

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM101719\
Data File : BM023252.D
Acq On : 18 Oct 2019 11:15
Operator : JU
Sample : K5235-15DL 2X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEPB5DL

Manual Integrations
APPROVED




mohammad
10/20/2019 8:07:27 PM

mohammad
10/20/2019 8:07:27 PM

Quant Time: Oct 18 15:31:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 18 07:48:41 2019
Response via : Initial Calibration

10/20/2019 8:07:27 PM

Ion 252.00 (251.70 to 252.70): BM023252.D
Ion 253.00 (252.70 to 253.70): BM023252.D
Ion 125.00 (124.70 to 125.70): BM023252.D

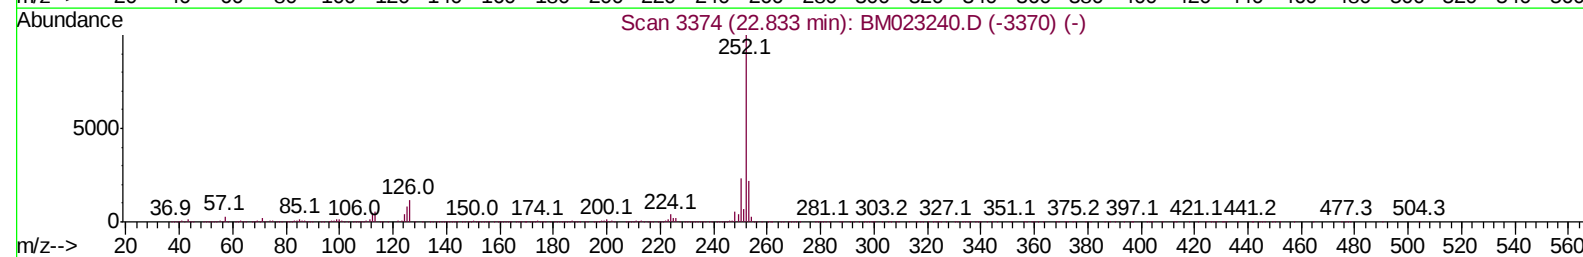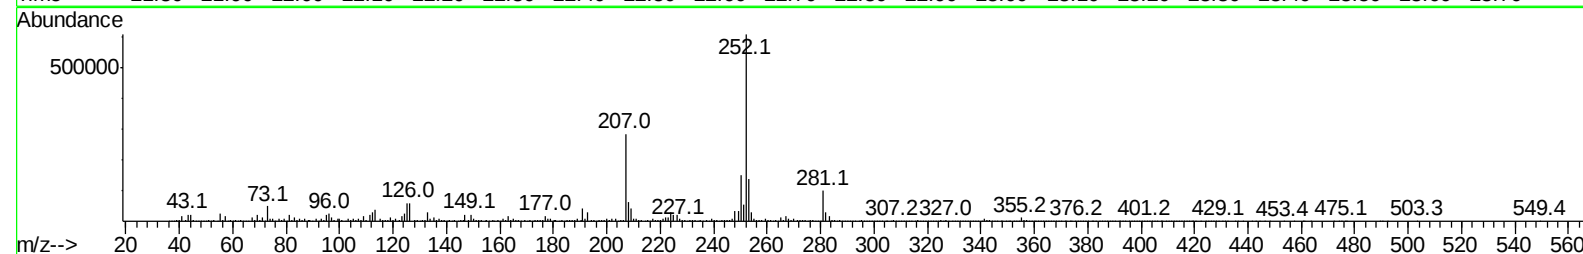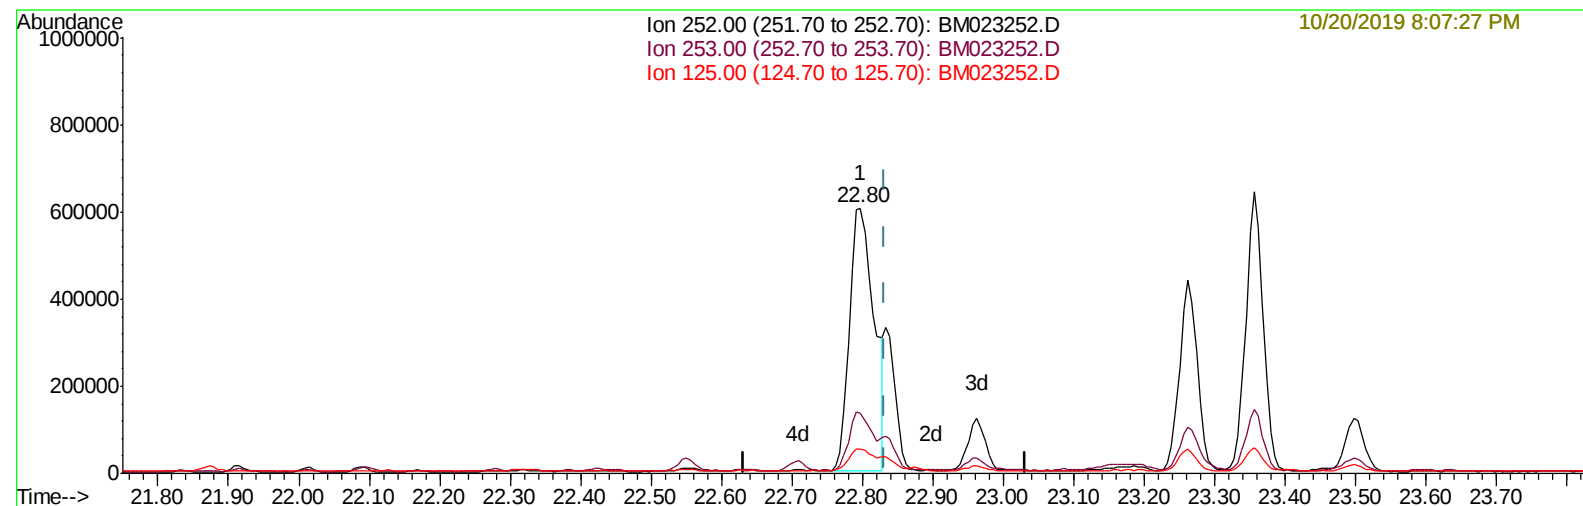

TIC: BM023252.D

(89) Benzo(k)fluoranthene
22.797min (-0.036) 7.78ng/ul
response 1453136

Ion	Exp%	Act%
252.00	100	100
253.00	21.70	22.68
125.00	8.10	9.43
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM101719\
Data File : BM023252.D
Acq On : 18 Oct 2019 11:15
Operator : JU
Sample : K5235-15DL 2X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEPB5DL




Manual Integrations
APPROVED

mohammad
10/20/2019 8:07:27 PM

mohammad
10/20/2019 8:07:27 PM

Quant Time: Oct 18 15:31:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 18 07:48:41 2019
Response via : Initial Calibration

10/20/2019 8:07:27 PM

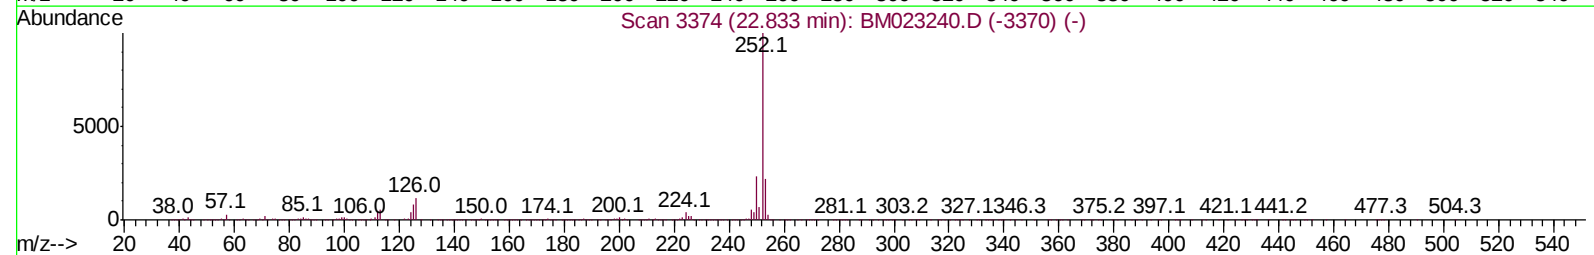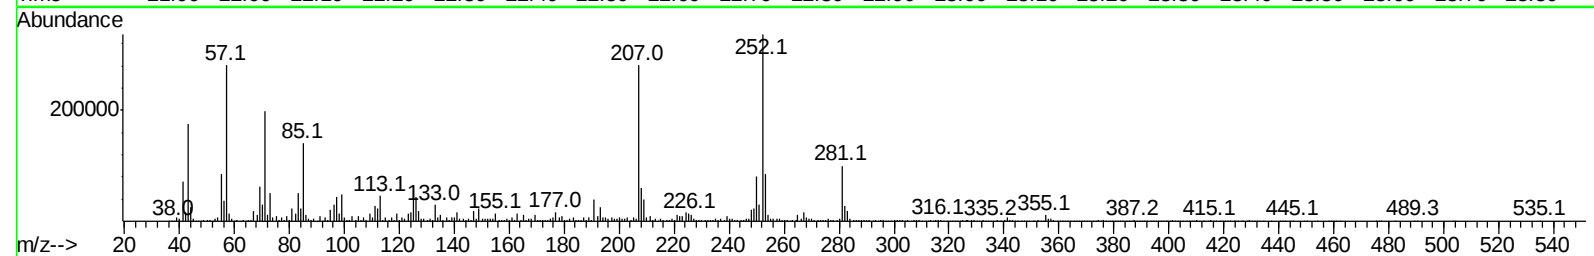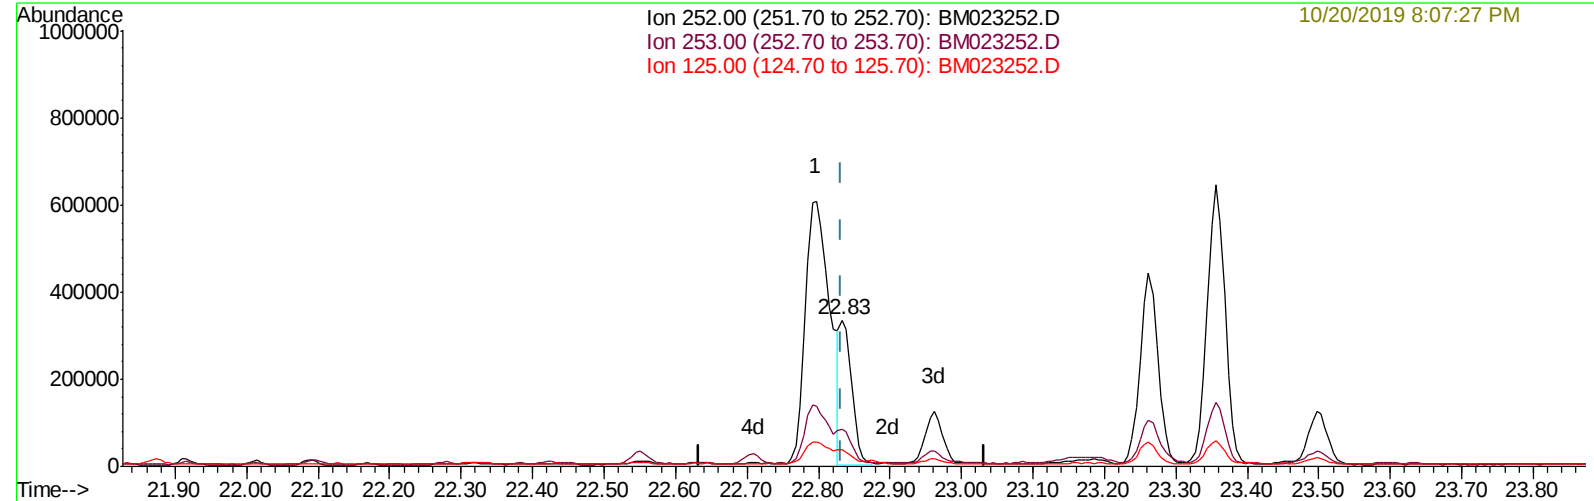

TIC: BM023252.D

(89) Benzo(k)fluoranthene

22.833min (-0.000) 2.00ng/ul m

response 373268

Ion	Exp%	Act%
252.00	100	100
253.00	21.70	25.46
125.00	8.10	11.45#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM101719\
 Data File : BM023252.D
 Acq On : 18 Oct 2019 11:15
 Operator : JU
 Sample : K5235-15DL 2X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BEPB5DL

Manual Integrations
 APPROVED

mohammad
 10/20/2019 8:07:27 PM

mohammad
 10/20/2019 8:07:27 PM

Quant Time: Oct 18 15:34:45 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 18 07:48:41 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)	10/20/2019 8:07:27 PM
1) 1,4-Dichlorobenzene-d4	7.66	152	470092	20.00	ng/ul	0.00	
18) Naphthalene-d8	10.44	136	1852234	20.00	ng/ul	0.00	
36) Acenaphthene-d10	14.30	164	1204972	20.00	ng/ul	0.00	
62) Phenanthrene-d10	17.05	188	2549076	20.00	ng/ul	0.00	
78) Chrysene-d12	21.24	240	2655997	20.00	ng/ul	0.00	
86) Perylene-d12	23.46	264	3207373	20.00	ng/ul	0.00	
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.17	96	16162	1.51	ng/uL	0.00	
5) Phenol-d5	6.83	99	314293	7.68	ng/ul	0.00	
7) Bis-(2-Chloroethyl)ether-d	7.00	67	183391	7.92	ng/ul	0.00	
9) 2-Chlorophenol-d4	7.19	132	265652	8.48	ng/ul	0.00	
13) 4-Methylphenol-d8	8.36	113	238150	7.24	ng/ul	0.00	
19) Nitrobenzene-d5	8.80	128	122078	9.74	ng/ul	0.00	
22) 2-Nitrophenol-d4	9.52	143	132861	11.13	ng/ul	0.00	
26) 2,4-Dichlorophenol-d3	10.06	165	268110	8.84	ng/ul	0.00	
29) 4-Chloroaniline-d4	10.57	131	219949	5.96	ng/ul	0.00	
44) Dimethylphthalate-d6	13.72	166	820410	8.88	ng/ul	0.00	
47) Acenaphthylene-d8	13.99	160	963552	8.90	ng/ul	0.00	
52) 4-Nitrophenol-d4	14.50	143	92751	6.20	ng/ul	0.00	
58) Fluorene-d10	15.30	176	727300	9.24	ng/ul	0.00	
63) 4,6-Dinitro-2-methylphenol	15.42	200	60643	6.00	ng/ul	0.00	
71) Anthracene-d10	17.14	188	1130927	9.20	ng/ul	0.00	
79) Pyrene-d10	19.44	212	1280146	9.95	ng/ul	0.00	
90) Benzo(a)pyrene-d12	23.31	264	1528697	9.40	ng/ul	0.00	
Target Compounds							
						Ovalue	
6) Phenol	6.86	94	49454	1.171	ng/ul	98	
45) Dimethylphthalate	13.77	163	274918	2.974	ng/ul	99	
70) Phenanthrene	17.09	178	639719	4.472	ng/ul	98	
72) Anthracene	17.18	178	200685	1.358	ng/ul	99	
77) Fluoranthene	19.11	202	1549517	9.108	ng/ul	100	
80) Pyrene	19.47	202	1826587	10.978	ng/ul	99	
83) Benzo(a)anthracene	21.23	228	1103976	6.134	ng/ul	97	
84) Bis(2-ethylhexyl)phthalate	21.19	149	2654716	28.850	ng/ul	99	
85) Chrysene	21.28	228	1136213	6.799	ng/ul	98	
88) Benzo(b)fluoranthene	22.80	252	1453136	7.472	ng/ul	98	
89) Benzo(k)fluoranthene	22.83	252	373268m	1.999	ng/ul		
91) Benzo(a)pyrene	23.36	252	1112053	5.960	ng/ul	98	
92) Indeno(1,2,3-cd)pyrene	25.67	276	694306	3.128	ng/ul	97	
93) Dibenzo(a,h)anthracene	25.67	278	207879	1.120	ng/ul#	82	
94) Benzo(g,h,i)perylene	26.34	276	714283	3.909	ng/ul	98	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM101719\
Data File : BM023252.D
Acq On : 18 Oct 2019 11:15
Operator : JU
Sample : K5235-15DL 2X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
BEPB5DL

Manual Integrations
APPROVED

mohammad
10/20/2019 8:07:27 PM

Quant Time: Oct 18 15:34:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 18 07:48:41 2019
Response via : Initial Calibration

mohammad
10/20/2019 8:07:27 PM

