

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM101719\
 Data File : BM023237.D
 Acq On : 18 Oct 2019 01:41
 Operator : JU
 Sample : K5236-14
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BEPM5

Quant Time: Oct 18 06:59:35 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 18 06:52:01 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	381536	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	1482664	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.31	164	914509	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.05	188	1850979	20.00	ng/ul	0.00
78) Chrysene-d12	21.24	240	1917925	20.00	ng/ul	-0.01
86) Perylene-d12	23.45	264	2326331	20.00	ng/ul	-0.01

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.18	96	26448	3.05	ng/uL	0.00
5) Phenol-d5	6.83	99	471866	14.20	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	281388	14.97	ng/ul	0.00
9) 2-Chlorophenol-d4	7.20	132	405230	15.93	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	357161	13.38	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	188188	18.76	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	205514	21.52	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	393653	16.21	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	483893	16.38	ng/ul	0.00
44) Dimethylphthalate-d6	13.72	166	1187186	16.94	ng/ul	0.00
47) Acenaphthylene-d8	14.00	160	1380258	16.79	ng/ul	0.00
52) 4-Nitrophenol-d4	14.50	143	134547	11.86	ng/ul	0.00
58) Fluorene-d10	15.30	176	1018496	17.06	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.42	200	102047	13.91	ng/ul	0.00
71) Anthracene-d10	17.15	188	1590272	17.82	ng/ul	0.00
79) Pyrene-d10	19.44	212	1955162	21.05	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.31	264	2377060	20.16	ng/ul	-0.01


Target Compounds					Ovalue	
6) Phenol	6.86	94	82097	2.396	ng/ul	98
45) Dimethylphthalate	13.77	163	438506	6.251	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM101719\
Data File : BM023237.D
Acq On : 18 Oct 2019 01:41
Operator : JU
Sample : K5236-14
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEPM5

Quant Time: Oct 18 06:59:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 18 06:52:01 2019
Response via : Initial Calibration

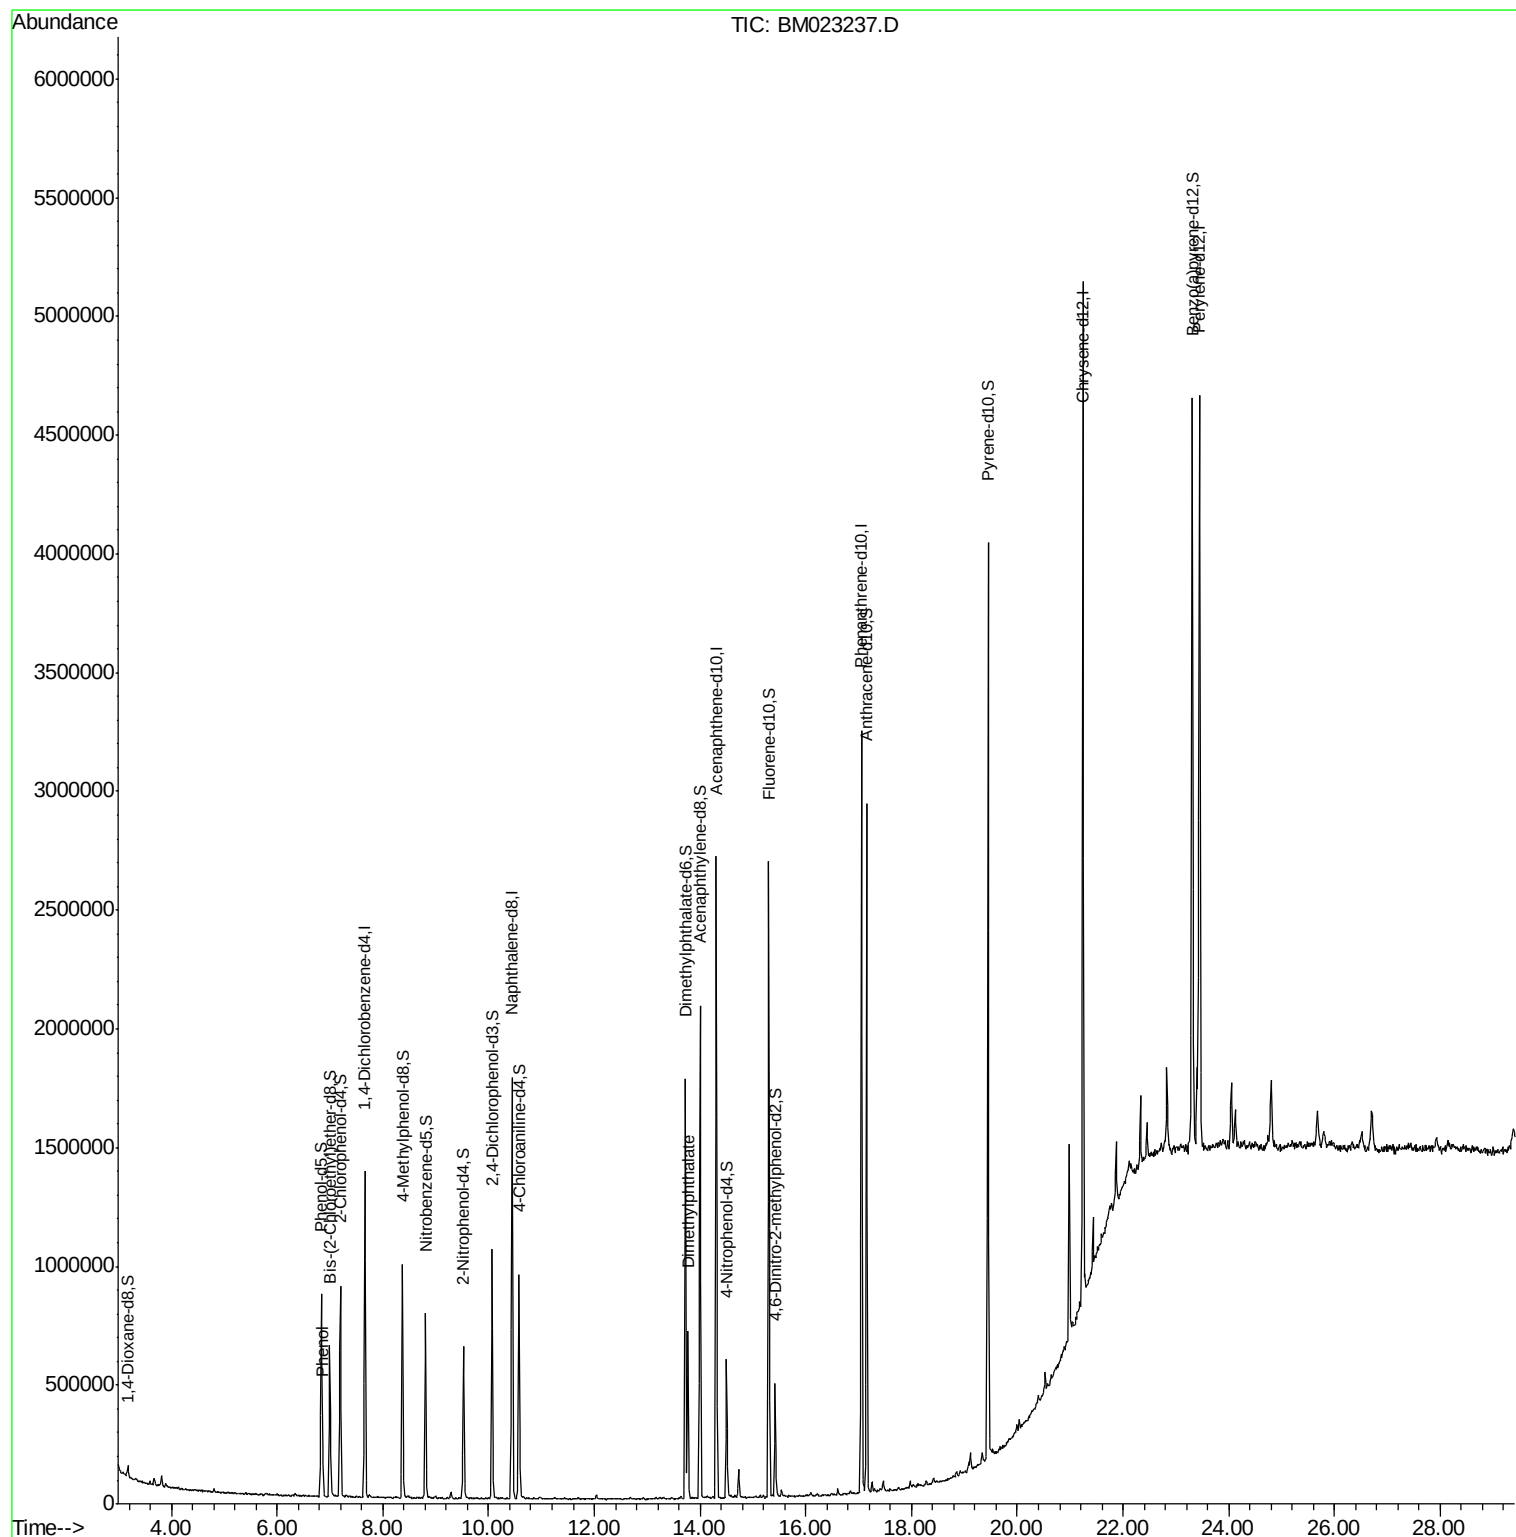

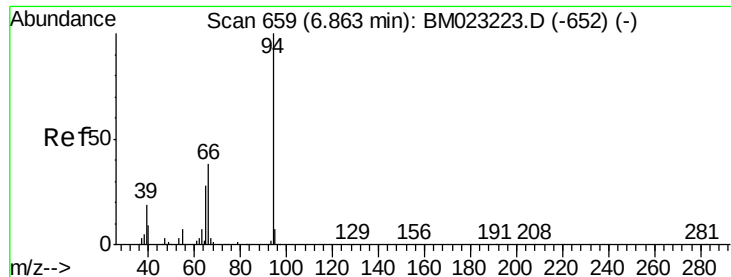

#6

Phenol

Concen: 2.396 ng/ul

RT: 6.86 min Scan# 659

Delta R.T. 0.00 min

Lab File: BM023237.D

Acq: 18 Oct 2019 01:41

Instrument :

BNA_M

ClientSampleId :

BEPM5


Tot Ion: 94 Resp: 82097

Ion Ratio Lower Upper

94 100

65 28.2 23.7 35.5




66 40.5 32.9 49.3

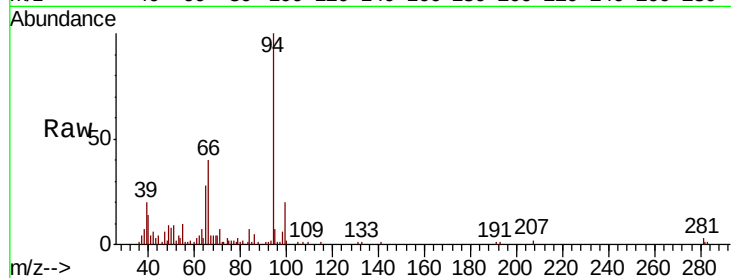

Abundance Ion 94.00 (93.70 to 94.70): BM023223.D (-652) (-)

Ion 65.00 (64.70 to 65.70): BM023223.D (-652) (-)

Ion 66.00 (65.70 to 66.70): BM023223.D (-652) (-)

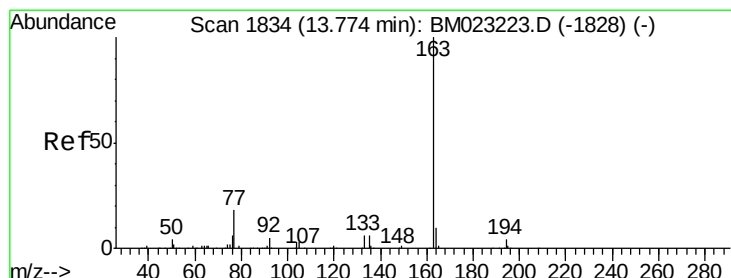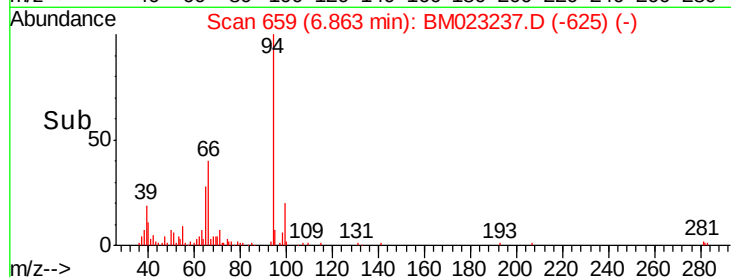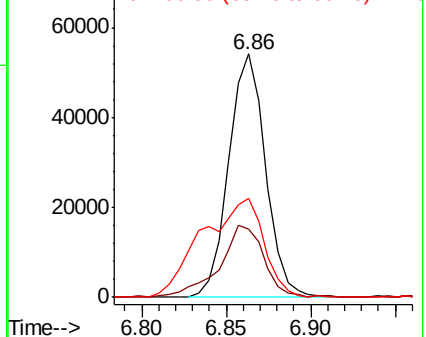

#45

Dimethylphthalate

Concen: 6.251 ng/ul

RT: 13.77 min Scan# 1833

Delta R.T. -0.01 min

Lab File: BM023237.D

Acq: 18 Oct 2019 01:41


Tgt Ion:163 Resp: 438506

Ion Ratio Lower Upper

163 100

194 4.5 3.5 5.3

164 10.2 8.0 12.0

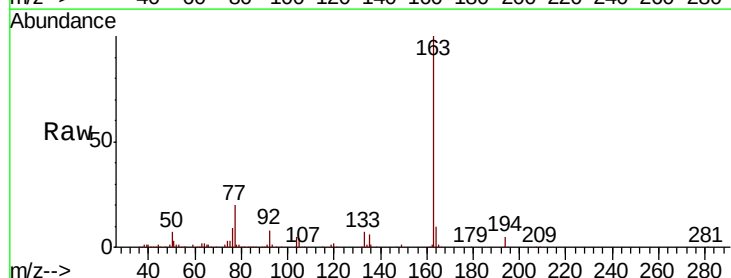

Abundance Ion 163.00 (162.70 to 163.70): BM023223.D (-1828) (-)

Ion 194.00 (193.70 to 194.70): BM023223.D (-1828) (-)

Ion 164.00 (163.70 to 164.70): BM023223.D (-1828) (-)

