

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM101719\
 Data File : BM023273.D
 Acq On : 19 Oct 2019 01:34
 Operator : JU
 Sample : K5345-15
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ETOK8

Quant Time: Oct 19 02:46:23 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 19 02:43:46 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	392593	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1545351	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.30	164	940181	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	1951076	20.00	ng/ul	0.00
78) Chrysene-d12	21.23	240	2083680	20.00	ng/ul	0.00
86) Perylene-d12	23.44	264	2473318	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.17	96	71690	8.04	ng/uL	0.00
5) Phenol-d5	6.83	99	1277011	37.35	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	750702	38.81	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	1037710	39.65	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	998328	36.35	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	493803	47.23	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	538695	54.11	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	1039397	41.05	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	1351413	43.88	ng/ul	0.00
44) Dimethylphthalate-d6	13.72	166	2980844	41.37	ng/ul	0.00
47) Acenaphthylene-d8	13.99	160	3569941	42.25	ng/ul	0.00
52) 4-Nitrophenol-d4	14.50	143	452235	38.77	ng/ul	0.00
58) Fluorene-d10	15.30	176	2581832	42.06	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.42	200	331999	42.92	ng/ul	0.00
71) Anthracene-d10	17.14	188	3976559	42.27	ng/ul	0.00
79) Pyrene-d10	19.44	212	4457093	44.17	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.30	264	5323642	42.46	ng/ul	0.00
Target Compounds						
6) Phenol	6.85	94	160217	4.544	ng/ul	97
45) Dimethylphthalate	13.76	163	898587	12.461	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM101719\
Data File : BM023273.D
Acq On : 19 Oct 2019 01:34
Operator : JU
Sample : K5345-15
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ETOK8

Quant Time: Oct 19 02:46:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 19 02:43:46 2019
Response via : Initial Calibration

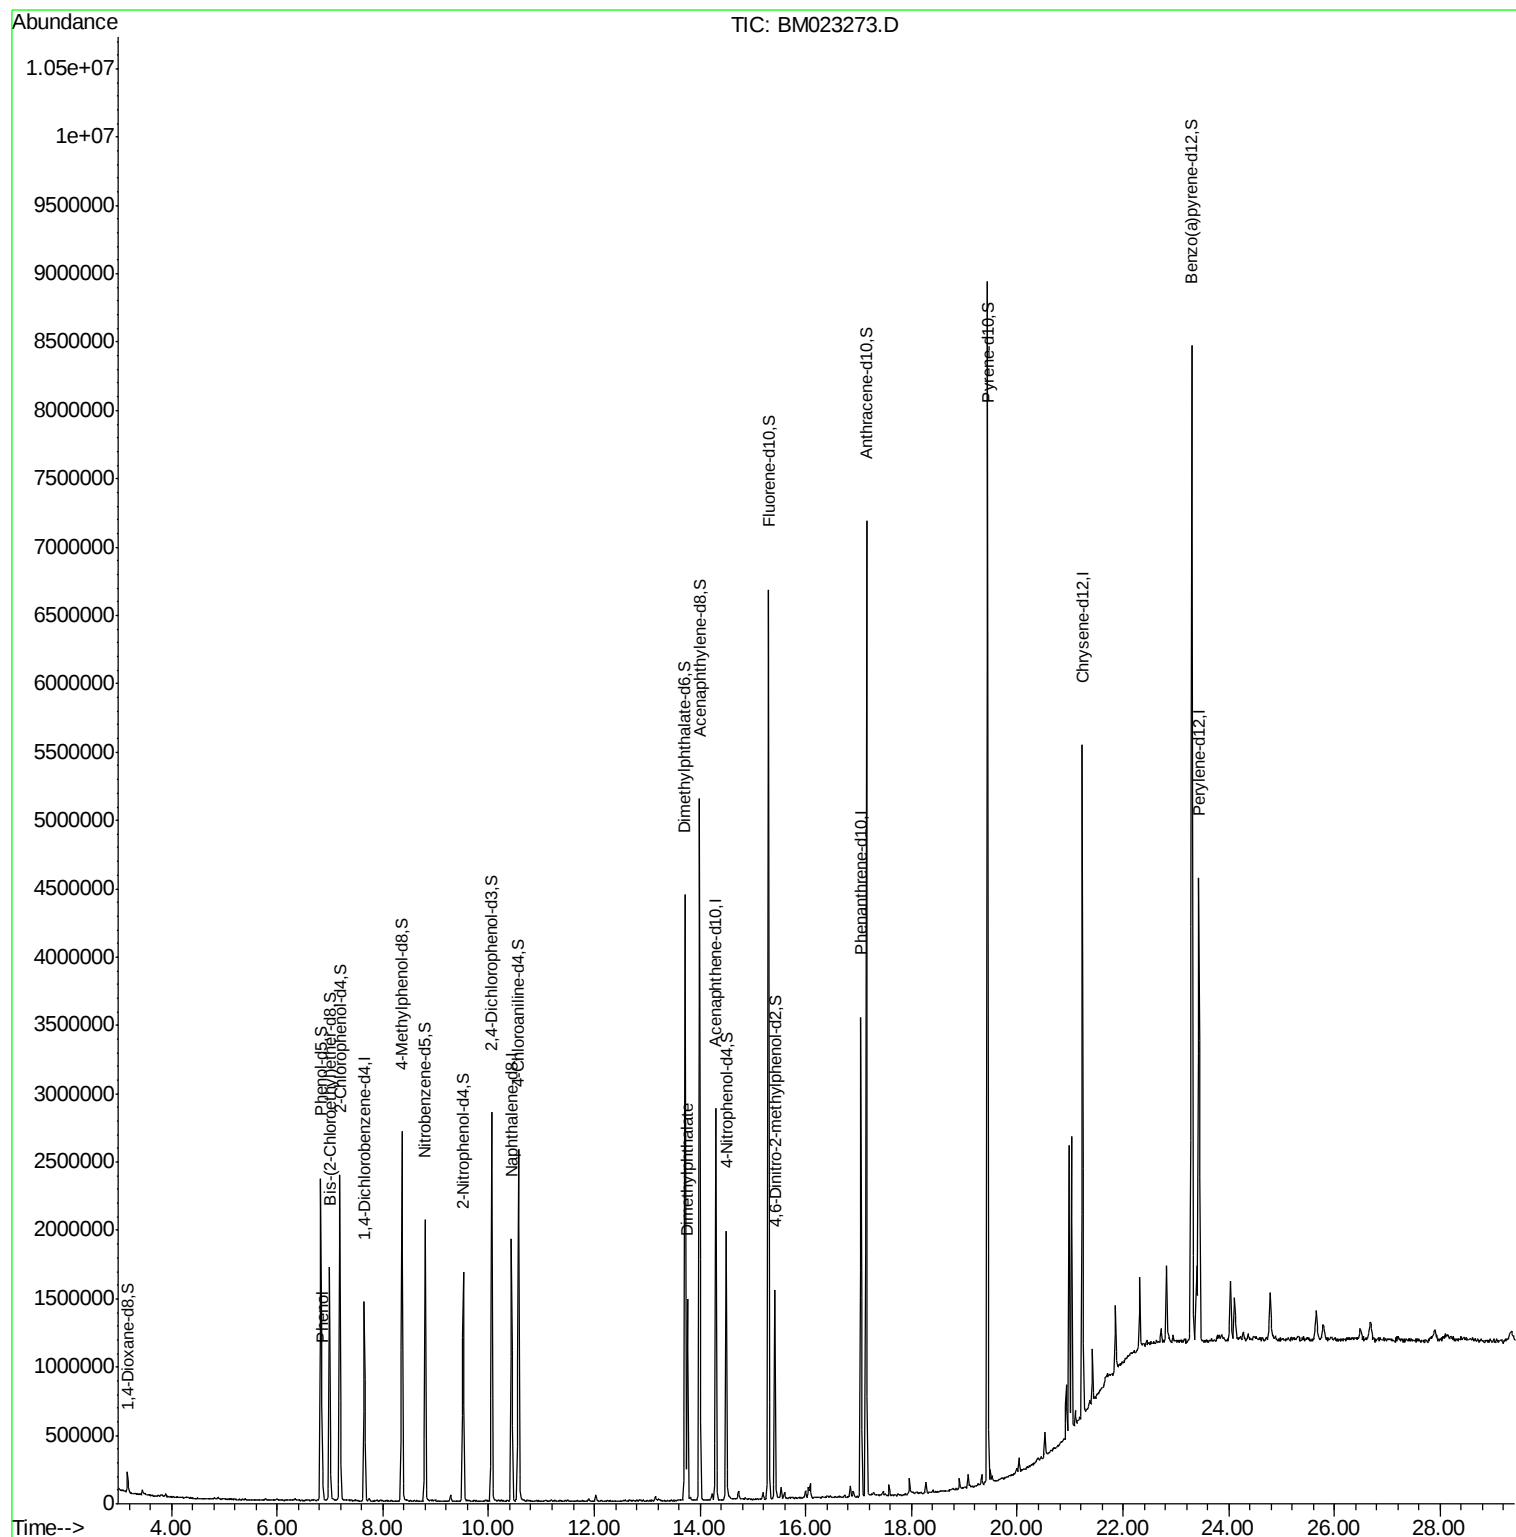

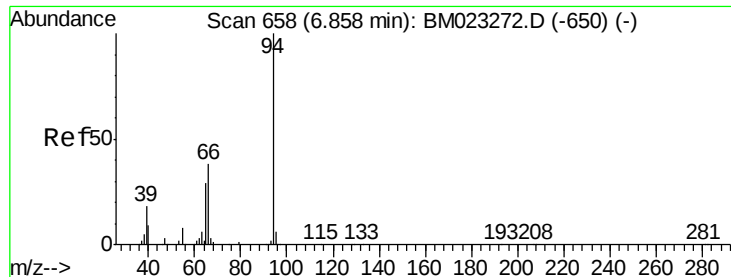

#6

Phenol

Concen: 4.544 ng/ul

RT: 6.85 min Scan# 657

Delta R.T. -0.01 min

Lab File: BM023273.D

Acq: 19 Oct 2019 01:34

Instrument :

BNA_M

ClientSampleId :

ETOK8


Tot Ion: 94 Resp: 160217

Ion Ratio Lower Upper




94 100

65 29.0 23.7 35.5

66 43.8 32.9 49.3

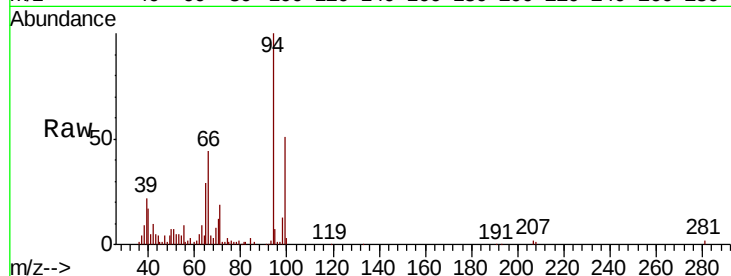

Abundance Ion 94.00 (93.70 to 94.70): BM023273.D (-624) (-)

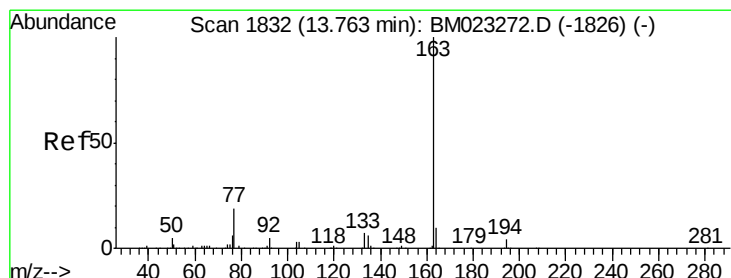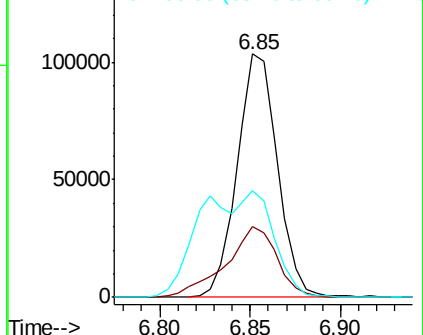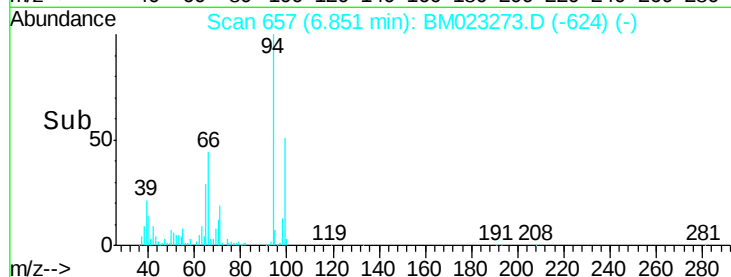

#45

Dimethylphthalate

Concen: 12.461 ng/ul

RT: 13.76 min Scan# 1832

Delta R.T. -0.00 min

Lab File: BM023273.D

Acq: 19 Oct 2019 01:34


Tgt Ion: 163 Resp: 898587

Ion Ratio Lower Upper

163 100

194 4.4 3.5 5.3

164 10.2 8.0 12.0

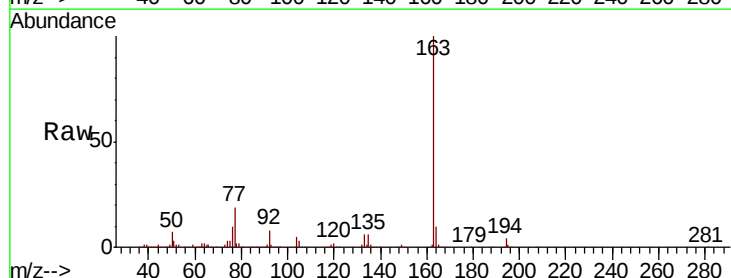

Abundance Ion 163.00 (162.70 to 163.70): BM023273.D (-1798) (-)

