

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101723\
 Data File : BM042333.D
 Acq On : 17 Oct 2023 22:41
 Operator : MA/JU
 Sample : 04885-02 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COM26

Quant Time: Oct 18 02:07:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 18 02:04:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.010	152	143161	20.000	ng/ul	0.00
20) Naphthalene-d8	10.833	136	644420	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.651	164	388908	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.404	188	831749	20.000	ng/ul	0.00
79) Chrysene-d12	21.580	240	750783	20.000	ng/ul	0.00
88) Perylene-d12	24.050	264	777912	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	9982	2.179	ng/uL	0.00
4) Pyridine-d5	3.810	84	127445	9.392	ng/ul	0.00
7) Phenol-d5	7.157	99	104533	6.589	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.351	67	315581	29.438	ng/ul	0.00
11) 2-Chlorophenol-d4	7.534	132	246956	22.627	ng/ul	0.00
15) 4-Methylphenol-d8	8.716	113	183461	14.601	ng/ul	0.00
21) Nitrobenzene-d5	9.210	128	158728	29.002	ng/ul	0.00
24) 2-Nitrophenol-d4	9.922	143	162405	27.759	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.445	165	286287	26.814	ng/ul	0.00
31) 4-Chloroaniline-d4	10.992	131	303164	18.034	ng/ul	0.00
46) Dimethylphthalate-d6	14.069	166	1035576	30.717	ng/ul	0.00
49) Acenaphthylene-d8	14.357	160	1120445	30.366	ng/ul	0.00
54) 4-Nitrophenol-d4	14.863	143	39787	5.868	ng/ul	0.00
60) Fluorene-d10	15.645	176	893448	32.239	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.768	200	150332	25.801	ng/ul	0.00
73) Anthracene-d10	17.504	188	1617316	37.959	ng/ul	0.00
81) Pyrene-d10	19.792	212	1952181	42.663	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.891	264	1759405	41.205	ng/ul	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.445	149	234881	6.547	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101723\
Data File : BM042333.D
Acq On : 17 Oct 2023 22:41
Operator : MA/JU
Sample : 04885-02 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COM26

Quant Time: Oct 18 02:07:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 18 02:04:27 2023
Response via : Initial Calibration

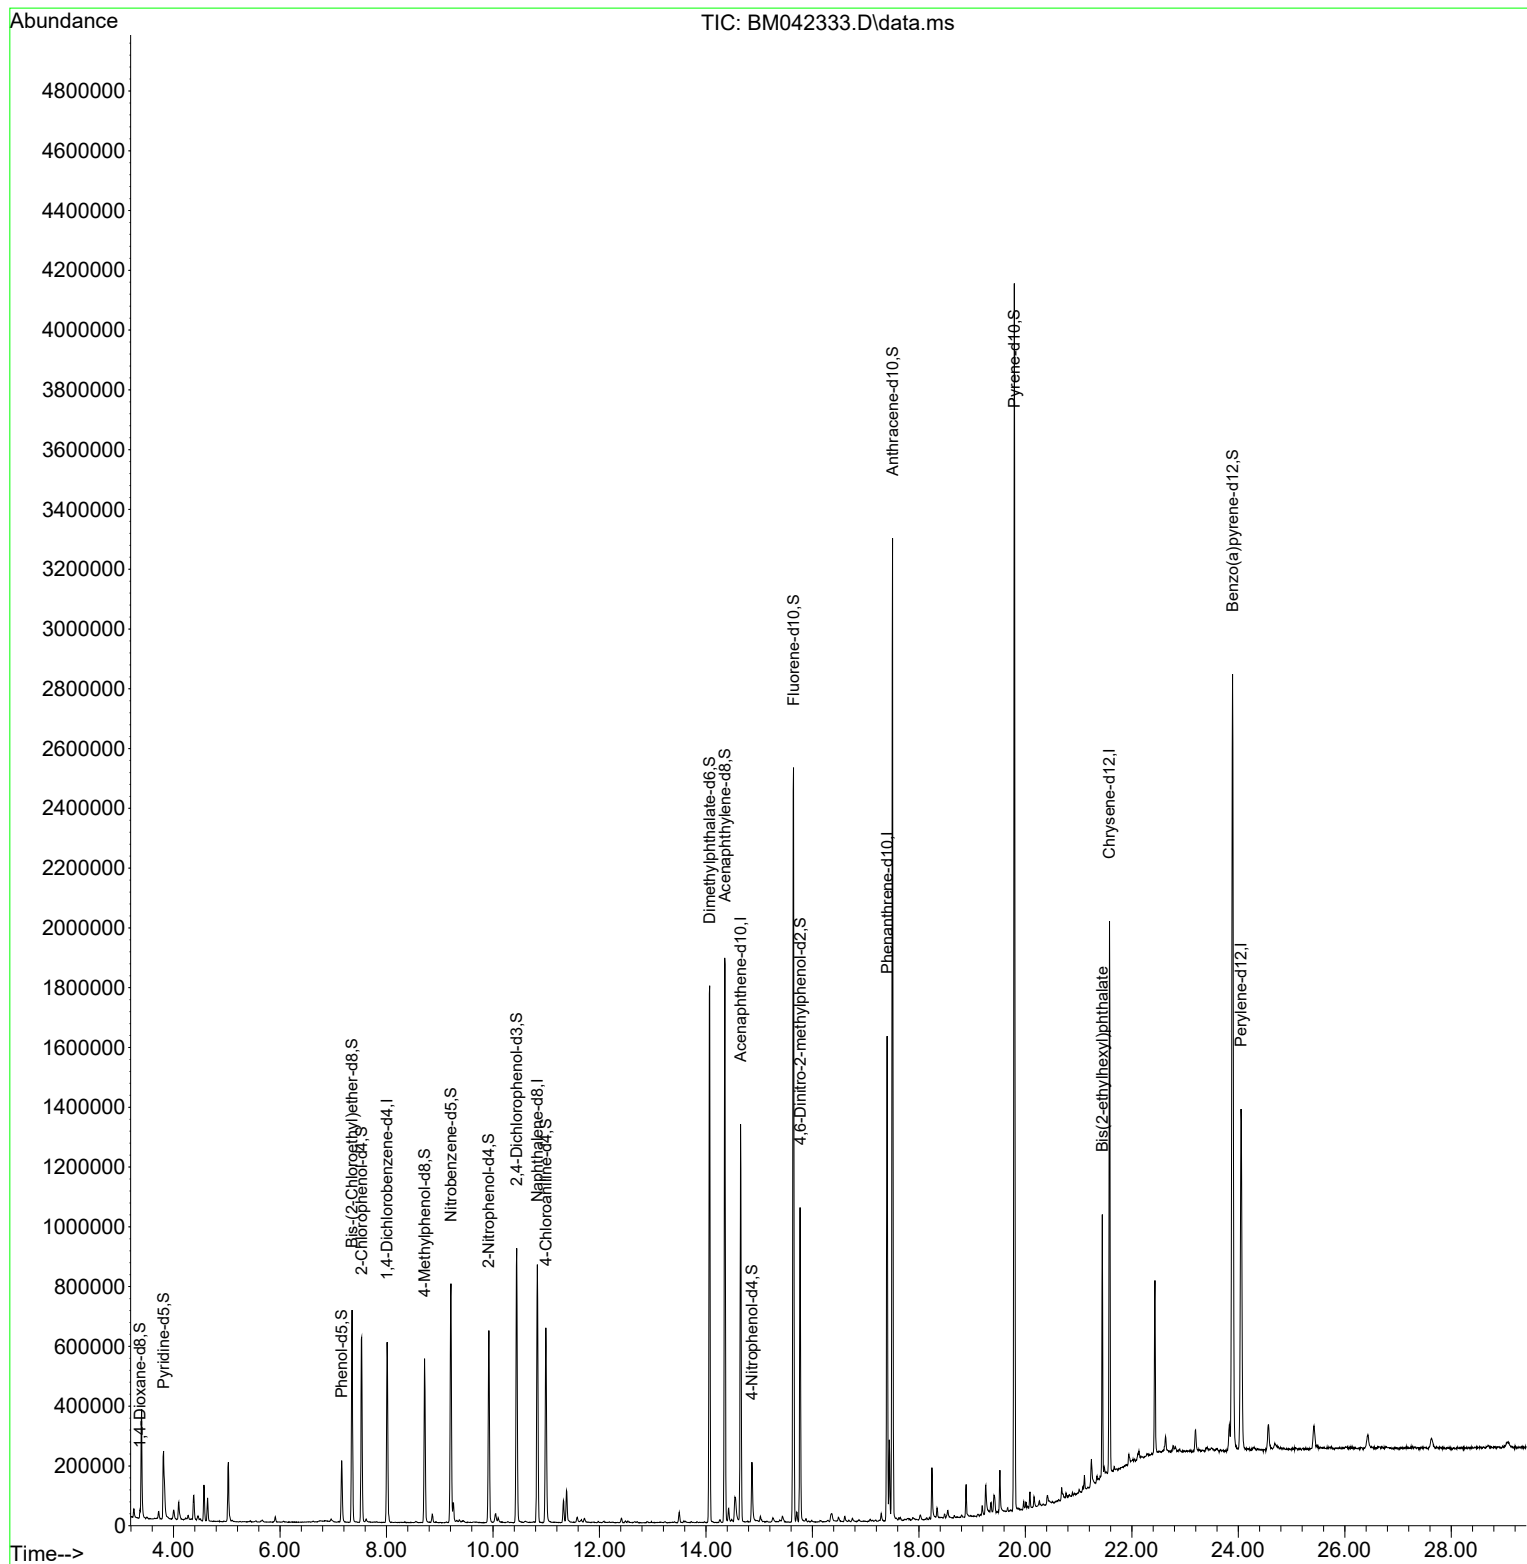

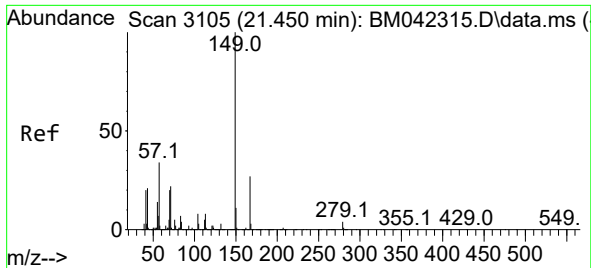

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 6.547 ng/ul
 RT: 21.445 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: BM042333.D
 Acq: 17 Oct 2023 22:41

Instrument :
 BNA_M
 ClientSampleId :
 COM26

Tgt Ion:149 Resp: 234881
 Ion Ratio Lower Upper
 149 100
 167 26.0 21.1 31.7
 279 3.0 2.4 3.6

