

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101723\
 Data File : BM042320.D
 Acq On : 17 Oct 2023 13:45
 Operator : MA/JU
 Sample : PB156335BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK335

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042320.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	27	31	43	rVB	69554	100130	1.87%	0.177%
2	3.804	101	105	125	rBV	842601	1395894	26.02%	2.466%
3	4.116	155	158	164	rVB	11069	16393	0.31%	0.029%
4	7.157	668	675	686	rBV	1074548	1647058	30.70%	2.910%
5	7.351	698	708	720	rBV	885799	1337129	24.92%	2.363%
6	7.528	731	738	751	rBV	983466	1560183	29.08%	2.757%
7	8.010	813	820	828	rVB	652959	1009844	18.82%	1.784%
8	8.716	933	940	951	rBV	1281794	1970643	36.73%	3.482%
9	9.210	1016	1024	1035	rBV	997674	1628499	30.35%	2.877%
10	9.922	1138	1145	1157	rBV	854073	1345773	25.08%	2.378%
11	10.445	1226	1234	1248	rBV	1172401	1919565	35.78%	3.392%
12	10.833	1292	1300	1308	rBV	970062	1568186	29.23%	2.771%
13	10.992	1319	1327	1342	rBV	1233525	2103047	39.20%	3.716%
14	12.416	1563	1569	1574	rBV2	17245	27753	0.52%	0.049%
15	13.498	1746	1753	1760	rBV	17501	26637	0.50%	0.047%
16	14.068	1843	1850	1857	rBV	2250488	2995172	55.82%	5.292%
17	14.357	1892	1899	1911	rBV	2360068	3410663	63.57%	6.026%
18	14.651	1942	1949	1961	rBV	1428244	2098685	39.11%	3.708%
19	14.863	1978	1985	1999	rBV	1193141	1670814	31.14%	2.952%
20	15.645	2111	2118	2125	rBV	3188776	4285497	79.87%	7.572%
21	15.768	2133	2139	2154	rBV	1086593	1431526	26.68%	2.529%
22	15.880	2154	2158	2162	rVB	12792	16888	0.31%	0.030%
23	17.404	2410	2417	2427	rBV	1849135	2506447	46.71%	4.429%
24	17.504	2427	2434	2451	rBV2	3425000	4630639	86.30%	8.182%
25	18.245	2556	2560	2564	rBV5	5576	9521	0.18%	0.017%
26	19.356	2744	2749	2753	rBV2	34378	48348	0.90%	0.085%
27	19.427	2757	2761	2765	rVB	36184	46382	0.86%	0.082%
28	19.662	2799	2801	2806	rVB5	9628	10626	0.20%	0.019%
29	19.797	2818	2824	2833	rBV	4241330	5365494	100.00%	9.480%
30	21.586	3123	3128	3137	rVB	2134255	2611555	48.67%	4.614%
31	23.897	3514	3521	3536	rVB2	2631122	5147055	95.93%	9.094%
32	24.062	3542	3549	3561	rVB	1289897	2653828	49.46%	4.689%




Sum of corrected areas: 56595874

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101723\
Data File : BM042320.D
Acq On : 17 Oct 2023 13:45
Operator : MA/JU
Sample : PB156335BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK335

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

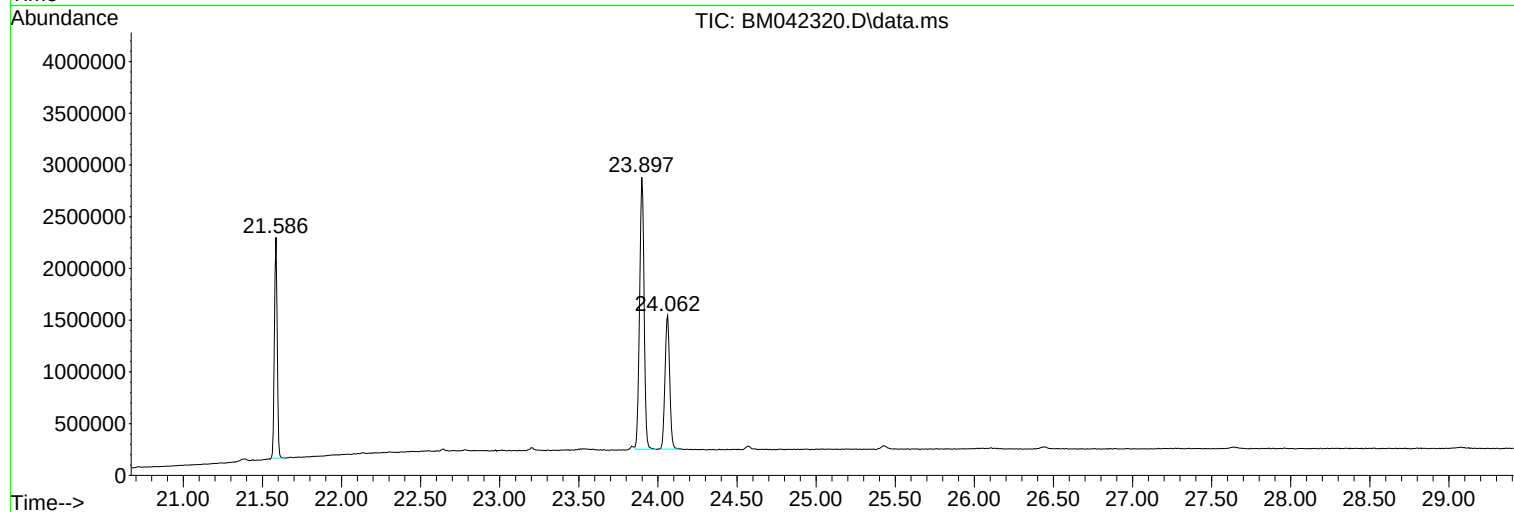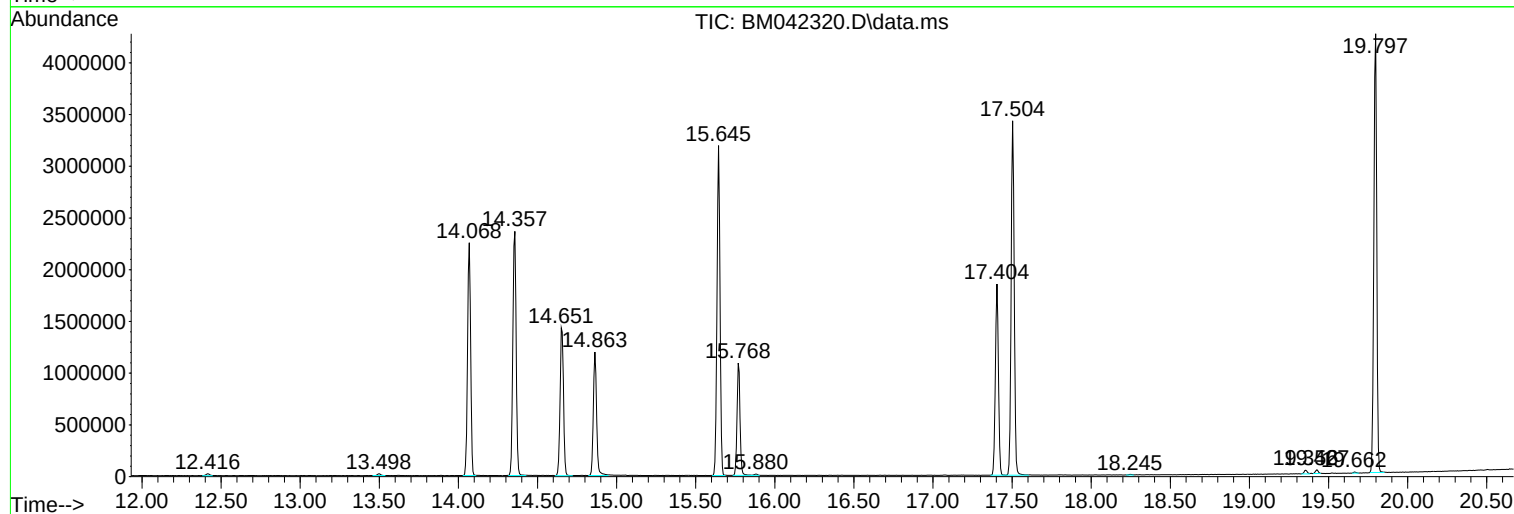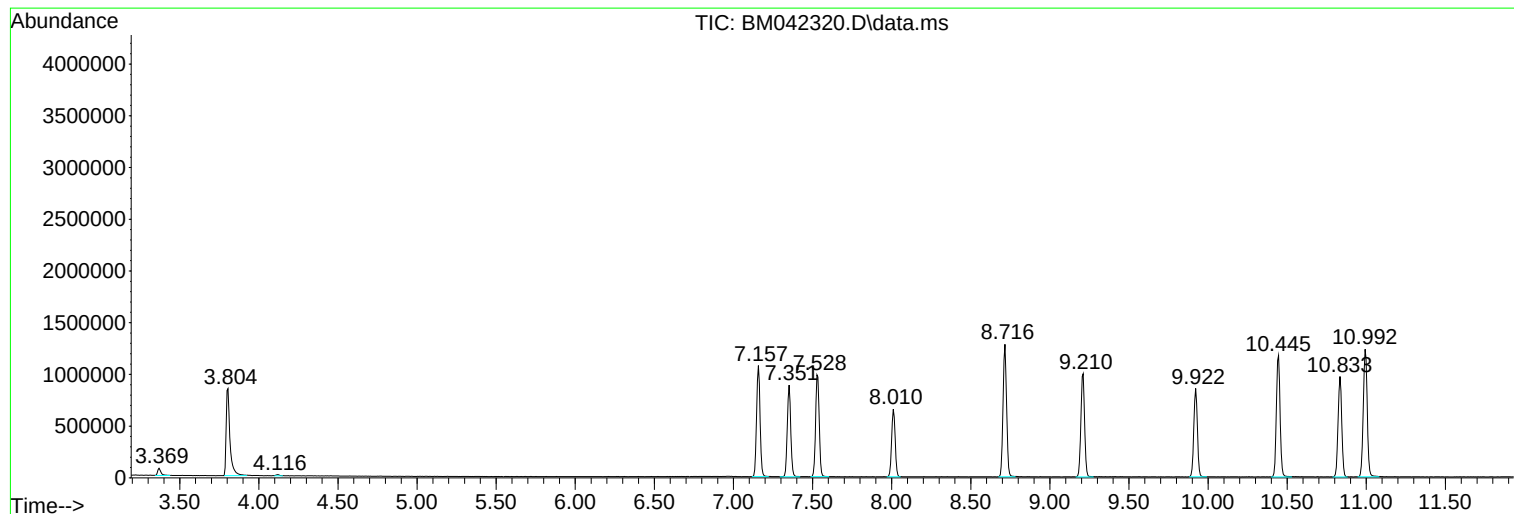

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101723\
Data File : BM042320.D
Acq On : 17 Oct 2023 13:45
Operator : MA/JU
Sample : PB156335BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK335

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101723\
Data File : BM042320.D
Acq On : 17 Oct 2023 13:45
Operator : MA/JU
Sample : PB156335BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK335

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------