

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101723\
 Data File : BM042326.D
 Acq On : 17 Oct 2023 18:23
 Operator : MA/JU
 Sample : PB156421BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK421

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042326.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	27	31	41	rVB	69100	99924	1.85%	0.175%
2	3.804	101	105	126	rBV	885747	1410844	26.10%	2.473%
3	4.116	155	158	165	rVB	15858	23393	0.43%	0.041%
4	7.157	668	675	691	rBV	1106543	1703473	31.52%	2.986%
5	7.351	701	708	718	rVB	911531	1374550	25.43%	2.409%
6	7.534	732	739	749	rBV	1038949	1604866	29.69%	2.813%
7	8.010	814	820	830	rVB	646819	1026573	18.99%	1.799%
8	8.716	933	940	949	rBV	1318958	2030852	37.58%	3.560%
9	9.210	1016	1024	1035	rBV	1063308	1679186	31.07%	2.943%
10	9.922	1138	1145	1154	rBV	867681	1385379	25.63%	2.428%
11	10.445	1226	1234	1253	rBV	1221107	1956189	36.19%	3.429%
12	10.833	1293	1300	1308	rVB	955492	1573621	29.12%	2.758%
13	10.992	1320	1327	1344	rBV	1274991	2190447	40.53%	3.839%
14	12.416	1561	1569	1578	rBV2	17880	34646	0.64%	0.061%
15	13.498	1748	1753	1758	rVB	15827	23292	0.43%	0.041%
16	14.068	1844	1850	1863	rVB	2299397	3041526	56.28%	5.331%
17	14.357	1892	1899	1908	rBV	2400896	3435559	63.57%	6.022%
18	14.651	1943	1949	1959	rVB	1405149	2099075	38.84%	3.679%
19	14.862	1979	1985	2003	rBV	1189907	1706503	31.57%	2.991%
20	15.645	2111	2118	2125	rBV	3114975	4279028	79.17%	7.500%
21	15.768	2133	2139	2152	rBV	1165013	1541752	28.53%	2.702%
22	15.880	2154	2158	2165	rVB4	14745	21060	0.39%	0.037%
23	17.404	2411	2417	2425	rVB	1827630	2457698	45.47%	4.308%
24	17.503	2427	2434	2453	rBV2	3435772	4685867	86.70%	8.214%
25	19.356	2744	2749	2753	rBV2	33894	44769	0.83%	0.078%
26	19.427	2757	2761	2766	rVB	36028	43853	0.81%	0.077%
27	19.668	2799	2802	2806	rBV4	10599	11831	0.22%	0.021%
28	19.797	2817	2824	2833	rBV	4293816	5404633	100.00%	9.473%
29	21.586	3123	3128	3135	rBV	1991055	2499573	46.25%	4.381%
30	23.838	3507	3511	3514	rBV	103282	163708	3.03%	0.287%
31	23.897	3514	3521	3533	rVB2	2514865	5027946	93.03%	8.813%
32	24.056	3541	3548	3558	rBV	1237371	2468984	45.68%	4.328%




Sum of corrected areas: 57050600

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101723\
Data File : BM042326.D
Acq On : 17 Oct 2023 18:23
Operator : MA/JU
Sample : PB156421BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK421

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

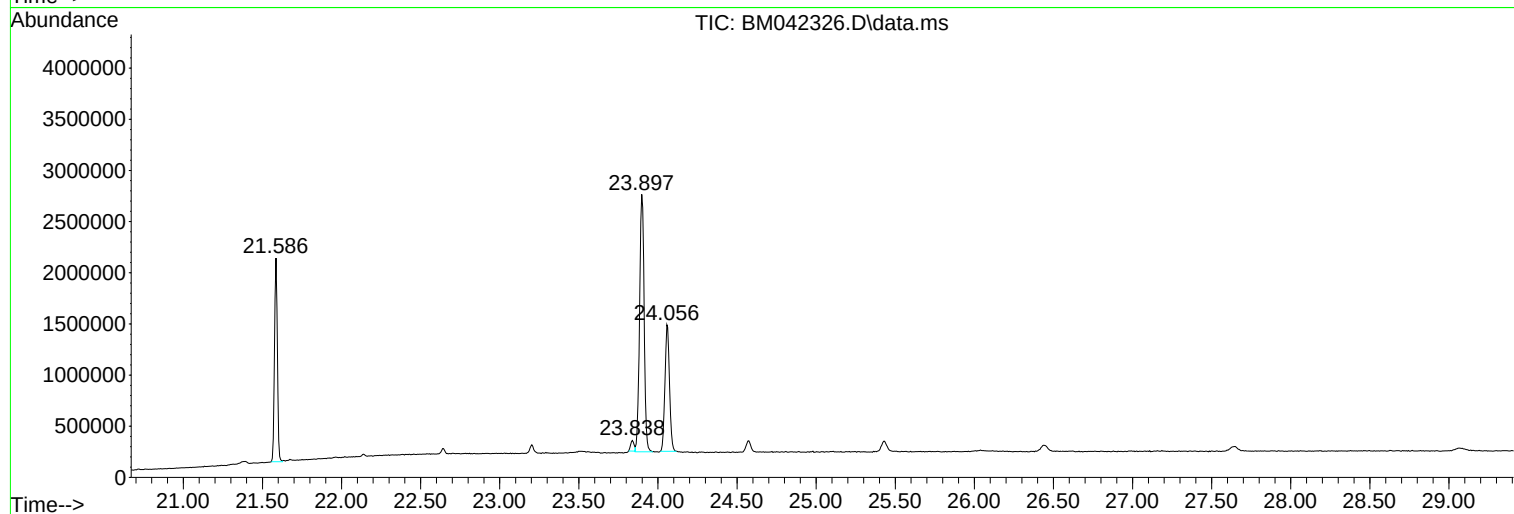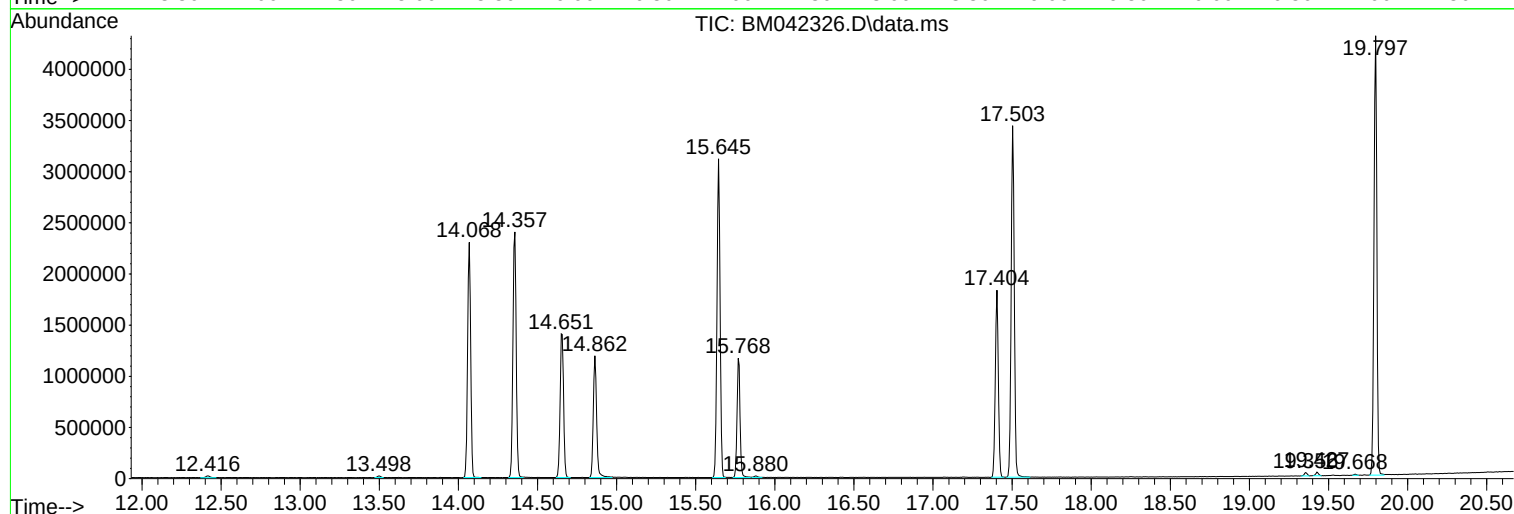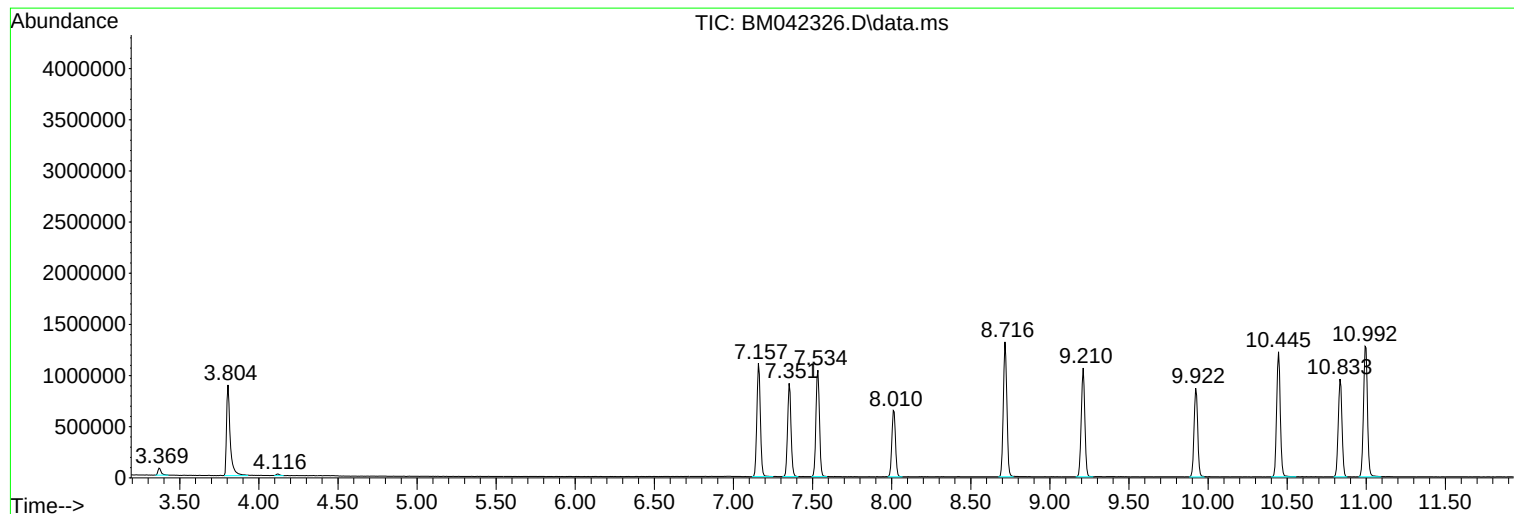

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101723\
Data File : BM042326.D
Acq On : 17 Oct 2023 18:23
Operator : MA/JU
Sample : PB156421BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK421

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101723\
Data File : BM042326.D
Acq On : 17 Oct 2023 18:23
Operator : MA/JU
Sample : PB156421BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK421

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc