

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101723\
 Data File : BM042334.D
 Acq On : 17 Oct 2023 23:17
 Operator : MA/JU
 Sample : 04885-03 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COM27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042334.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	28	31	34	rBV	24654	35543	1.50%	0.129%
2	3.399	34	36	47	rVB	28294	40099	1.70%	0.145%
3	3.805	101	105	123	rBV	296515	506818	21.46%	1.832%
4	4.116	152	158	166	rVB2	11265	22951	0.97%	0.083%
5	4.375	200	202	208	rVB2	9357	12767	0.54%	0.046%
6	4.575	232	236	240	rVV	9300	13091	0.55%	0.047%
7	4.640	243	247	253	rVB5	5443	8380	0.35%	0.030%
8	5.028	308	313	317	rBV	15962	20174	0.85%	0.073%
9	5.351	364	368	371	rVB6	1654	2475	0.10%	0.009%
10	6.957	638	641	643	rBV3	2115	2407	0.10%	0.009%
11	7.157	668	675	685	rBV	370189	568753	24.08%	2.056%
12	7.351	700	708	717	rBV	361006	554301	23.47%	2.004%
13	7.422	717	720	723	rVB5	2025	2830	0.12%	0.010%
14	7.528	732	738	750	rVB	375655	602088	25.49%	2.177%
15	8.010	813	820	834	rVB	666429	1033366	43.75%	3.736%
16	8.716	932	940	950	rBV	445884	702423	29.74%	2.540%
17	9.210	1016	1024	1032	rBV	377177	628071	26.59%	2.271%
18	9.328	1040	1044	1045	rBV4	3107	2822	0.12%	0.010%
19	9.922	1138	1145	1152	rBV	296732	479207	20.29%	1.733%
20	10.269	1201	1204	1207	rBV4	2225	2673	0.11%	0.010%
21	10.445	1225	1234	1243	rBV	427444	702000	29.72%	2.538%
22	10.686	1271	1275	1279	rVB5	1908	2746	0.12%	0.010%
23	10.833	1293	1300	1310	rVB	932663	1530983	64.83%	5.535%
24	10.992	1320	1327	1340	rBV	429154	732238	31.00%	2.647%
25	11.339	1383	1386	1388	rVB4	3382	4127	0.17%	0.015%
26	11.392	1393	1395	1402	rVB4	3425	5998	0.25%	0.022%
27	11.592	1423	1429	1431	rBV4	1843	3166	0.13%	0.011%
28	11.904	1477	1482	1487	rVB5	2368	4777	0.20%	0.017%
29	12.228	1536	1537	1543	rBV5	1610	2794	0.12%	0.010%
30	12.416	1565	1569	1575	rBV4	6047	10930	0.46%	0.040%
31	13.498	1747	1753	1757	rBV	15209	23656	1.00%	0.086%
32	14.063	1843	1849	1856	rBV	828112	1127501	47.74%	4.076%
33	14.351	1890	1898	1906	rBV	883151	1254143	53.10%	4.534%
34	14.651	1942	1949	1957	rBV	1424371	2028583	85.89%	7.334%
35	14.763	1965	1968	1971	rVB4	1984	2800	0.12%	0.010%
36	14.863	1977	1985	1998	rBV	275098	456160	19.31%	1.649%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101723\
 Data File : BM042334.D
 Acq On : 17 Oct 2023 23:17
 Operator : MA/JU
 Sample : 04885-03 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COM27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
 Title : SVOA CALIBRATION

37	15.586	2103	2108	2110	rBV3	1633	2437	0.10%	0.009%
38	15.639	2111	2117	2125	rVB	1140774	1621467	68.66%	5.862%
39	15.768	2133	2139	2152	rBV	324254	427547	18.10%	1.546%
40	15.874	2155	2157	2164	rVB5	4467	5598	0.24%	0.020%
41	16.292	2224	2228	2231	rBV6	2483	4146	0.18%	0.015%
42	16.951	2333	2340	2343	rBV8	1365	3201	0.14%	0.012%
43	17.086	2361	2363	2371	rBV9	1709	2956	0.13%	0.011%
44	17.192	2378	2381	2385	rVB3	2637	3421	0.14%	0.012%
45	17.262	2387	2393	2397	rBV8	1553	3037	0.13%	0.011%
46	17.404	2410	2417	2425	rBV	1656762	2361716	100.00%	8.539%
47	17.504	2427	2434	2446	rBV2	1187377	1673083	70.84%	6.049%
48	18.021	2517	2522	2527	rBV9	3866	6934	0.29%	0.025%
49	18.245	2556	2560	2569	rBV	33742	48853	2.07%	0.177%
50	18.521	2604	2607	2610	rBV5	2864	4205	0.18%	0.015%
51	18.604	2618	2621	2624	rBV5	1740	2624	0.11%	0.009%
52	19.356	2744	2749	2754	rBV5	12174	21213	0.90%	0.077%
53	19.421	2754	2760	2765	rVV	17171	28648	1.21%	0.104%
54	19.521	2773	2777	2783	rBV6	19130	26865	1.14%	0.097%
55	19.662	2798	2801	2806	rVB6	11186	12873	0.55%	0.047%
56	19.792	2817	2823	2830	rBV	1495278	1844854	78.11%	6.670%
57	21.580	3122	3127	3133	rBV	1890906	2307554	97.71%	8.343%
58	23.197	3398	3402	3410	rVB	90592	140041	5.93%	0.506%
59	23.827	3506	3509	3513	rBV	89230	142769	6.05%	0.516%
60	23.886	3513	3519	3529	rVB2	813311	1570802	66.51%	5.679%
61	24.050	3540	3547	3563	rVB	1125580	2258514	95.63%	8.166%




Sum of corrected areas: 27659199

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101723\
Data File : BM042334.D
Acq On : 17 Oct 2023 23:17
Operator : MA/JU
Sample : 04885-03 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COM27

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

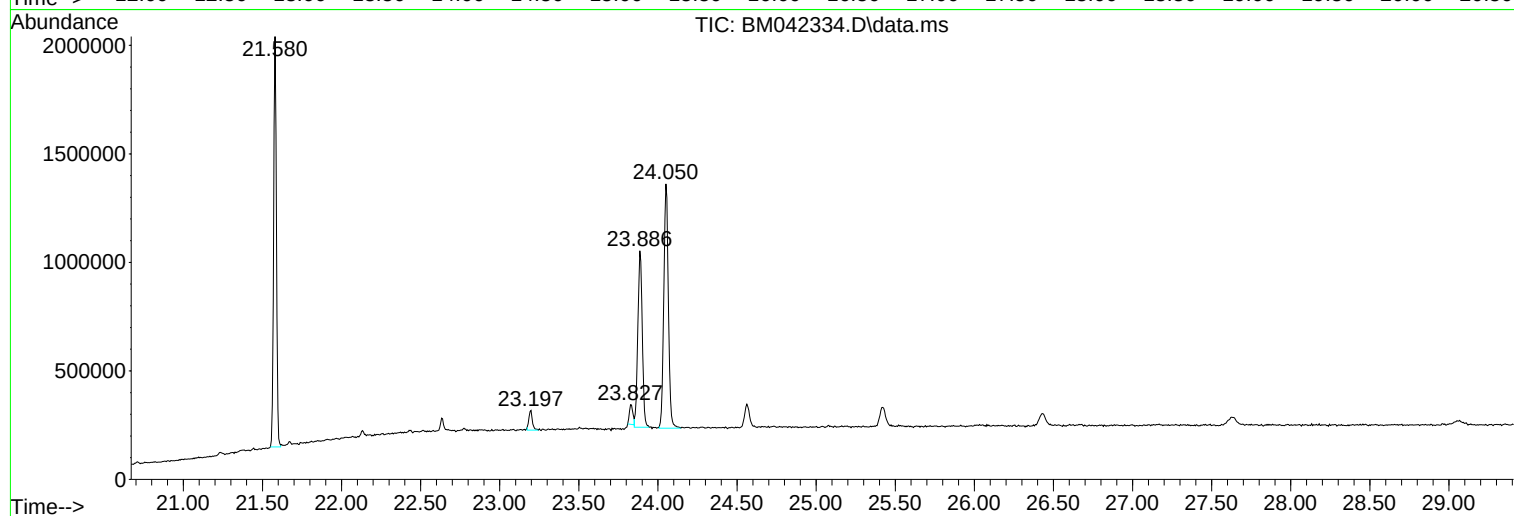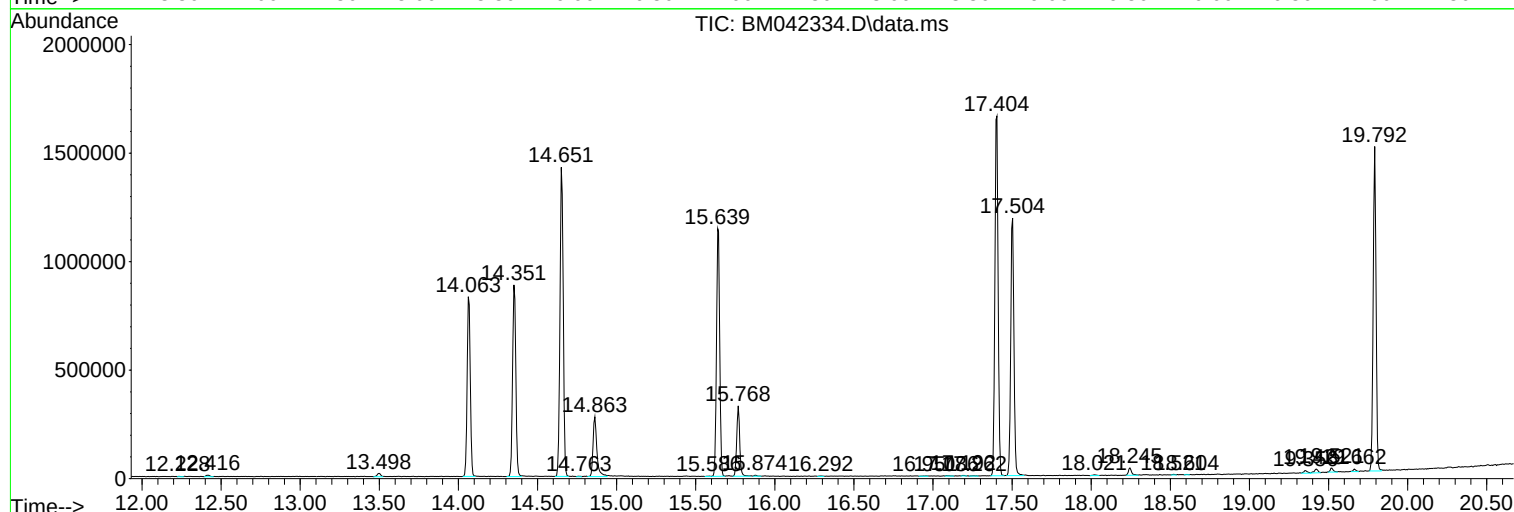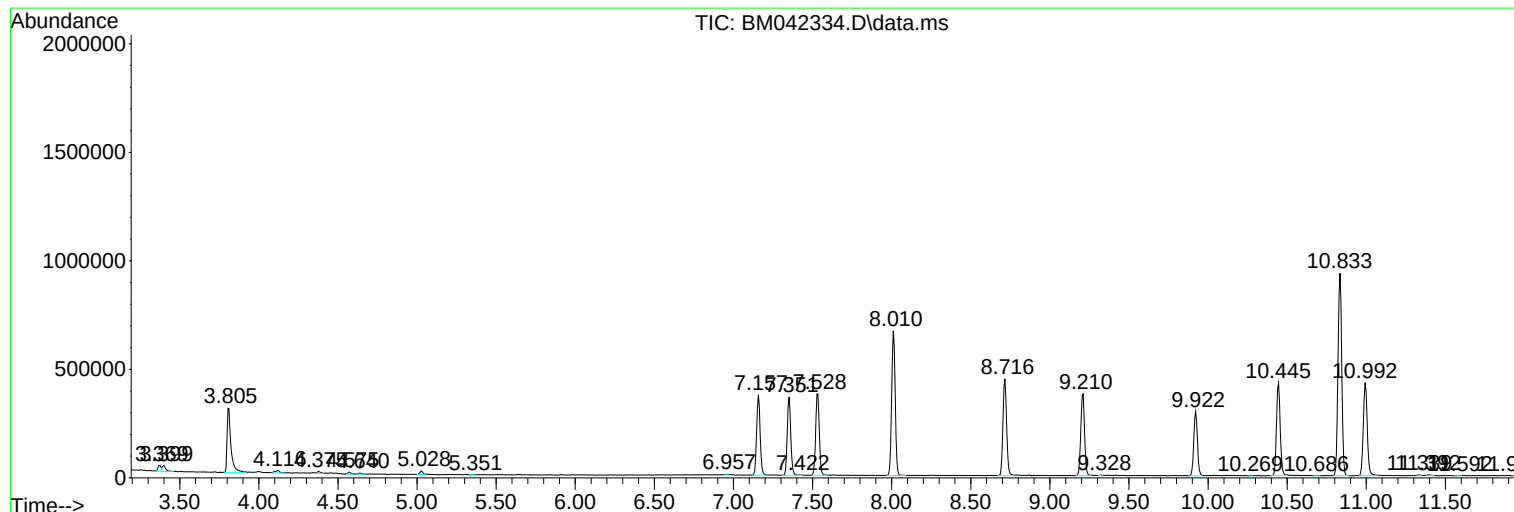

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101723\
Data File : BM042334.D
Acq On : 17 Oct 2023 23:17
Operator : MA/JU
Sample : 04885-03 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COM27

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101723\
Data File : BM042334.D
Acq On : 17 Oct 2023 23:17
Operator : MA/JU
Sample : 04885-03 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COM27

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc