

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101723\
 Data File : BM042339.D
 Acq On : 18 Oct 2023 02:19
 Operator : MA/JU
 Sample : 04885-10 10X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COM32

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042339.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	28	31	42	rVB	24923	37654	0.64%	0.073%
2	3.716	87	90	98	rVB	23865	33721	0.57%	0.066%
3	3.810	102	106	124	rVV	189708	328520	5.57%	0.640%
4	4.004	133	139	148	rVB	32538	54018	0.92%	0.105%
5	4.116	155	158	163	rBV2	18137	25367	0.43%	0.049%
6	5.057	312	318	322	rBV	14017	20460	0.35%	0.040%
7	7.157	669	675	684	rBV	202733	319503	5.42%	0.623%
8	7.351	699	708	719	rBV	910693	1387298	23.51%	2.704%
9	7.528	730	738	748	rBV	771579	1211824	20.54%	2.362%
10	7.628	751	755	761	rVB6	4133	6898	0.12%	0.013%
11	8.010	813	820	834	rBV	588080	924125	15.66%	1.801%
12	8.716	933	940	951	rBV	573666	917073	15.54%	1.787%
13	8.857	959	964	969	rVB	29916	47478	0.80%	0.093%
14	9.133	1005	1011	1016	rBV	28811	45709	0.77%	0.089%
15	9.204	1016	1023	1035	rVB	1027211	1679266	28.46%	3.273%
16	9.633	1091	1096	1098	rBV6	5027	8746	0.15%	0.017%
17	9.692	1104	1106	1114	rVB6	4243	6840	0.12%	0.013%
18	9.922	1133	1145	1155	rBV	823701	1318139	22.34%	2.569%
19	10.039	1160	1165	1171	rVB5	4300	9666	0.16%	0.019%
20	10.439	1225	1233	1243	rBV	1043721	1742226	29.53%	3.395%
21	10.763	1282	1288	1292	rBV6	4214	7427	0.13%	0.014%
22	10.833	1292	1300	1307	rBV	811536	1343365	22.77%	2.618%
23	10.992	1316	1327	1340	rBV	959413	1581914	26.81%	3.083%
24	11.322	1377	1383	1388	rBV	58879	91998	1.56%	0.179%
25	11.380	1388	1393	1403	rVB	80772	126388	2.14%	0.246%
26	12.410	1563	1568	1574	rVB2	17814	29150	0.49%	0.057%
27	12.663	1607	1611	1615	rBV6	5905	7775	0.13%	0.015%
28	12.974	1659	1664	1670	rBV5	9519	14761	0.25%	0.029%
29	13.157	1689	1695	1700	rBV7	4384	7693	0.13%	0.015%
30	13.498	1746	1753	1757	rBV2	29631	50534	0.86%	0.098%
31	13.910	1814	1823	1831	rBV	17443	35068	0.59%	0.068%
32	14.063	1843	1849	1856	rBV	2193343	3024773	51.27%	5.895%
33	14.110	1856	1857	1863	rVB2	10442	10093	0.17%	0.020%
34	14.257	1877	1882	1888	rBV2	12867	20523	0.35%	0.040%
35	14.351	1891	1898	1912	rBV	2415936	3416150	57.90%	6.657%
36	14.651	1942	1949	1956	rVB	1245631	1769475	29.99%	3.448%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101723\
 Data File : BM042339.D
 Acq On : 18 Oct 2023 02:19
 Operator : MA/JU
 Sample : 04885-10 10X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COM32

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
 Title : SVOA CALIBRATION

37	14.863	1979	1985	1995	rBV	164471	270474	4.58%	0.527%
38	15.021	2005	2012	2014	rBV6	3512	6555	0.11%	0.013%
39	15.286	2053	2057	2062	rBV2	30386	40713	0.69%	0.079%
40	15.386	2069	2074	2078	rBV	9832	13804	0.23%	0.027%
41	15.639	2111	2117	2125	rBV	3078475	4388438	74.38%	8.552%
42	15.768	2133	2139	2153	rBV	1239931	1595653	27.05%	3.110%
43	15.880	2153	2158	2162	rVV4	14327	21177	0.36%	0.041%
44	15.927	2162	2166	2171	rVB3	9071	11080	0.19%	0.022%
45	17.180	2376	2379	2386	rBV4	4706	7777	0.13%	0.015%
46	17.404	2410	2417	2423	rBV	1485462	2071946	35.12%	4.038%
47	17.504	2427	2434	2445	rBV	3640039	5109637	86.61%	9.958%
48	17.792	2480	2483	2489	rBV5	3520	6821	0.12%	0.013%
49	18.027	2518	2523	2528	rVB7	6843	11572	0.20%	0.023%
50	18.245	2555	2560	2565	rBV	65429	85606	1.45%	0.167%
51	18.462	2593	2597	2604	rBV4	13748	22396	0.38%	0.044%
52	18.968	2680	2683	2688	rBV7	2737	6041	0.10%	0.012%
53	19.350	2744	2748	2753	rVV2	38426	52211	0.88%	0.102%
54	19.421	2755	2760	2767	rVB	42446	63662	1.08%	0.124%
55	19.515	2773	2776	2785	rBV4	48834	64868	1.10%	0.126%
56	19.662	2798	2801	2805	rVB4	11411	13318	0.23%	0.026%
57	19.792	2817	2823	2833	rBV	4708708	5899920	100.00%	11.498%
58	21.580	3121	3127	3137	rBV2	1598632	2098041	35.56%	4.089%
59	22.627	3303	3305	3310	rVB	56013	71413	1.21%	0.139%
60	23.827	3505	3509	3512	rBV	106866	164013	2.78%	0.320%
61	23.885	3512	3519	3532	rVB2	2791727	5490075	93.05%	10.699%
62	24.050	3540	3547	3559	rVB	996431	2064246	34.99%	4.023%




Sum of corrected areas: 51313075

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101723\
Data File : BM042339.D
Acq On : 18 Oct 2023 02:19
Operator : MA/JU
Sample : 04885-10 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COM32

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

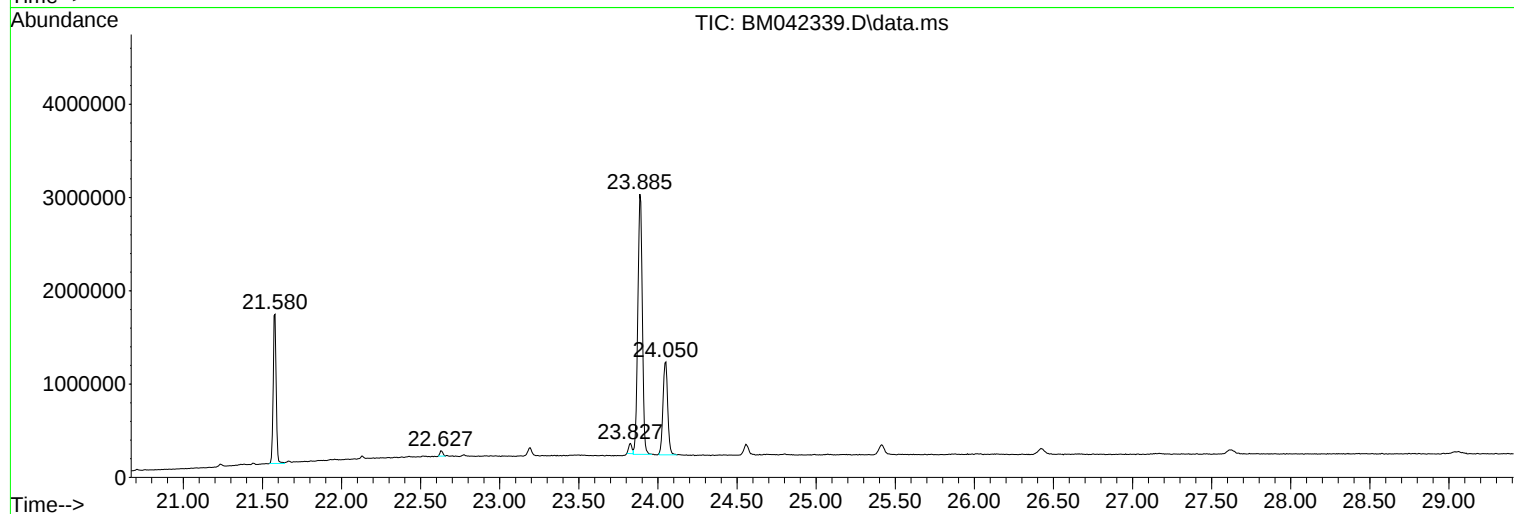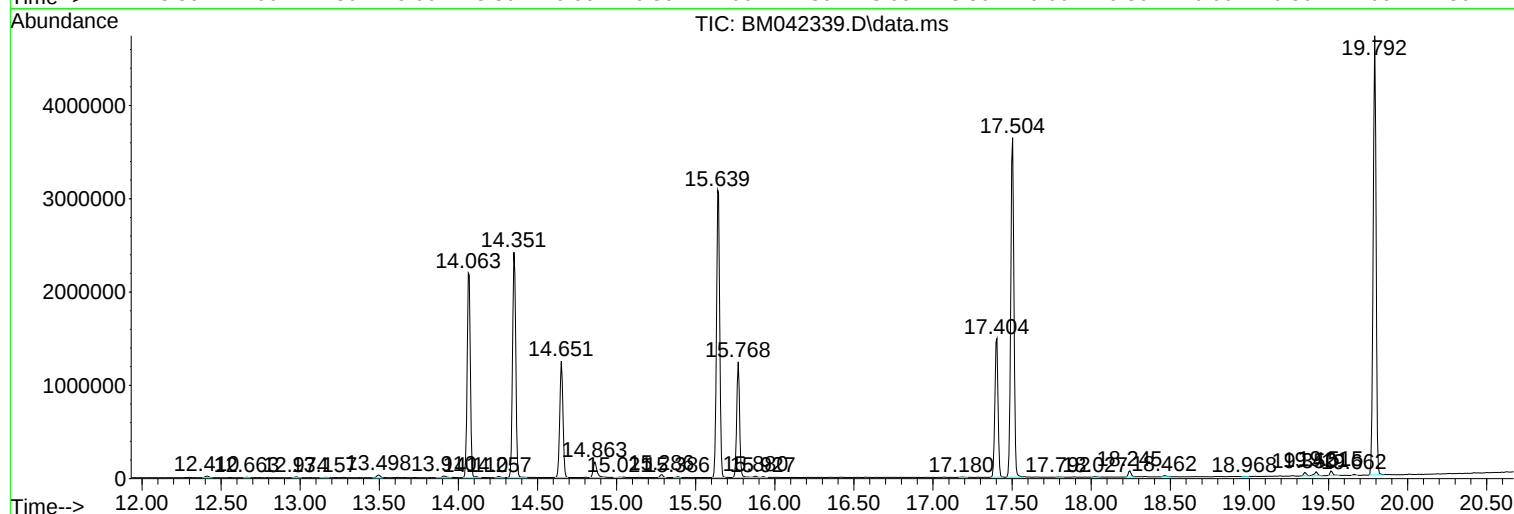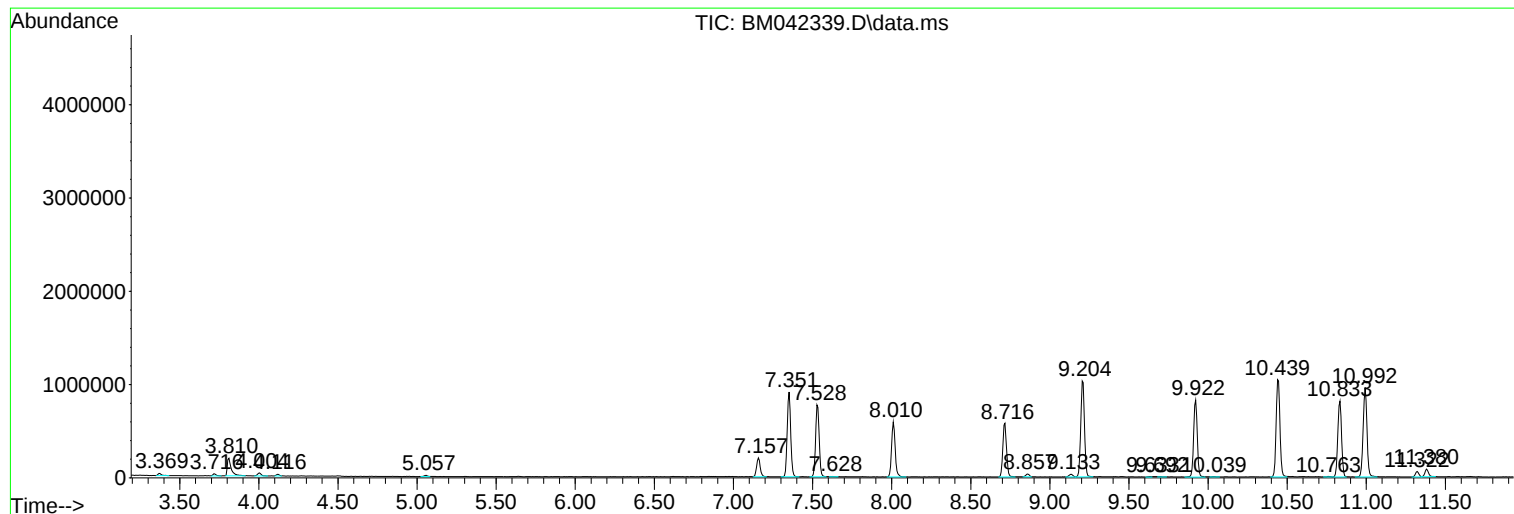

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101723\
Data File : BM042339.D
Acq On : 18 Oct 2023 02:19
Operator : MA/JU
Sample : 04885-10 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COM32

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101723\
Data File : BM042339.D
Acq On : 18 Oct 2023 02:19
Operator : MA/JU
Sample : 04885-10 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COM32

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------