

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM101918\
 Data File : BM017257.D
 Acq On : 20 Oct 2018 10:13
 Operator : MJ/SJ
 Sample : J5195-04
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Oct 22 02:48:05 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM101718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 17 14:23:17 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	308141	20.00	ng	-0.01
21) Naphthalene-d8	10.44	136	1236043	20.00	ng	-0.01
39) Acenaphthene-d10	14.30	164	740075	20.00	ng	-0.01
64) Phenanthrene-d10	17.06	188	1744839	20.00	ng	-0.01
76) Chrysene-d12	21.25	240	1816251	20.00	ng	-0.01
87) Perylene-d12	23.46	264	1639532	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.28	112	2107565	115.68	ng	0.00
7) Phenol-d6	6.85	99	2644472	106.58	ng	-0.01
23) Nitrobenzene-d5	8.82	82	1867909	88.38	ng	-0.02
42) 2,4,6-Tribromophenol	15.80	330	1361915	136.08	ng	-0.01
45) 2-Fluorobiphenyl	12.92	172	4308430	77.46	ng	-0.01
79) Terphenyl-d14	19.70	244	7267725	90.19	ng	0.00
Target Compounds						
80) Butylbenzylphthalate	20.39	149	321	7.183	ng	# 27
84) Bis(2-ethylhexyl)phthalate	21.18	149	2004	5.338	ng	# 91
85) Di-n-octyl phthalate	22.07	149	1103	5.581	ng	# 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM101918\
Data File : BM017257.D
Acq On : 20 Oct 2018 10:13
Operator : MJ/SJ
Sample : J5195-04
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Oct 22 02:48:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM101718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 17 14:23:17 2018
Response via : Initial Calibration

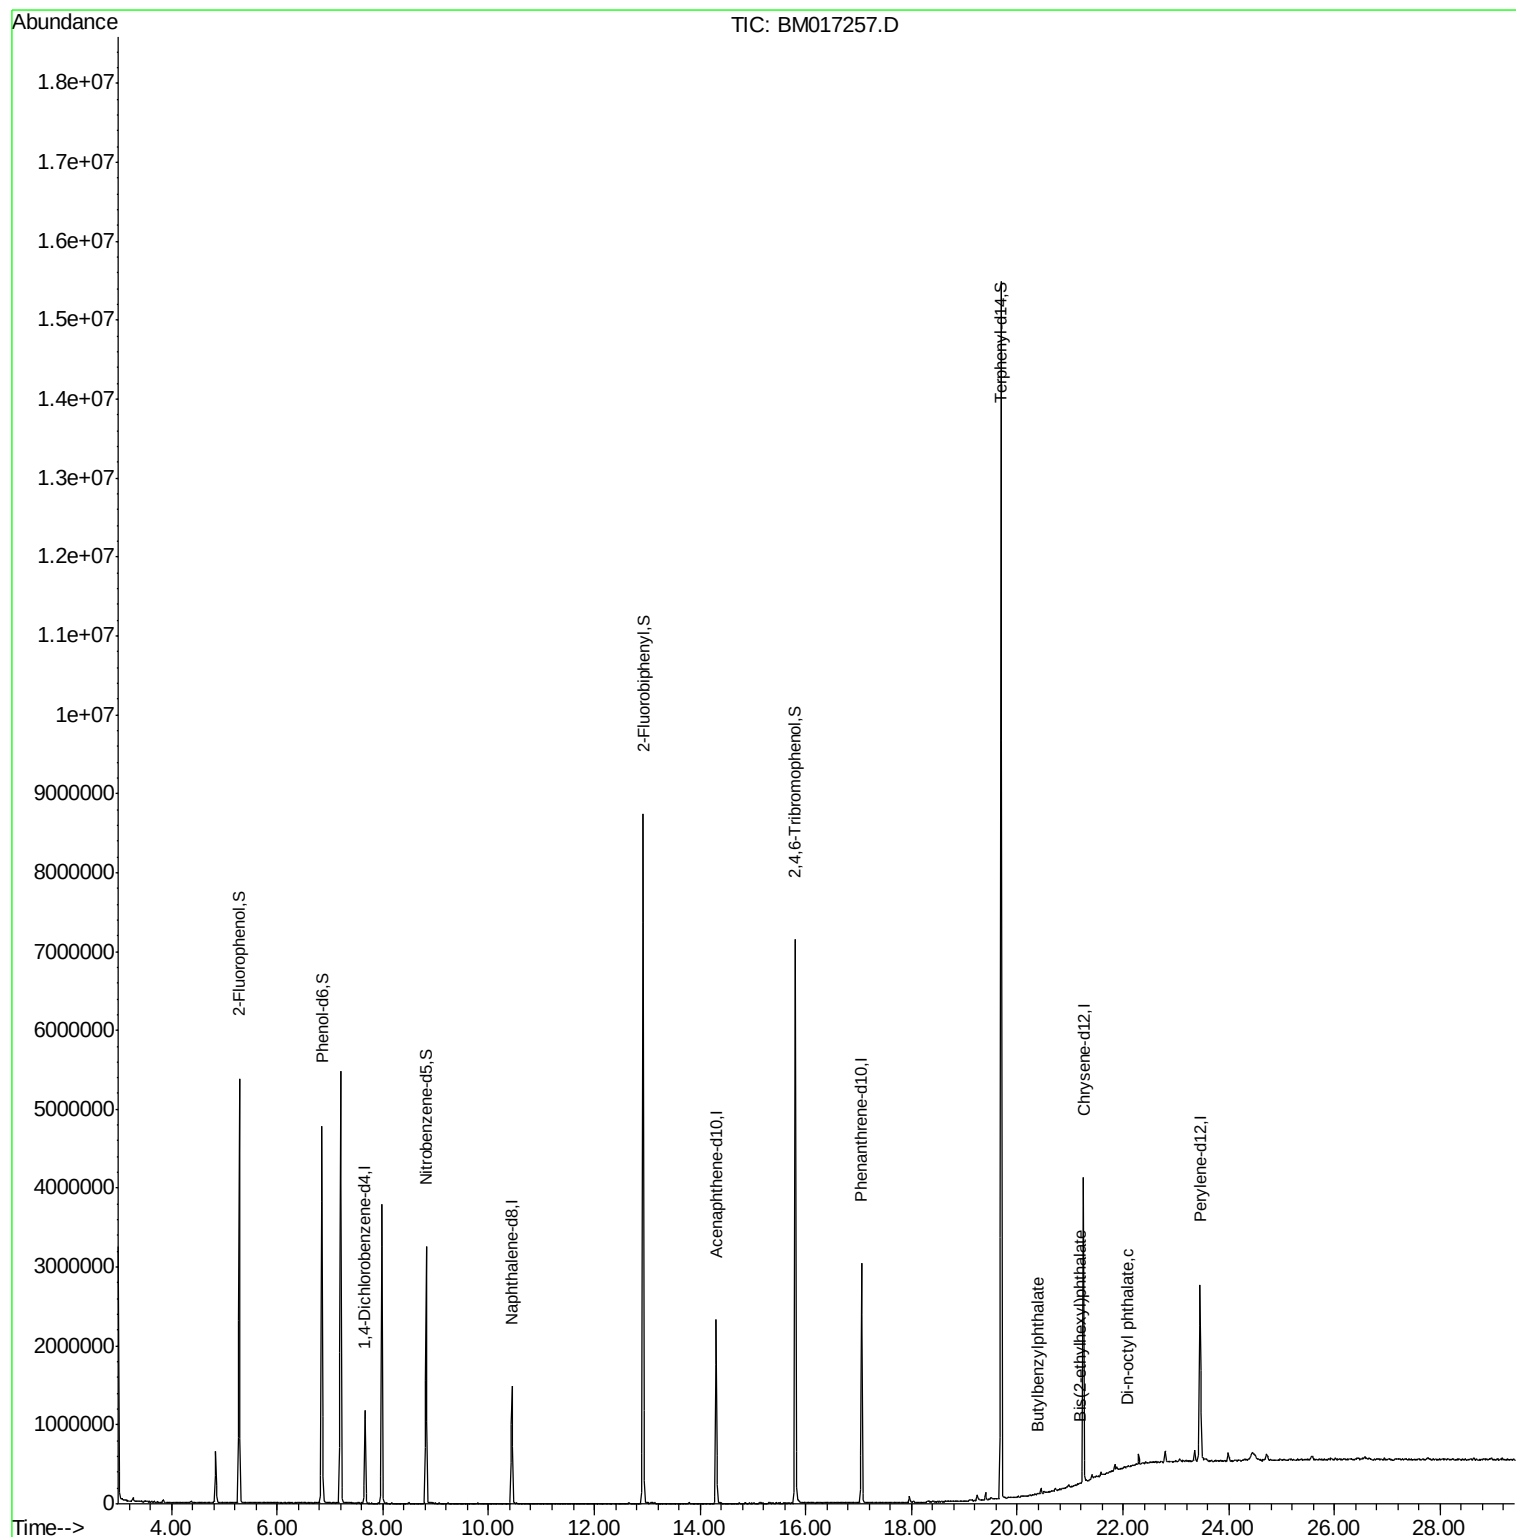

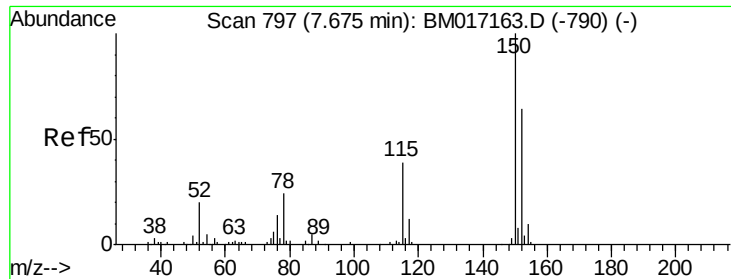


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.66 min Scan# 795
Delta R.T. -0.01 min
Lab File: BM017257.D
Acq: 20 Oct 2018 10:13

Instrument :
BNA_M
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	157.7	124.3	186.5
115	61.1	48.1	72.1



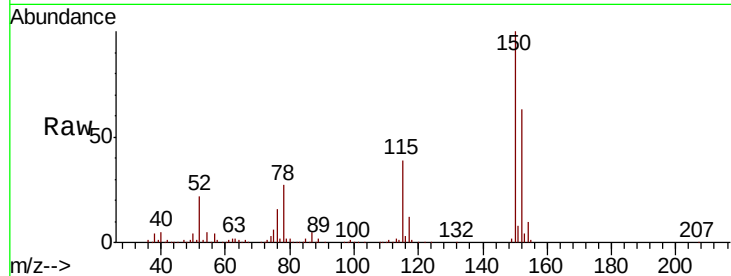


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

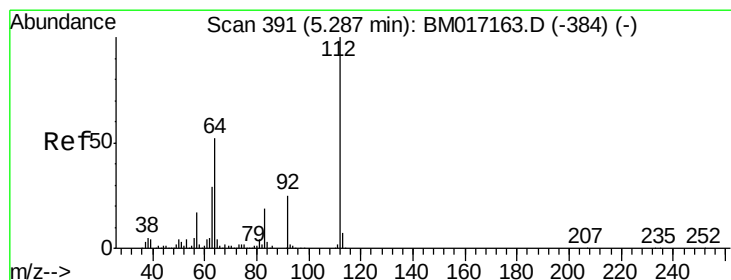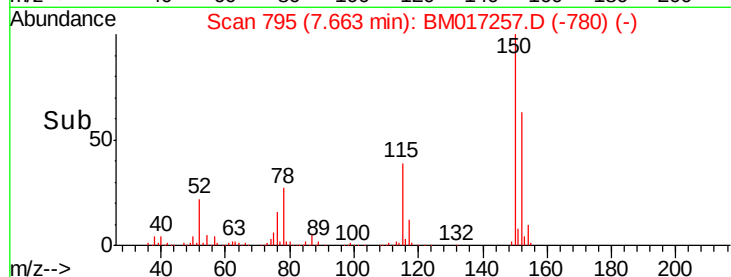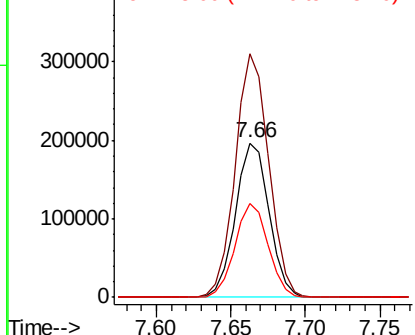

#5

2-Fluorophenol
Concen: 115.681 ng
RT: 5.28 min Scan# 390
Delta R.T. -0.01 min
Lab File: BM017257.D
Acq: 20 Oct 2018 10:13

Tgt Ion	Ratio	Lower	Upper
112	100		
64	58.7	41.7	62.5
63	30.8	23.0	34.4


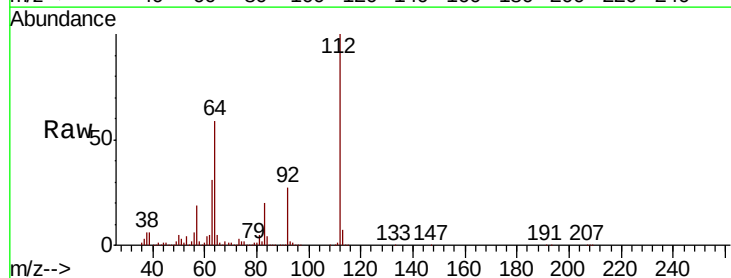



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 63.00 (62.70 to 63.70): BM0

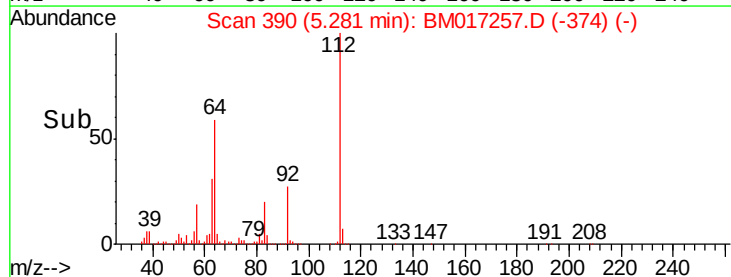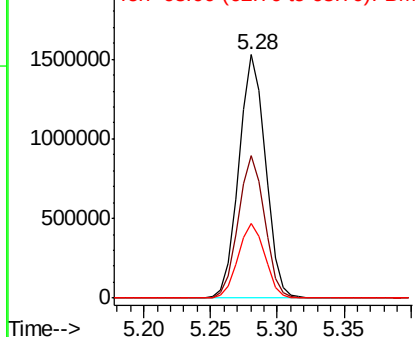

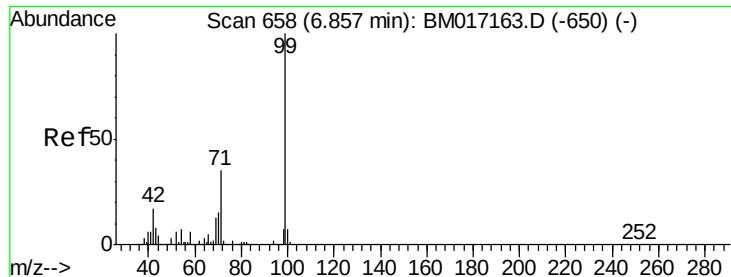

#7

Phenol-d6

Concen: 106.576 ng

RT: 6.85 min Scan# 656

Delta R.T. -0.01 min

Lab File: BM017257.D

Acq: 20 Oct 2018 10:13


Instrument :

BNA_M

ClientSampleId :

Tot Ion: 99 Resp: 2644472

Ion	Ratio	Lower	Upper
99	100		
42	17.4	13.3	19.9
71	35.8	28.0	42.0



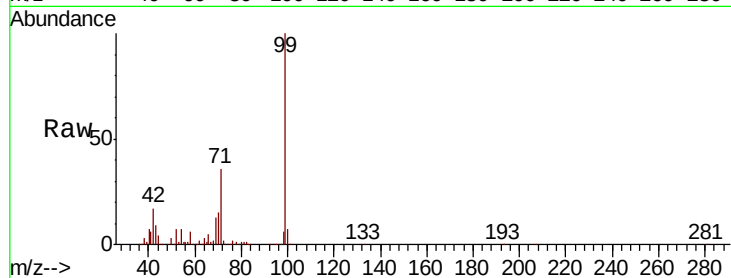


Abundance

Ion 99.00 (98.70 to 99.70): BM017163.D (-650) (-)

Ion 42.00 (41.70 to 42.70): BM017163.D (-650) (-)

Ion 71.00 (70.70 to 71.70): BM017163.D (-650) (-)

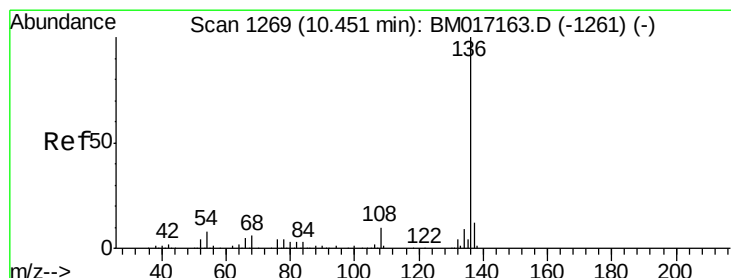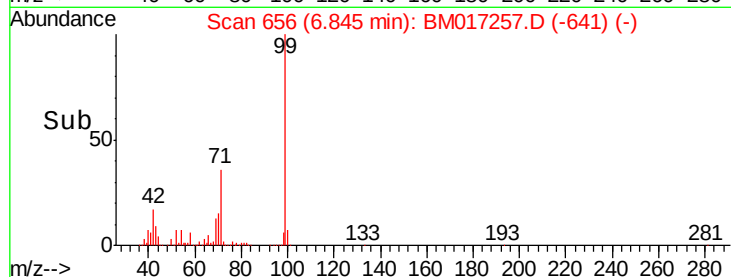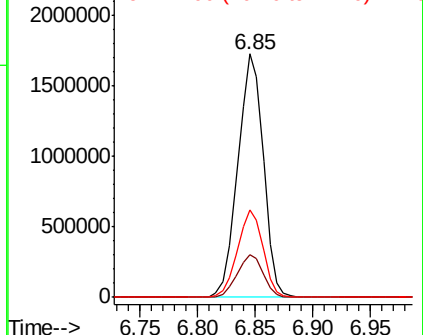

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.44 min Scan# 1267


Delta R.T. -0.01 min

Lab File: BM017257.D

Acq: 20 Oct 2018 10:13

Tgt Ion: 136 Resp: 1236043

Ion	Ratio	Lower	Upper
136	100		
137	11.2	9.2	13.8
54	7.5	6.7	10.1
68	5.7	4.7	7.1

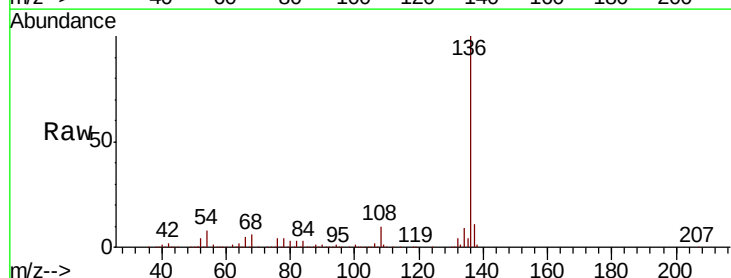



Abundance


Ion 136.00 (135.70 to 136.70): BM017163.D (-1261) (-)

Ion 137.00 (136.70 to 137.70): BM017163.D (-1261) (-)

Ion 54.00 (53.70 to 54.70): BM017163.D (-1261) (-)

Ion 68.00 (67.70 to 68.70): BM017163.D (-1261) (-)



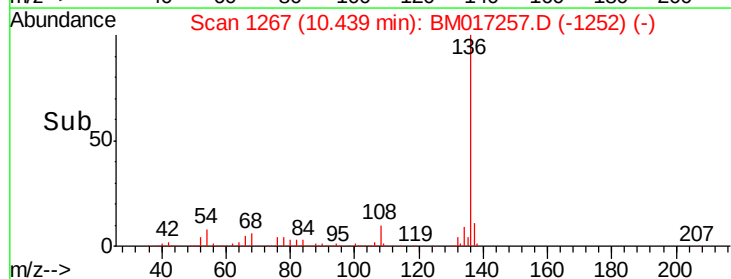
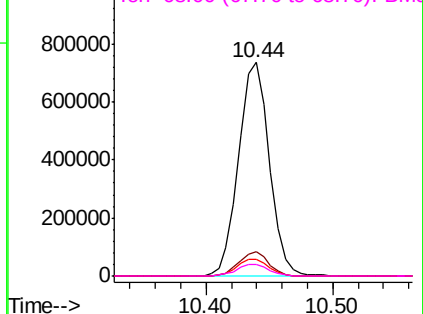


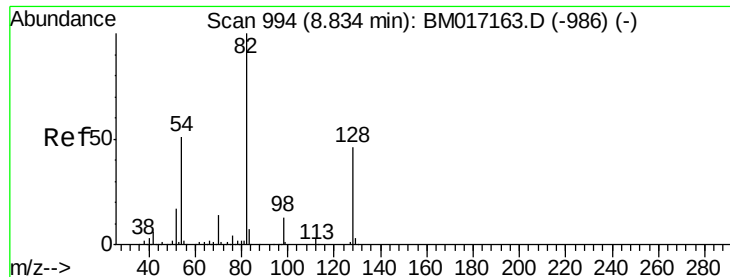

#23
Nitrobenzene-d5
Concen: 88.384 ng
RT: 8.82 min Scan# 991
Delta R.T. -0.02 min
Lab File: BM017257.D
Acq: 20 Oct 2018 10:13




Instrument :
BNA_M
ClientSampled :


Tot Ion: 82 Resp: 1867909
Ion Ratio Lower Upper
82 100
128 41.3 37.0 55.6
54 49.1 40.7 61.1

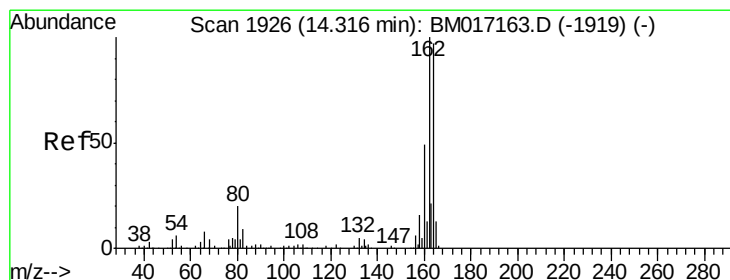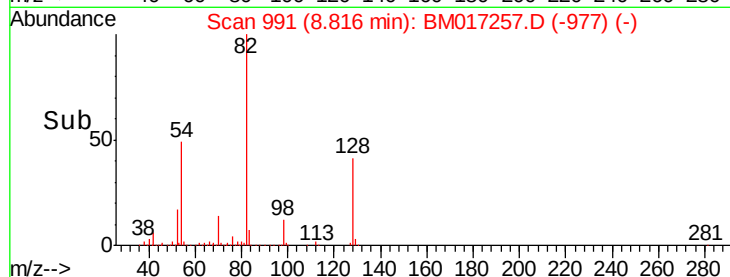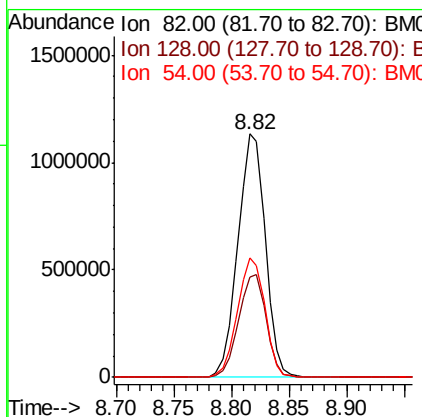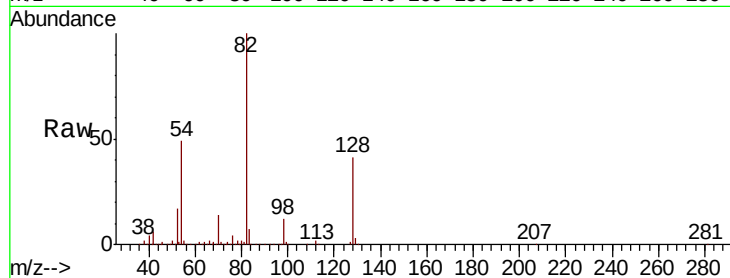

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.30 min Scan# 1924
Delta R.T. -0.01 min
Lab File: BM017257.D
Acq: 20 Oct 2018 10:13

Tgt Ion:164 Resp: 740075
Ion Ratio Lower Upper
164 100
162 103.3 82.1 123.1
160 45.2 40.2 60.2

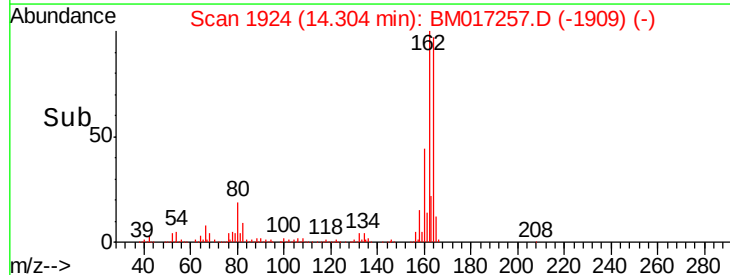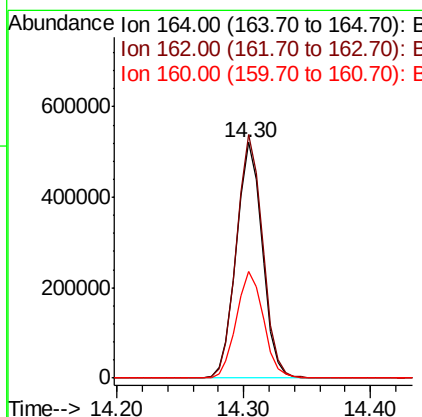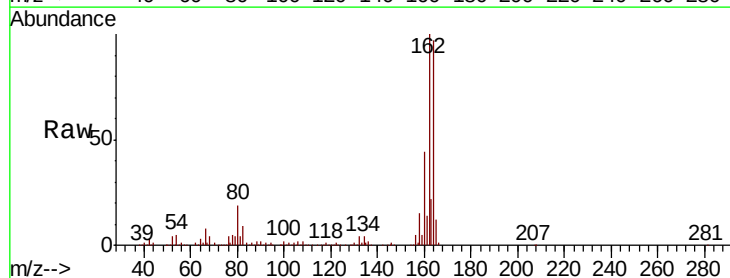


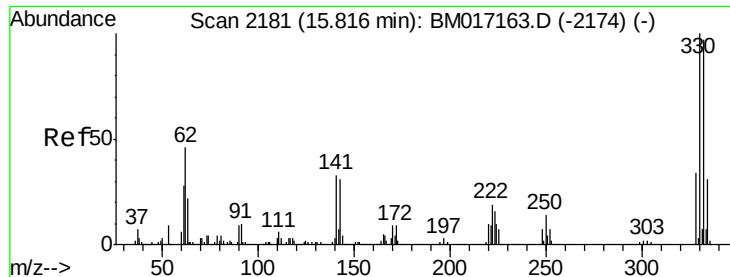




#42
 2,4,6-Tribromophenol
 Concen: 136.077 ng
 RT: 15.80 min Scan# 2179
 Delta R.T. -0.01 min
 Lab File: BM017257.D
 Acq: 20 Oct 2018 10:13

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion:330 Resp: 1361915
 Ion Ratio Lower Upper
 330 100
 332 96.8 77.3 115.9
 141 33.8 27.4 41.0

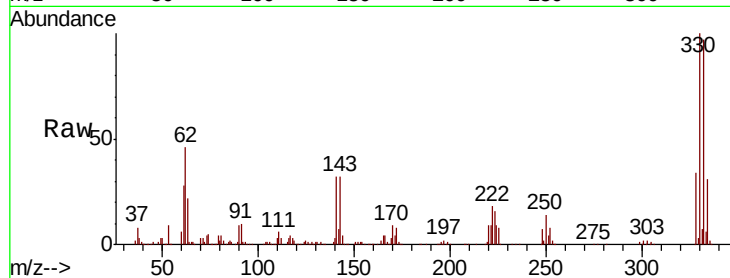


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

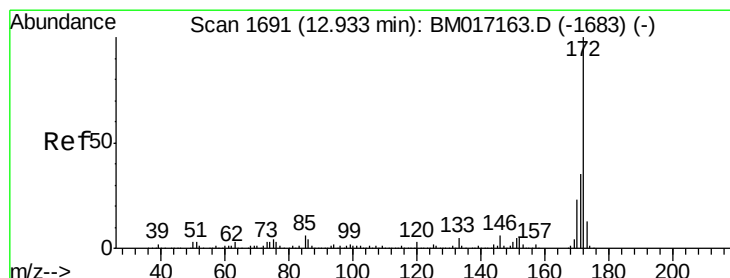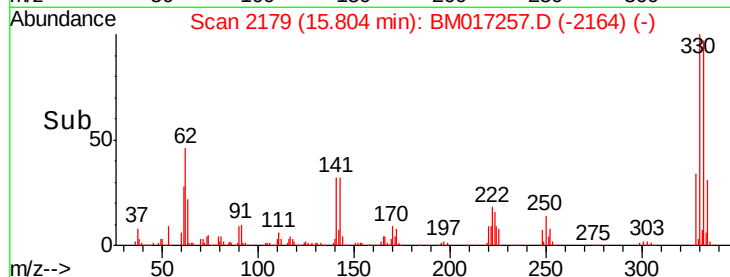
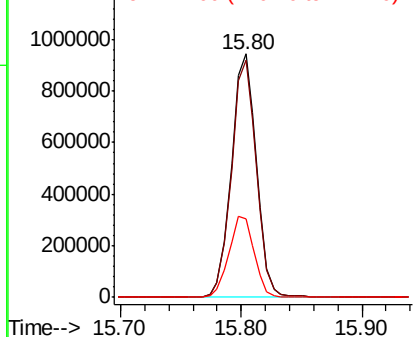



#45
 2-Fluorobiphenyl
 Concen: 77.459 ng
 RT: 12.92 min Scan# 1689
 Delta R.T. -0.01 min
 Lab File: BM017257.D
 Acq: 20 Oct 2018 10:13

Tgt Ion:172 Resp: 4308430
 Ion Ratio Lower Upper
 172 100
 171 35.3 28.3 42.5
 170 22.7 18.3 27.5

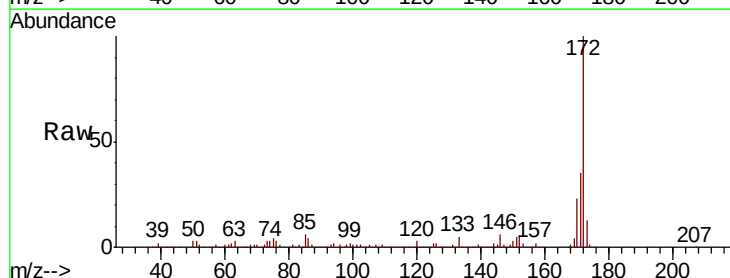

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

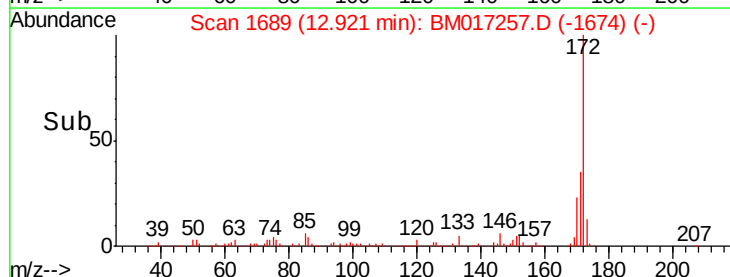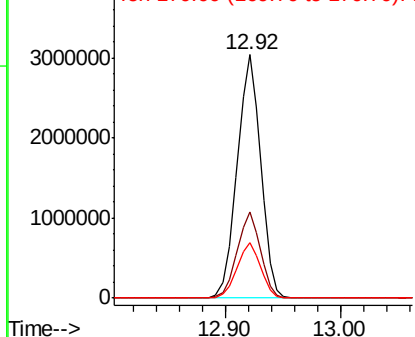

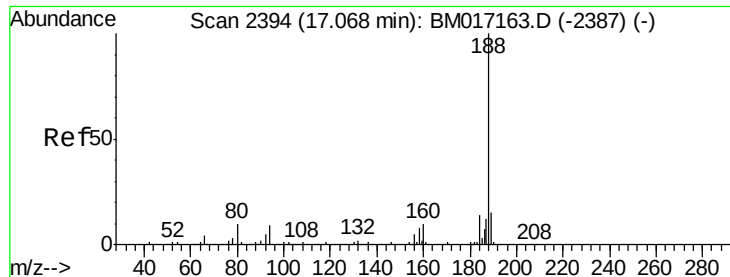

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.06 min Scan# 2392

Delta R.T. -0.01 min

Lab File: BM017257.D

Acq: 20 Oct 2018 10:13

Instrument :

BNA_M

ClientSampleId :


Tot Ion:188 Resp: 1744839

Ion Ratio Lower Upper

188 100

94 8.7 7.0 10.4




80 10.0 7.7 11.5

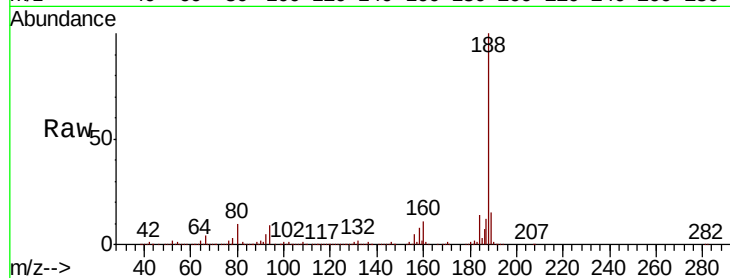

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM0

Ion 80.00 (79.70 to 80.70): BM0

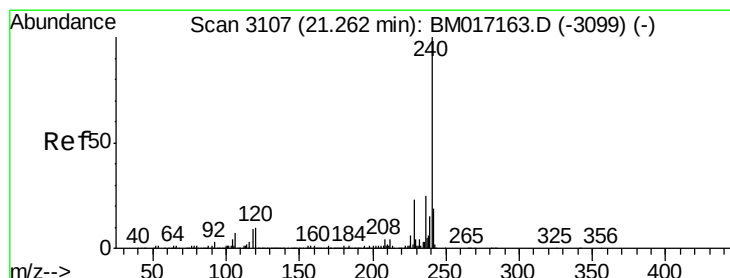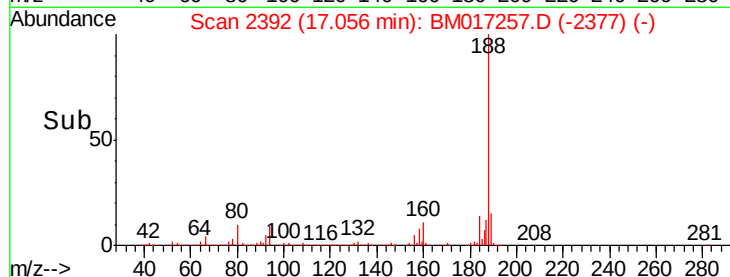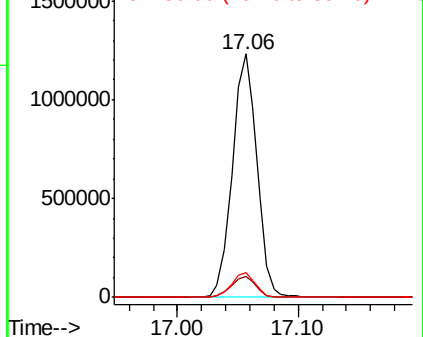

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.25 min Scan# 3105

Delta R.T. -0.01 min

Lab File: BM017257.D

Acq: 20 Oct 2018 10:13


Tgt Ion:240 Resp: 1816251

Ion Ratio Lower Upper

240 100

120 9.5 8.1 12.1



236 25.0 19.9 29.9

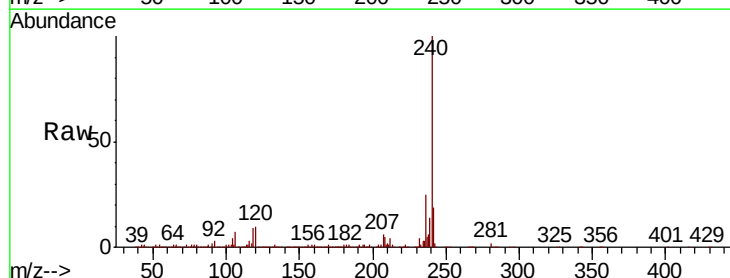


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

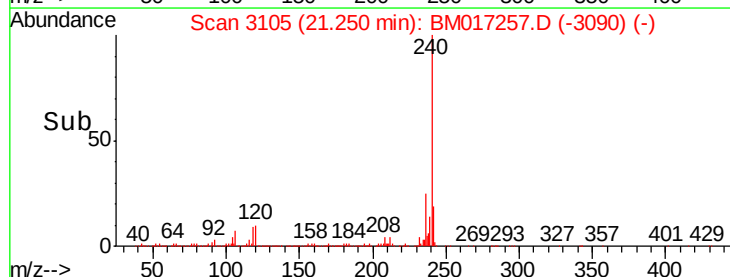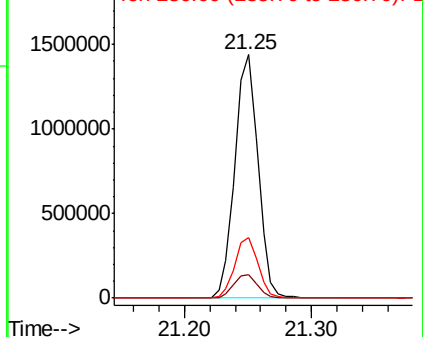


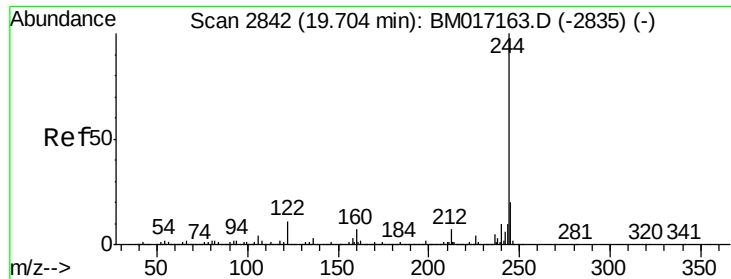




#79
 Terphenyl-d14
 Concen: 90.194 ng
 RT: 19.70 min Scan# 2841
 Delta R.T. -0.01 min
 Lab File: BM017257.D
 Acq: 20 Oct 2018 10:13

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion:244 Resp: 7267725
 Ion Ratio Lower Upper
 244 100
 212 7.2 5.5 8.3
 122 10.0 8.4 12.6

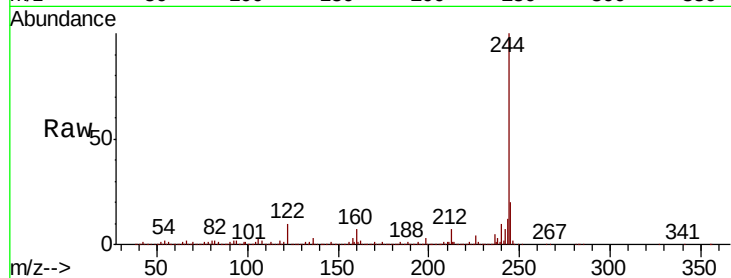


Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

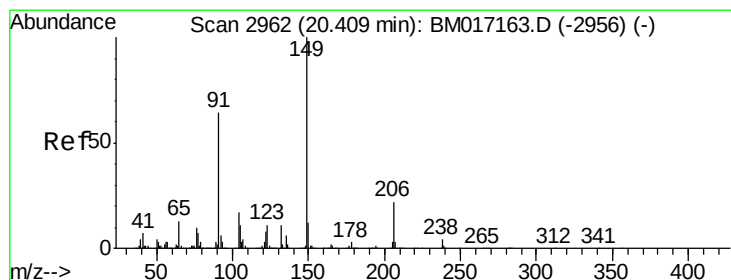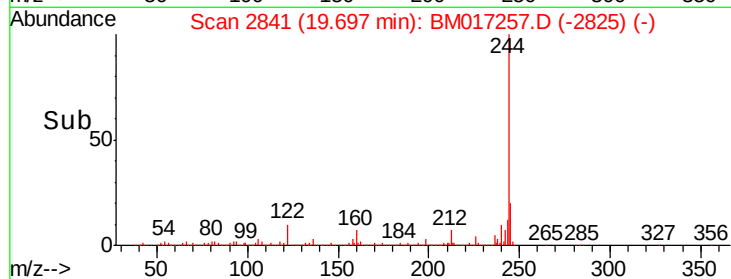
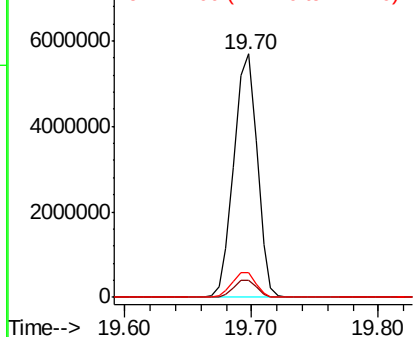



#80
 Butylbenzylphthalate
 Concen: 7.183 ng
 RT: 20.39 min Scan# 2959
 Delta R.T. -0.02 min
 Lab File: BM017257.D
 Acq: 20 Oct 2018 10:13

Tgt Ion:149 Resp: 321
 Ion Ratio Lower Upper
 149 100
 91 0.0 51.3 76.9#
 206 0.0 18.0 27.0#

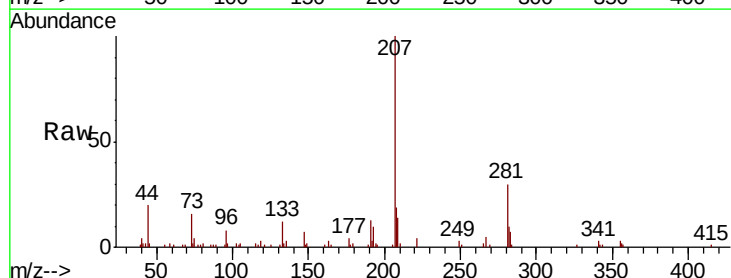

Abundance Ion 149.00 (148.70 to 149.70): E
 Ion 91.00 (90.70 to 91.70): BM0
 Ion 206.00 (205.70 to 206.70): E

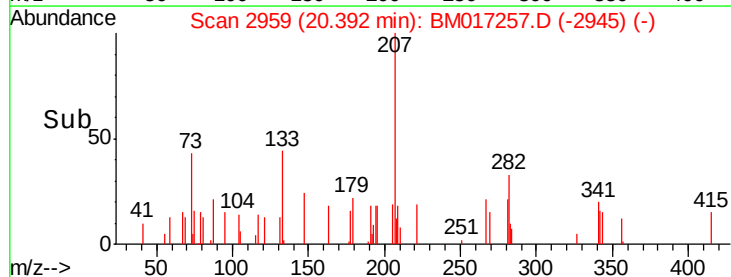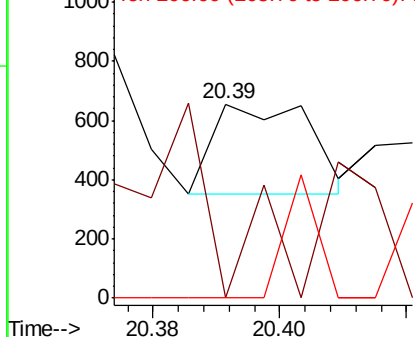

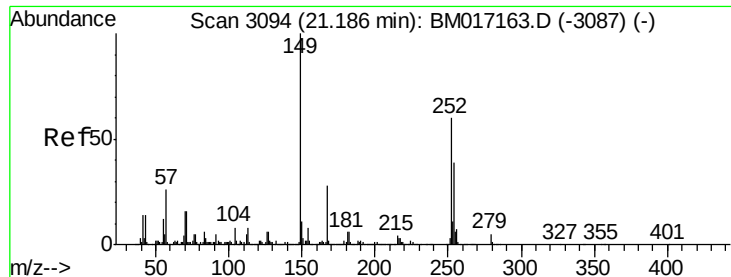

#84

Bis(2-ethylhexyl)phthalate

Concen: 5.338 ng

RT: 21.18 min Scan# 3093

Delta R.T. -0.01 min

Lab File: BM017257.D

Acq: 20 Oct 2018 10:13

Instrument :

BNA_M

ClientSampled :


Tot Ion:149 Resp: 2004

Ion Ratio Lower Upper

149 100

167 23.5 22.2 33.4




279 0.0 3.6 5.4#

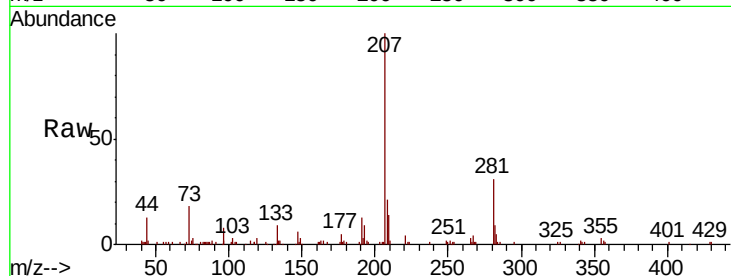

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

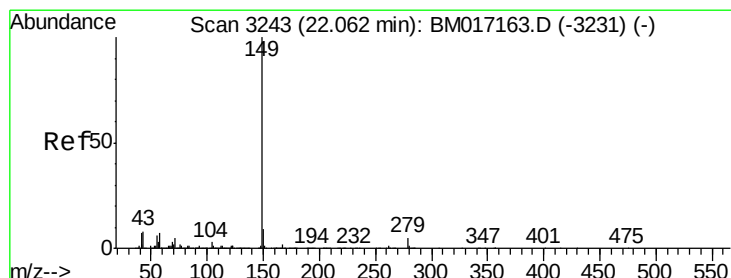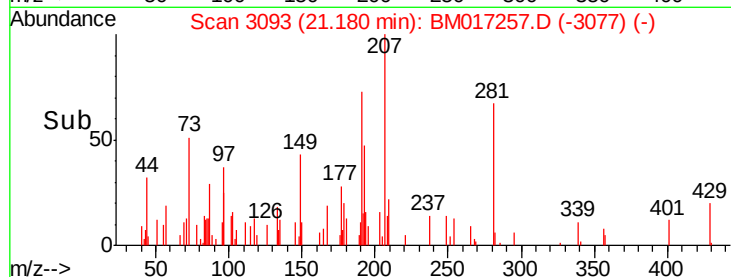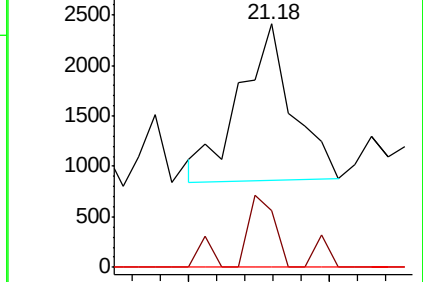

#85

Di-n-octyl phthalate

Concen: 5.581 ng

RT: 22.07 min Scan# 3245

Delta R.T. 0.01 min

Lab File: BM017257.D

Acq: 20 Oct 2018 10:13


Tgt Ion:149 Resp: 1103

Ion Ratio Lower Upper

149 100

167 24.8 1.4 2.0#



43 0.0 7.2 10.8#

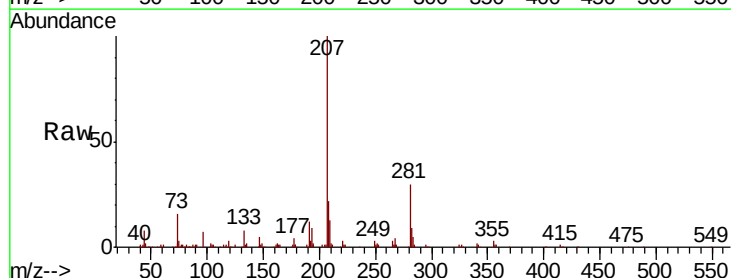


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 43.00 (42.70 to 43.70): BM

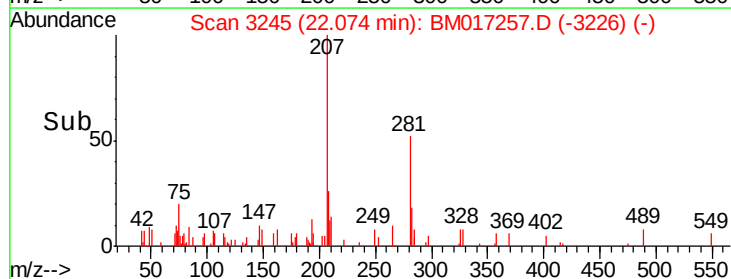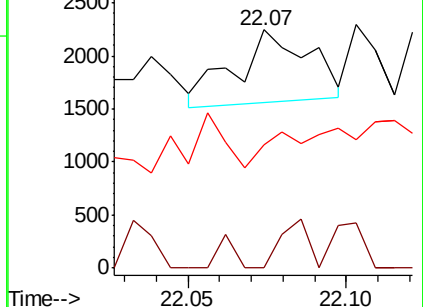

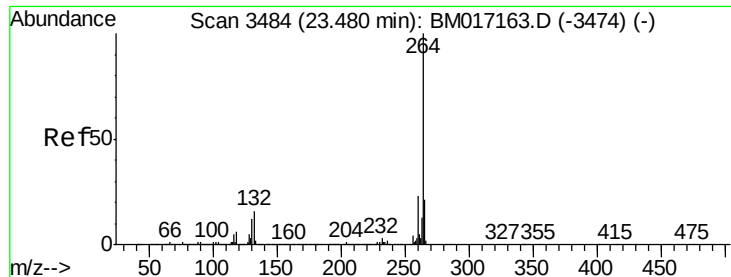

#87
Pervlene-d12
Concen: 20.000 ng
RT: 23.46 min Scan# 3481
Delta R.T. -0.02 min
Lab File: BM017257.D
Acq: 20 Oct 2018 10:13

Instrument :
BNA_M
ClientSampleId :

Tot Ion:264 Resp: 1639532

Ion	Ratio	Lower	Upper
264	100		
260	22.5	18.6	27.8
265	21.9	17.8	26.8

