

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM101918\
 Data File : BM017269.D
 Acq On : 20 Oct 2018 17:27
 Operator : MJ/SJ
 Sample : J5590-08
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Oct 22 06:39:20 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM101718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 17 14:23:17 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	332699	20.00	ng	-0.01
21) Naphthalene-d8	10.43	136	1351491	20.00	ng	-0.02
39) Acenaphthene-d10	14.30	164	797567	20.00	ng	-0.01
64) Phenanthrene-d10	17.06	188	1794042	20.00	ng	-0.01
76) Chrysene-d12	21.25	240	1579020	20.00	ng	-0.01
87) Perylene-d12	23.46	264	1426881	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.28	112	2312907	117.58	ng	0.00
7) Phenol-d6	6.85	99	2884875	107.68	ng	-0.01
23) Nitrobenzene-d5	8.82	82	2015557	87.22	ng	-0.02
42) 2,4,6-Tribromophenol	15.80	330	1323281	122.69	ng	-0.01
45) 2-Fluorobiphenyl	12.92	172	4618112	77.04	ng	-0.01
79) Terphenyl-d14	19.70	244	6825182	97.43	ng	0.00
Target Compounds						
80) Butylbenzylphthalate	20.40	149	424	7.187	ng	# 55
84) Bis(2-ethylhexyl)phthalate	21.17	149	2459	5.350	ng	# 84
85) Di-n-octyl phthalate	22.03	149	883	5.580	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM101918\
Data File : BM017269.D
Acq On : 20 Oct 2018 17:27
Operator : MJ/SJ
Sample : J5590-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Oct 22 06:39:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM101718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 17 14:23:17 2018
Response via : Initial Calibration

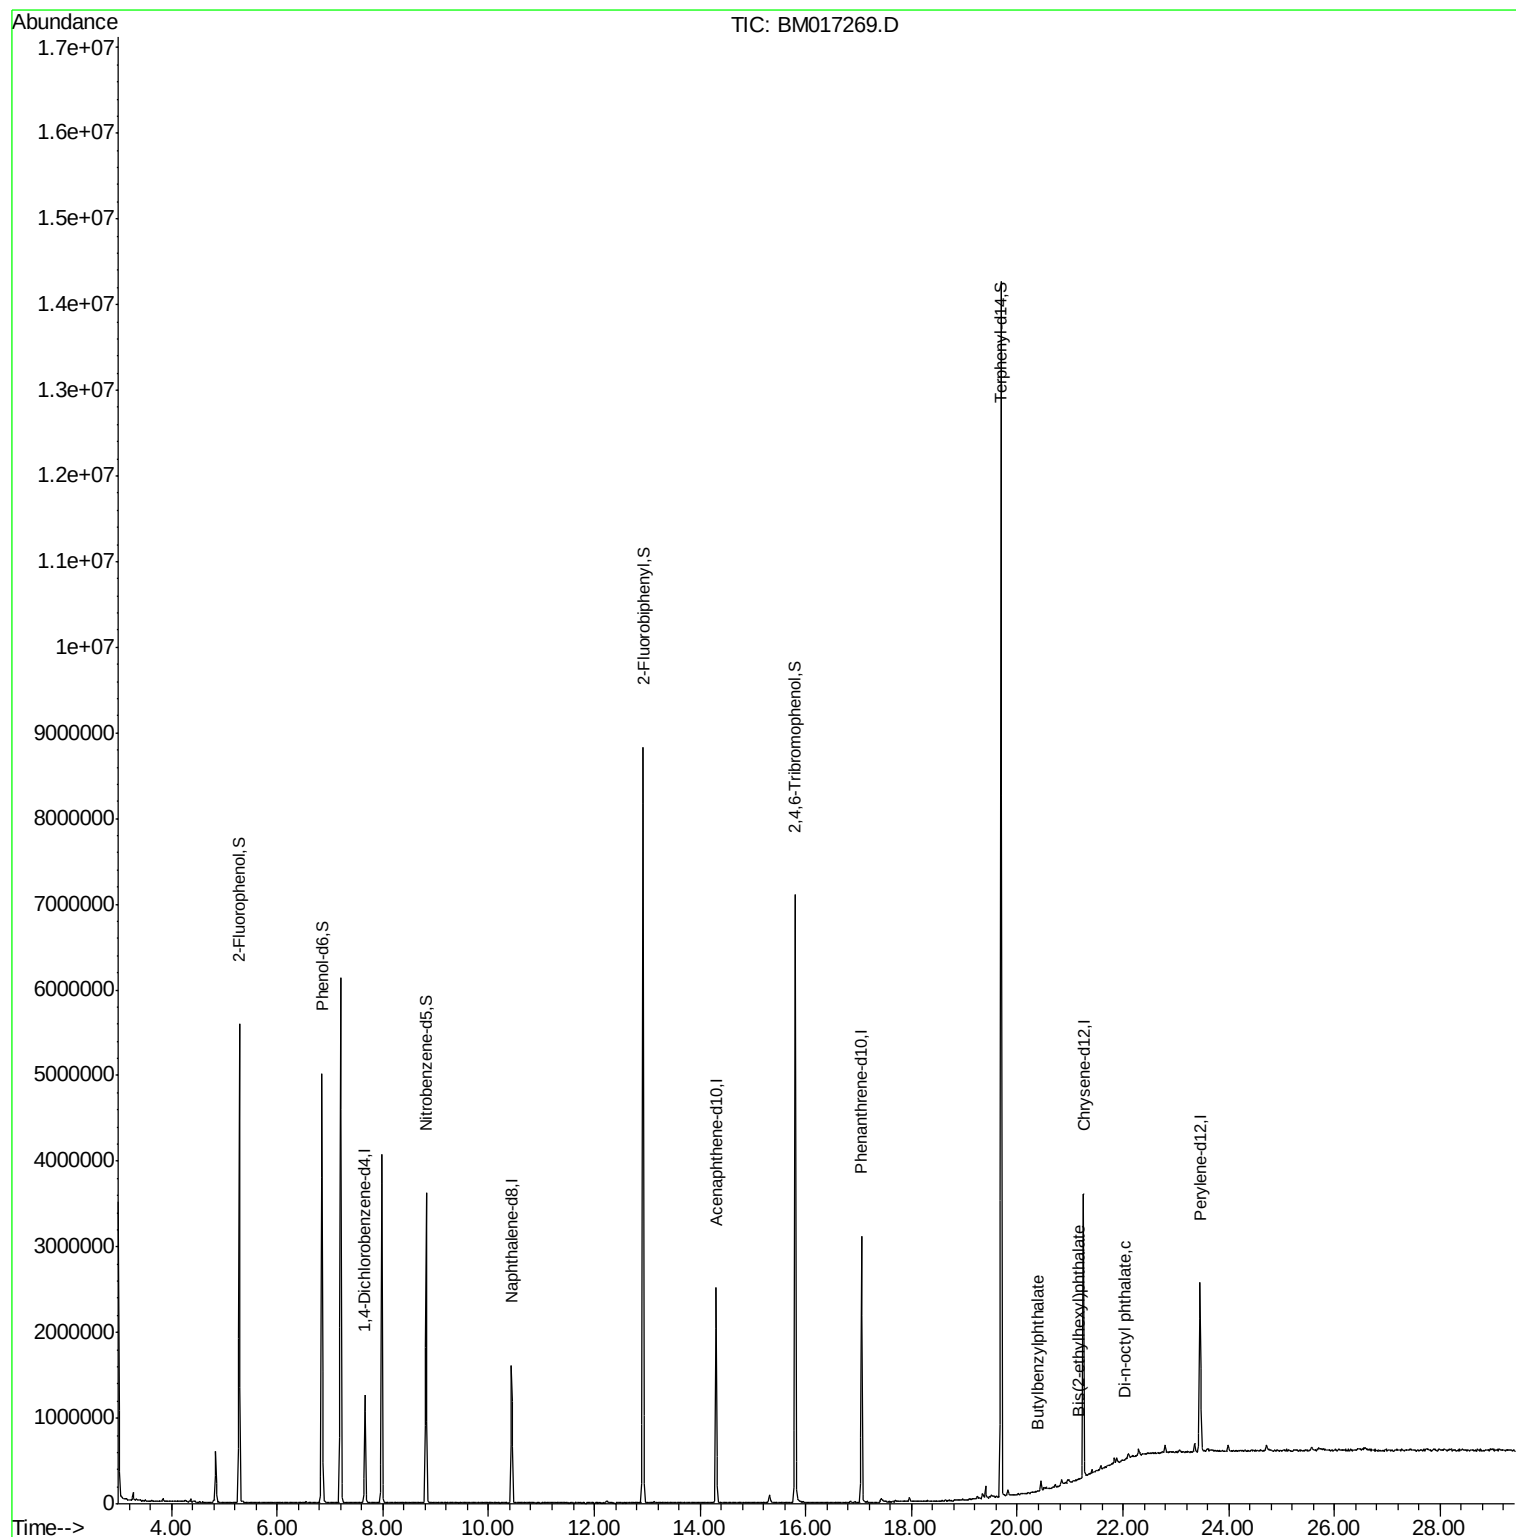

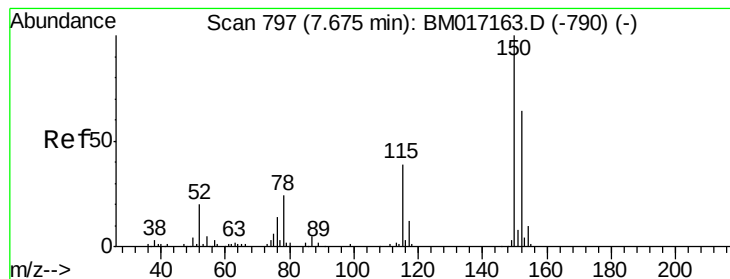


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.66 min Scan# 795
Delta R.T. -0.01 min
Lab File: BM017269.D
Acq: 20 Oct 2018 17:27

Instrument :
BNA_M
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	151.9	124.3	186.5
115	57.1	48.1	72.1






Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

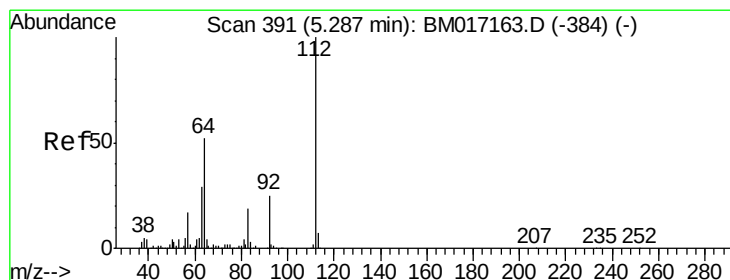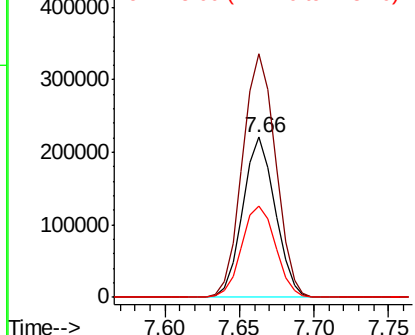

#5

2-Fluorophenol
Concen: 117.581 ng
RT: 5.28 min Scan# 390
Delta R.T. -0.01 min
Lab File: BM017269.D
Acq: 20 Oct 2018 17:27

Tgt Ion	Ratio	Lower	Upper
112	100		
64	59.1	41.7	62.5
63	31.1	23.0	34.4






Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 63.00 (62.70 to 63.70): BM0

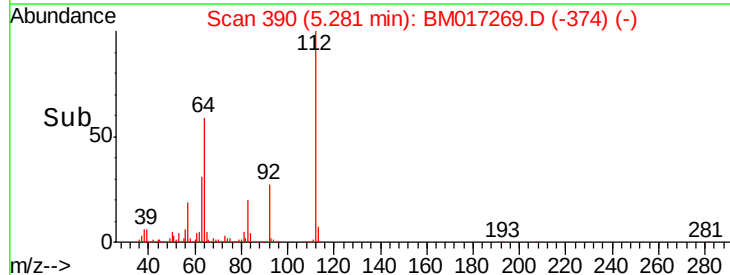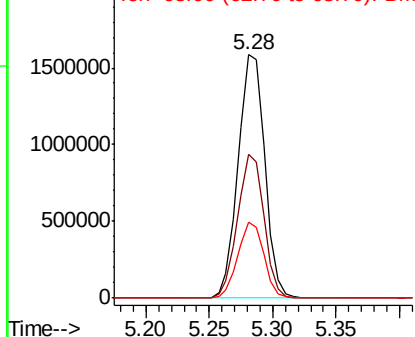



#7

Phenol-d6

Concen: 107.683 ng

RT: 6.85 min Scan# 656

Delta R.T. -0.01 min

Lab File: BM017269.D

Acq: 20 Oct 2018 17:27

Instrument :

BNA_M

ClientSampled :


Tot Ion: 99 Resp: 2884875

Ion Ratio Lower Upper

99 100

42 17.7 13.3 19.9

71 35.8 28.0 42.0






Abundance

Ion 99.00 (98.70 to 99.70): BM017163.D (-650) (-)

Ion 42.00 (41.70 to 42.70): BM017163.D (-650) (-)

Ion 71.00 (70.70 to 71.70): BM017163.D (-650) (-)

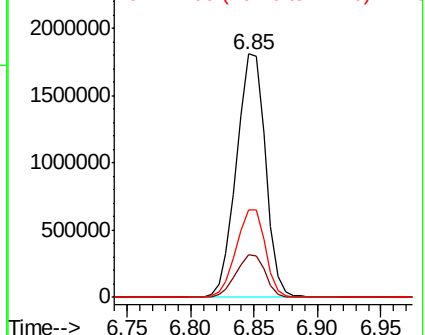

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.43 min Scan# 1266

Delta R.T. -0.02 min

Lab File: BM017269.D

Acq: 20 Oct 2018 17:27

Tgt Ion: 136 Resp: 1351491


Ion Ratio Lower Upper

136 100

137 11.3 9.2 13.8

54 7.6 6.7 10.1

68 5.7 4.7 7.1





Abundance


Ion 136.00 (135.70 to 136.70): BM017163.D (-1261) (-)

Ion 137.00 (136.70 to 137.70): BM017163.D (-1261) (-)

Ion 54.00 (53.70 to 54.70): BM017163.D (-1261) (-)

Ion 68.00 (67.70 to 68.70): BM017163.D (-1261) (-)

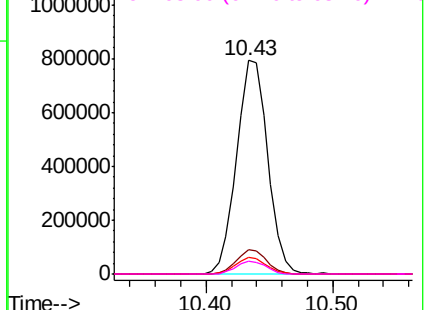







#23
 Nitrobenzene-d5
 Concen: 87.223 ng
 RT: 8.82 min Scan# 991
 Delta R.T. -0.02 min
 Lab File: BM017269.D
 Acq: 20 Oct 2018 17:27

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion: 82 Resp: 201557




Ion	Ratio	Lower	Upper
82	100		
128	43.1	37.0	55.6
54	48.6	40.7	61.1

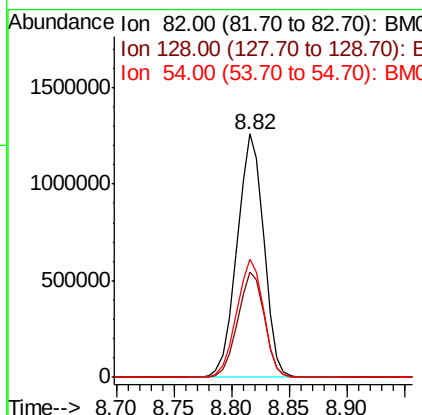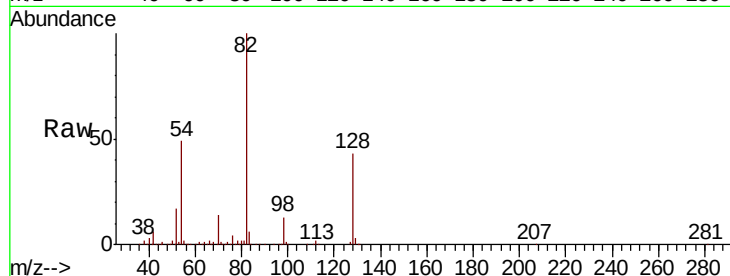


#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.30 min Scan# 1924
 Delta R.T. -0.01 min
 Lab File: BM017269.D
 Acq: 20 Oct 2018 17:27

Tgt Ion: 164 Resp: 797567

Ion	Ratio	Lower	Upper
164	100		
162	103.2	82.1	123.1
160	45.5	40.2	60.2

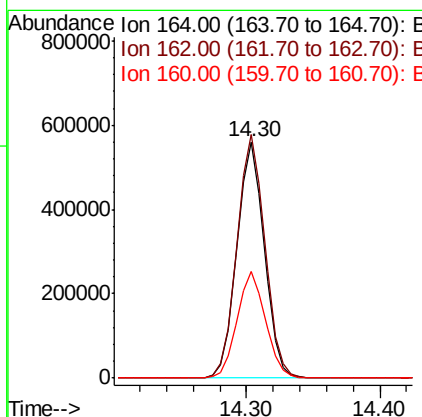


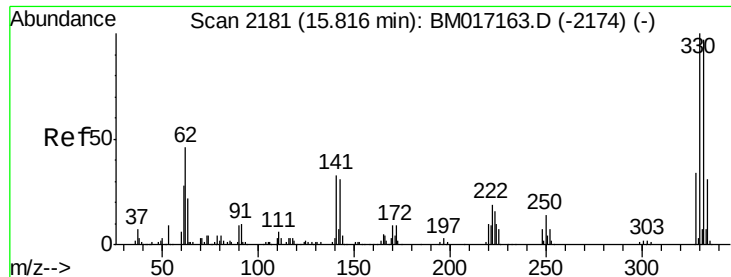




#42
 2,4,6-Tribromophenol
 Concen: 122.686 ng
 RT: 15.80 min Scan# 2179
 Delta R.T. -0.01 min
 Lab File: BM017269.D
 Acq: 20 Oct 2018 17:27

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion:330 Resp: 1323281
 Ion Ratio Lower Upper
 330 100
 332 96.4 77.3 115.9
 141 33.5 27.4 41.0

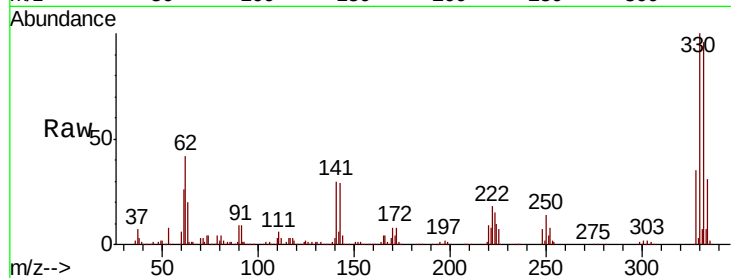


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

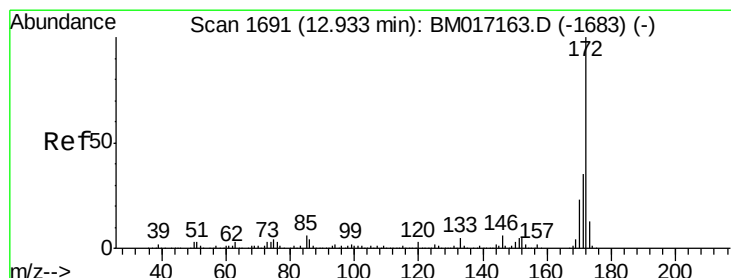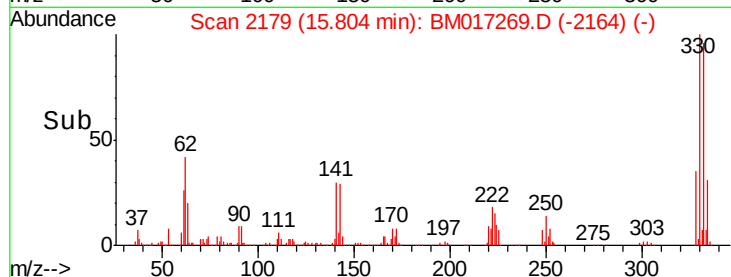
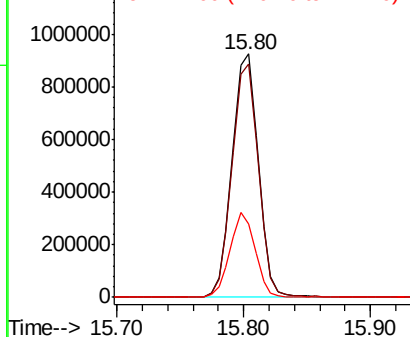



#45
 2-Fluorobiphenyl
 Concen: 77.042 ng
 RT: 12.92 min Scan# 1689
 Delta R.T. -0.01 min
 Lab File: BM017269.D
 Acq: 20 Oct 2018 17:27

Tgt Ion:172 Resp: 4618112
 Ion Ratio Lower Upper
 172 100
 171 34.8 28.3 42.5
 170 22.8 18.3 27.5

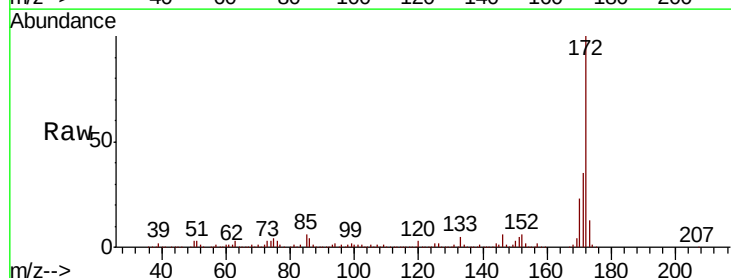

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



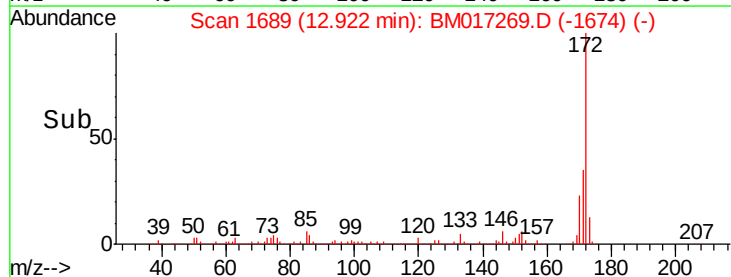
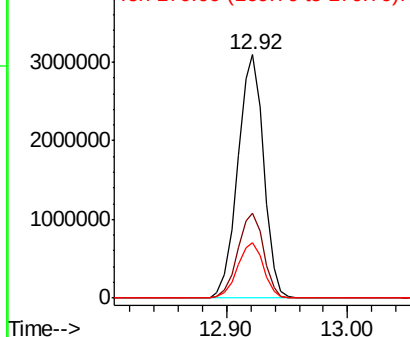




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.06 min Scan# 2392
Delta R.T. -0.01 min
Lab File: BM017269.D
Acq: 20 Oct 2018 17:27




Instrument :
BNA_M
ClientSampleId :


Tot Ion:188 Resp: 1794042
Ion Ratio Lower Upper
188 100
94 8.7 7.0 10.4
80 9.5 7.7 11.5

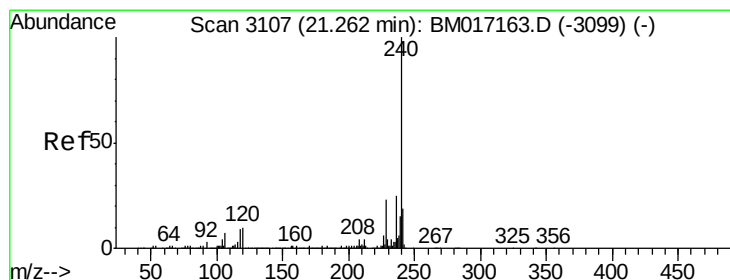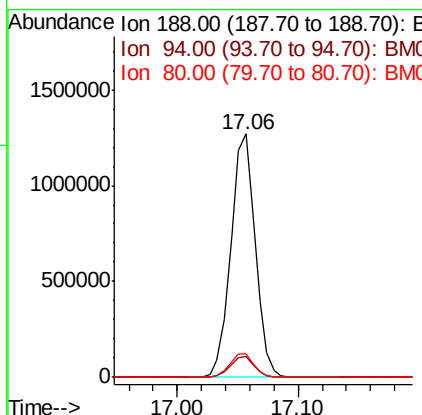

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.25 min Scan# 3105
Delta R.T. -0.01 min
Lab File: BM017269.D
Acq: 20 Oct 2018 17:27

Tgt Ion:240 Resp: 1579020
Ion Ratio Lower Upper
240 100
120 9.5 8.1 12.1
236 25.2 19.9 29.9

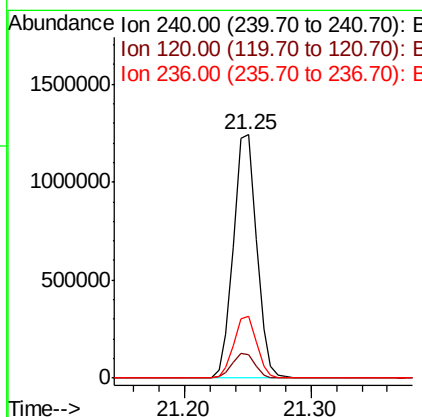

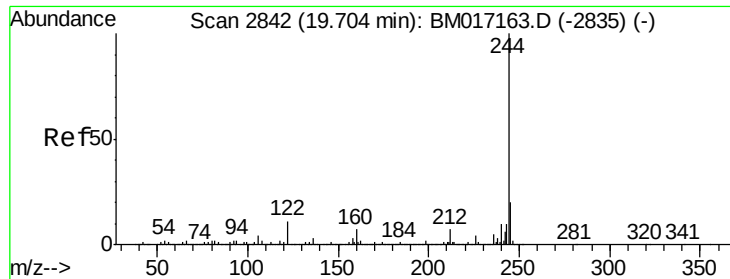

#79

Terphenyl-d14

Concen: 97.427 ng

RT: 19.70 min Scan# 2841

Delta R.T. -0.01 min

Lab File: BM017269.D

Acq: 20 Oct 2018 17:27

Instrument :

BNA_M

ClientSampleId :


Tot Ion:244 Resp: 6825182

Ion Ratio Lower Upper

244 100

212 7.2 5.5 8.3




122 10.0 8.4 12.6



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

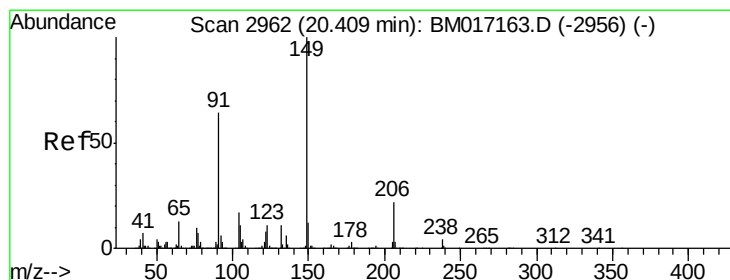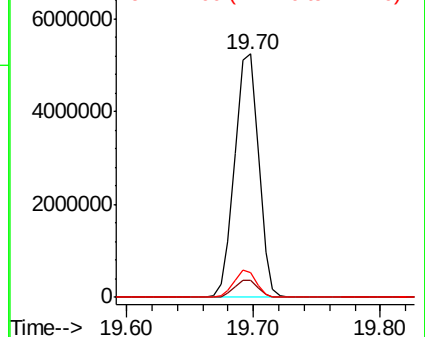

#80

Butylbenzylphthalate

Concen: 7.187 ng

RT: 20.40 min Scan# 2961

Delta R.T. -0.01 min

Lab File: BM017269.D

Acq: 20 Oct 2018 17:27


Tgt Ion:149 Resp: 424

Ion Ratio Lower Upper

149 100

91 100.9 51.3 76.9#



206 42.0 18.0 27.0#




Abundance Ion 149.00 (148.70 to 149.70): E

Ion 91.00 (90.70 to 91.70): BM0

Ion 206.00 (205.70 to 206.70): E

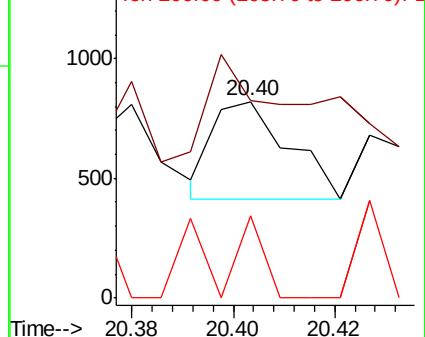

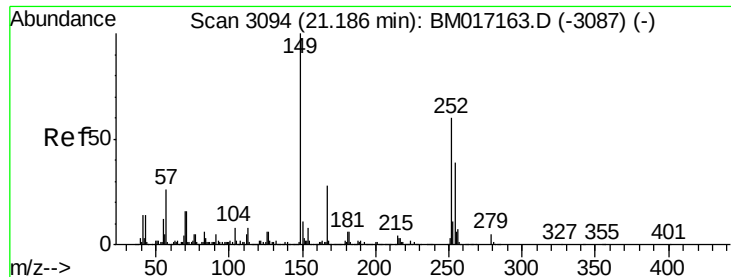

#84

Bis(2-ethylhexyl)phthalate

Concen: 5.350 ng

RT: 21.17 min Scan# 3092

Delta R.T. -0.01 min

Lab File: BM017269.D

Acq: 20 Oct 2018 17:27

Instrument :

BNA_M

ClientSampleId :


Tot Ion:149 Resp: 2459

Ion Ratio Lower Upper

149 100

167 18.9 22.2 33.4#




279 0.0 3.6 5.4#

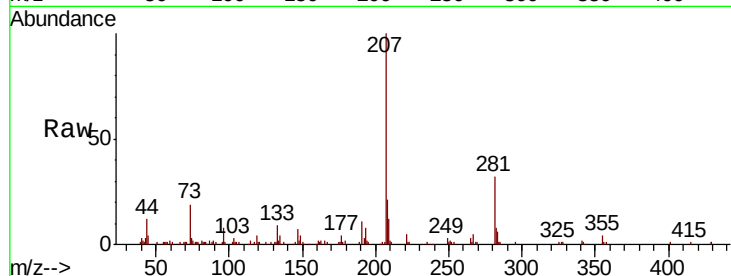

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

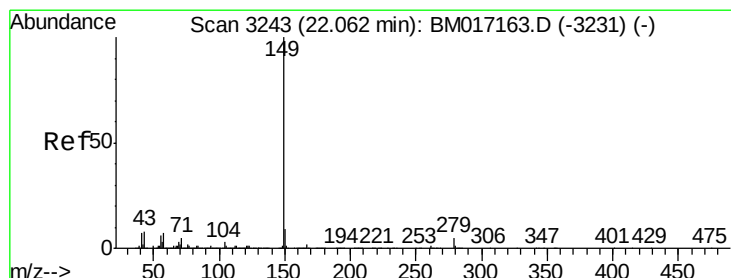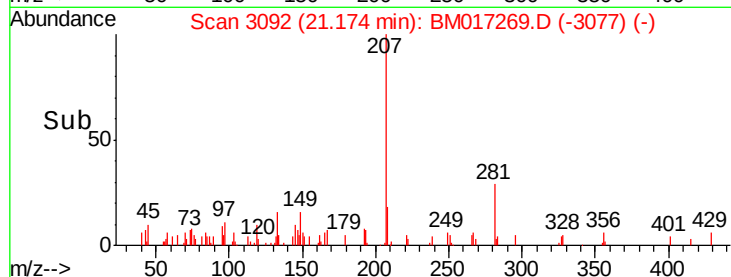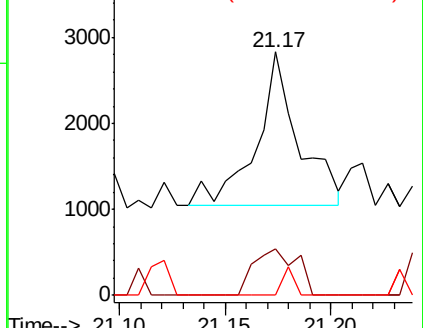

#85

Di-n-octyl phthalate

Concen: 5.580 ng

RT: 22.03 min Scan# 3238

Delta R.T. -0.03 min

Lab File: BM017269.D

Acq: 20 Oct 2018 17:27


Tgt Ion:149 Resp: 883

Ion Ratio Lower Upper

149 100

167 14.6 1.4 2.0#



43 209.5 7.2 10.8#

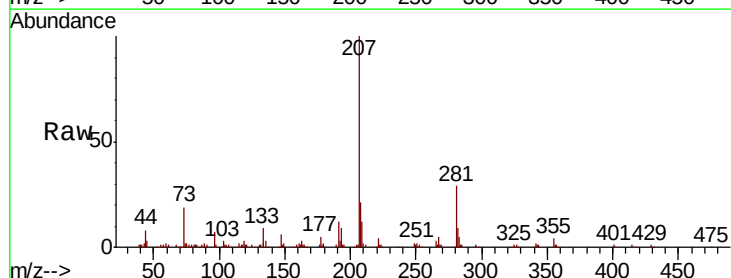


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 43.00 (42.70 to 43.70): BM

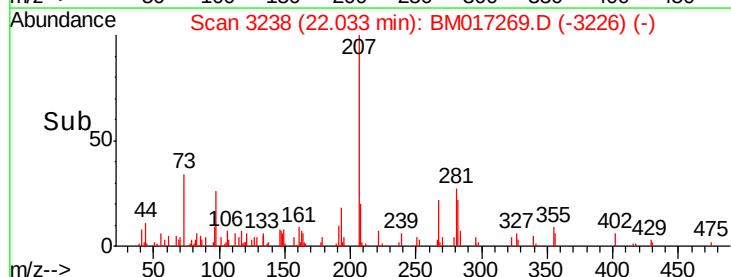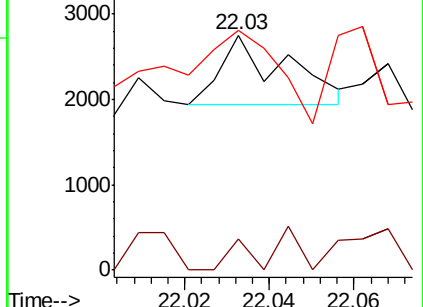

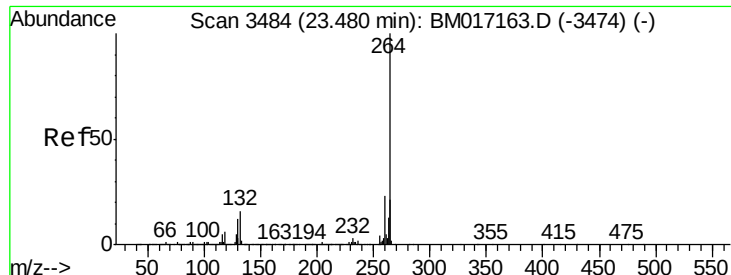


#87
Pervlene-d12
Concen: 20.000 ng
RT: 23.46 min Scan# 3481
Delta R.T. -0.02 min
Lab File: BM017269.D
Acq: 20 Oct 2018 17:27

Instrument :
BNA_M
ClientSampleId :

Tot Ion:264 Resp: 1426881

Ion	Ratio	Lower	Upper
264	100		
260	23.0	18.6	27.8
265	22.5	17.8	26.8

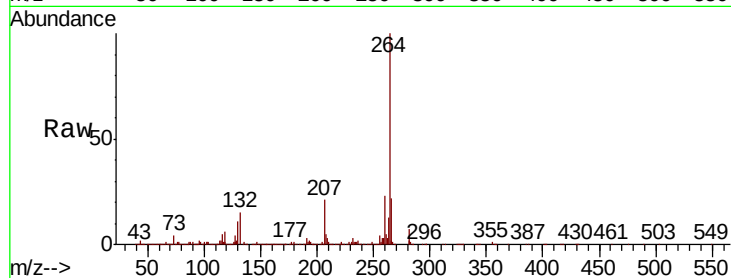

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

