
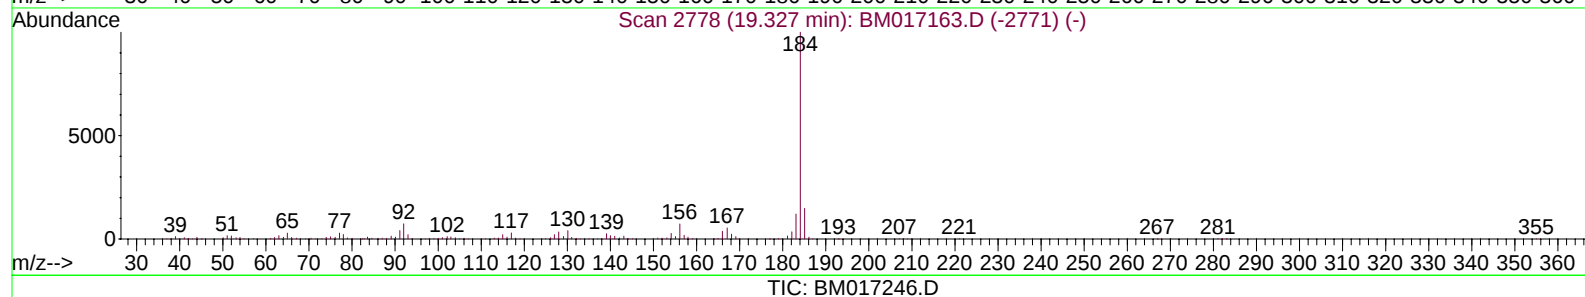
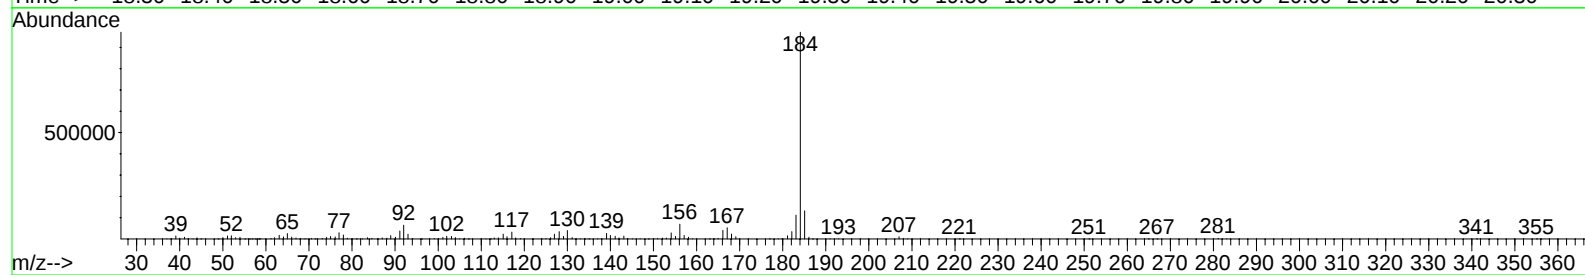


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM101918\
 Data File : BM017246.D
 Acq On : 20 Oct 2018 02:10
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 22 08:31:56 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM101718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 17 14:23:17 2018
 Response via : Initial Calibration

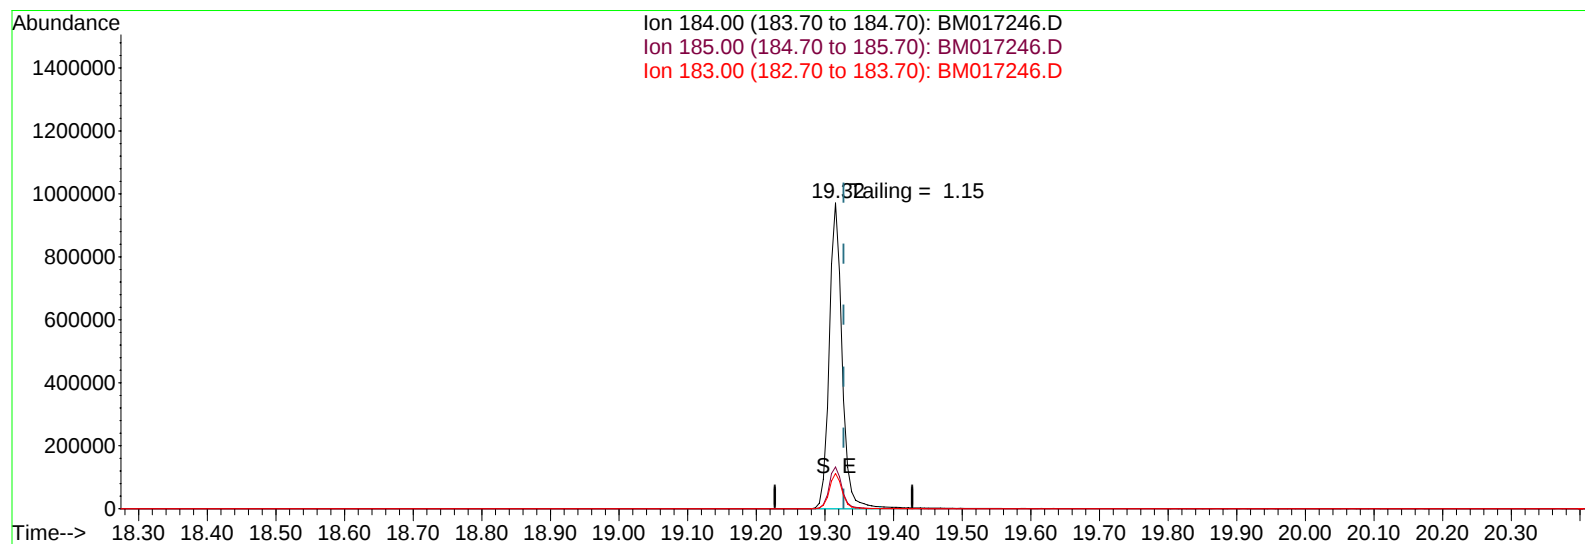

(77) Benzidine




19.315min (-0.012) 54714.37ng

response 1265277

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	13.68
183.00	12.10	11.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM101918\
Data File : BM017246.D
Acq On : 20 Oct 2018 02:10
Operator : MJ/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 22 08:31:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM101718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 17 14:23:17 2018
Response via : Initial Calibration

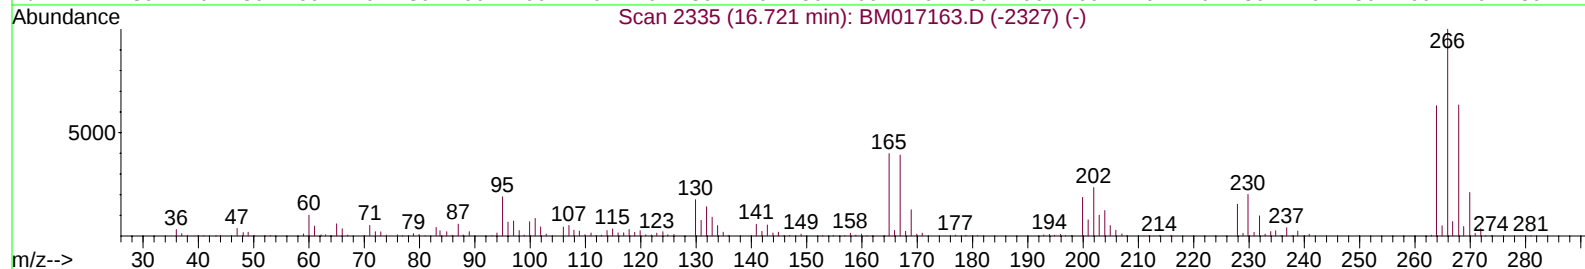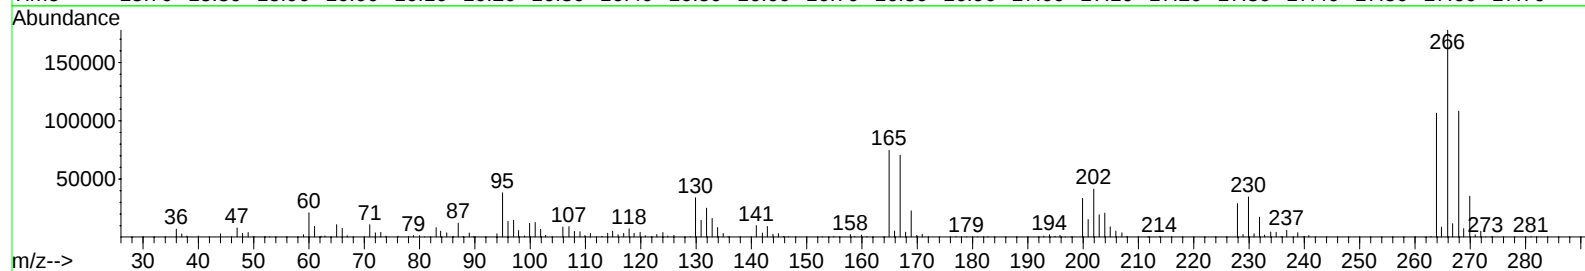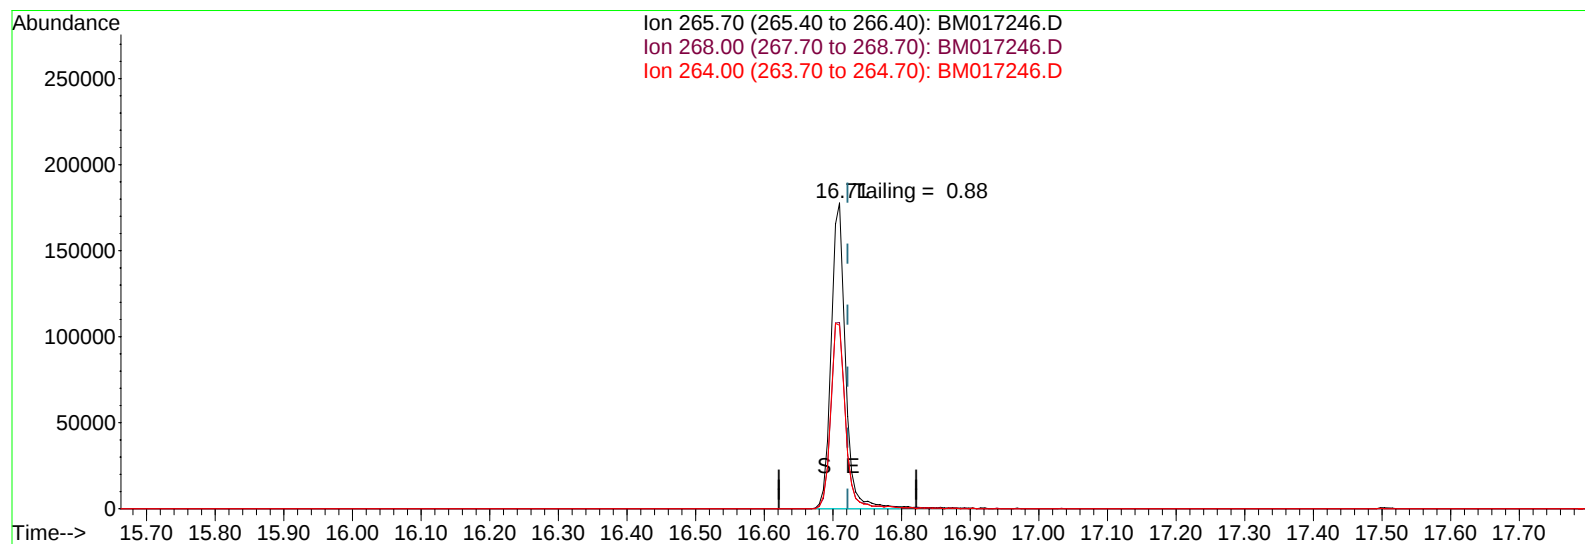

TIC: BM017246.D

(70) Pentachlorophenol (C)

16.710min (-0.012) 0.00ng

response 257756

Ion	Exp%	Act%
265.70	100	100
268.00	63.40	60.89
264.00	63.00	60.02
0.00	0.00	0.00