

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM101918\
 Data File : BM017251.D
 Acq On : 20 Oct 2018 05:24
 Operator : MJ/SJ
 Sample : J5565-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 RLF-SD-4

Quant Time: Oct 22 02:51:56 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM101718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 17 14:23:17 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	269756	20.00	ng	-0.01
21) Naphthalene-d8	10.44	136	1135269	20.00	ng	-0.01
39) Acenaphthene-d10	14.30	164	708973	20.00	ng	-0.01
64) Phenanthrene-d10	17.06	188	1626812	20.00	ng	-0.01
76) Chrysene-d12	21.24	240	1532635	20.00	ng	-0.02
87) Perylene-d12	23.46	264	1307678	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.28	112	753601	47.25	ng	-0.01
7) Phenol-d6	6.84	99	1035083	47.65	ng	-0.02
23) Nitrobenzene-d5	8.82	82	631483	32.53	ng	-0.02
42) 2,4,6-Tribromophenol	15.80	330	436739	45.55	ng	-0.02
45) 2-Fluorobiphenyl	12.92	172	1489443	27.95	ng	-0.01
79) Terphenyl-d14	19.69	244	2055617	30.23	ng	-0.01
Target Compounds						
10) Phenol	6.86	94	47626	2.037	ng	92
50) Dimethylphthalate	13.77	163	266200	4.867	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM101918\
Data File : BM017251.D
Acq On : 20 Oct 2018 05:24
Operator : MJ/SJ
Sample : J5565-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
RLF-SD-4

Quant Time: Oct 22 02:51:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM101718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 17 14:23:17 2018
Response via : Initial Calibration

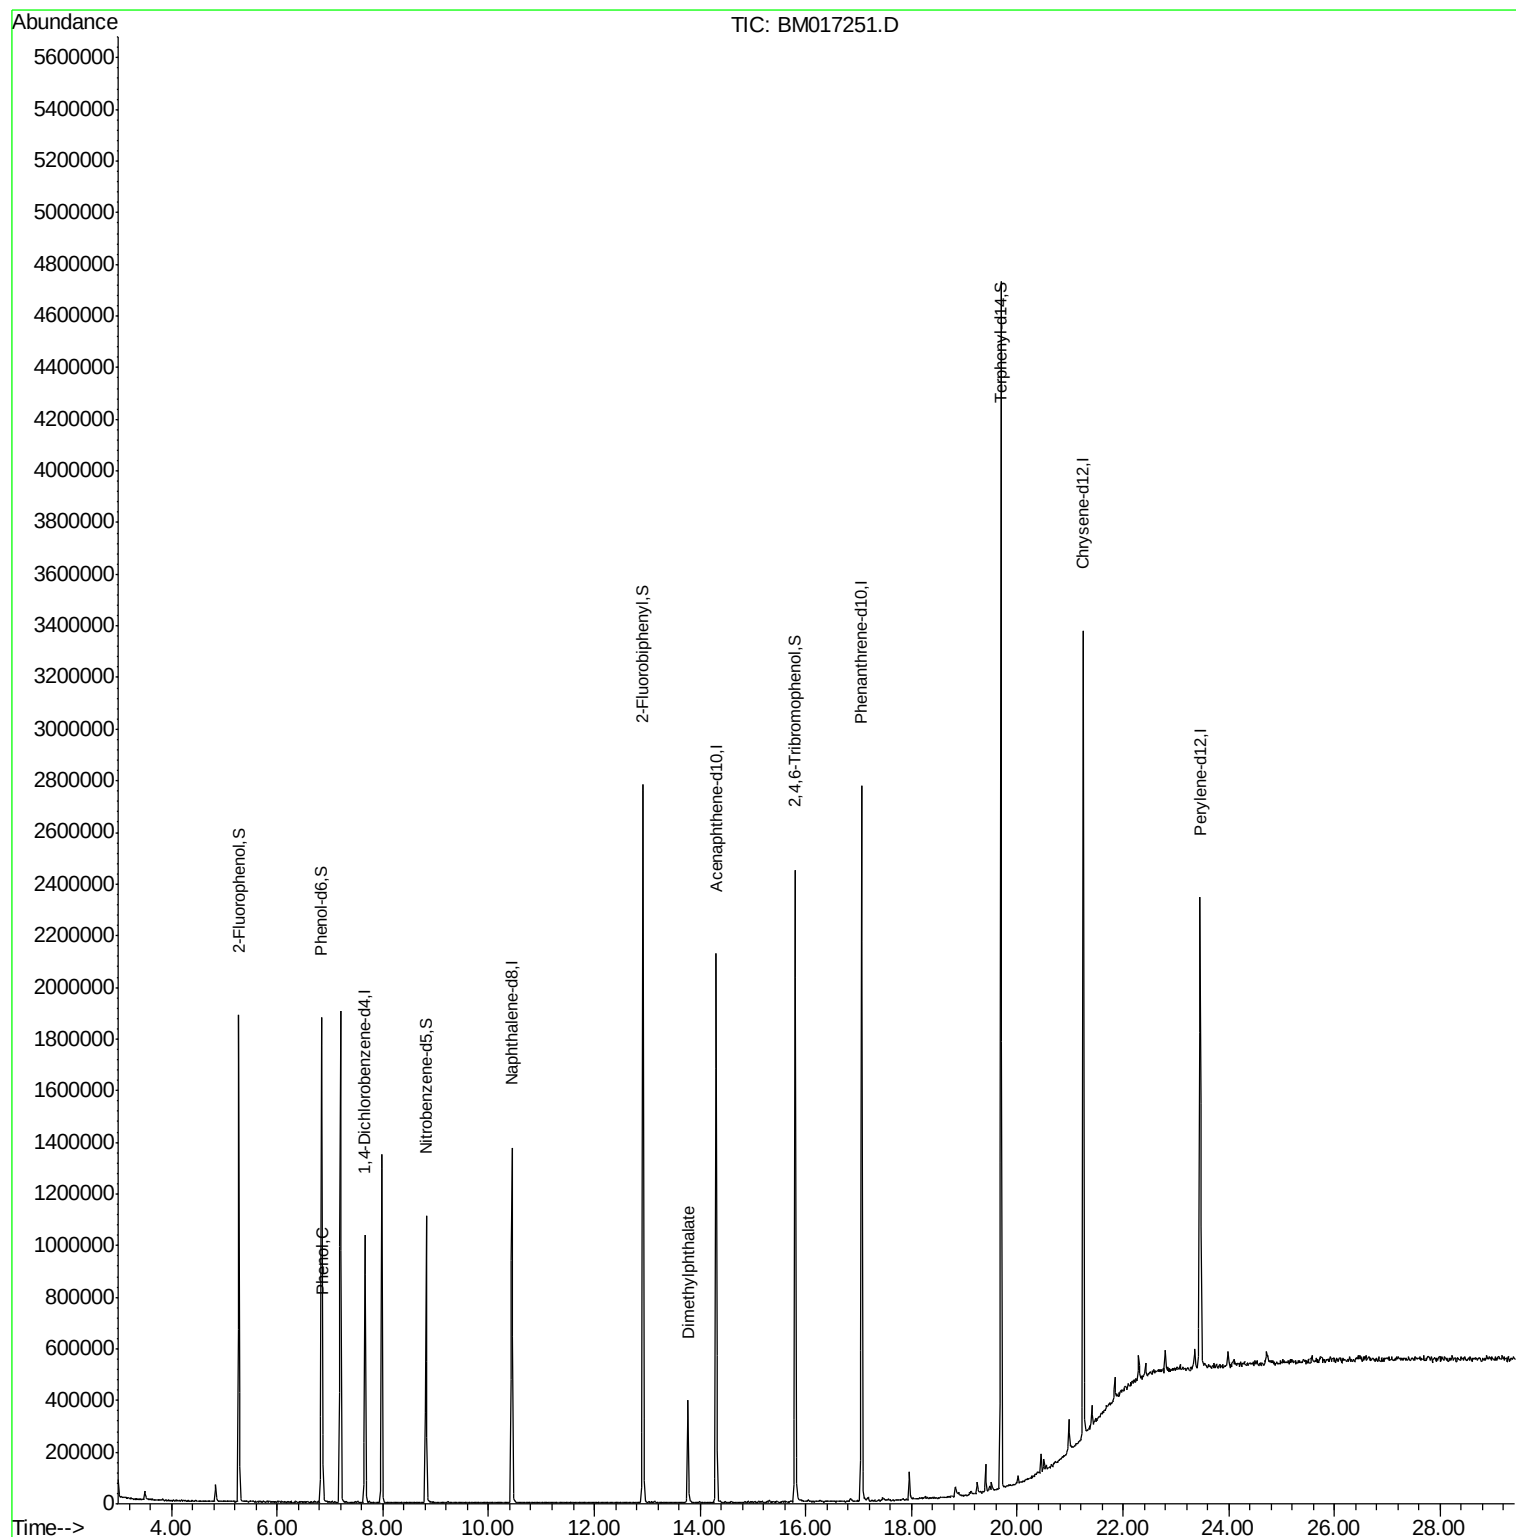

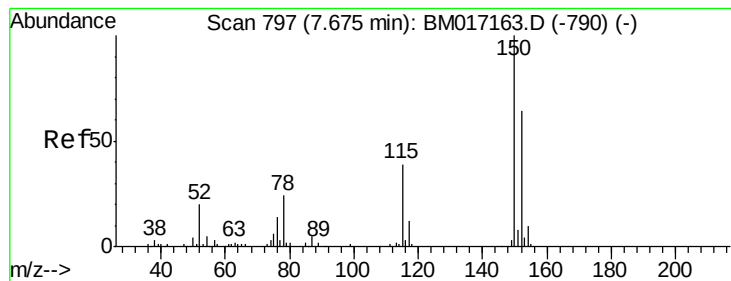


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.66 min Scan# 795
Delta R.T. -0.01 min
Lab File: BM017251.D
Acq: 20 Oct 2018 05:24

Instrument :
BNA_M
ClientSampleId :
RLF-SD-4

Tgt Ion	Ratio	Lower	Upper
152	100		
150	152.4	124.3	186.5
115	60.0	48.1	72.1

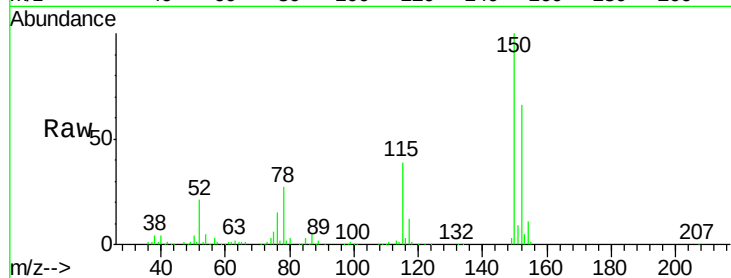


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

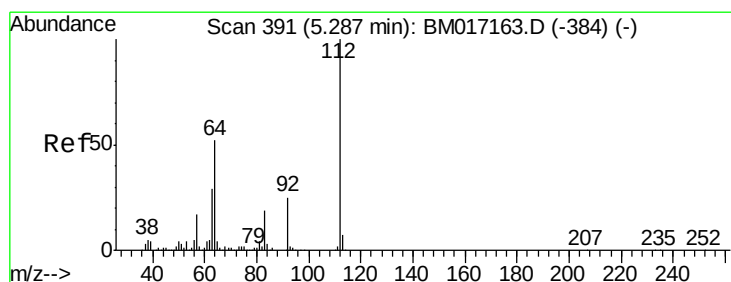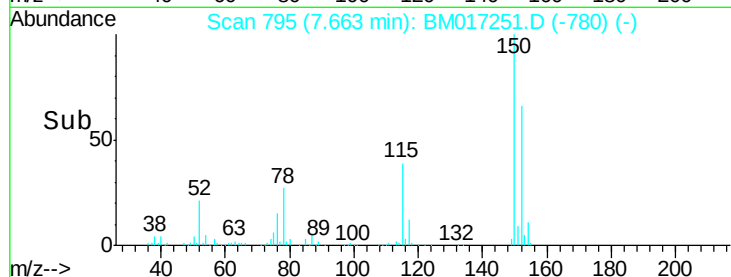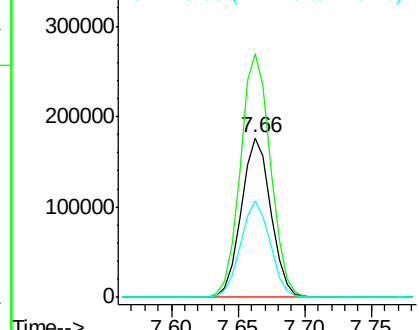



#5




2-Fluorophenol
Concen: 47.250 ng
RT: 5.28 min Scan# 389
Delta R.T. -0.01 min
Lab File: BM017251.D
Acq: 20 Oct 2018 05:24

Tgt Ion	Ratio	Lower	Upper
112	100		
64	57.5	41.7	62.5
63	30.5	23.0	34.4

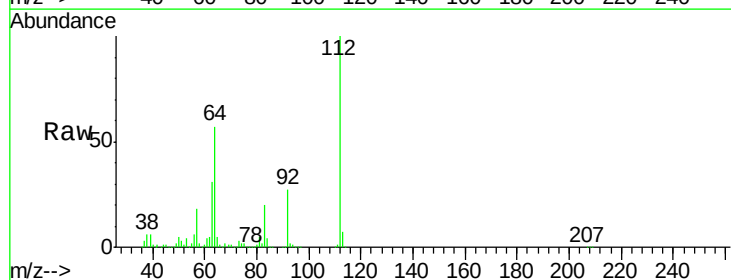

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

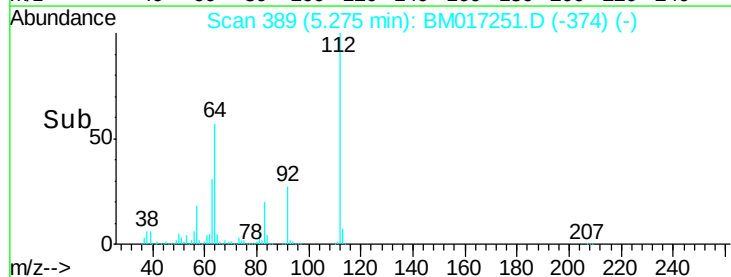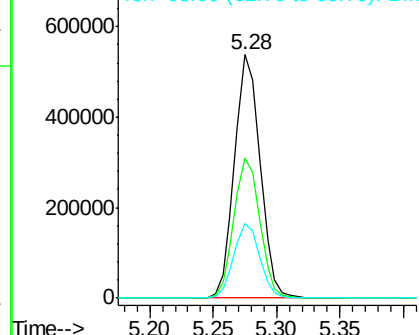

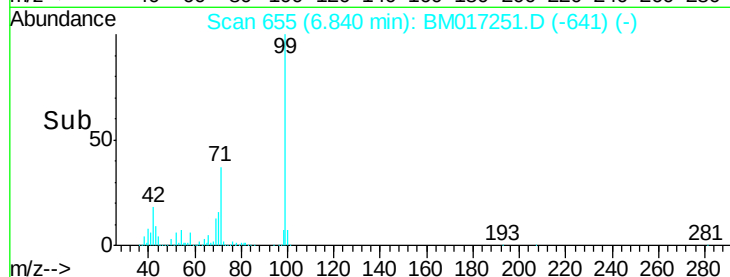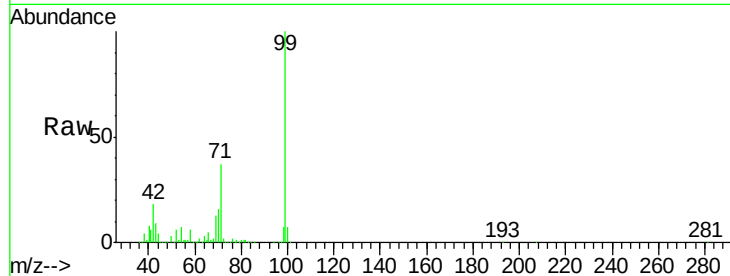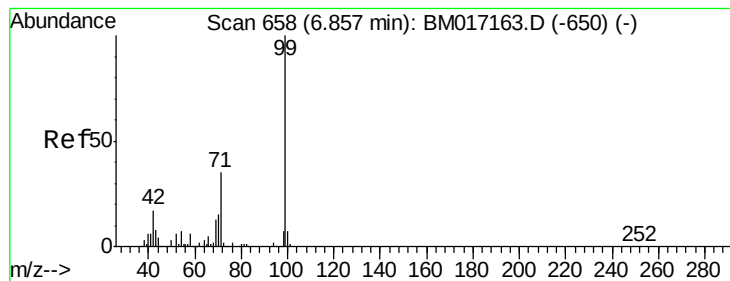

#7

Phenol-d6

Concen: 47.651 ng

RT: 6.84 min Scan# 655

Delta R.T. -0.02 min

Lab File: BM017251.D

Acq: 20 Oct 2018 05:24

Instrument :

BNA_M

ClientSampleId :

RLF-SD-4





Tgt Ion: 99 Resp: 1035083

Ion Ratio Lower Upper

99 100

42 17.9 13.3 19.9

71 37.2 28.0 42.0

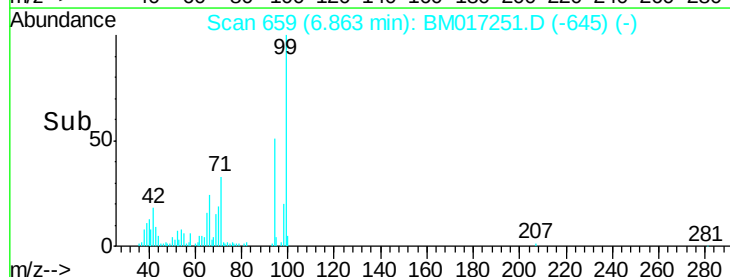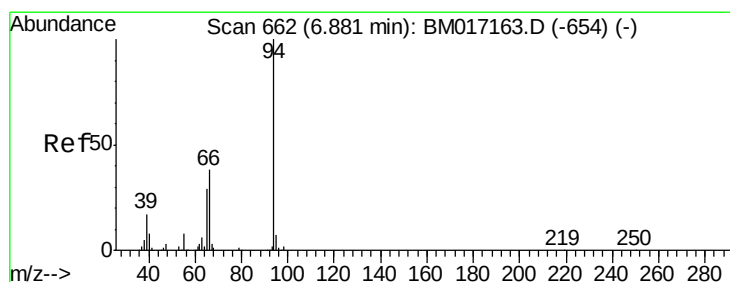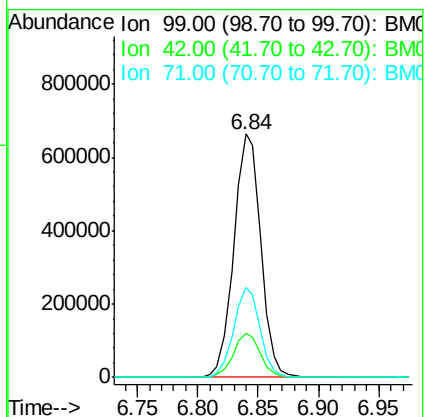

#10

Phenol

Concen: 2.037 ng

RT: 6.86 min Scan# 659

Delta R.T. -0.02 min

Lab File: BM017251.D

Acq: 20 Oct 2018 05:24


Tgt Ion: 94 Resp: 47626


Ion Ratio Lower Upper

94 100

65 30.4 9.4 49.4

66 46.8 19.0 59.0

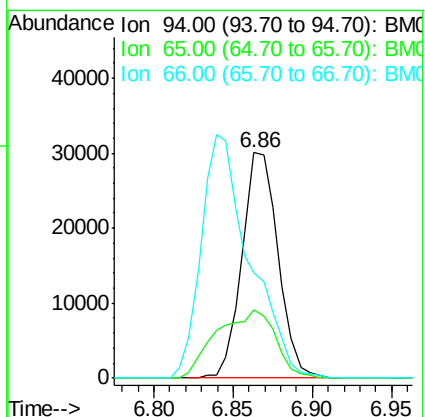

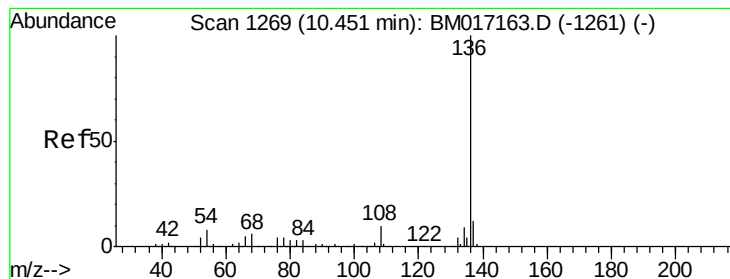

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.44 min Scan# 1267

Delta R.T. -0.01 min

Lab File: BM017251.D

Acq: 20 Oct 2018 05:24

Instrument :

BNA_M

ClientSampleId :

RLF-SD-4

Tgt Ion:136 Resp: 1135269


Ion Ratio Lower Upper

136 100

137 10.8 9.2 13.8

54 7.9 6.7 10.1

68 5.8 4.7 7.1




Abundance Ion 136.00 (135.70 to 136.70): E


Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BM

Ion 68.00 (67.70 to 68.70): BM

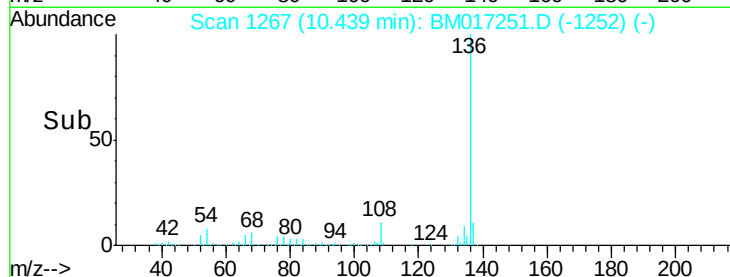

Time-->

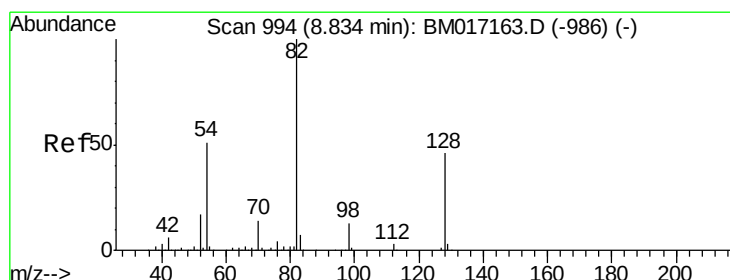

#23

Nitrobenzene-d5

Concen: 32.532 ng

RT: 8.82 min Scan# 991

Delta R.T. -0.02 min

Lab File: BM017251.D

Acq: 20 Oct 2018 05:24


Tgt Ion: 82 Resp: 631483

Ion Ratio Lower Upper

82 100

128 41.8 37.0 55.6


54 49.2 40.7 61.1




Abundance Ion 82.00 (81.70 to 82.70): BM

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BM

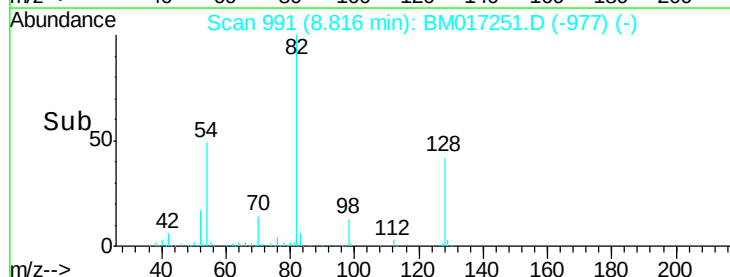





Time-->

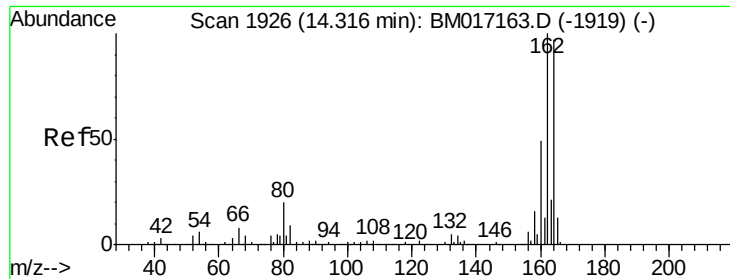

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.30 min Scan# 1924
Delta R.T. -0.01 min
Lab File: BM017251.D
Acq: 20 Oct 2018 05:24




Instrument :
BNA_M
ClientSampleId :
RLF-SD-4


Tgt Ion:164 Resp: 708973
Ion Ratio Lower Upper
164 100
162 99.8 82.1 123.1
160 45.8 40.2 60.2

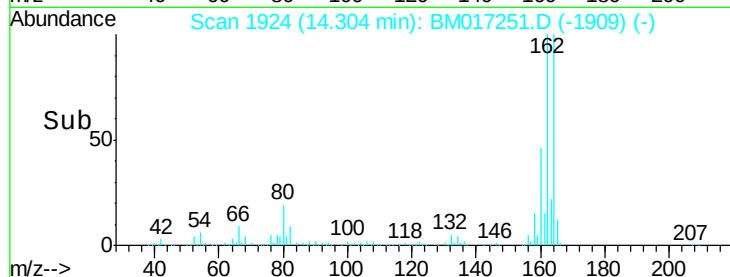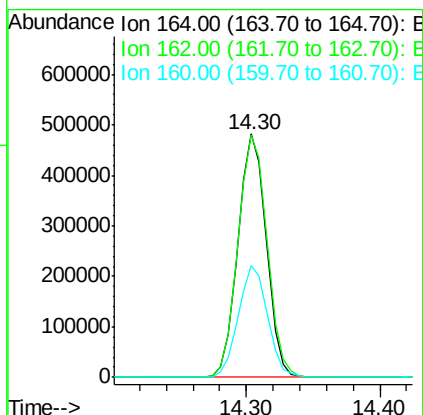

#42
2,4,6-Tribromophenol
Concen: 45.551 ng
RT: 15.80 min Scan# 2178
Delta R.T. -0.02 min
Lab File: BM017251.D
Acq: 20 Oct 2018 05:24

Tgt Ion:330 Resp: 436739
Ion Ratio Lower Upper
330 100
332 96.3 77.3 115.9
141 34.3 27.4 41.0


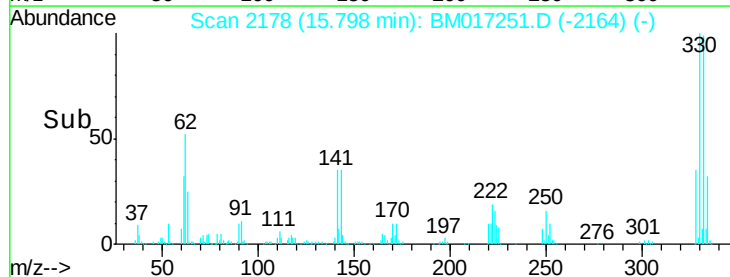
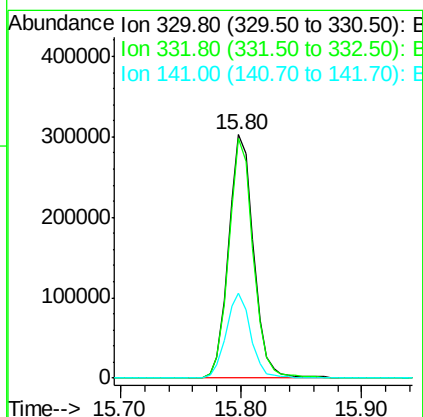



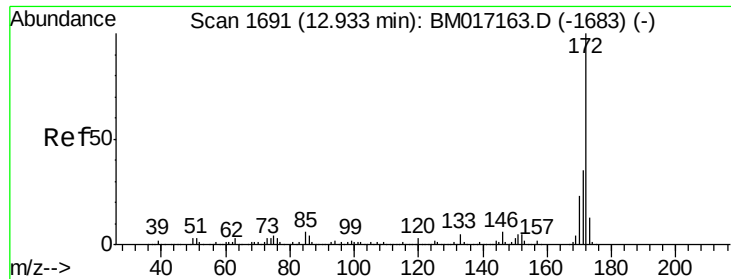

#45
 2-Fluorobiphenyl
 Concen: 27.953 ng
 RT: 12.92 min Scan# 1689
 Delta R.T. -0.01 min
 Lab File: BM017251.D
 Acq: 20 Oct 2018 05:24




Instrument :
 BNA_M
 ClientSampleId :
 RLF-SD-4


Tgt Ion:172 Resp: 1489443
 Ion Ratio Lower Upper
 172 100
 171 35.3 28.3 42.5
 170 22.2 18.3 27.5

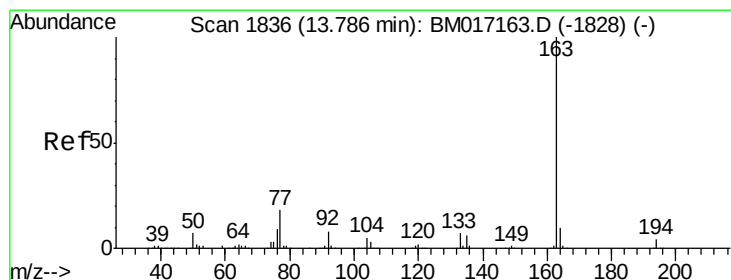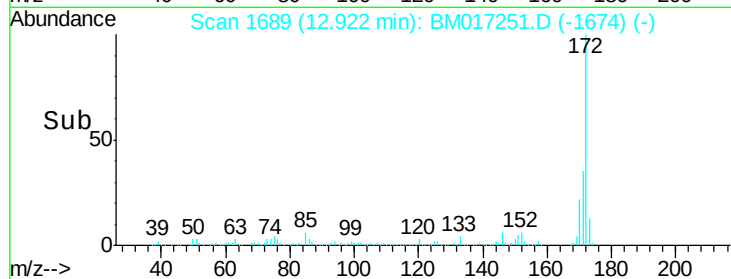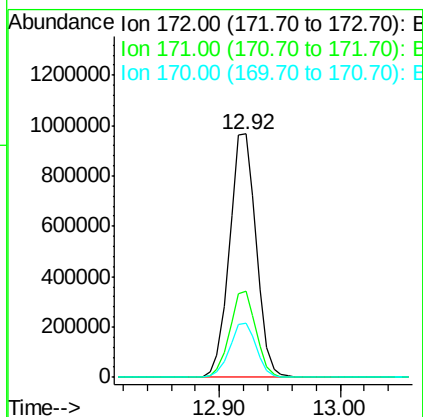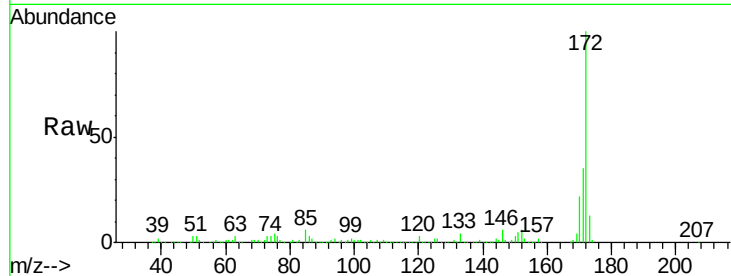

#50
 Dimethylphthalate
 Concen: 4.867 ng
 RT: 13.77 min Scan# 1833
 Delta R.T. -0.02 min
 Lab File: BM017251.D
 Acq: 20 Oct 2018 05:24

Tgt Ion:163 Resp: 266200
 Ion Ratio Lower Upper
 163 100
 194 3.7 3.3 4.9
 164 9.5 7.8 11.8


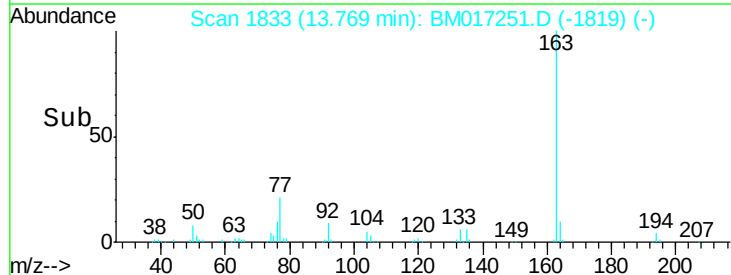
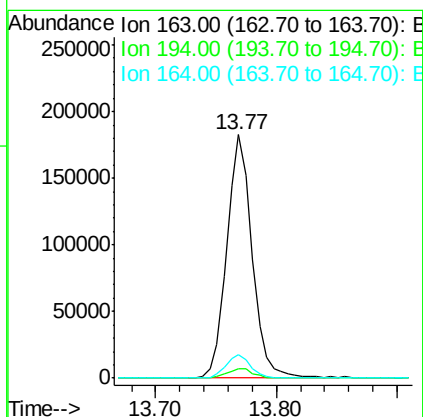
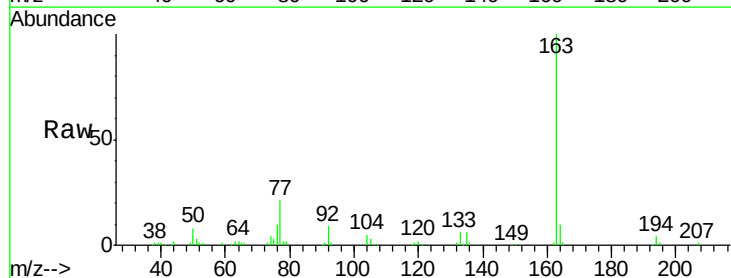


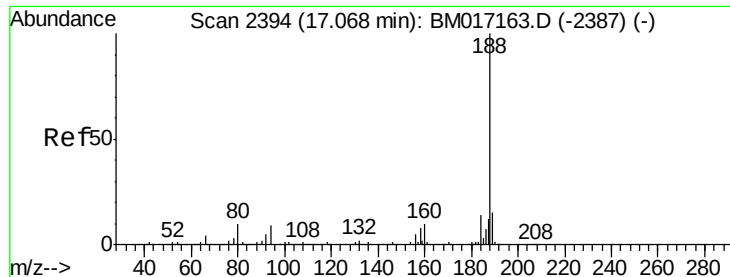

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.06 min Scan# 2392
Delta R.T. -0.01 min
Lab File: BM017251.D
Acq: 20 Oct 2018 05:24




Instrument :
BNA_M
ClientSampleId :
RLF-SD-4


Tgt Ion:188 Resp: 1626812
Ion Ratio Lower Upper
188 100
94 8.6 7.0 10.4
80 9.4 7.7 11.5

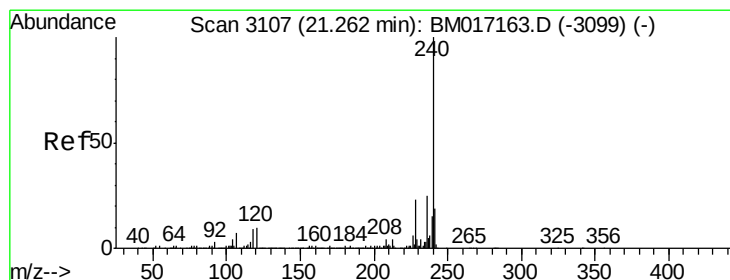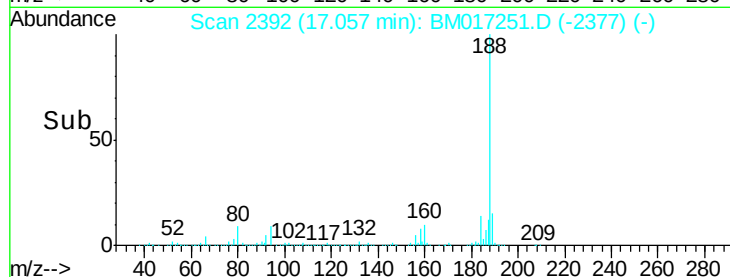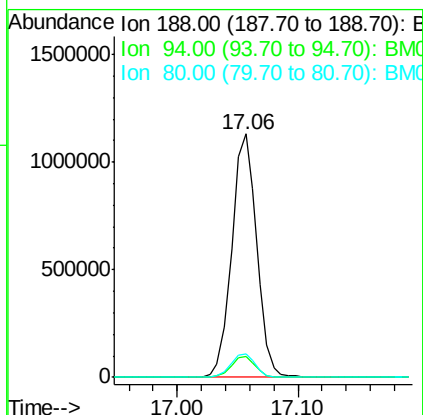

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.24 min Scan# 3104
Delta R.T. -0.02 min
Lab File: BM017251.D
Acq: 20 Oct 2018 05:24

Tgt Ion:240 Resp: 1532635
Ion Ratio Lower Upper
240 100
120 10.1 8.1 12.1
236 24.8 19.9 29.9

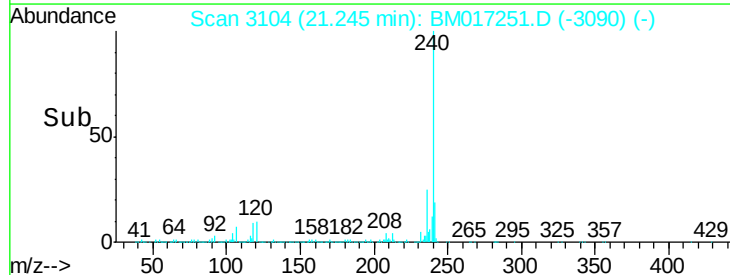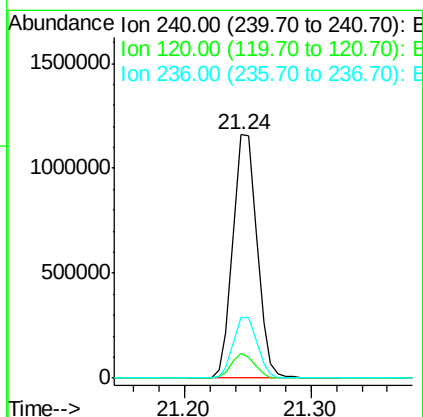

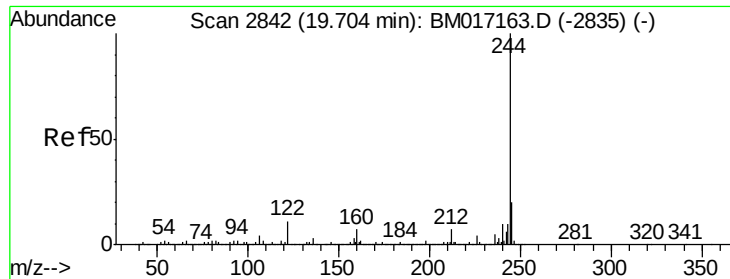

#79

Terphenyl-d14

Concen: 30.231 ng

RT: 19.69 min Scan# 2840

Delta R.T. -0.01 min

Lab File: BM017251.D

Acq: 20 Oct 2018 05:24

Instrument :

BNA_M

ClientSampleId :

RLF-SD-4


Tgt Ion:244 Resp: 2055617

Ion Ratio Lower Upper

244 100

212 7.2 5.5 8.3




122 10.2 8.4 12.6

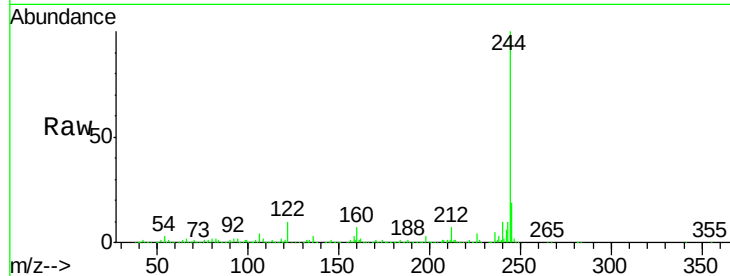

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

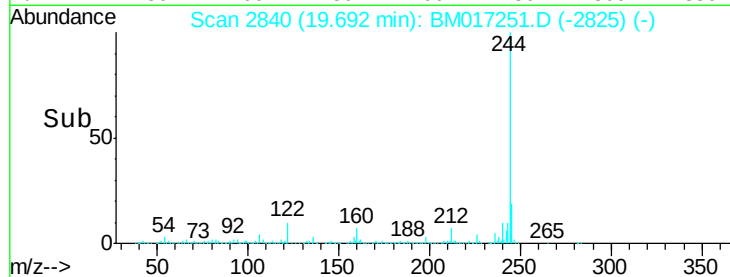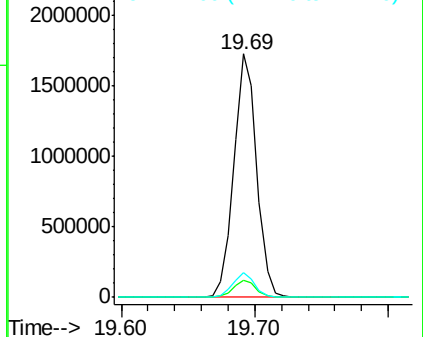

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.46 min Scan# 3481

Delta R.T. -0.02 min

Lab File: BM017251.D

Acq: 20 Oct 2018 05:24


Tgt Ion:264 Resp: 1307678

Ion Ratio Lower Upper

264 100

260 23.1 18.6 27.8

265 21.5 17.8 26.8



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

