

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM101918\
 Data File : BM017252.D
 Acq On : 20 Oct 2018 06:01
 Operator : MJ/SJ
 Sample : J5575-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSSI-1015-S-DH-25A-T

Quant Time: Oct 22 03:45:35 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM101718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 17 14:23:17 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	292087	20.00	ng	-0.01
21) Naphthalene-d8	10.44	136	1202554	20.00	ng	-0.01
39) Acenaphthene-d10	14.30	164	727076	20.00	ng	-0.01
64) Phenanthrene-d10	17.06	188	1595998	20.00	ng	-0.01
76) Chrysene-d12	21.25	240	1495373	20.00	ng	-0.01
87) Perylene-d12	23.46	264	1370899	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.28	112	1356498	78.55	ng	0.00
7) Phenol-d6	6.85	99	1858274	79.01	ng	-0.01
23) Nitrobenzene-d5	8.82	82	1124283	54.68	ng	-0.02
42) 2,4,6-Tribromophenol	15.80	330	750640	76.34	ng	-0.01
45) 2-Fluorobiphenyl	12.92	172	2691717	49.26	ng	-0.01
79) Terphenyl-d14	19.69	244	3551543	53.53	ng	-0.01
Target Compounds						
10) Phenol	6.87	94	171420	6.772	ng	96
50) Dimethylphthalate	13.77	163	259345	4.623	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM101918\
Data File : BM017252.D
Acq On : 20 Oct 2018 06:01
Operator : MJ/SJ
Sample : J5575-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSSI-1015-S-DH-25A-T

Quant Time: Oct 22 03:45:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM101718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 17 14:23:17 2018
Response via : Initial Calibration

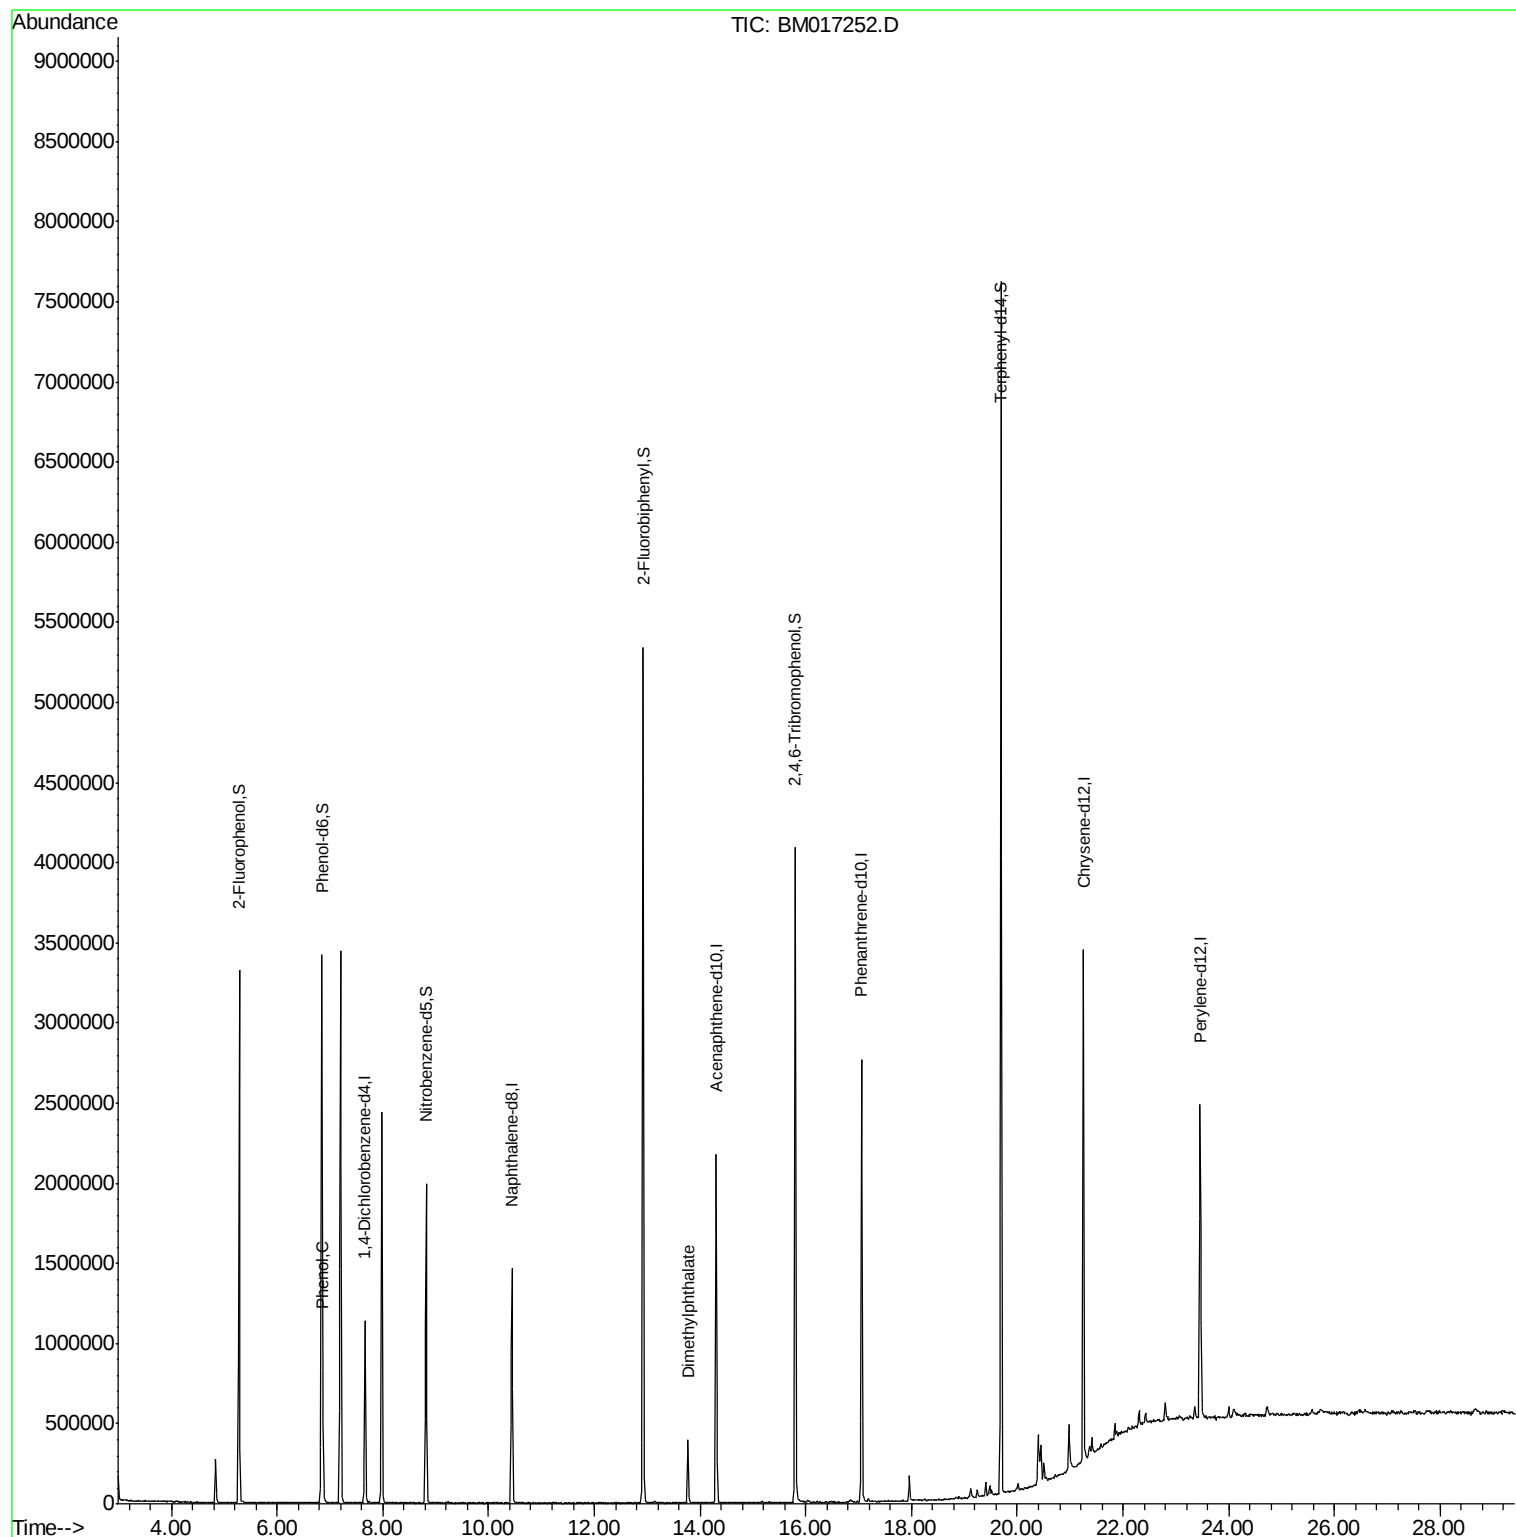

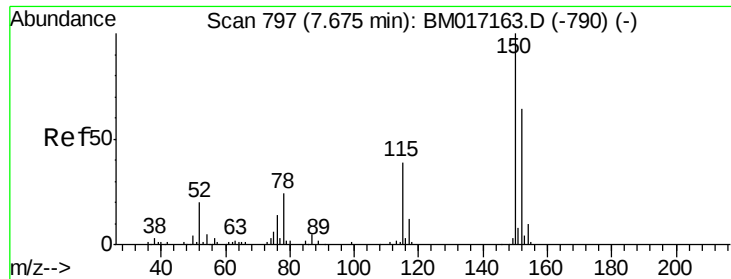


#1


1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.66 min Scan# 795
Delta R.T. -0.01 min
Lab File: BM017252.D
Acq: 20 Oct 2018 06:01

Instrument :
BNA_M
ClientSampleId :
SSSI-1015-S-DH-25A-T



Tgt Ion:152 Resp: 292087
Ion Ratio Lower Upper
152 100
150 155.4 124.3 186.5
115 59.9 48.1 72.1

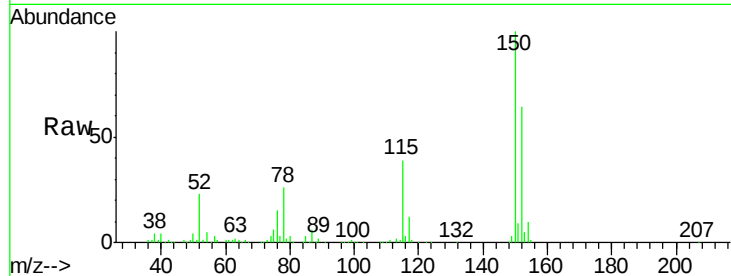

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

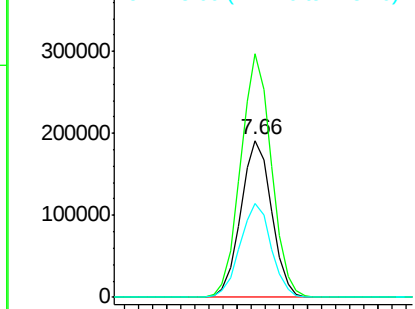


Time-->

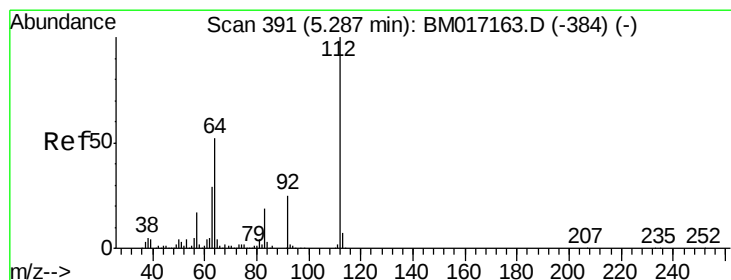


#5

2-Fluorophenol
Concen: 78.548 ng
RT: 5.28 min Scan# 390
Delta R.T. -0.01 min
Lab File: BM017252.D
Acq: 20 Oct 2018 06:01


Tgt Ion:112 Resp: 1356498
Ion Ratio Lower Upper
112 100
64 57.2 41.7 62.5
63 30.9 23.0 34.4






Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

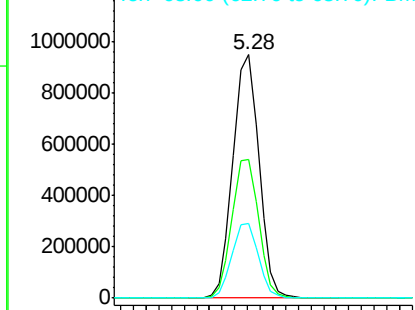

Time-->



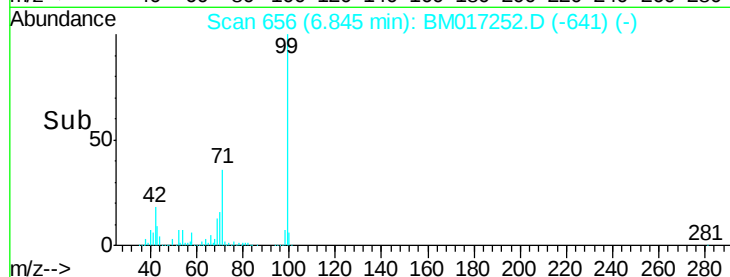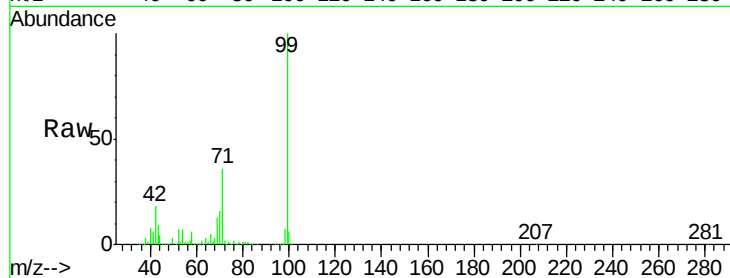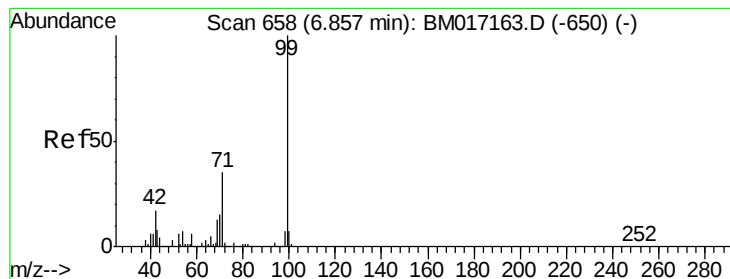

#7

Phenol-d6

Concen: 79.007 ng

RT: 6.85 min Scan# 656

Delta R.T. -0.01 min

Lab File: BM017252.D

Acq: 20 Oct 2018 06:01

Instrument :

BNA_M

ClientSampleId :

SSSI-1015-S-DH-25A-T





Tgt Ion: 99 Resp: 1858274

Ion Ratio Lower Upper

99 100

42 17.8 13.3 19.9

71 36.5 28.0 42.0

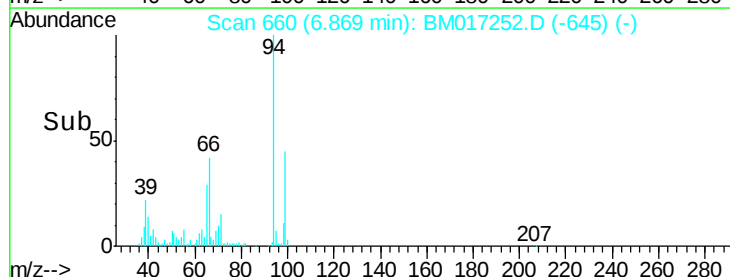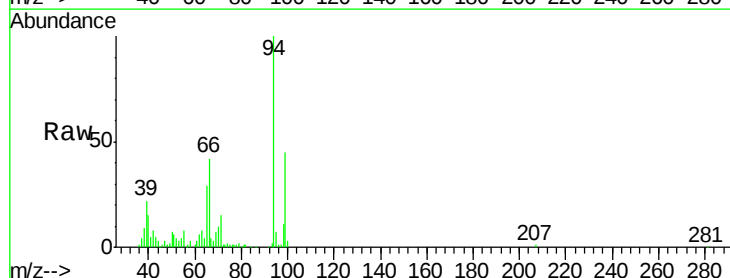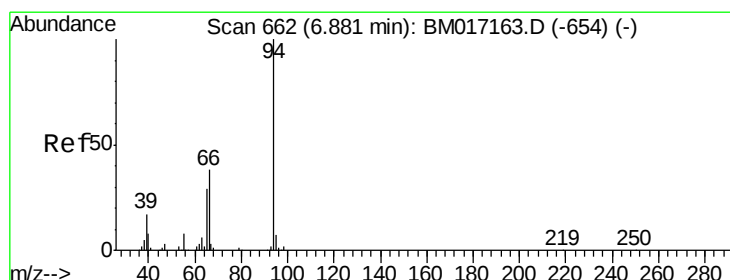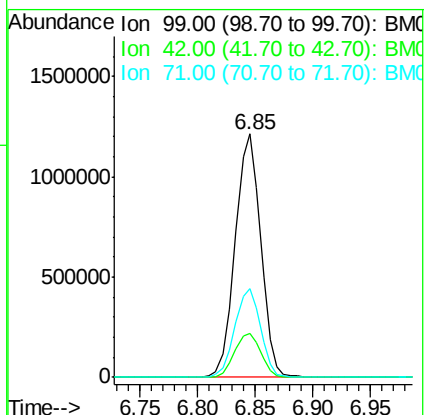

#10

Phenol

Concen: 6.772 ng

RT: 6.87 min Scan# 660

Delta R.T. -0.01 min

Lab File: BM017252.D

Acq: 20 Oct 2018 06:01


Tgt Ion: 94 Resp: 171420


Ion Ratio Lower Upper

94 100

65 28.6 9.4 49.4

66 42.3 19.0 59.0

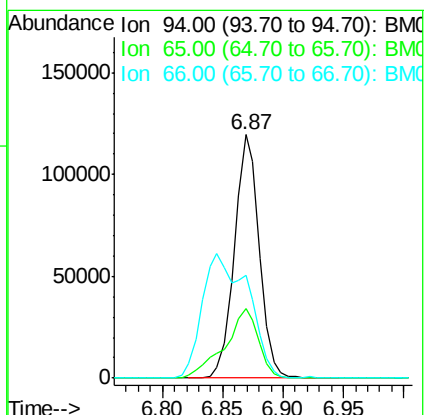







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.44 min Scan# 1267
Delta R.T. -0.01 min
Lab File: BM017252.D
Acq: 20 Oct 2018 06:01

Instrument :
BNA_M
ClientSampleId :
SSSI-1015-S-DH-25A-T

Tgt Ion: 136 Resp: 1202554
Ion Ratio Lower Upper
136 100
137 10.4 9.2 13.8
54 8.1 6.7 10.1
68 5.4 4.7 7.1

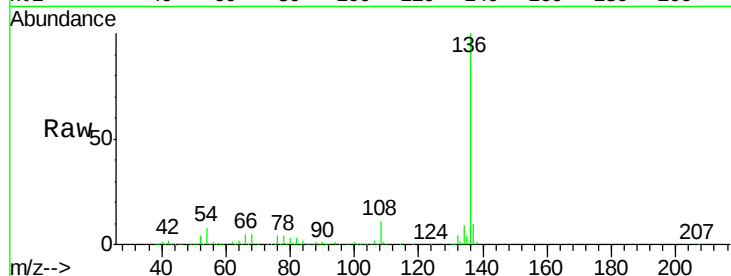


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BM
Ion 68.00 (67.70 to 68.70): BM


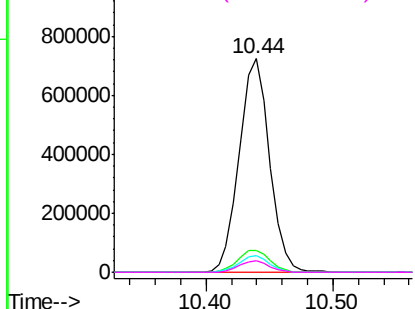



#23
Nitrobenzene-d5
Concen: 54.679 ng
RT: 8.82 min Scan# 991
Delta R.T. -0.02 min
Lab File: BM017252.D
Acq: 20 Oct 2018 06:01

Tgt Ion: 82 Resp: 1124283
Ion Ratio Lower Upper
82 100
128 41.6 37.0 55.6
54 50.1 40.7 61.1



Abundance Ion 82.00 (81.70 to 82.70): BM
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BM

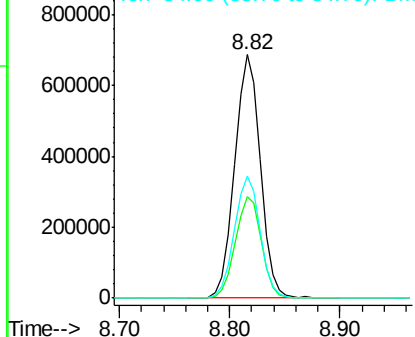


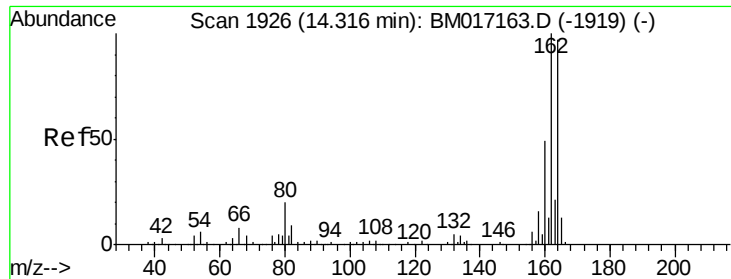




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.30 min Scan# 1924
Delta R.T. -0.01 min
Lab File: BM017252.D
Acq: 20 Oct 2018 06:01

Instrument :
BNA_M
ClientSampleId :
SSSI-1015-S-DH-25A-T

Tgt Ion:164 Resp: 727076
Ion Ratio Lower Upper
164 100
162 101.7 82.1 123.1
160 45.7 40.2 60.2

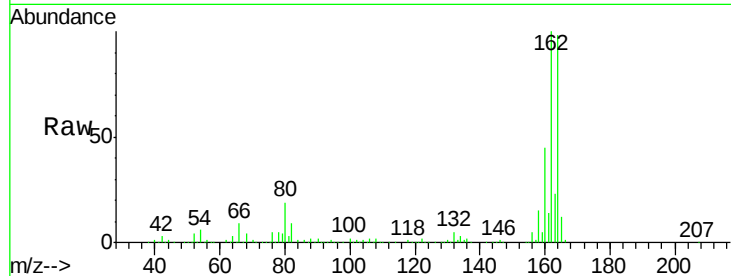


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E


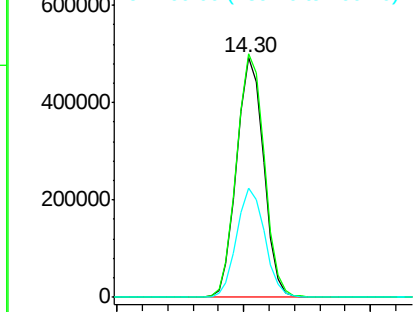



#42
2,4,6-Tribromophenol
Concen: 76.342 ng
RT: 15.80 min Scan# 2179
Delta R.T. -0.01 min
Lab File: BM017252.D
Acq: 20 Oct 2018 06:01

Tgt Ion:330 Resp: 750640
Ion Ratio Lower Upper
330 100
332 96.6 77.3 115.9
141 34.4 27.4 41.0



Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E




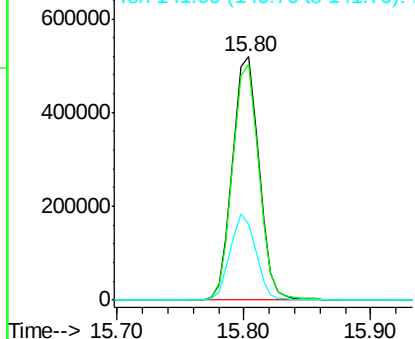


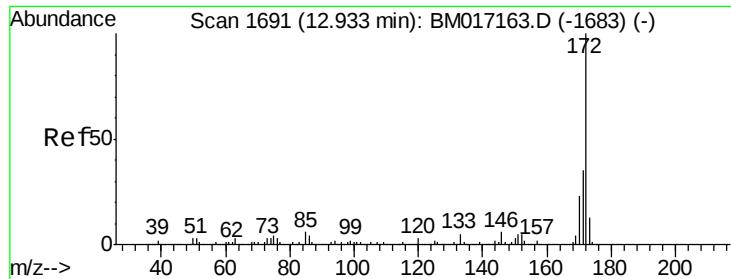

#45
2-Fluorobiphenyl
Concen: 49.258 ng
RT: 12.92 min Scan# 1689
Delta R.T. -0.01 min
Lab File: BM017252.D
Acq: 20 Oct 2018 06:01




Instrument :
BNA_M
ClientSampleId :
SSSI-1015-S-DH-25A-T


Tgt Ion:172 Resp: 2691717
Ion Ratio Lower Upper
172 100
171 34.5 28.3 42.5
170 22.6 18.3 27.5

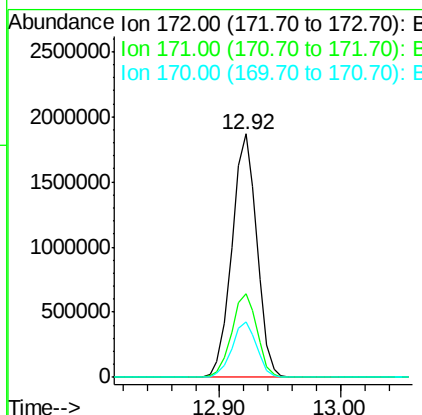

#50
Dimethylphthalate
Concen: 4.623 ng
RT: 13.77 min Scan# 1833
Delta R.T. -0.02 min
Lab File: BM017252.D
Acq: 20 Oct 2018 06:01

Tgt Ion:163 Resp: 259345
Ion Ratio Lower Upper
163 100
194 4.4 3.3 4.9
164 10.1 7.8 11.8

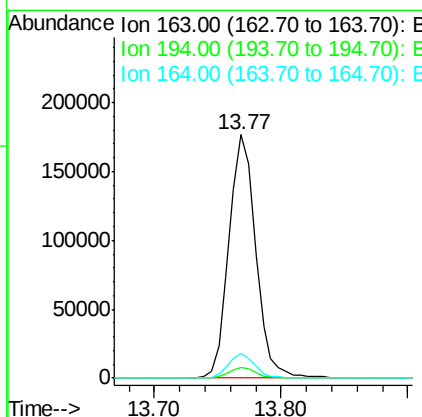



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.06 min Scan# 2392

Delta R.T. -0.01 min

Lab File: BM017252.D

Acq: 20 Oct 2018 06:01

Instrument :

BNA_M

ClientSampleId :

SSSI-1015-S-DH-25A-T


Tgt Ion:188 Resp: 1595998

Ion Ratio Lower Upper

188 100

94 8.4 7.0 10.4




80 9.1 7.7 11.5



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM017252.D (-2377) (-)

Ion 80.00 (79.70 to 80.70): BM017252.D (-2377) (-)

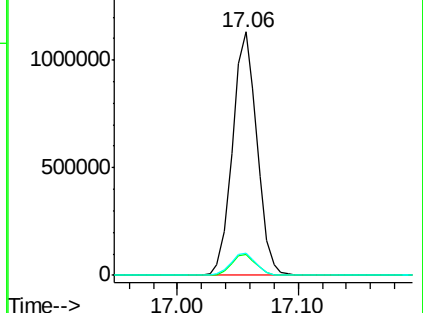

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.25 min Scan# 3105

Delta R.T. -0.01 min

Lab File: BM017252.D

Acq: 20 Oct 2018 06:01


Tgt Ion:240 Resp: 1495373

Ion Ratio Lower Upper

240 100

120 9.9 8.1 12.1



236 25.0 19.9 29.9




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

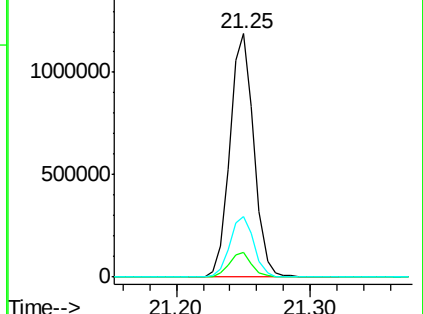

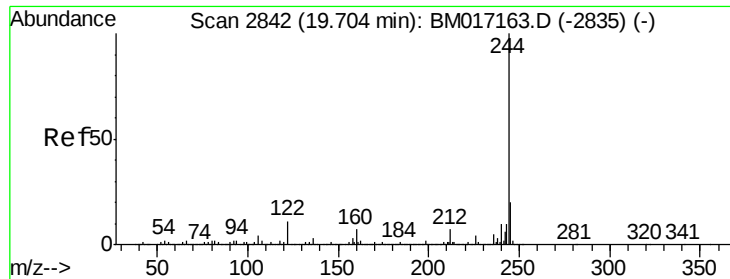

#79

Terphenyl-d14

Concen: 53.533 ng

RT: 19.69 min Scan# 2840

Delta R.T. -0.01 min

Lab File: BM017252.D

Acq: 20 Oct 2018 06:01

Instrument :

BNA_M

ClientSampleId :

SSSI-1015-S-DH-25A-T


Tgt Ion:244 Resp: 3551543

Ion Ratio Lower Upper

244 100

212 7.1 5.5 8.3




122 10.1 8.4 12.6

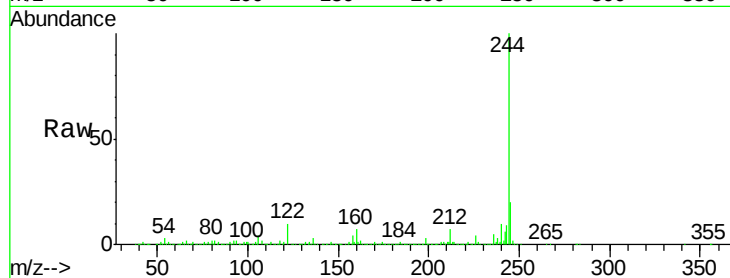

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

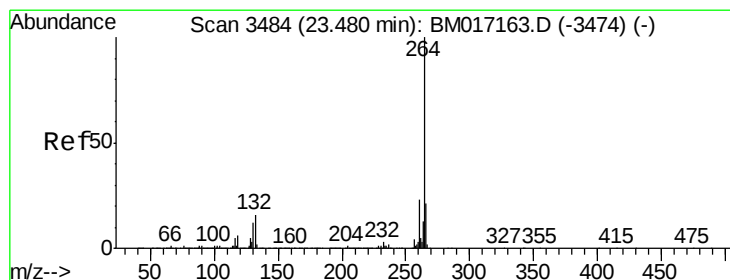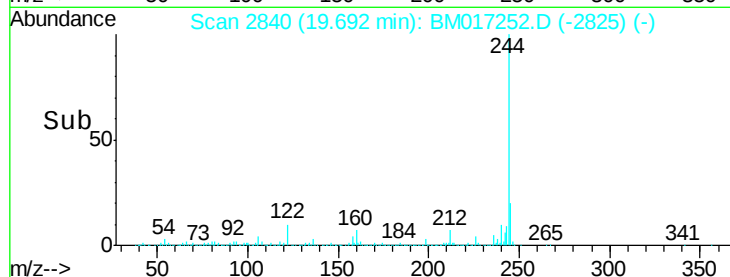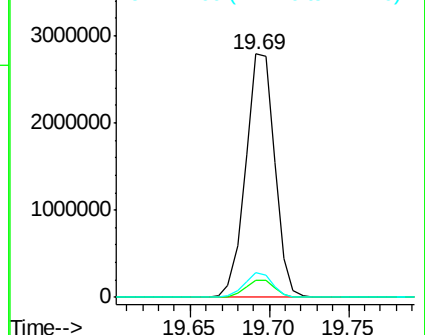

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.46 min Scan# 3481

Delta R.T. -0.02 min

Lab File: BM017252.D

Acq: 20 Oct 2018 06:01


Tgt Ion:264 Resp: 1370899

Ion Ratio Lower Upper

264 100

260 23.4 18.6 27.8

265 21.9 17.8 26.8

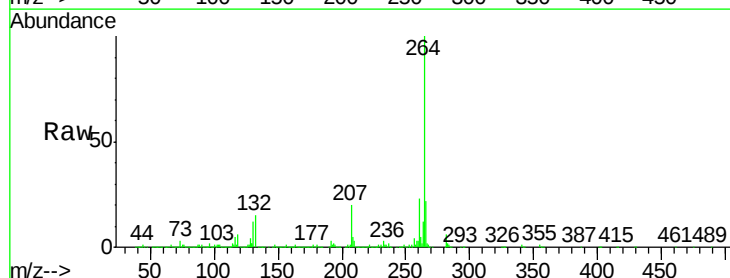

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

