


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM101918\
 Data File : BM017227.D
 Acq On : 19 Oct 2018 13:21
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM101718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 17 14:23:17 2018

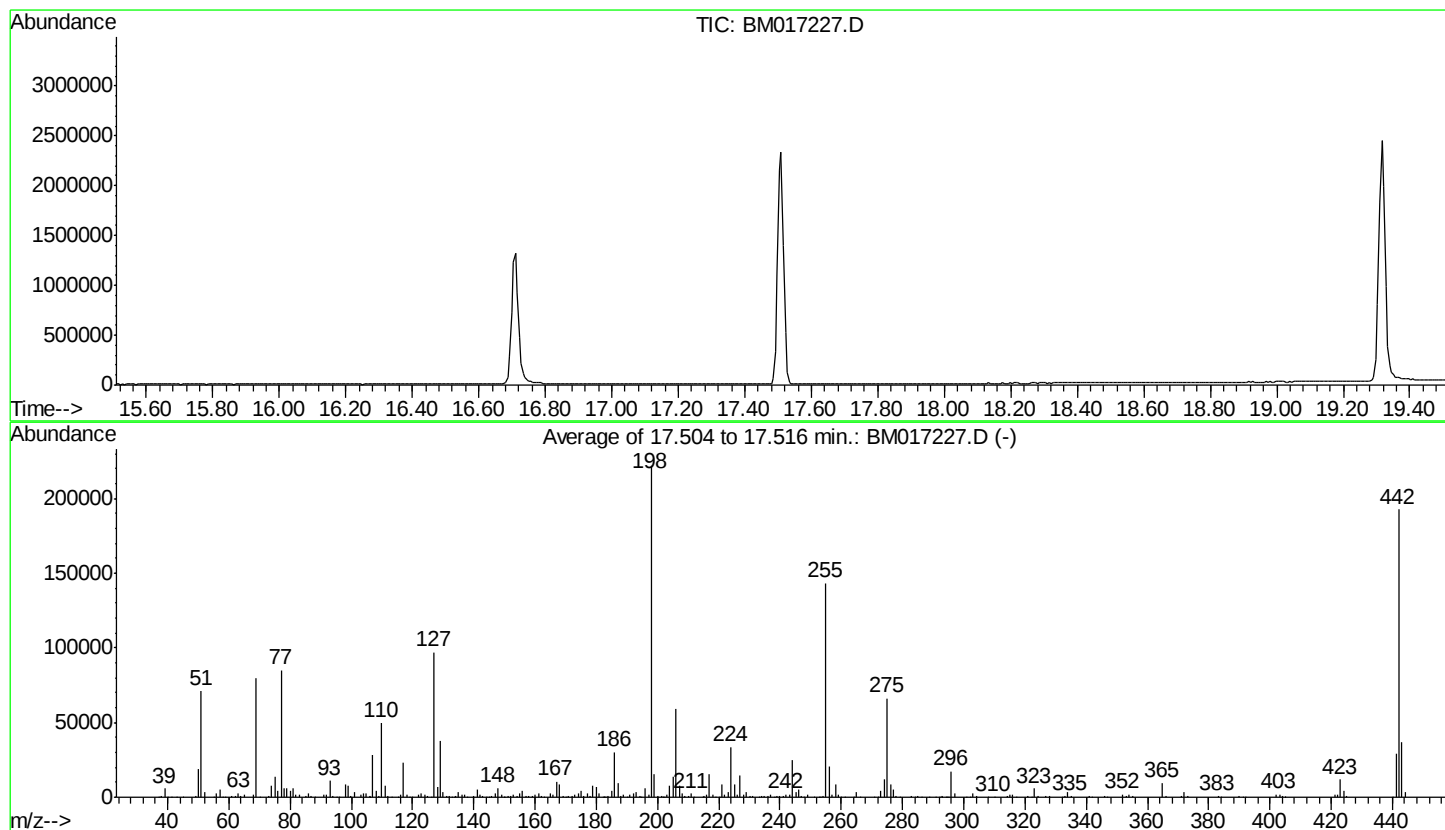

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	71562	PASS
68	69	0.00	2	1.9	1541	PASS
69	198	0.00	100	35.8	79450	PASS
70	69	0.00	2	0.5	374	PASS
127	198	10	80	43.8	97280	PASS
197	198	0.00	2	0.6	1337	PASS
198	198	100	100	100.0	221973	PASS
199	198	5	9	7.0	15600	PASS
275	198	10	60	29.8	66205	PASS
365	198	1	100	4.3	9499	PASS
441	198	0.01	100	13.0	28829	PASS
442	198	50	100	86.8	192768	PASS
443	442	15	24	19.0	36648	PASS