


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM101918\
Data File : BM017246.D
Acq On : 20 Oct 2018 02:10
Operator : MJ/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM101718.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 17 14:23:17 2018

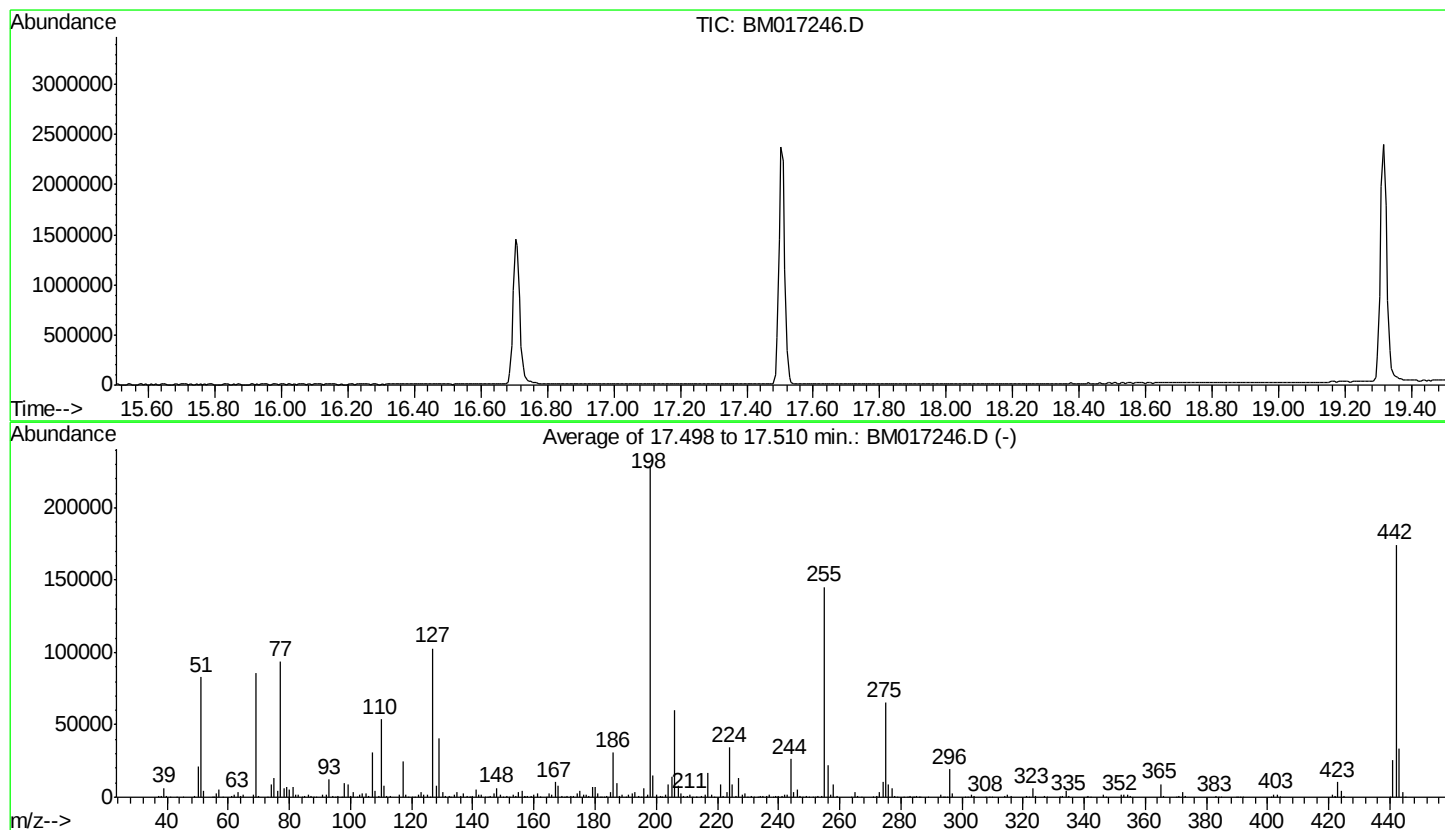

AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	82786	PASS
68	69	0.00	2	1.9	1612	PASS
69	198	0.00	100	37.5	85805	PASS
70	69	0.00	2	0.7	560	PASS
127	198	10	80	45.0	103024	PASS
197	198	0.00	2	0.6	1432	PASS
198	198	100	100	100.0	229098	PASS
199	198	5	9	6.7	15387	PASS
275	198	10	60	28.4	65080	PASS
365	198	1	100	3.9	9044	PASS
441	198	0.01	100	11.4	26056	PASS
442	198	50	100	76.2	174669	PASS
443	442	15	24	19.1	33357	PASS