


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM101918\
 Data File : BM017255.D
 Acq On : 20 Oct 2018 09:01
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM101718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 17 14:23:17 2018

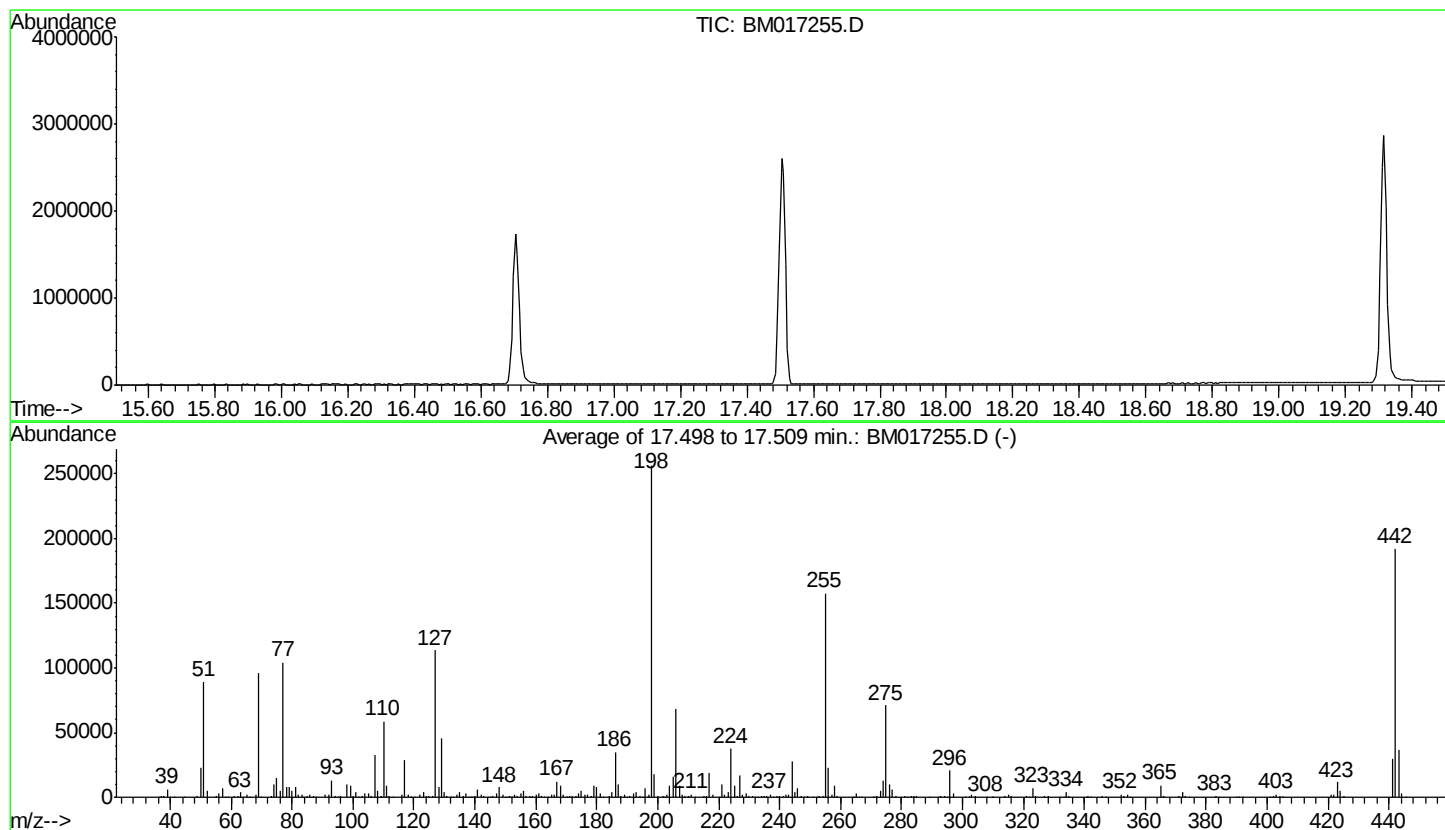

AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	89429	PASS
68	69	0.00	2	1.9	1815	PASS
69	198	0.00	100	37.5	96138	PASS
70	69	0.00	2	0.5	447	PASS
127	198	10	80	44.3	113698	PASS
197	198	0.00	2	0.6	1595	PASS
198	198	100	100	100.0	256426	PASS
199	198	5	9	7.1	18116	PASS
275	198	10	60	27.7	71074	PASS
365	198	1	100	3.5	8958	PASS
441	198	0.01	100	11.8	30202	PASS
442	198	50	100	74.9	192064	PASS
443	442	15	24	19.1	36664	PASS