

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM101919\
 Data File : BM023303.D
 Acq On : 20 Oct 2019 01:14
 Operator : JU
 Sample : K5378-21
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0025

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101419MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	28	31	38	rVB	55080	78679	1.20%	0.116%
2	3.810	134	140	146	rVB	59093	99438	1.52%	0.147%
3	3.893	150	154	159	rVB	26358	36842	0.56%	0.054%
4	4.799	304	308	312	rBV	15618	24893	0.38%	0.037%
5	5.022	345	346	353	rBV4	4722	9512	0.15%	0.014%
6	6.334	565	569	570	rBV4	7708	9735	0.15%	0.014%
7	6.822	644	652	663	rVV2	933288	1646263	25.15%	2.432%
8	6.987	674	680	693	rVB	661028	1087049	16.60%	1.606%
9	7.187	707	714	723	rBV	943730	1538014	23.49%	2.272%
10	7.298	732	733	739	rVB6	10974	13416	0.20%	0.020%
11	7.651	785	793	802	rBV	1519377	2414155	36.88%	3.567%
12	7.734	802	807	810	rBV6	7435	10018	0.15%	0.015%
13	8.357	905	913	926	rBV	1066094	1765692	26.97%	2.609%
14	8.463	926	931	934	rVB6	4835	7845	0.12%	0.012%
15	8.792	980	987	998	rBV	787363	1348452	20.60%	1.992%
16	8.975	1016	1018	1025	rVB6	8859	12143	0.19%	0.018%
17	9.281	1064	1070	1076	rVB6	12054	22539	0.34%	0.033%
18	9.516	1103	1110	1119	rBV	634870	1019652	15.58%	1.506%
19	10.051	1194	1201	1208	rBV	1115591	1810727	27.66%	2.675%
20	10.428	1258	1265	1273	rBV	1947706	3274478	50.02%	4.838%
21	10.563	1279	1288	1297	rBV	1003775	1736446	26.52%	2.565%
22	11.239	1399	1403	1404	rBV4	5927	7117	0.11%	0.011%
23	11.675	1470	1477	1482	rVB6	9436	19200	0.29%	0.028%
24	12.027	1531	1537	1541	rVB	20504	34453	0.53%	0.051%
25	12.916	1685	1688	1695	rVB7	7605	14518	0.22%	0.021%
26	13.145	1721	1727	1730	rBV7	9152	12004	0.18%	0.018%
27	13.216	1734	1739	1745	rVV5	6440	12691	0.19%	0.019%
28	13.627	1806	1809	1811	rBV3	8976	10394	0.16%	0.015%
29	13.710	1817	1823	1827	rBV	1825739	2529642	38.64%	3.737%
30	13.757	1827	1831	1842	rVB	800313	1084004	16.56%	1.602%
31	13.986	1863	1870	1880	rBV	2057501	3074852	46.97%	4.543%
32	14.292	1916	1922	1930	rVV	2879866	4293731	65.59%	6.344%
33	14.421	1942	1944	1949	rBV5	4163	6703	0.10%	0.010%
34	14.492	1949	1956	1967	rBV	221059	364361	5.57%	0.538%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM101919\
 Data File : BM023303.D
 Acq On : 20 Oct 2019 01:14
 Operator : JU
 Sample : K5378-21
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0025

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101419MA.M
 Title : SVOA CALIBRATION

35	14.721	1991	1995	2003	rVB3	74169	109545	1.67%	0.162%
36	15.127	2060	2064	2070	rBV7	11705	20024	0.31%	0.030%
37	15.180	2070	2073	2076	rBV4	7181	9630	0.15%	0.014%
38	15.292	2083	2092	2103	rBV	2707665	3879192	59.26%	5.731%
39	15.410	2106	2112	2121	rVB	200848	298669	4.56%	0.441%
40	15.533	2127	2133	2139	rVB3	32638	46154	0.71%	0.068%
41	16.074	2222	2225	2230	rVB6	8132	12267	0.19%	0.018%
42	16.510	2295	2299	2301	rVV5	5735	6787	0.10%	0.010%
43	16.727	2329	2336	2338	rBV7	6577	13014	0.20%	0.019%
44	16.827	2348	2353	2357	rBV5	13972	25289	0.39%	0.037%
45	17.039	2383	2389	2396	rBV2	3580162	5015246	76.61%	7.410%
46	17.139	2399	2406	2416	rBV	2993587	4259236	65.06%	6.293%
47	17.239	2420	2423	2429	rVV6	23999	32974	0.50%	0.049%
48	17.457	2456	2460	2463	rBV6	9035	11792	0.18%	0.017%
49	17.956	2541	2545	2551	rBV3	57725	83971	1.28%	0.124%
50	18.151	2576	2578	2581	rVB4	8523	7941	0.12%	0.012%
51	19.068	2731	2734	2736	rBV2	31282	34612	0.53%	0.051%
52	19.433	2790	2796	2803	rBV	3798662	5134499	78.43%	7.586%
53	20.980	3055	3059	3064	rBV3	283217	391225	5.98%	0.578%
54	21.227	3096	3101	3107	rBV	4728524	6102157	93.21%	9.015%
55	21.421	3131	3134	3137	rBV3	189734	215283	3.29%	0.318%
56	22.315	3283	3286	3290	rVB	294565	357652	5.46%	0.528%
57	23.291	3446	3452	3460	rVB	3183796	5643083	86.20%	8.337%
58	23.433	3470	3476	3485	rVB	3617785	6546558	100.00%	9.672%


Sum of corrected areas: 67686458

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM101919\
Data File : BM023303.D
Acq On : 20 Oct 2019 01:14
Operator : JU
Sample : K5378-21
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0025

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

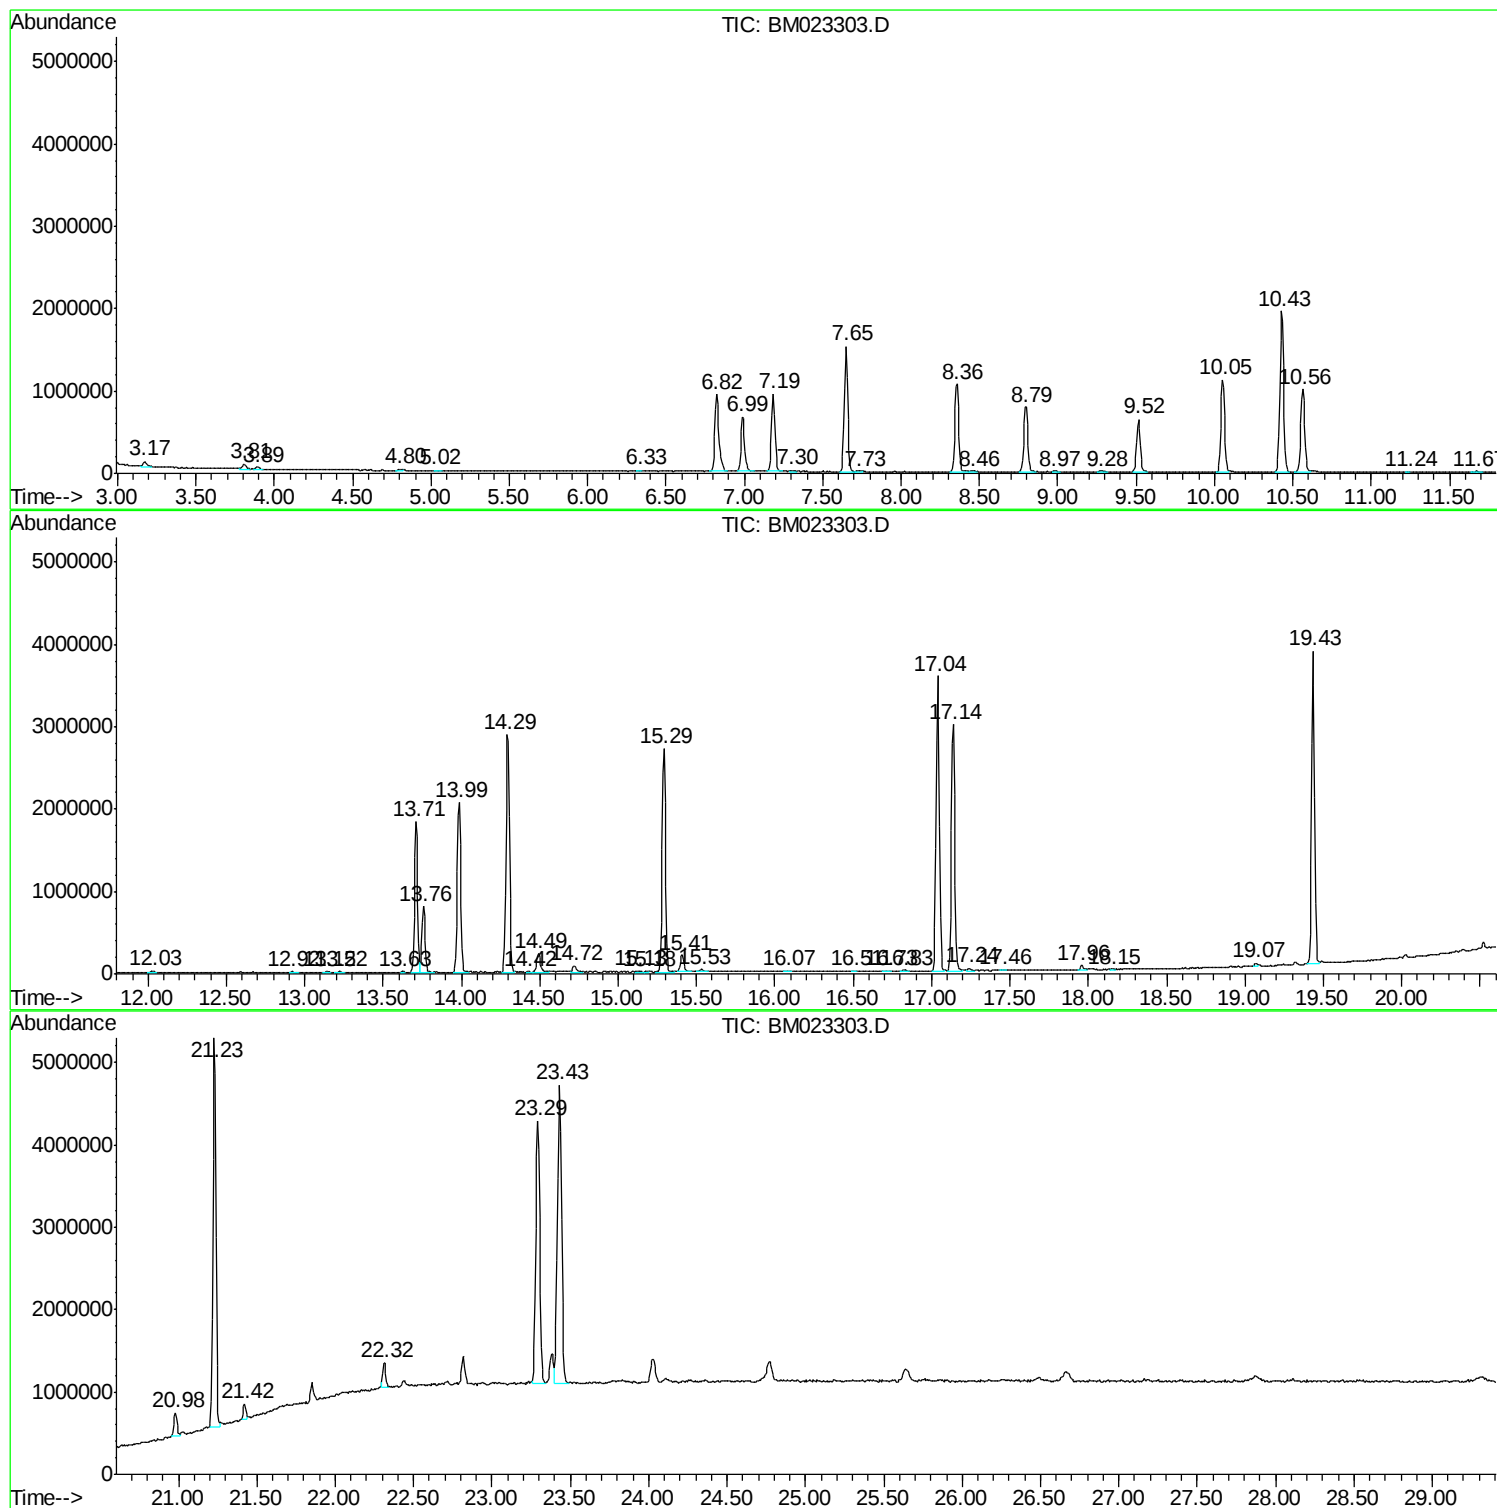

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM101919\
Data File : BM023303.D
Acq On : 20 Oct 2019 01:14
Operator : JU
Sample : K5378-21
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0025

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM101919\
Data File : BM023303.D
Acq On : 20 Oct 2019 01:14
Operator : JU
Sample : K5378-21
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0025

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc