


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102123\
Data File : BM042382.D
Acq On : 20 Oct 2023 17:47
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Oct 21 02:32:53 2023

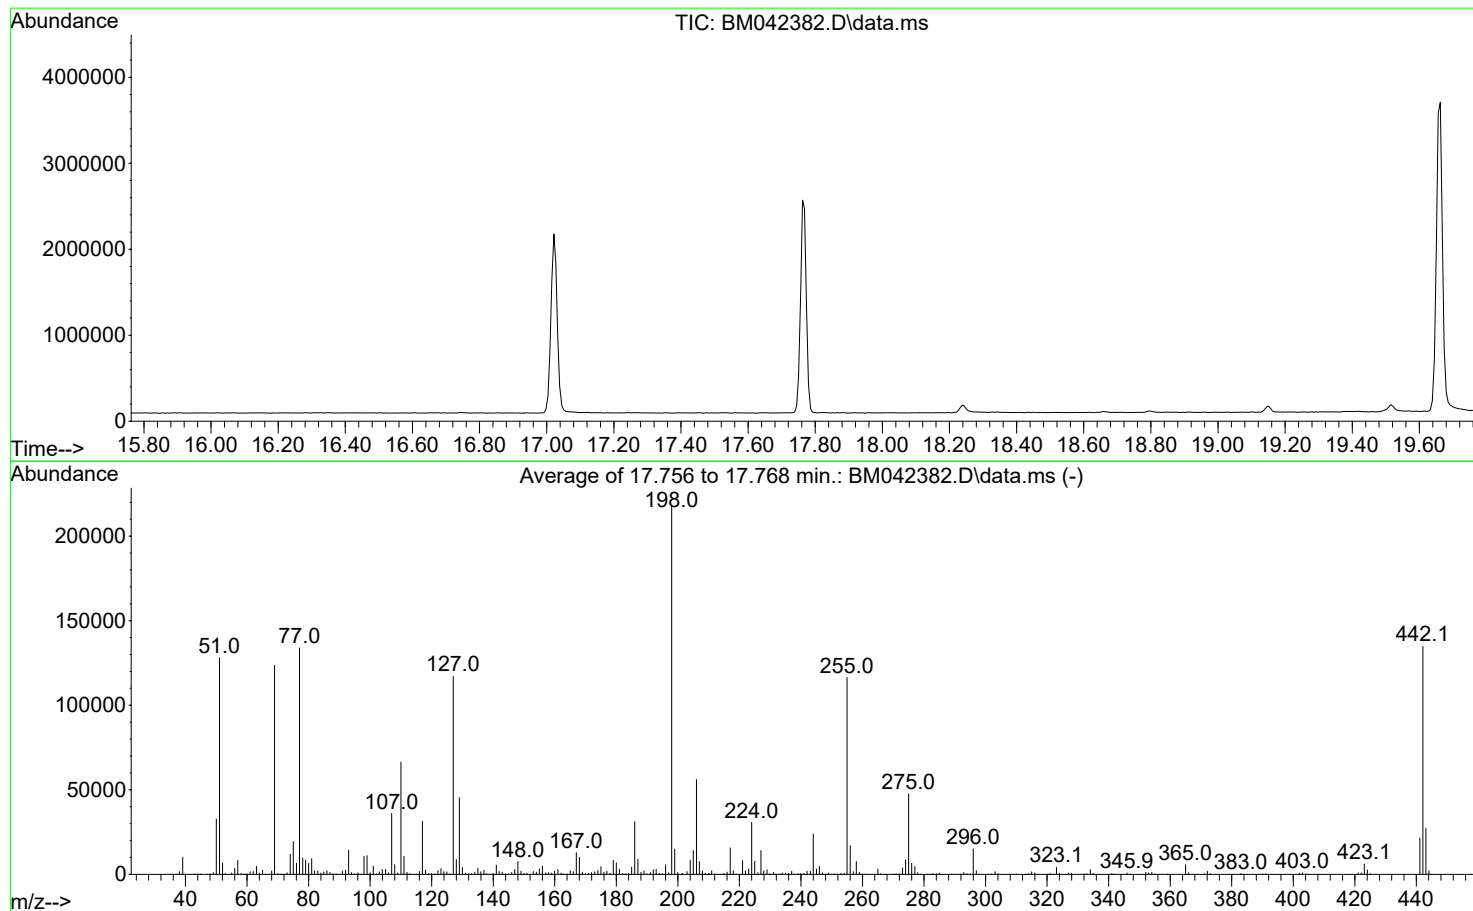

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.8	127985	PASS
68	69	0.00	2	1.6	1971	PASS
69	198	0.00	100	56.9	123661	PASS
70	69	0.00	2	0.4	499	PASS
127	198	10	80	53.9	117157	PASS
197	198	0.00	2	0.4	944	PASS
198	198	100	100	100.0	217515	PASS
199	198	5	9	6.9	14962	PASS
275	198	10	60	21.9	47587	PASS
365	198	1	100	2.6	5675	PASS
441	198	0.01	100	9.9	21478	PASS
442	442	50	100	100.0	134853	PASS
443	442	15	24	20.1	27167	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/21/2023	BNA_M	<u>BM042382.D</u>
Compound Name	Response	Retention Time
DDT	780690	20.85
DDD	5588	20.456
DDE	124	19.898
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5712	786402	0.73

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102123\
Data File : BM042382.D
Acq On : 20 Oct 2023 17:47
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Oct 21 02:39:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 21 02:32:53 2023
Response via : Initial Calibration

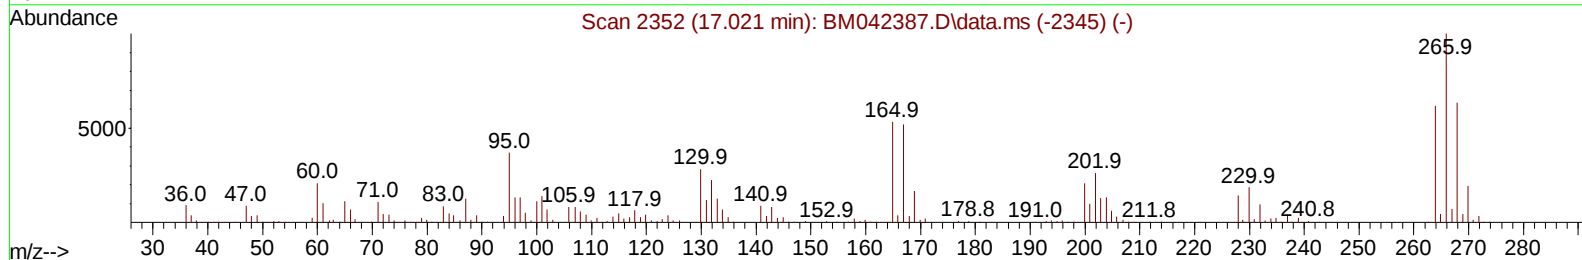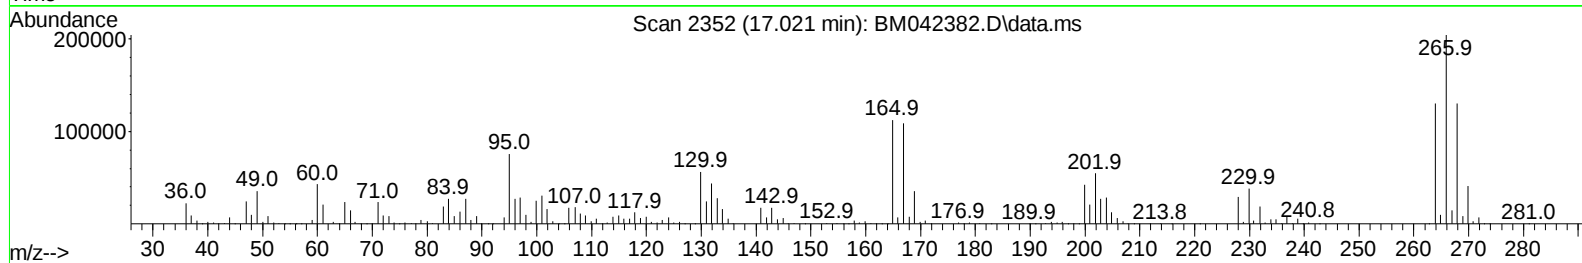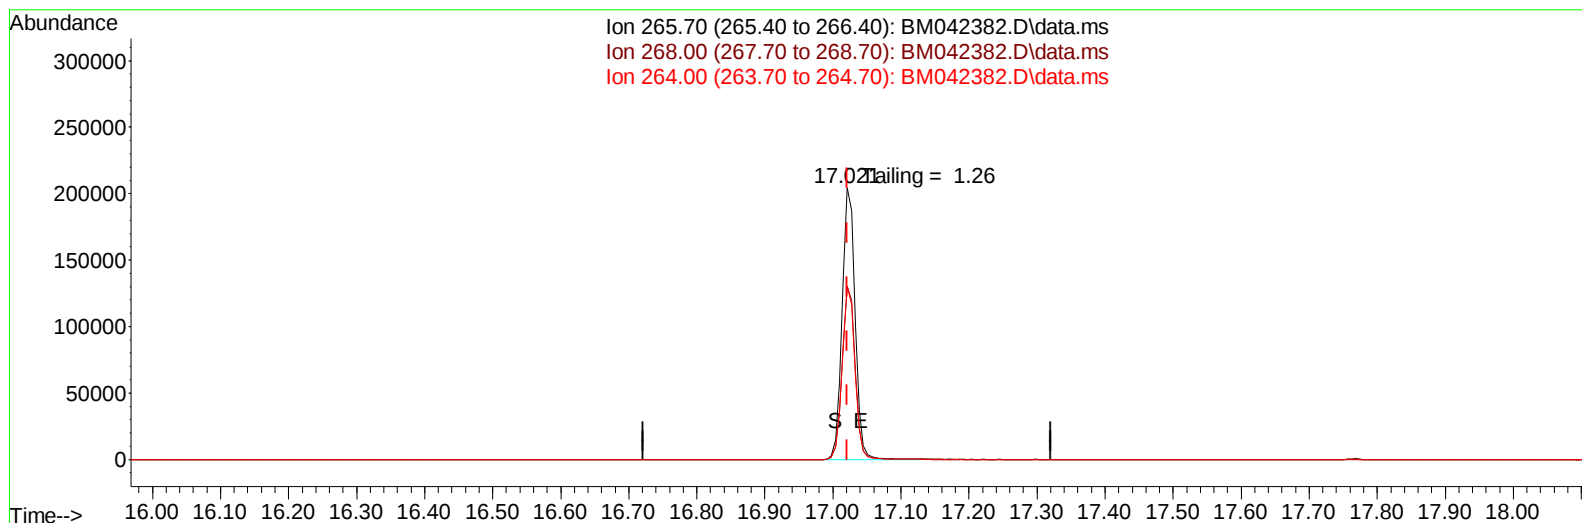

TIC: BM042382.D\data.ms

(70) Pentachlorophenol (C)

17.021min (+ 0.000) 220381.88 ng




response 269891

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	63.77
264.00	61.70	63.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102123\
Data File : BM042382.D
Acq On : 20 Oct 2023 17:47
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Oct 21 02:39:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 21 02:32:53 2023
Response via : Initial Calibration

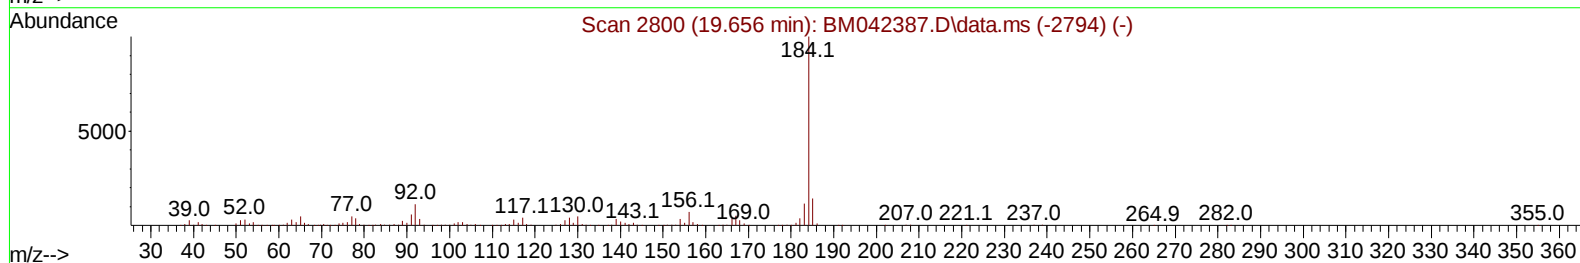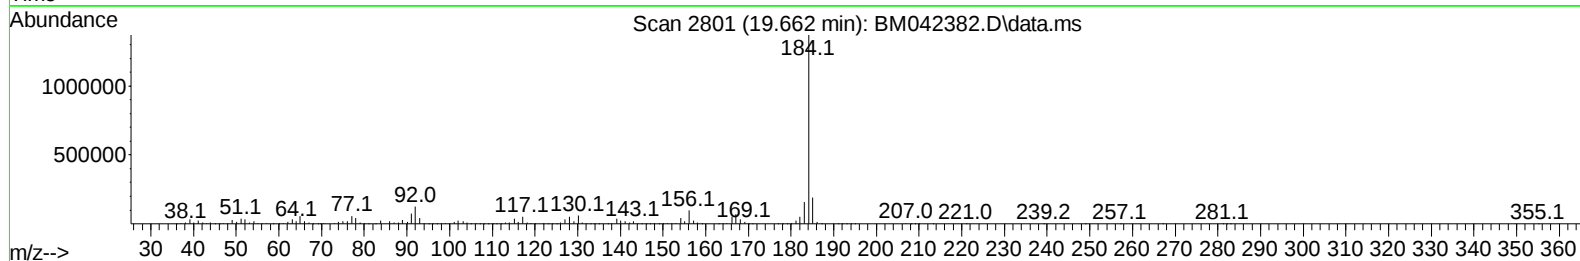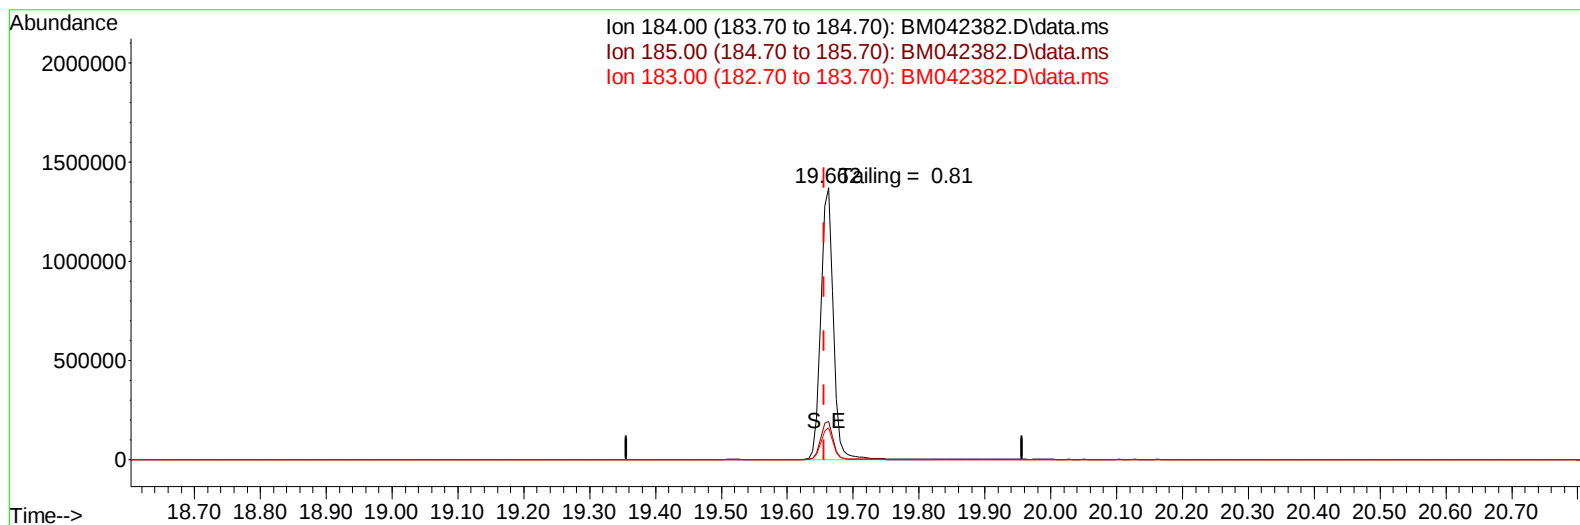

TIC: BM042382.D\data.ms

(77) Benzidine

19.662min (+ 0.006) 182773.25 ng

response 1763334

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.01
183.00	11.50	11.60
0.00	0.00	0.00