
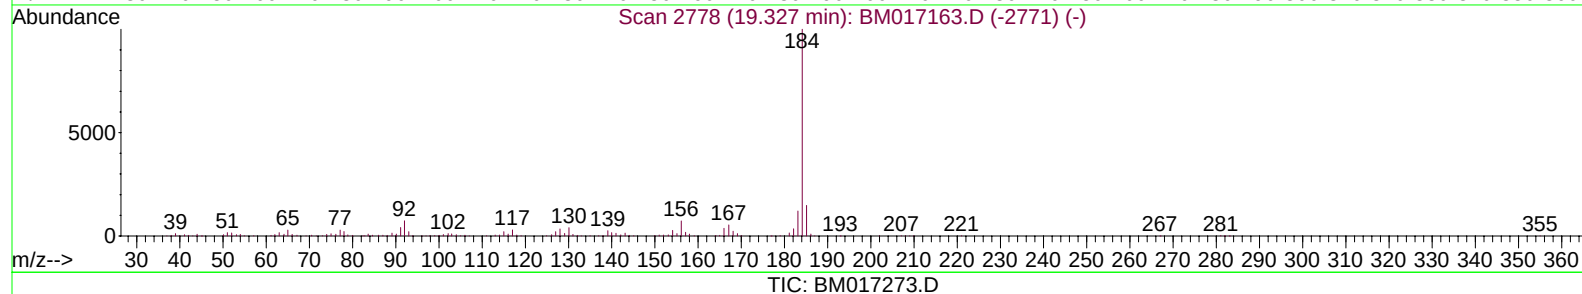
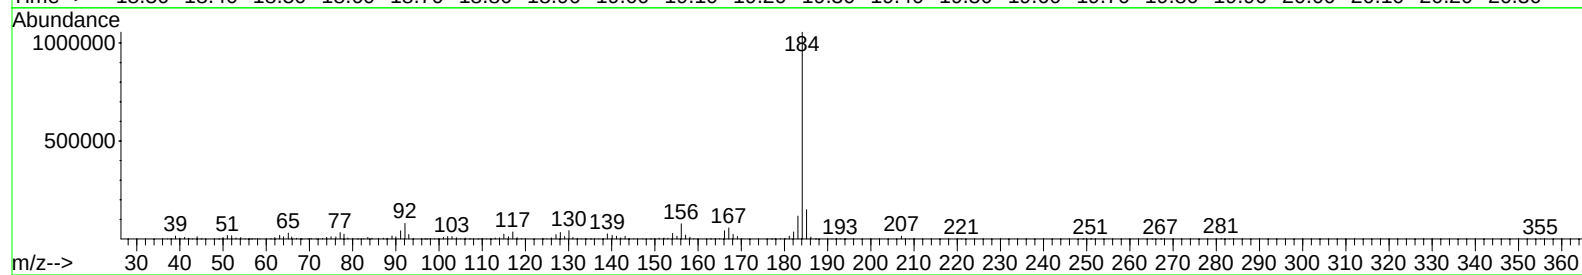


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM102218\
Data File : BM017273.D
Acq On : 22 Oct 2018 10:51
Operator : MJ/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 23 08:18:57 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM101718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 17 14:23:17 2018
Response via : Initial Calibration

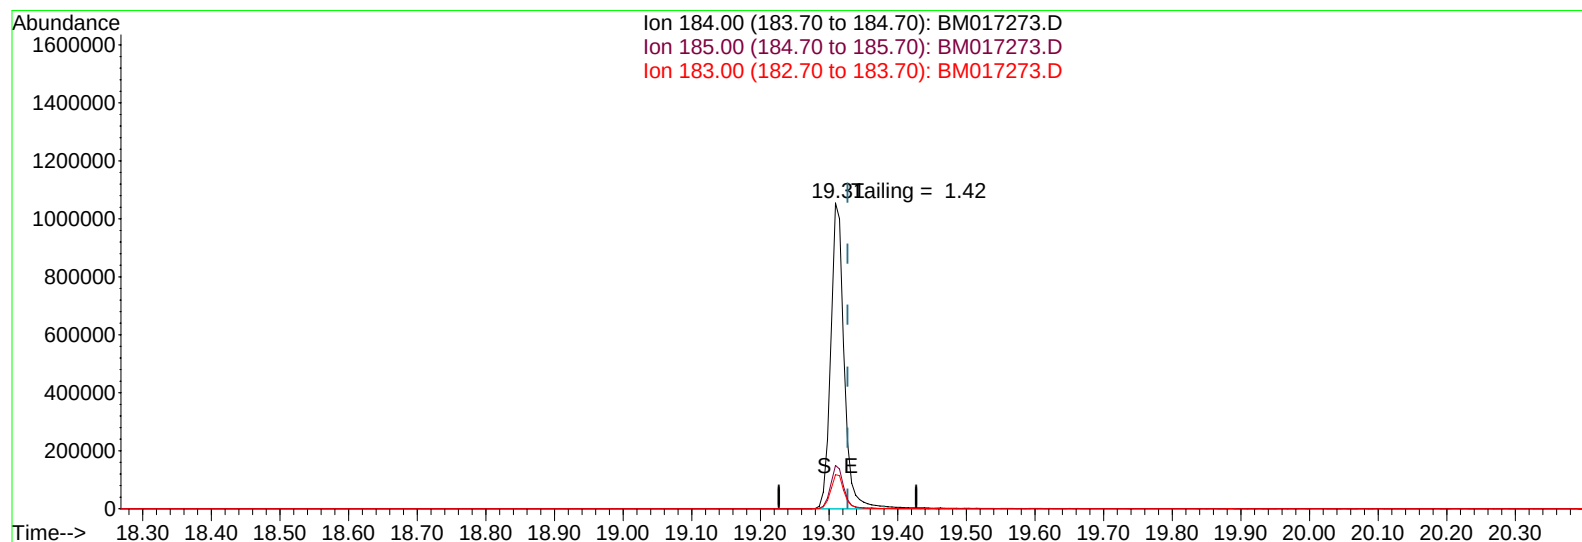

(77) Benzidine




19.309min (-0.018) 148177.78ng

response 1431520

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.21
183.00	12.10	11.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM102218\
Data File : BM017273.D
Acq On : 22 Oct 2018 10:51
Operator : MJ/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 23 08:18:57 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM101718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 17 14:23:17 2018
Response via : Initial Calibration

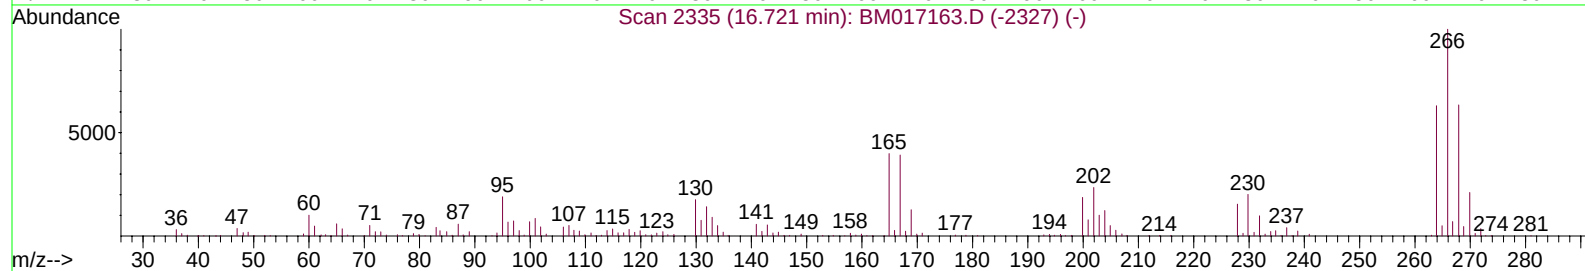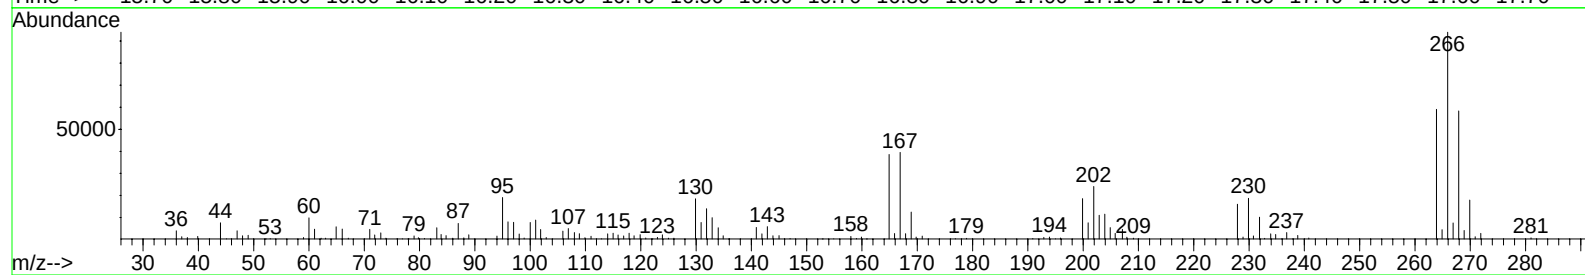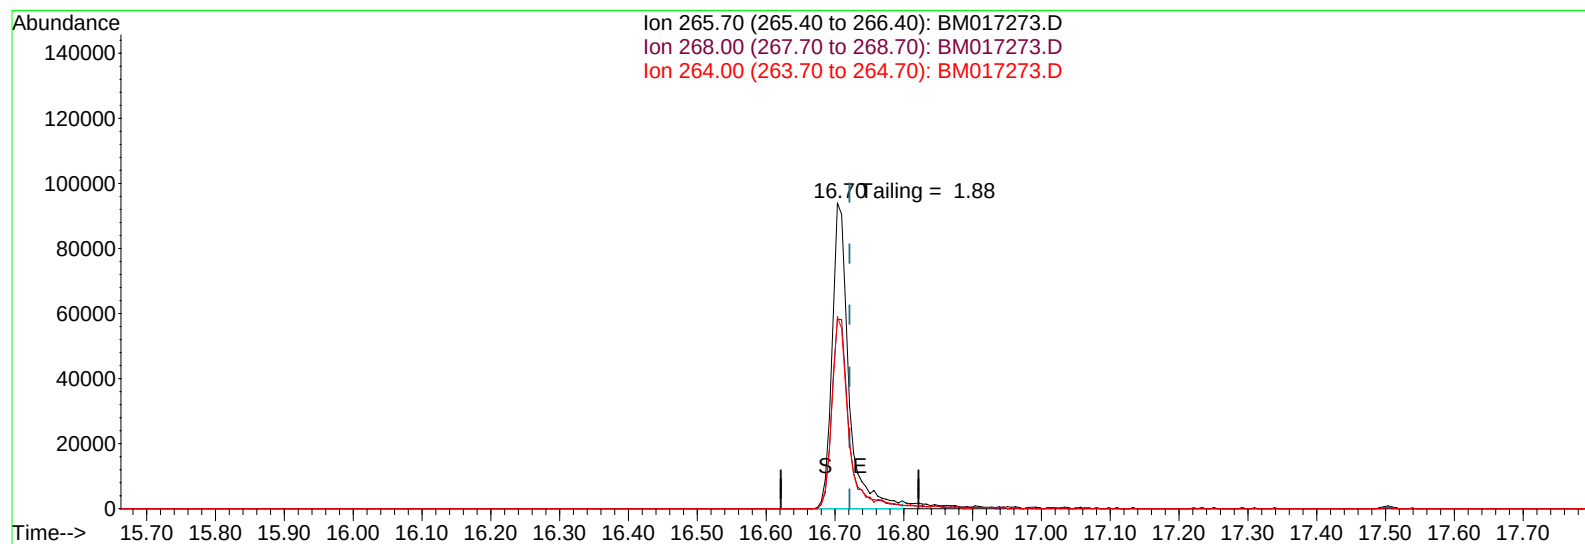

TIC: BM017273.D

(70) Pentachlorophenol (C)

16.704min (-0.018) 0.00ng

response 158343

Ion	Exp%	Act%
265.70	100	100
268.00	63.40	62.04
264.00	63.00	62.79
0.00	0.00	0.00