


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM102218\
 Data File : BM017273.D
 Acq On : 22 Oct 2018 10:51
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM101718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 17 14:23:17 2018

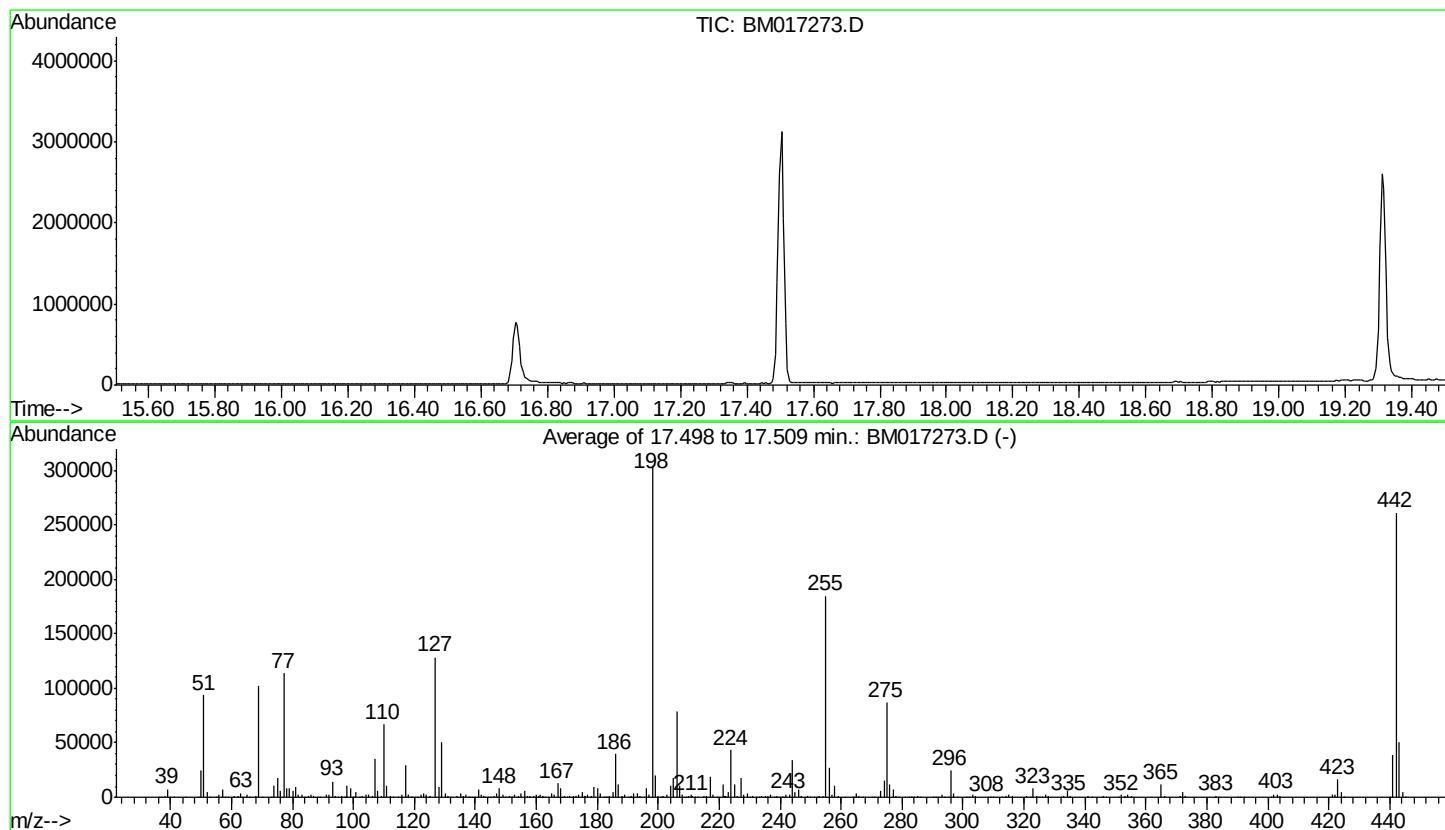

AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.9	93890	PASS
68	69	0.00	2	1.5	1550	PASS
69	198	0.00	100	33.5	102048	PASS
70	69	0.00	2	0.6	586	PASS
127	198	10	80	42.2	128514	PASS
197	198	0.00	2	0.6	1972	PASS
198	198	100	100	100.0	304341	PASS
199	198	5	9	6.6	20213	PASS
275	198	10	60	28.4	86456	PASS
365	198	1	100	3.8	11523	PASS
441	198	0.01	100	12.7	38578	PASS
442	198	50	100	85.9	261333	PASS
443	442	15	24	19.5	50976	PASS