

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102219\
 Data File : BM023330.D
 Acq On : 22 Oct 2019 21:56
 Operator : JU
 Sample : K5354-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFB88

Manual Integrations
 APPROVED

mohammad
 10/24/2019 8:08:53 AM

Quant Time: Oct 23 03:03:01 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 23 01:39:41 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	412125	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1664216	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	1056417	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	2218540	20.00	ng/ul	0.00
78) Chrysene-d12	21.23	240	2293751	20.00	ng/ul	0.00
86) Perylene-d12	23.44	264	2808122	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.17	96	37725	4.03	ng/uL	0.00
5) Phenol-d5	6.82	99	728245	20.29	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	411636	20.27	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	604939	22.02	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	557029	19.32	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	293780	26.09	ng/ul	0.00
22) 2-Nitrophenol-d4	9.51	143	329581	30.74	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	634246	23.26	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	303026	9.14	ng/ul	0.00
44) Dimethylphthalate-d6	13.71	166	1940392	23.97	ng/ul	0.00
47) Acenaphthylene-d8	13.98	160	2307254	24.30	ng/ul	0.00
52) 4-Nitrophenol-d4	14.50	143	255731	19.51	ng/ul	0.00
58) Fluorene-d10	15.29	176	1721875	24.96	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.41	200	206774	23.51	ng/ul	0.00
71) Anthracene-d10	17.14	188	2755782	25.76	ng/ul	0.00
79) Pyrene-d10	19.43	212	3038131	27.35	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.30	264	3690809	25.93	ng/ul	0.00

Target Compounds

					Ovalue
6) Phenol	6.85	94	76907	2.078	ng/ul 98
45) Dimethylphthalate	13.76	163	757122	9.344	ng/ul 99
48) Acenaphthylene	14.01	152	245690	2.531	ng/ul 96
59) Fluorene	15.34	166	82968	1.054	ng/ul 99
70) Phenanthrene	17.08	178	1386332	11.135	ng/ul 99
72) Anthracene	17.17	178	418228	3.251	ng/ul 99
77) Fluoranthene	19.10	202	2659157	17.958	ng/ul 99
80) Pyrene	19.46	202	2805623	19.525	ng/ul 98
83) Benzo(a)anthracene	21.22	228	1738553	11.186	ng/ul 95
84) Bis(2-ethylhexyl)phthalate	21.17	149	136916	1.723	ng/ul# 97
85) Chrysene	21.27	228	1635596	11.334	ng/ul 97
88) Benzo(b)fluoranthene	22.79	252	2447525	14.375	ng/ul 97
89) Benzo(k)fluoranthene	22.82	252	828876m	5.070	ng/ul
91) Benzo(a)pyrene	23.34	252	1783588	10.919	ng/ul 96
92) Indeno(1,2,3-cd)pyrene	25.65	276	1327060	6.829	ng/ul 97
93) Dibenzo(a,h)anthracene	25.66	278	364037	2.241	ng/ul# 91
94) Benzo(g,h,i)perylene	26.33	276	1307392	8.172	ng/ul 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102219\
Data File : BM023330.D
Acq On : 22 Oct 2019 21:56
Operator : JU
Sample : K5354-02
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BFB88

Manual Integrations
APPROVED

mohammad
10/24/2019 8:08:53 AM

Quant Time: Oct 23 03:03:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 23 01:39:41 2019
Response via : Initial Calibration

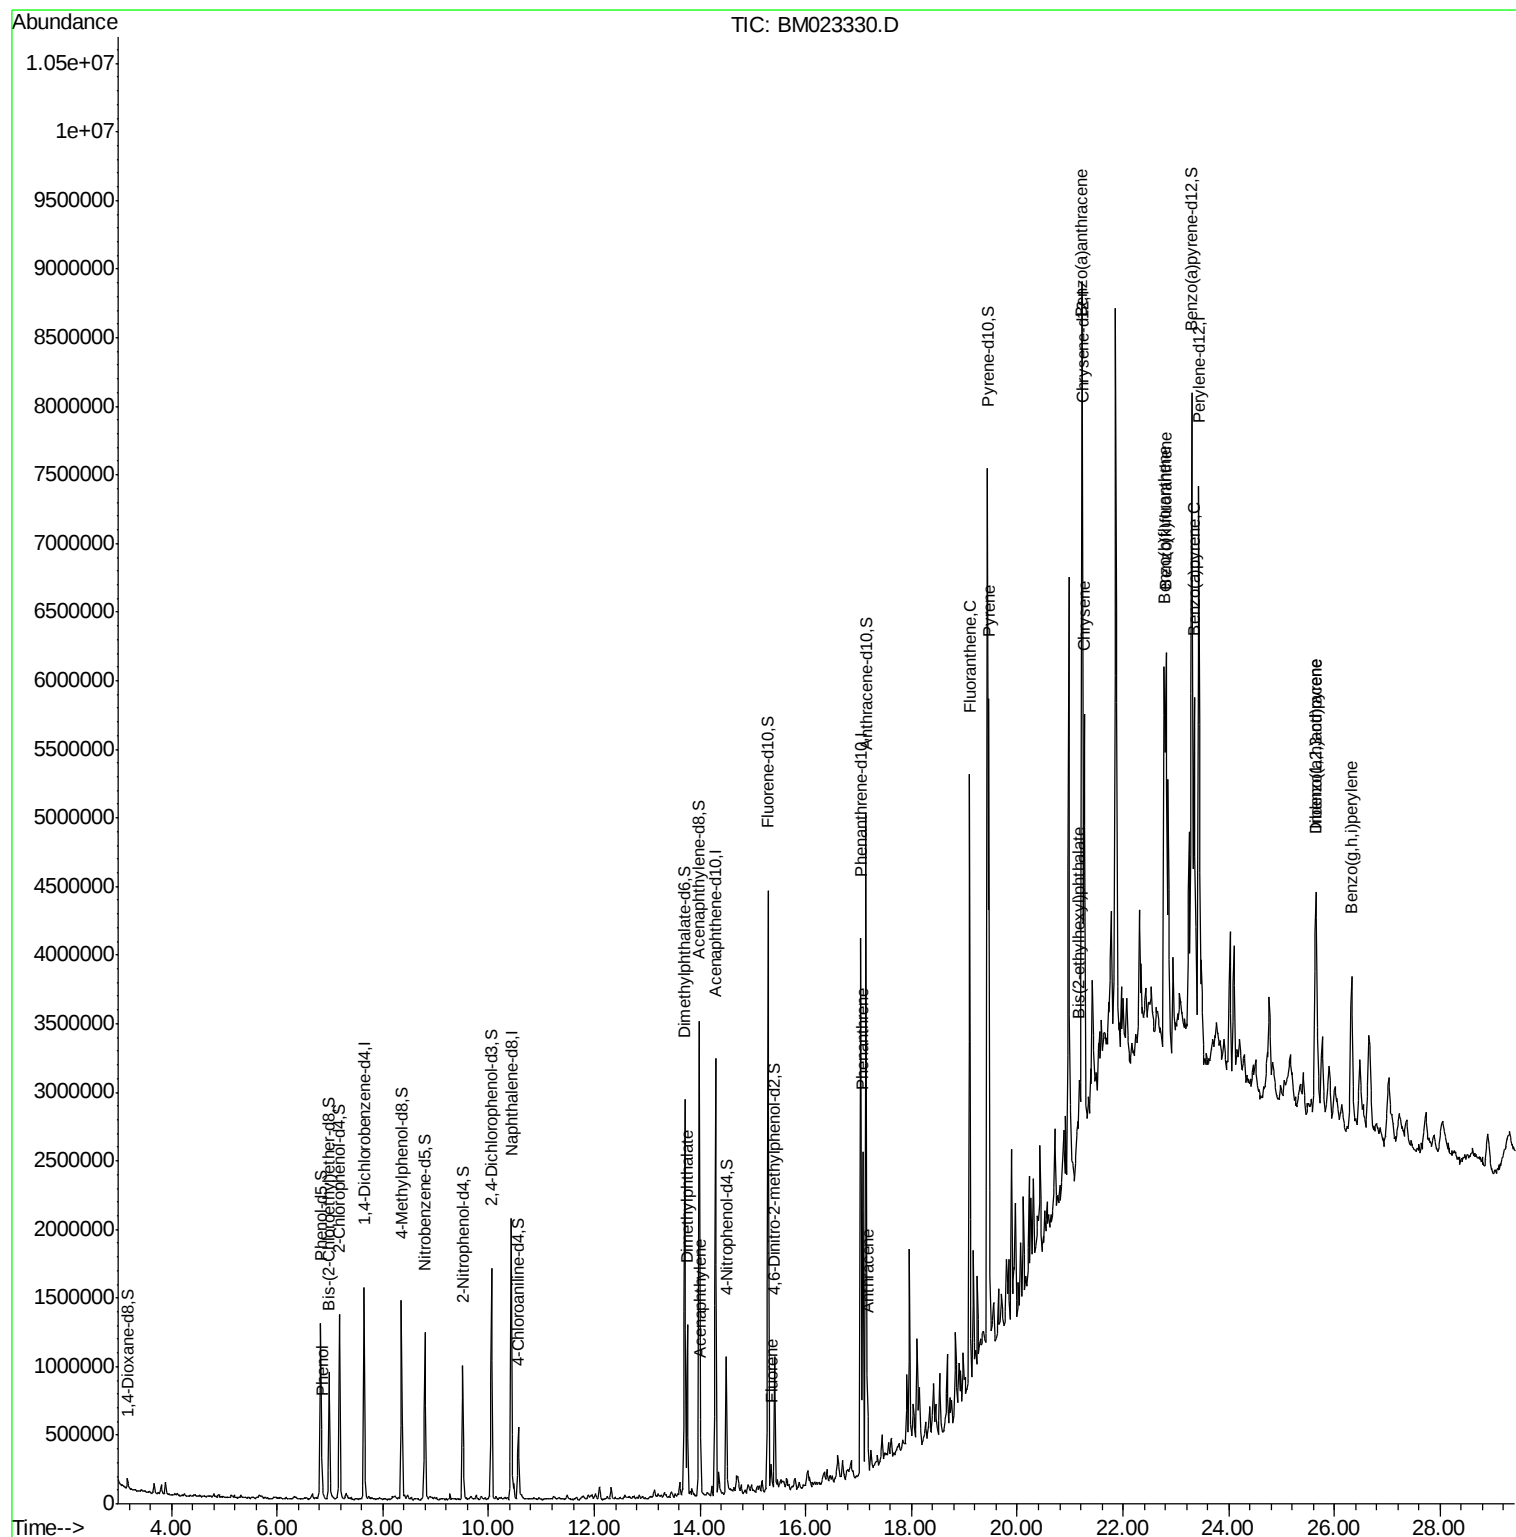

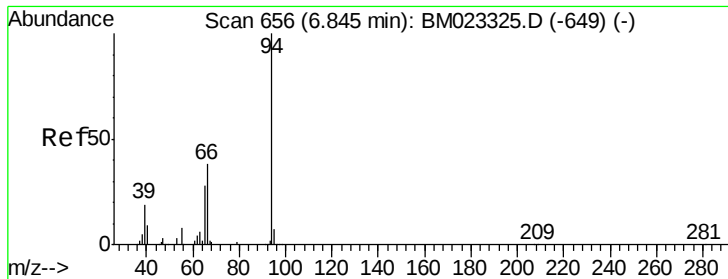

#6

Phenol

Concen: 2.078 ng/ul

RT: 6.85 min Scan# 657

Delta R.T. 0.01 min

Lab File: BM023330.D

Acq: 22 Oct 2019 21:56

Instrument :

BNA_M





ClientSampleId :

BFB88

Tot Ion:	94	Resp:	76907
Ion	Ratio	Lower	Upper
94	100		
65	27.0	23.2	34.8
66	40.4	32.9	49.3

Manual Integrations
APPROVED

mohammad
10/24/2019 8:08:53 AM

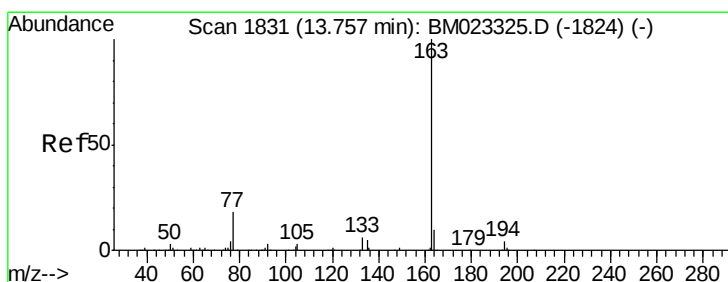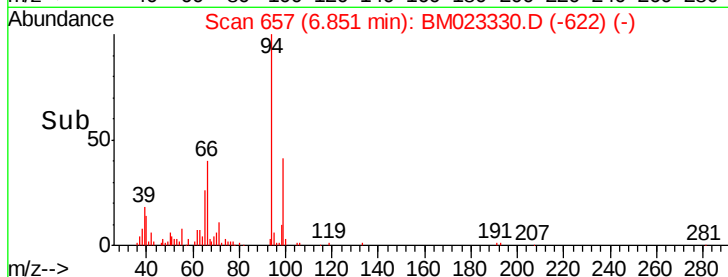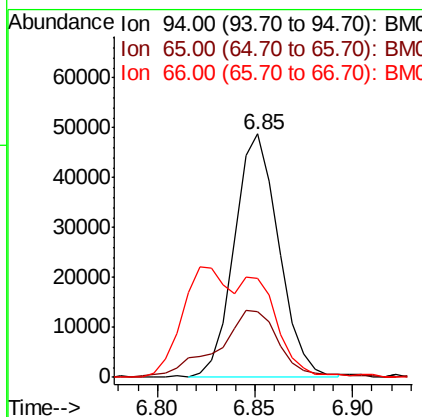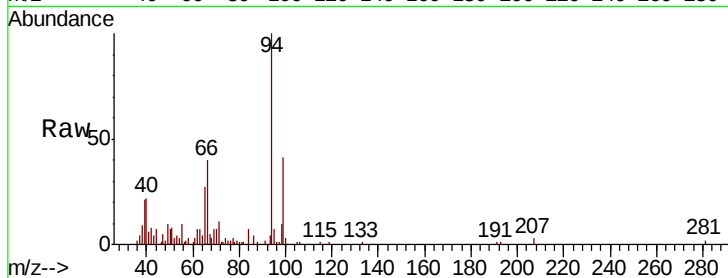

#45

Dimethylphthalate

Concen: 9.344 ng/ul




RT: 13.76 min Scan# 1831


Delta R.T. -0.00 min

Lab File: BM023330.D

Acq: 22 Oct 2019 21:56

Tgt Ion:	163	Resp:	757122
Ion	Ratio	Lower	Upper
163	100		
194	4.3	3.4	5.2
164	10.0	7.8	11.6

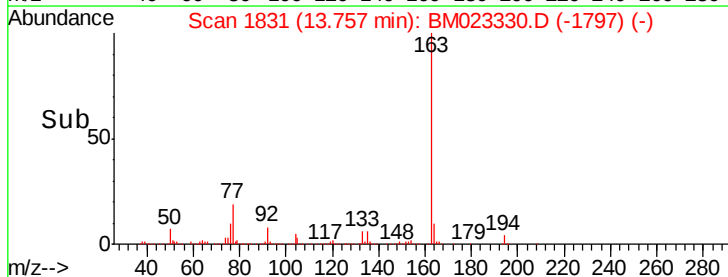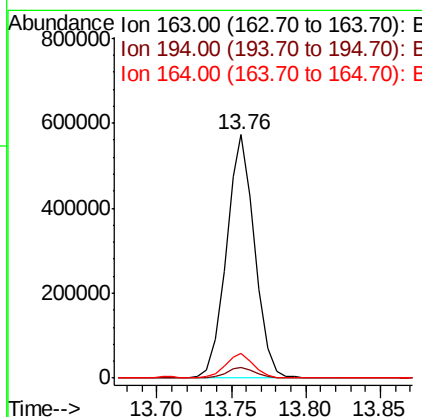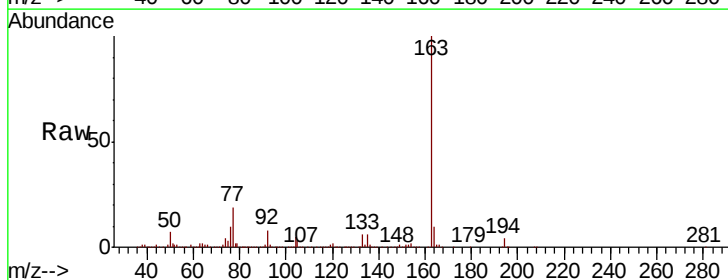

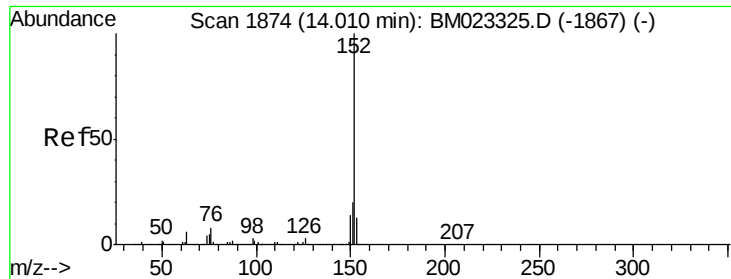





#48
Acenaphthylene
Concen: 2.531 ng/ul
RT: 14.01 min Scan# 1874
Delta R.T. -0.00 min
Lab File: BM023330.D
Acq: 22 Oct 2019 21:56

Instrument :
BNA_M
ClientSampleId :
BFB88

Tot Ion	Ratio	Resp	Lower	Upper
152	100	245690		
151	21.8		15.9	23.9
153	14.1		10.3	15.5




Manual Integrations
APPROVED


mohammad
10/24/2019 8:08:53 AM

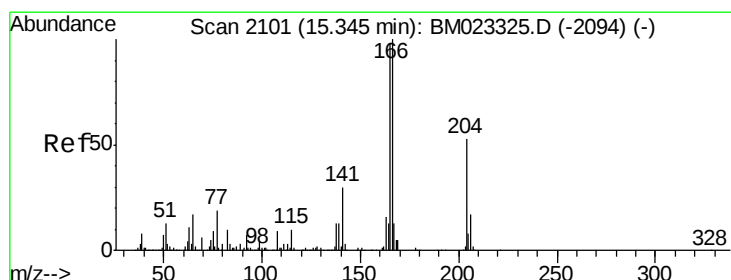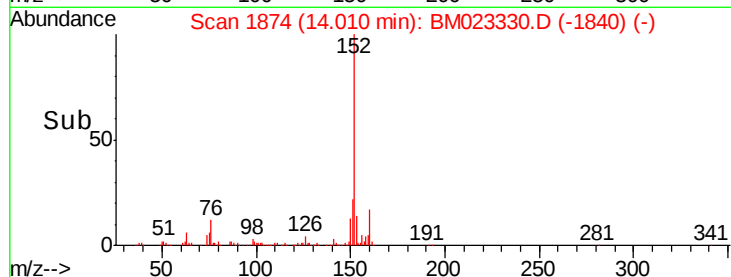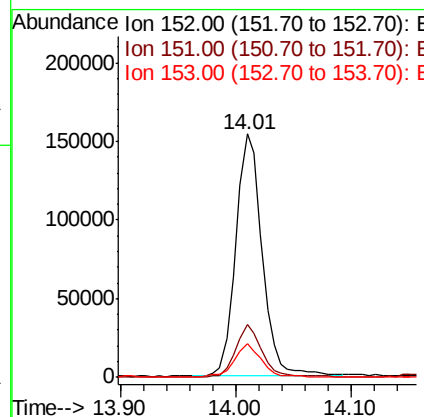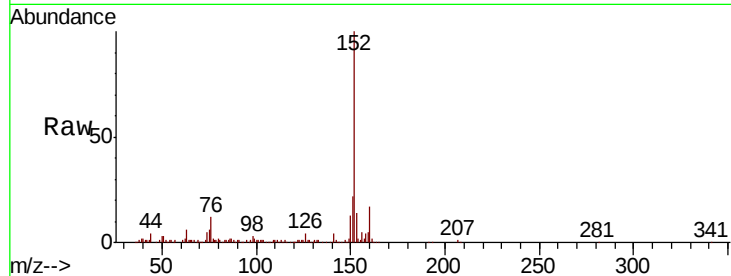

#59
Fluorene
Concen: 1.054 ng/ul
RT: 15.34 min Scan# 2101
Delta R.T. -0.00 min
Lab File: BM023330.D
Acq: 22 Oct 2019 21:56

Tgt Ion	Ratio	Resp	Lower	Upper
166	100	82968		
165	97.0		78.3	117.5
167	15.1		10.7	16.1

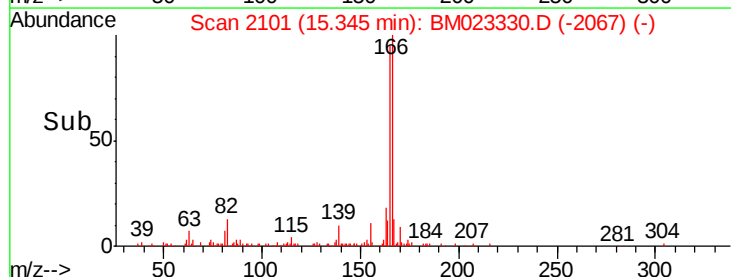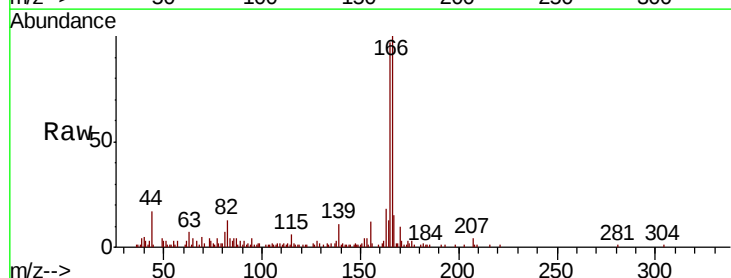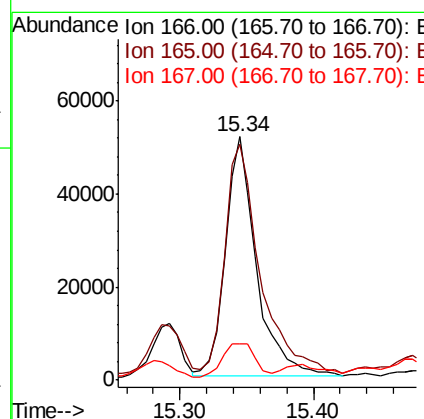

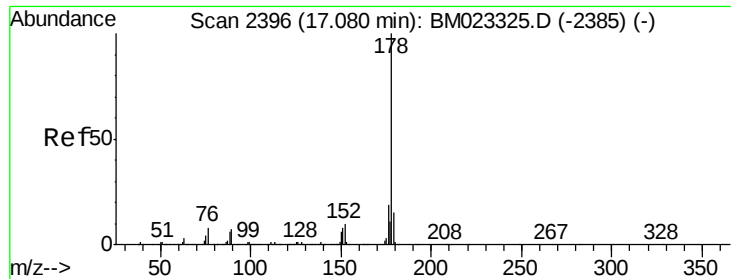





#70
Phenanthrene
Concen: 11.135 ng/ul
RT: 17.08 min Scan# 2396
Delta R.T. -0.00 min
Lab File: BM023330.D
Acq: 22 Oct 2019 21:56

Instrument :
BNA_M
ClientSampleId :
BFB88

Tot Ion	Ratio	Lower	Upper
178	100		
179	15.5	11.7	17.5
176	18.9	15.0	22.4




Manual Integrations
APPROVED


mohammad
10/24/2019 8:08:53 AM

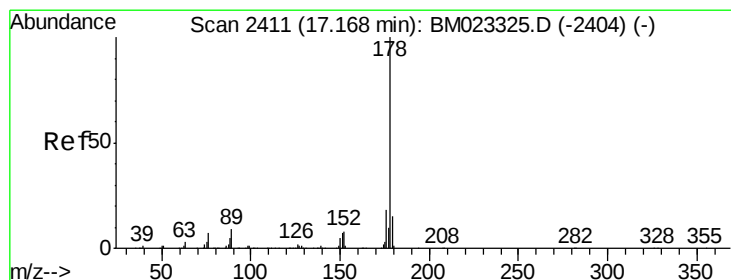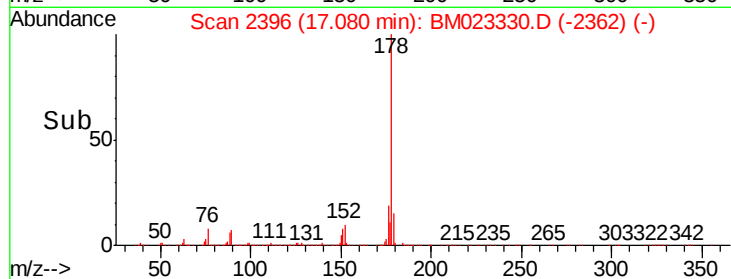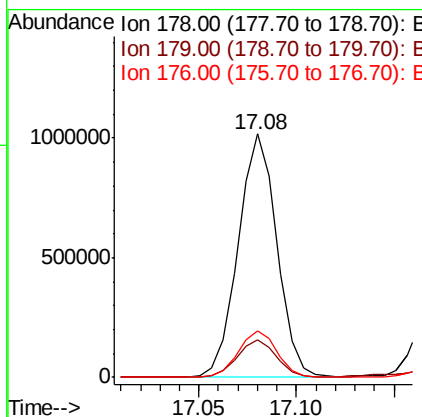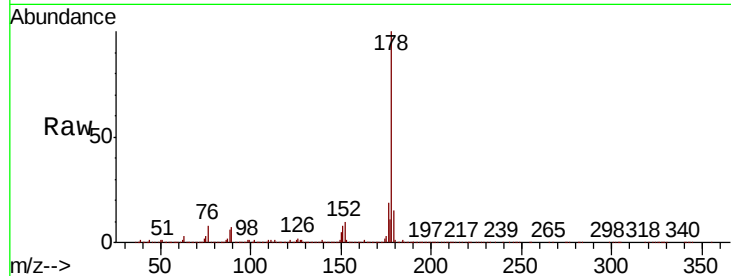

#72
Anthracene
Concen: 3.251 ng/ul
RT: 17.17 min Scan# 2411
Delta R.T. -0.00 min
Lab File: BM023330.D
Acq: 22 Oct 2019 21:56

Tgt Ion	Ratio	Lower	Upper
178	100		
179	15.0	12.5	18.7
176	18.2	14.8	22.2

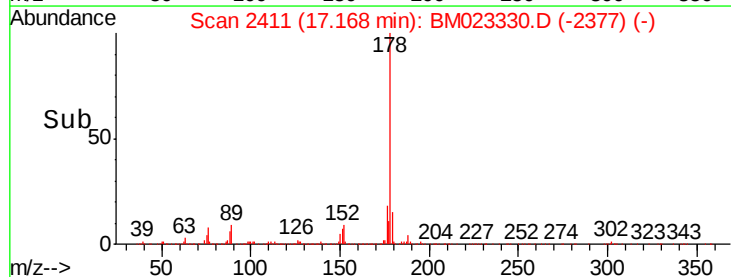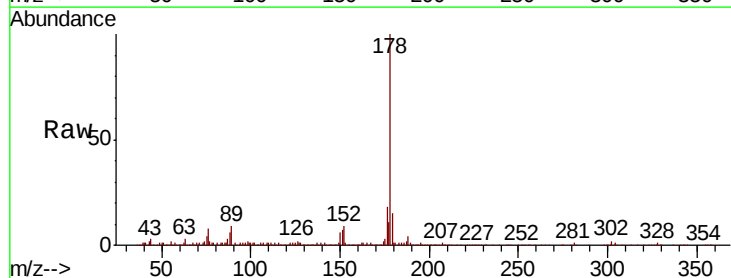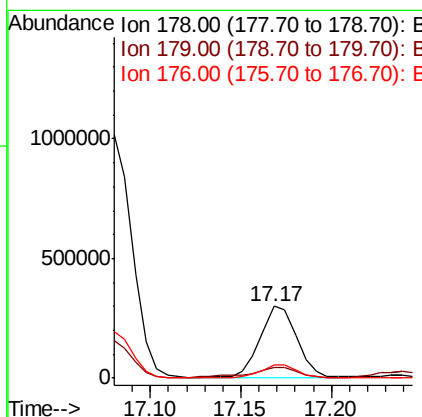

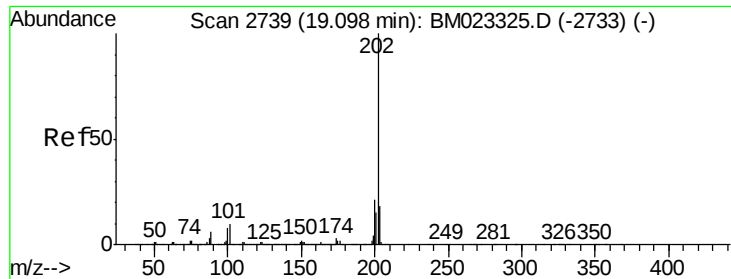





#77
 Fluoranthene
 Concen: 17.958 ng/ul
 RT: 19.10 min Scan# 2740
 Delta R.T. 0.01 min
 Lab File: BM023330.D
 Acq: 22 Oct 2019 21:56

Instrument :
 BNA_M
 ClientSampleId :
 BFB88

Tot Ion	Ion	Ratio	Resp	Lower	Upper
202	100		2659157		
101	9.5	8.2	12.4		
100	7.4	6.1	9.1		




Manual Integrations
 APPROVED


mohammad
 10/24/2019 8:08:53 AM

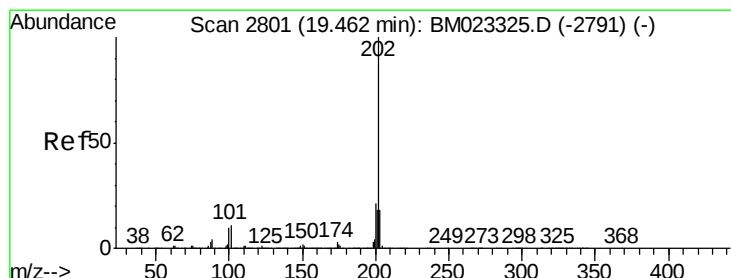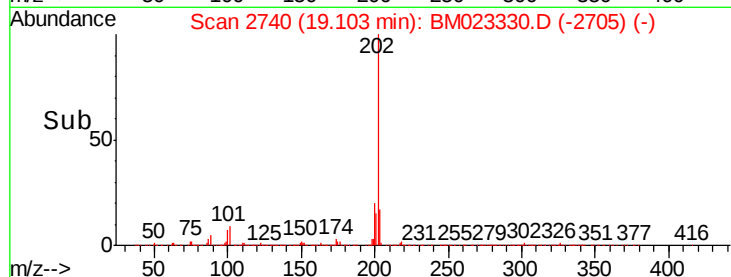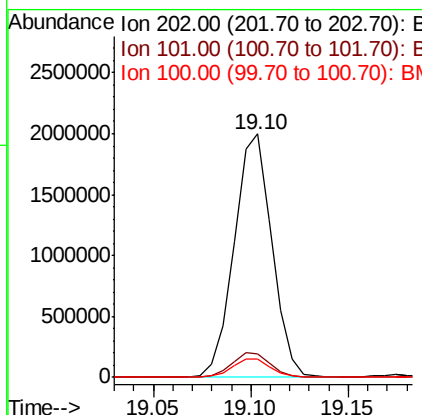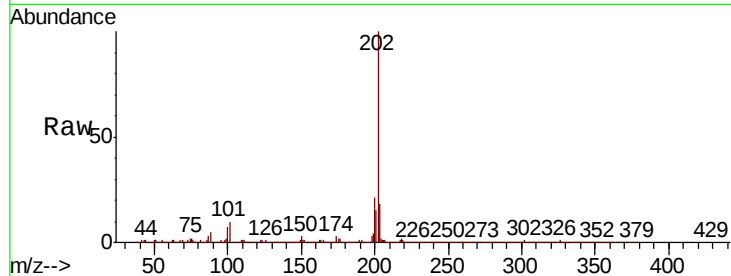

#80
 Pyrene
 Concen: 19.525 ng/ul
 RT: 19.46 min Scan# 2801
 Delta R.T. -0.00 min
 Lab File: BM023330.D
 Acq: 22 Oct 2019 21:56

Tgt Ion	Ion	Ratio	Resp	Lower	Upper
202	100		2805623		
101	12.0	9.0	13.6		
100	10.2	7.5	11.3		

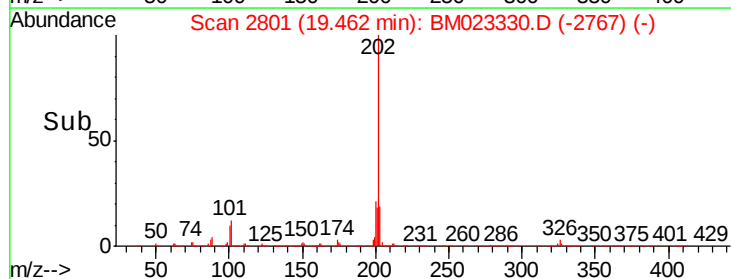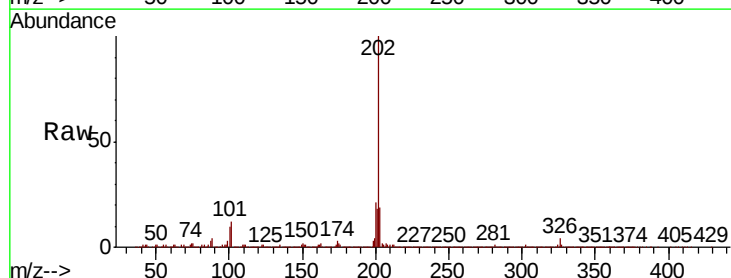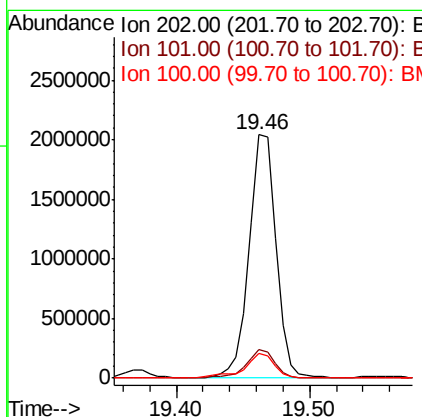

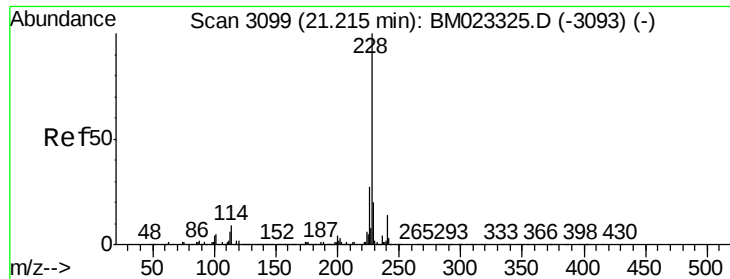





#83
Benzo(a)anthracene
Concen: 11.186 ng/ul
RT: 21.22 min Scan# 3099
Delta R.T. -0.00 min
Lab File: BM023330.D
Acq: 22 Oct 2019 21:56

Instrument :
BNA_M
ClientSampleId :
BFB88

Tot Ion	Ratio	Lower	Upper
228	100		
229	21.3	15.8	23.8
226	30.4	21.5	32.3




Manual Integrations
APPROVED


mohammad
10/24/2019 8:08:53 AM

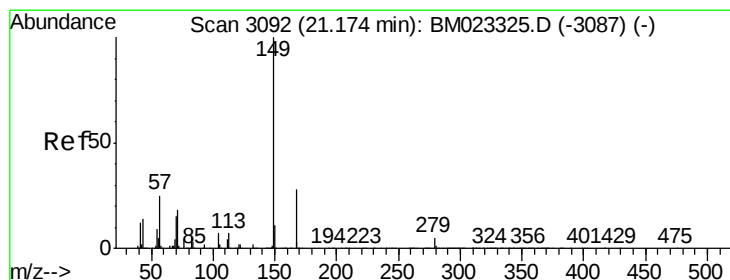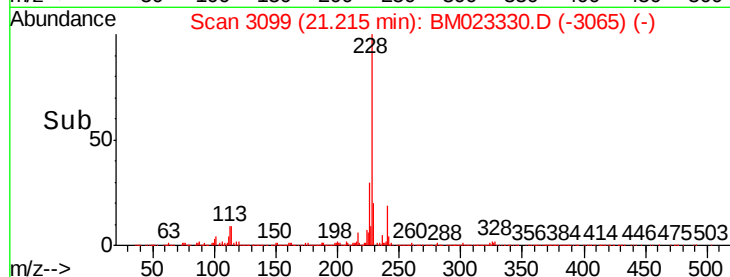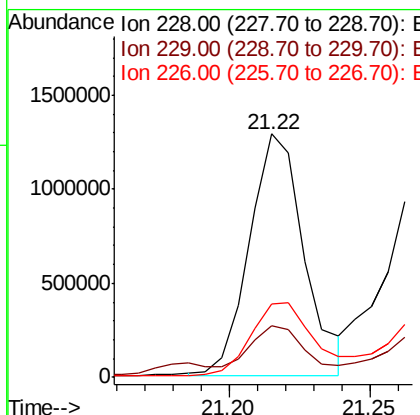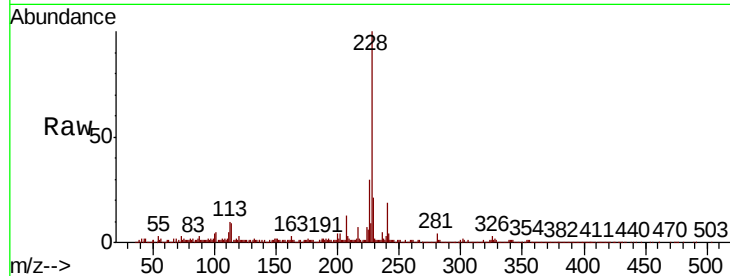

#84
Bis(2-ethylhexyl)phthalate
Concen: 1.723 ng/ul
RT: 21.17 min Scan# 3092
Delta R.T. -0.00 min
Lab File: BM023330.D
Acq: 22 Oct 2019 21:56

Tgt Ion	Ratio	Lower	Upper
149	100		
167	29.2	22.1	33.1
279	7.2	4.3	6.5#

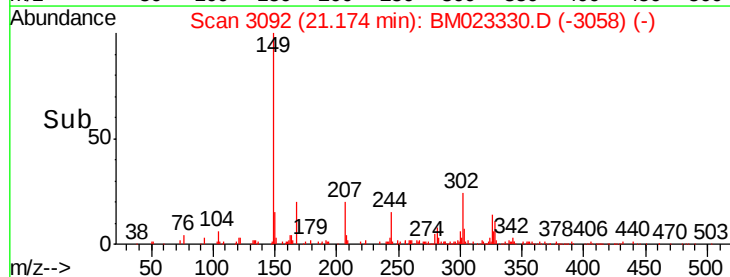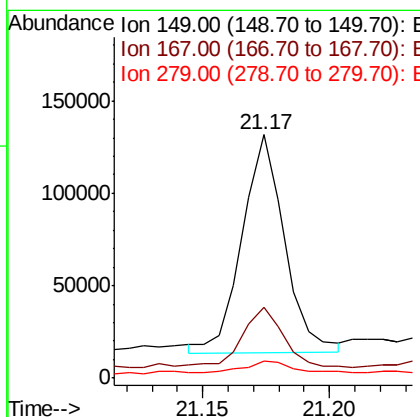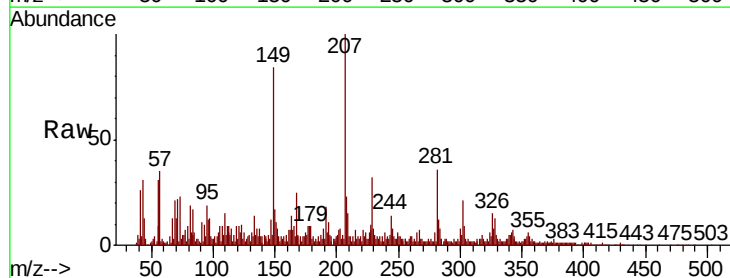

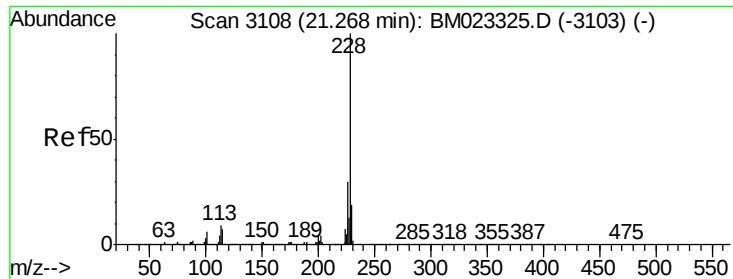





#85
Chrysene
Concen: 11.334 ng/ul
RT: 21.27 min Scan# 3108
Delta R.T. -0.00 min
Lab File: BM023330.D
Acq: 22 Oct 2019 21:56

Instrument :
BNA_M
ClientSampleId :
BFB88

Tot Ion	Ratio	Lower	Upper
228	100		
226	30.1	23.4	35.0
229	22.2	15.5	23.3




Manual Integrations
APPROVED


mohammad
10/24/2019 8:08:53 AM

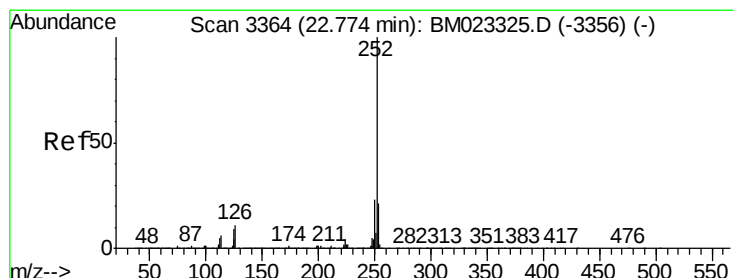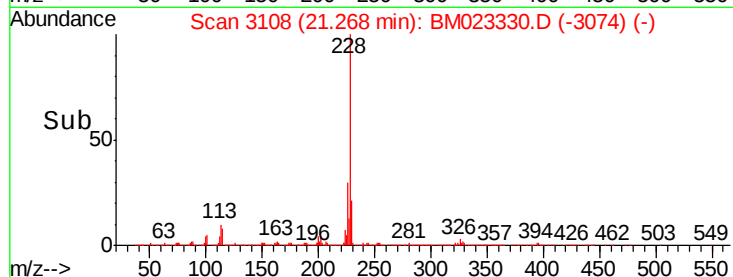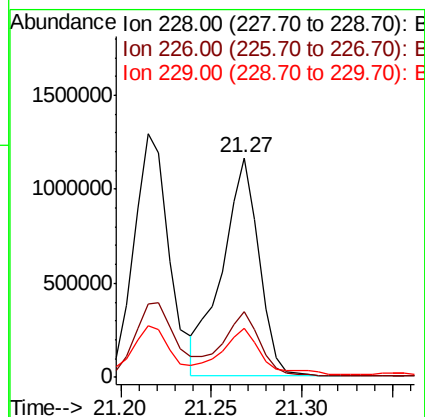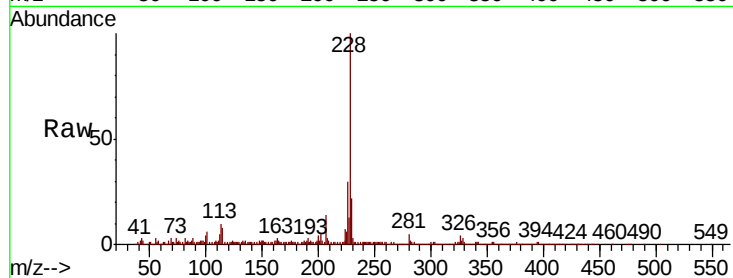

#88
Benzo(b)fluoranthene
Concen: 14.375 ng/ul
RT: 22.79 min Scan# 3366
Delta R.T. 0.01 min
Lab File: BM023330.D
Acq: 22 Oct 2019 21:56

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.2	17.3	25.9
125	9.7	7.0	10.4

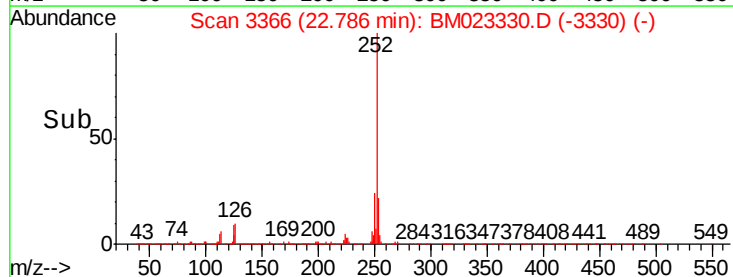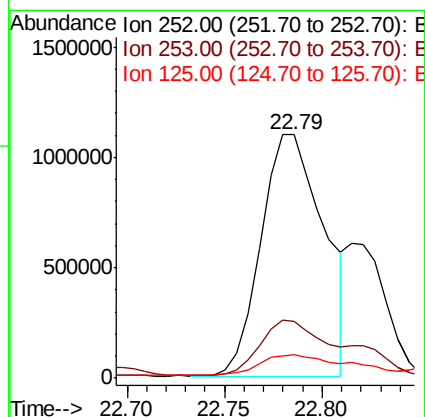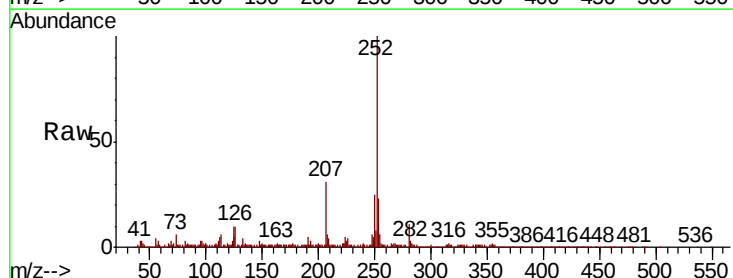

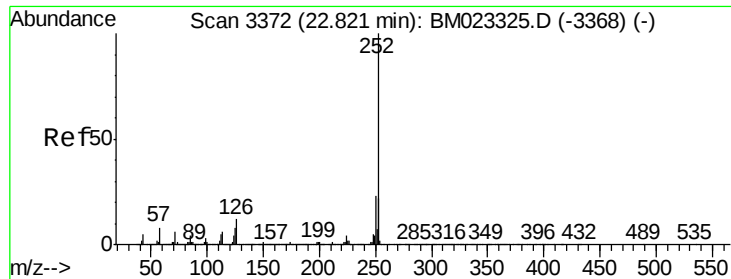





#89
Benzo(k)fluoranthene
Concen: 5.070 ng/ul m
RT: 22.82 min Scan# 3371
Delta R.T. -0.01 min
Lab File: BM023330.D
Acq: 22 Oct 2019 21:56

Instrument :
BNA_M
ClientSampleId :
BFB88

Tot Ion	Ratio	Lower	Upper
252	100		
253	24.0	17.5	26.3
125	11.3	6.6	9.8




Manual Integrations
APPROVED


mohammad
10/24/2019 8:08:53 AM

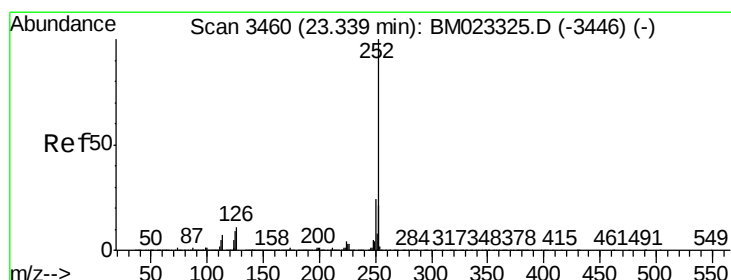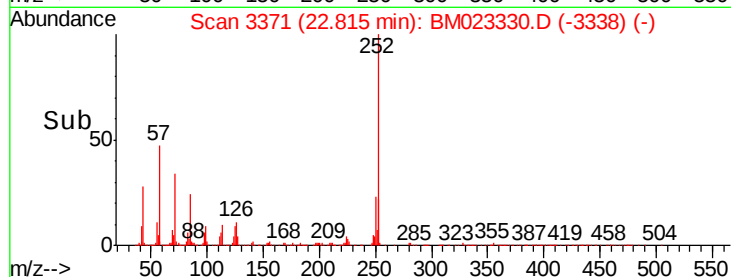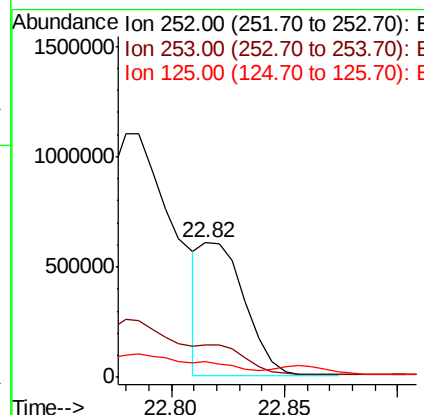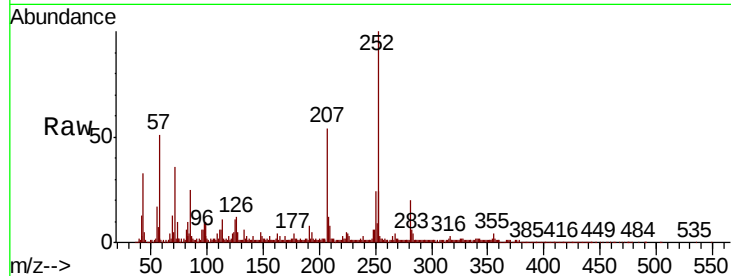

#91
Benzo(a)pyrene
Concen: 10.919 ng/ul
RT: 23.34 min Scan# 3461
Delta R.T. 0.01 min
Lab File: BM023330.D
Acq: 22 Oct 2019 21:56

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.7	17.0	25.6
125	10.0	7.1	10.7

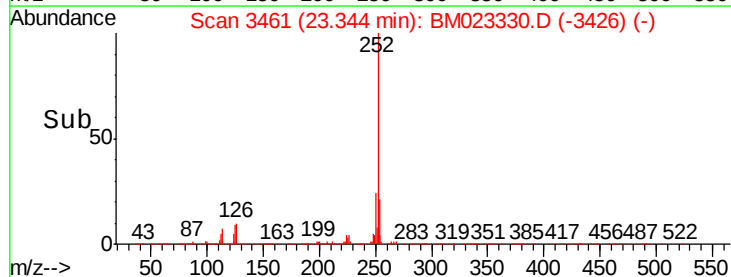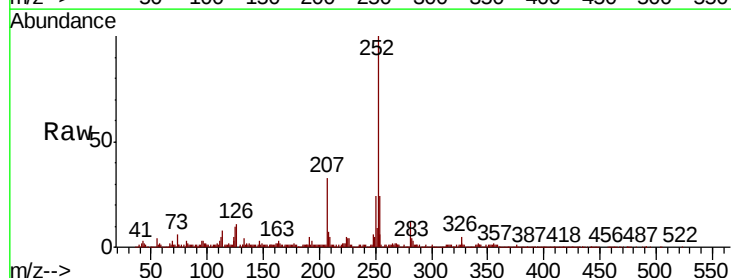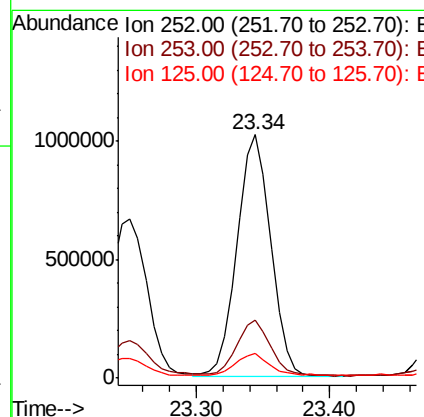

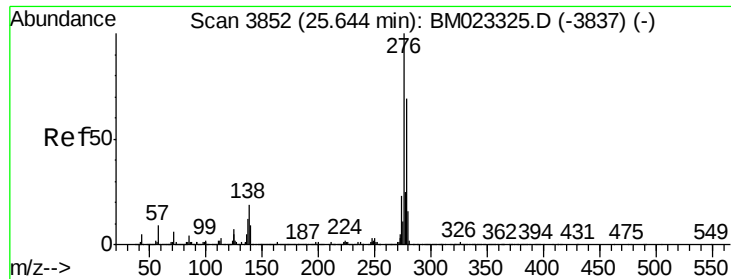





#92
 Indeno(1,2,3-cd)pyrene
 Concen: 6.829 ng/ul
 RT: 25.65 min Scan# 3853
 Delta R.T. 0.01 min
 Lab File: BM023330.D
 Acq: 22 Oct 2019 21:56

Instrument :
 BNA_M
 ClientSampleId :
 BFB88

Tot Ion	Ratio	Lower	Upper
276	100		
138	16.8	15.8	23.6
277	25.2	19.8	29.8




Manual Integrations
 APPROVED




mohammad
 10/24/2019 8:08:53 AM

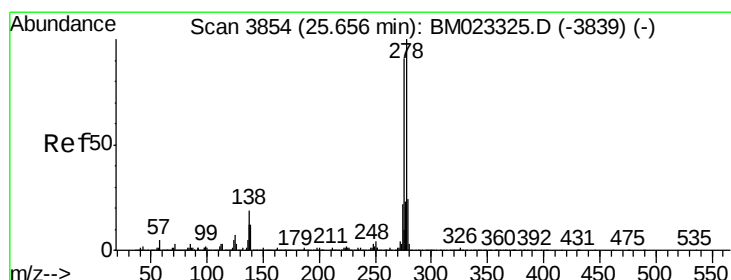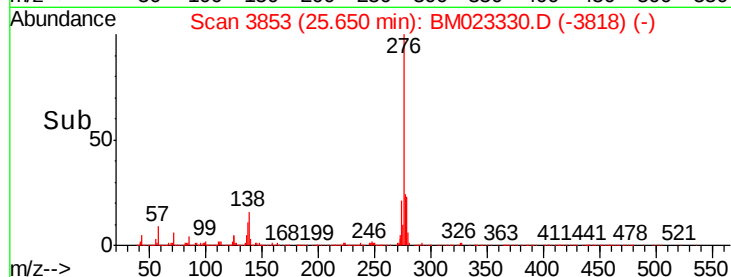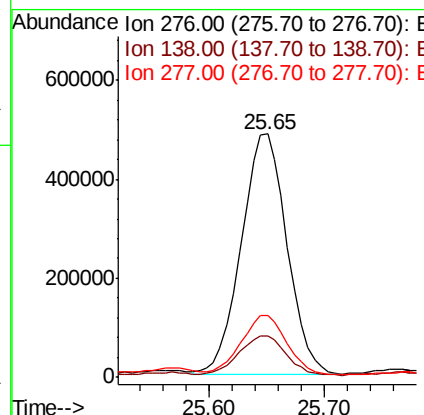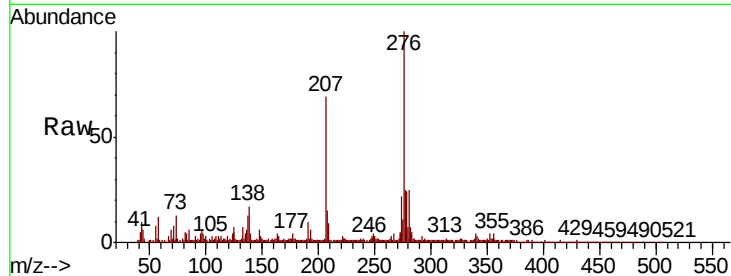

#93
 Dibenzo(a,h)anthracene
 Concen: 2.241 ng/ul
 RT: 25.66 min Scan# 3854
 Delta R.T. -0.00 min
 Lab File: BM023330.D
 Acq: 22 Oct 2019 21:56

Tgt Ion	Ratio	Lower	Upper
278	100		
139	17.5	10.5	15.7#
279	28.5	19.7	29.5

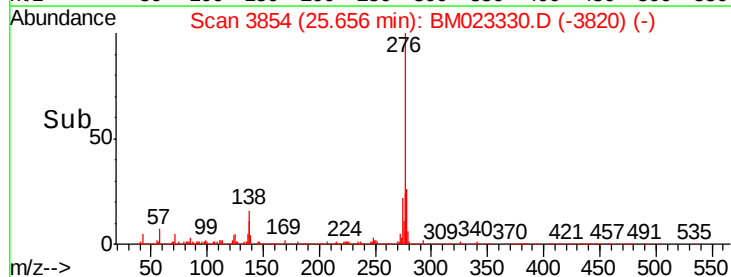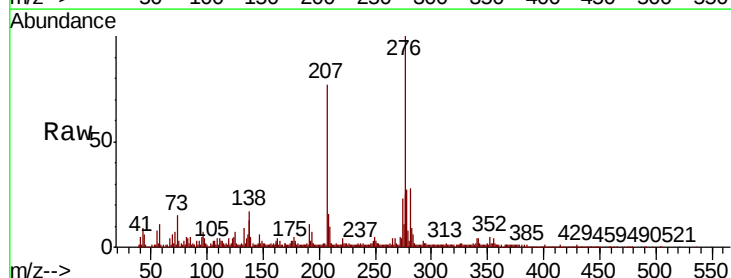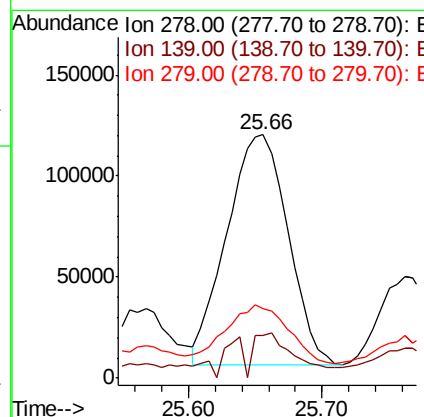

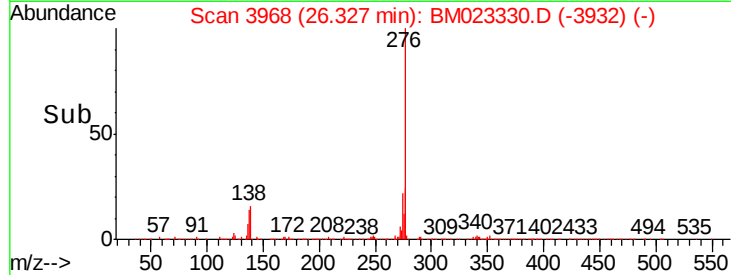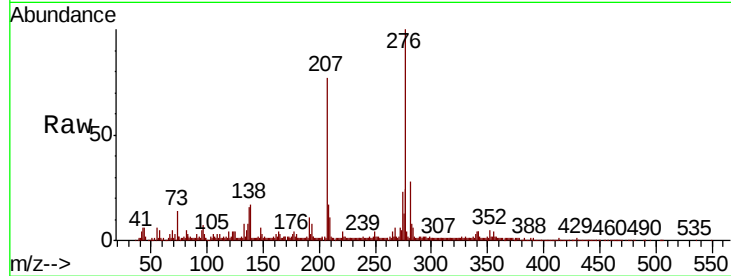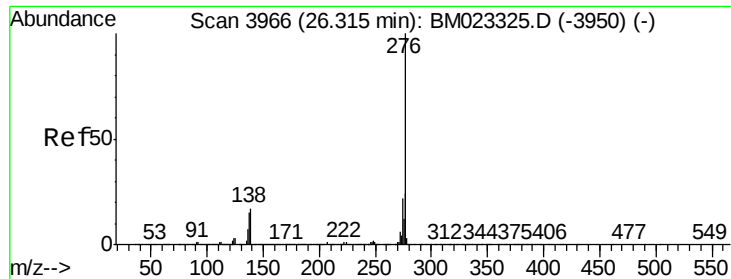

#94
 Benzo(a,h,i)perylene
 Concen: 8.172 ng/ul
 RT: 26.33 min Scan# 3968
 Delta R.T. 0.01 min
 Lab File: BM023330.D
 Acq: 22 Oct 2019 21:56

Instrument :
 BNA_M
 ClientSampleId :
 BFB88

Tot Ion	Ratio	Lower	Upper
276	100		
138	17.2	13.9	20.9
277	24.5	18.7	28.1

Manual Integrations
 APPROVED

mohammad
 10/24/2019 8:08:53 AM

