

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102318\
 Data File : BM017295.D
 Acq On : 23 Oct 2018 21:29
 Operator : MJ/SJ
 Sample : J5605-12
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Oct 24 06:58:23 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM101718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 17 14:23:17 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	273797	20.00	ng	-0.02
21) Naphthalene-d8	10.43	136	1024056	20.00	ng	-0.02
39) Acenaphthene-d10	14.30	164	584551	20.00	ng	-0.02
64) Phenanthrene-d10	17.05	188	1400897	20.00	ng	-0.02
76) Chrysene-d12	21.24	240	1510422	20.00	ng	-0.02
87) Perylene-d12	23.46	264	1279647	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.28	112	1716156	106.01	ng	0.00
7) Phenol-d6	6.85	99	2001645	90.79	ng	-0.01
23) Nitrobenzene-d5	8.81	82	1534224	87.62	ng	-0.02
42) 2,4,6-Tribromophenol	15.80	330	1104767	139.75	ng	-0.02
45) 2-Fluorobiphenyl	12.92	172	3526910	80.28	ng	-0.02
79) Terphenyl-d14	19.69	244	6180623	92.23	ng	-0.01
Target Compounds						
80) Butylbenzylphthalate	20.40	149	832	7.198	ng	# 77
84) Bis(2-ethylhexyl)phthalate	21.17	149	9614	5.482	ng	# 89
85) Di-n-octyl phthalate	22.04	149	1049	5.583	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102318\
Data File : BM017295.D
Acq On : 23 Oct 2018 21:29
Operator : MJ/SJ
Sample : J5605-12
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Oct 24 06:58:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM101718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 17 14:23:17 2018
Response via : Initial Calibration

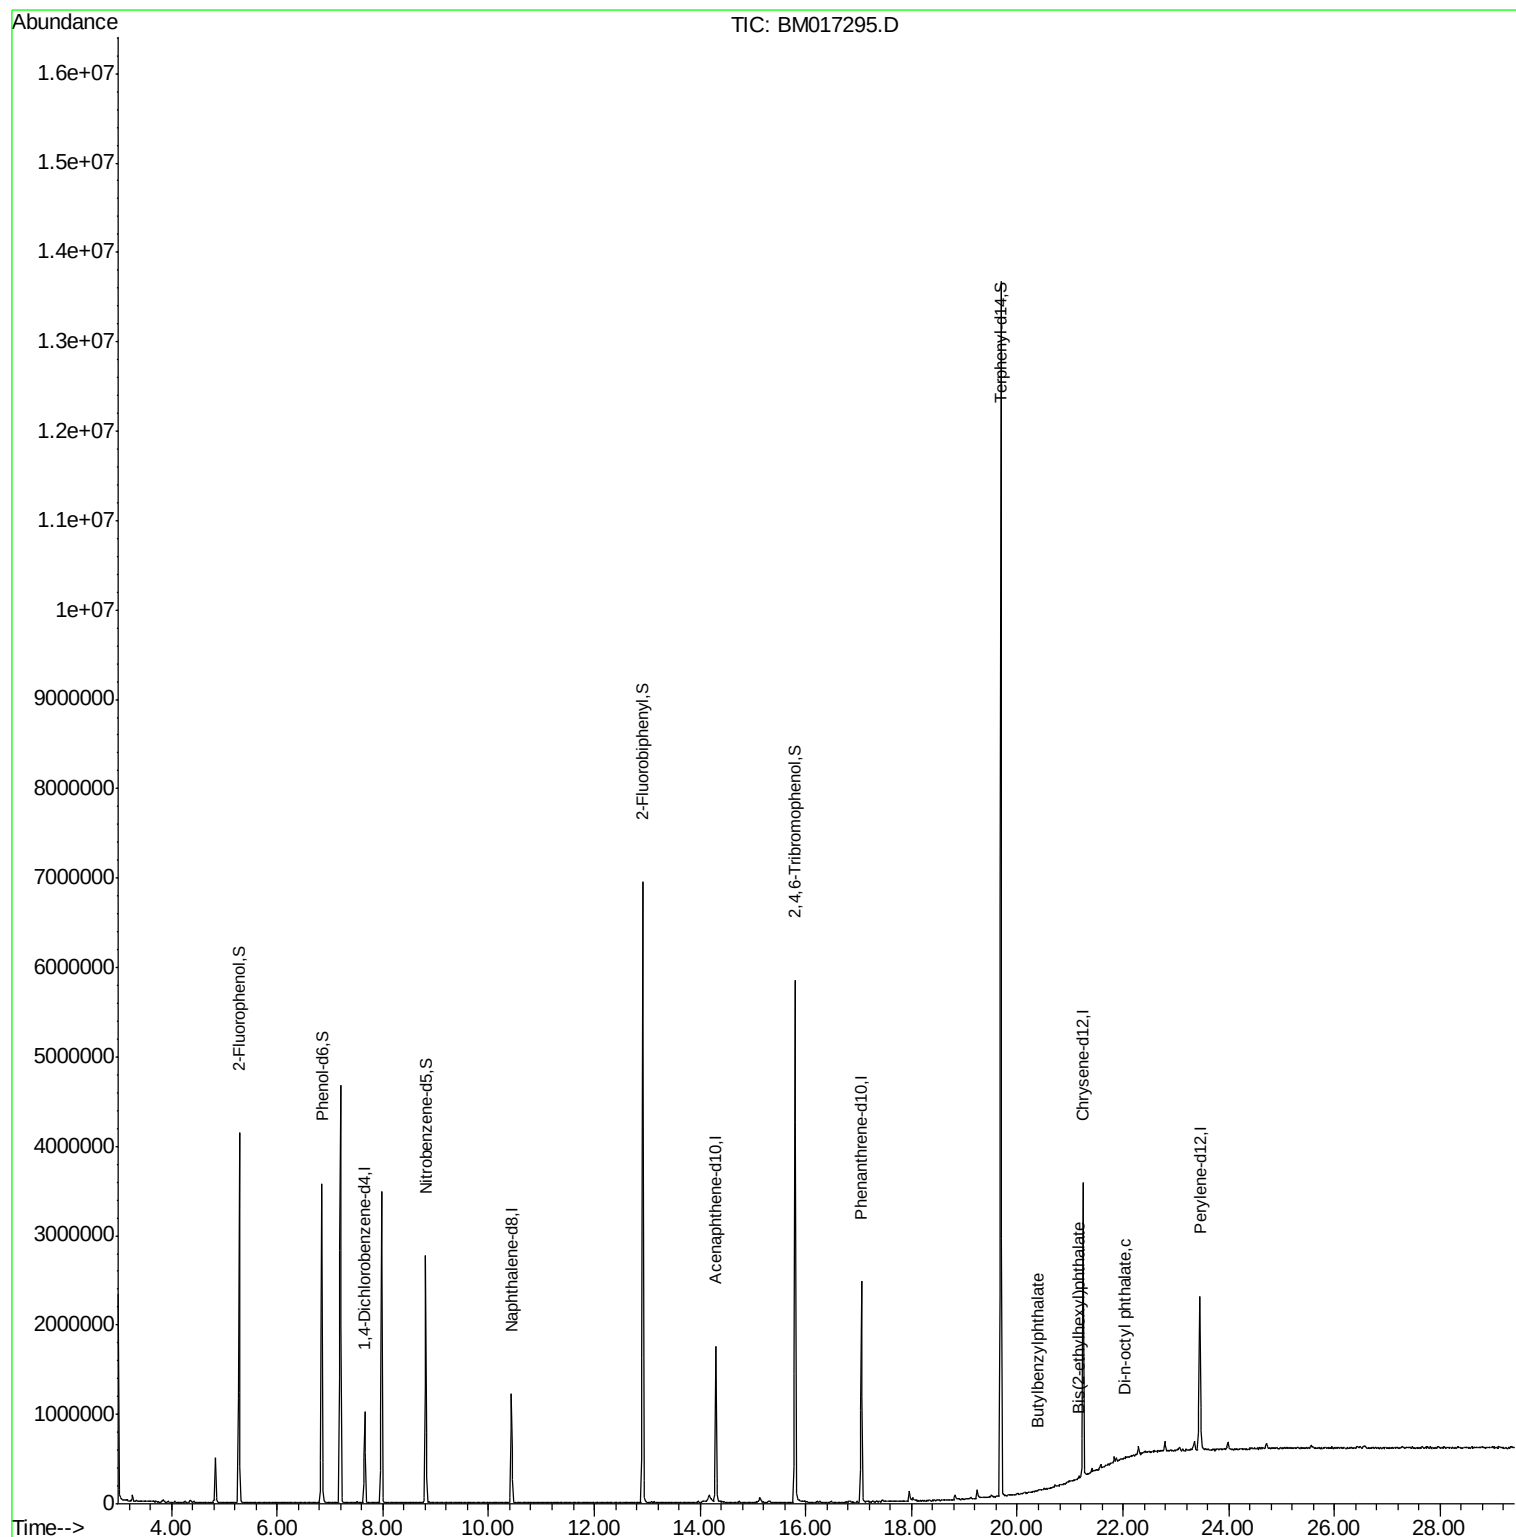

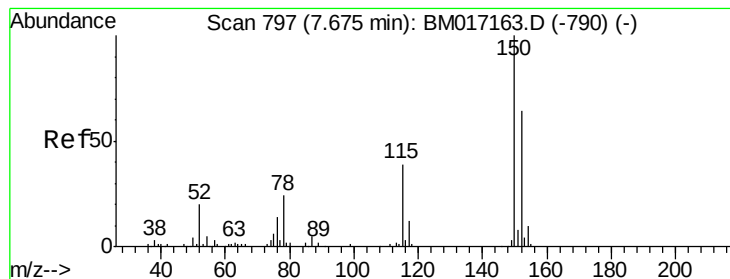


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.66 min Scan# 794
Delta R.T. -0.02 min
Lab File: BM017295.D
Acq: 23 Oct 2018 21:29

Instrument :
BNA_M
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	150.7	124.3	186.5
115	58.6	48.1	72.1






Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

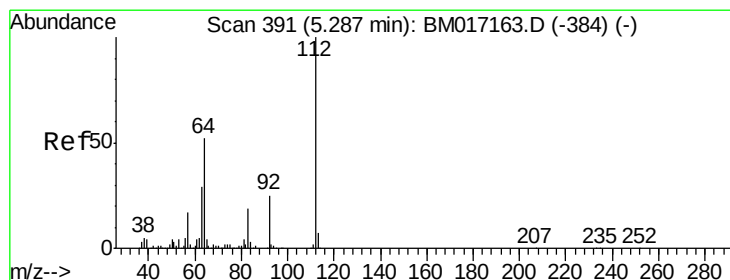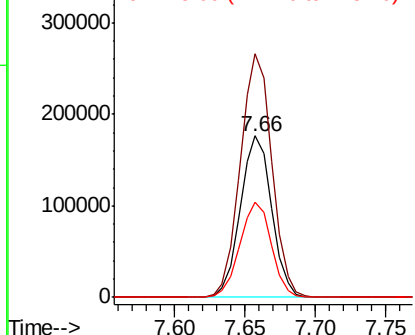

#5

2-Fluorophenol
Concen: 106.013 ng
RT: 5.28 min Scan# 390
Delta R.T. -0.01 min
Lab File: BM017295.D
Acq: 23 Oct 2018 21:29

Tgt Ion	Ratio	Lower	Upper
112	100		
64	56.8	41.7	62.5
63	29.4	23.0	34.4






Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 63.00 (62.70 to 63.70): BM0

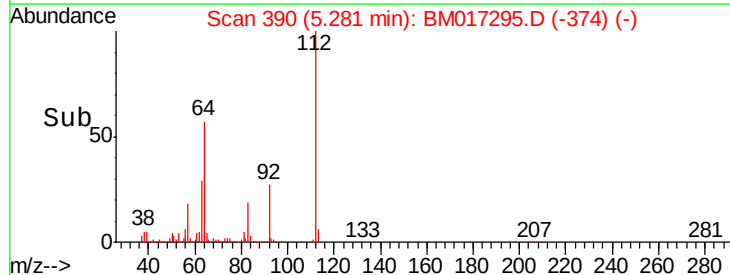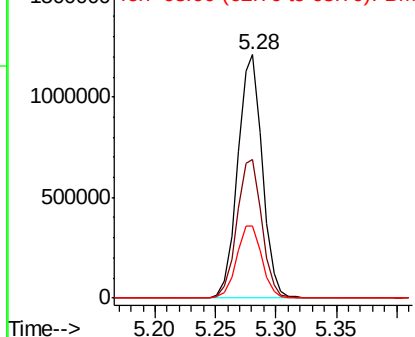

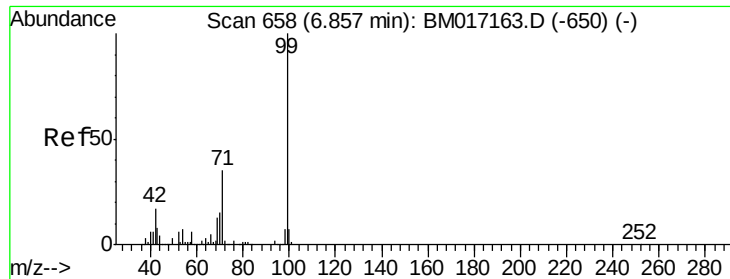

#7

Phenol-d6

Concen: 90.788 ng

RT: 6.85 min Scan# 656

Delta R.T. -0.01 min

Lab File: BM017295.D

Acq: 23 Oct 2018 21:29


Instrument :

BNA_M

ClientSampleId :

Tot Ion: 99 Resp: 2001645

Ion	Ratio	Lower	Upper
99	100		
42	17.1	13.3	19.9
71	35.1	28.0	42.0






Abundance

Ion 99.00 (98.70 to 99.70): BM017163.D (-650) (-)

Ion 42.00 (41.70 to 42.70): BM017163.D (-650) (-)

Ion 71.00 (70.70 to 71.70): BM017163.D (-650) (-)

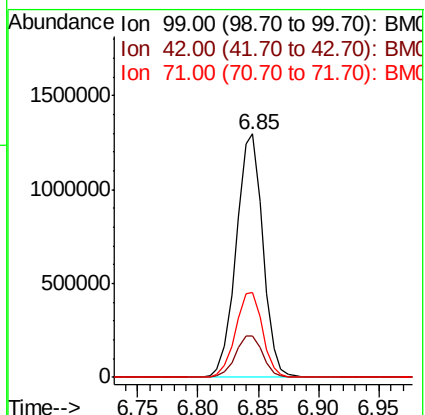

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.43 min Scan# 1266


Delta R.T. -0.02 min

Lab File: BM017295.D

Acq: 23 Oct 2018 21:29

Tgt Ion: 136 Resp: 1024056

Ion	Ratio	Lower	Upper
136	100		
137	10.9	9.2	13.8
54	7.9	6.7	10.1
68	6.0	4.7	7.1





Abundance


Ion 136.00 (135.70 to 136.70): BM017163.D (-1261) (-)

Ion 137.00 (136.70 to 137.70): BM017163.D (-1261) (-)

Ion 54.00 (53.70 to 54.70): BM017163.D (-1261) (-)

Ion 68.00 (67.70 to 68.70): BM017163.D (-1261) (-)

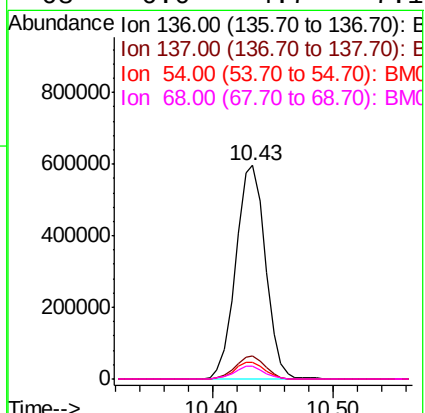




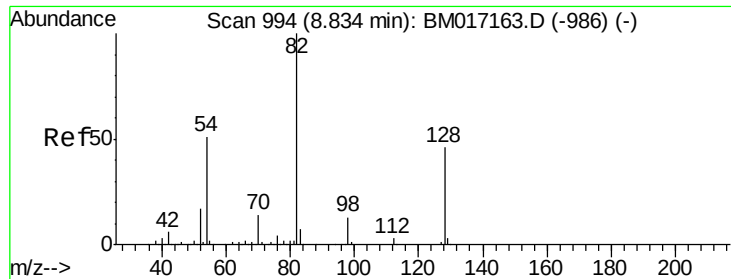


#23
 Nitrobenzene-d5
 Concen: 87.622 ng
 RT: 8.81 min Scan# 990
 Delta R.T. -0.02 min
 Lab File: BM017295.D
 Acq: 23 Oct 2018 21:29

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion: 82 Resp: 1534224




Ion	Ratio	Lower	Upper
82	100		
128	43.3	37.0	55.6
54	49.3	40.7	61.1

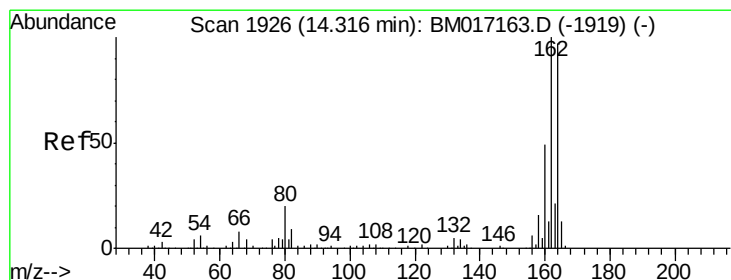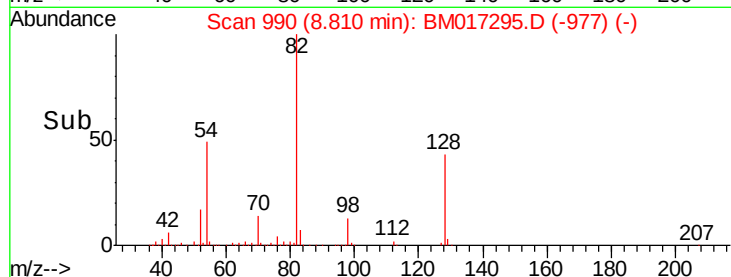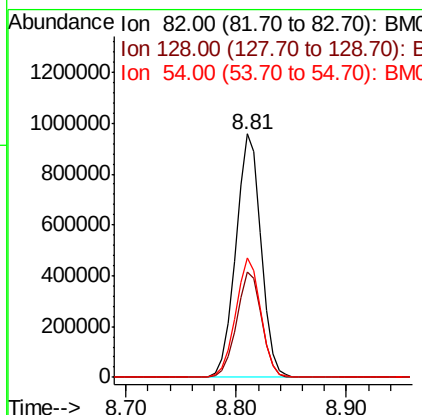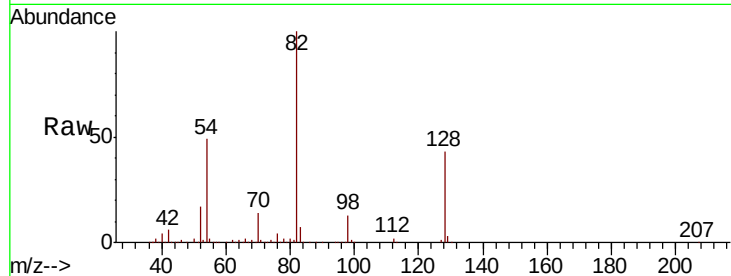


#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.30 min Scan# 1923
 Delta R.T. -0.02 min
 Lab File: BM017295.D
 Acq: 23 Oct 2018 21:29

Tgt Ion: 164 Resp: 584551

Ion	Ratio	Lower	Upper
164	100		
162	100.9	82.1	123.1
160	44.3	40.2	60.2

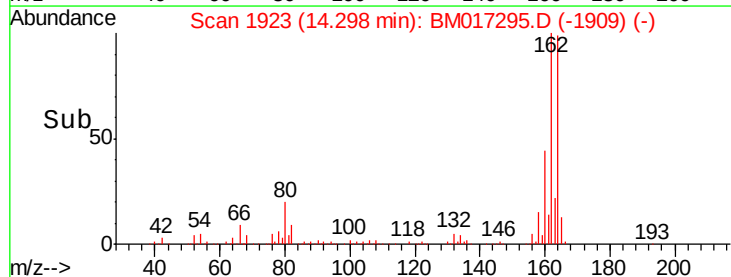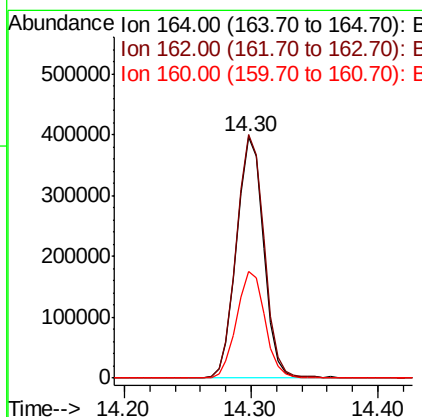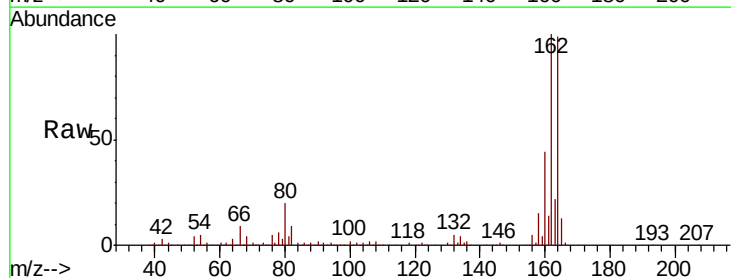







#42
 2,4,6-Tribromophenol
 Concen: 139.752 ng
 RT: 15.80 min Scan# 2178
 Delta R.T. -0.02 min
 Lab File: BM017295.D
 Acq: 23 Oct 2018 21:29

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion:330 Resp: 1104767
 Ion Ratio Lower Upper
 330 100
 332 97.1 77.3 115.9
 141 33.2 27.4 41.0

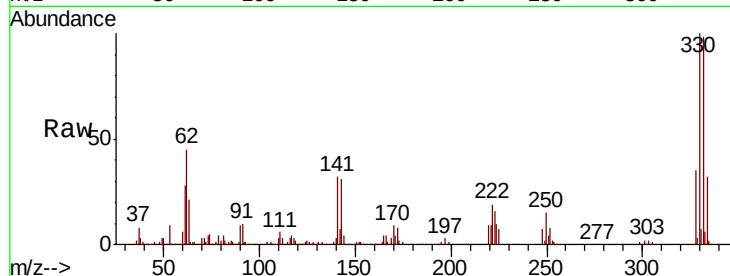


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


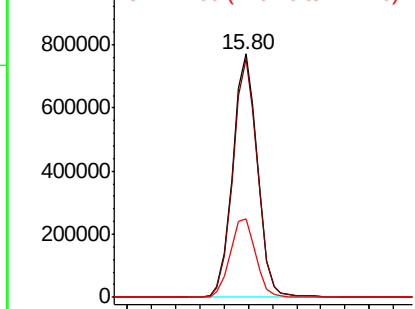



#45
 2-Fluorobiphenyl
 Concen: 80.279 ng
 RT: 12.92 min Scan# 1688
 Delta R.T. -0.02 min
 Lab File: BM017295.D
 Acq: 23 Oct 2018 21:29

Tgt Ion:172 Resp: 3526910
 Ion Ratio Lower Upper
 172 100
 171 35.1 28.3 42.5
 170 22.8 18.3 27.5



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E




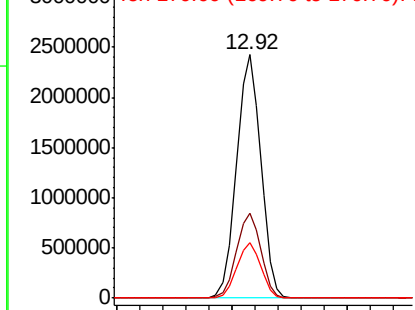




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.05 min Scan# 2391
Delta R.T. -0.02 min
Lab File: BM017295.D
Acq: 23 Oct 2018 21:29




Instrument :
BNA_M
ClientSampleId :


Tot Ion:188 Resp: 1400897
Ion Ratio Lower Upper
188 100
94 8.9 7.0 10.4
80 10.2 7.7 11.5

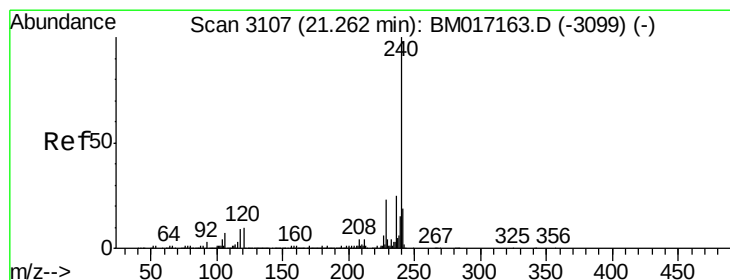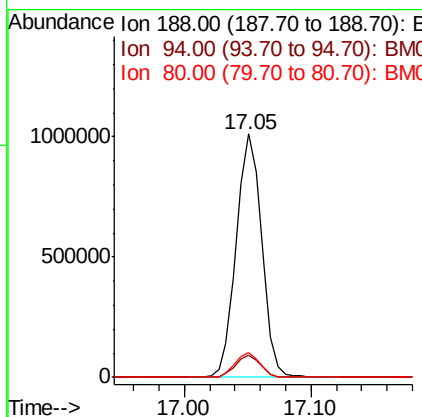

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.24 min Scan# 3104
Delta R.T. -0.02 min
Lab File: BM017295.D
Acq: 23 Oct 2018 21:29

Tgt Ion:240 Resp: 1510422
Ion Ratio Lower Upper
240 100
120 9.8 8.1 12.1
236 25.3 19.9 29.9

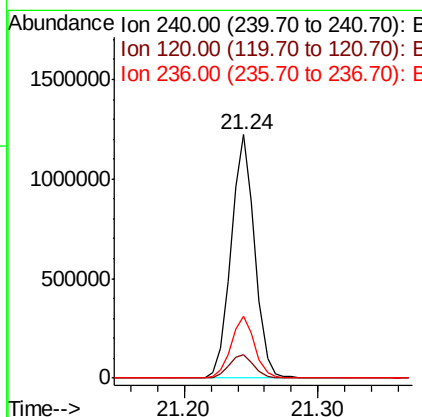



#79

Terphenyl-d14

Concen: 92.233 ng

RT: 19.69 min Scan# 2840

Delta R.T. -0.01 min

Lab File: BM017295.D

Acq: 23 Oct 2018 21:29

Instrument :

BNA_M

ClientSampleId :


Tot Ion:244 Resp: 6180623

Ion Ratio Lower Upper

244 100

212 7.2 5.5 8.3




122 10.3 8.4 12.6

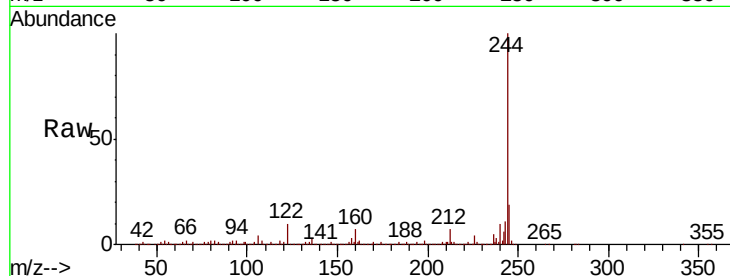

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

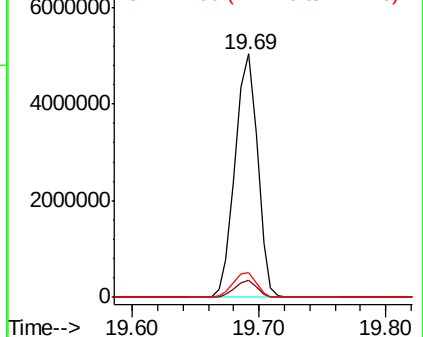

#80

Butylbenzylphthalate

Concen: 7.198 ng

RT: 20.40 min Scan# 2960

Delta R.T. -0.01 min

Lab File: BM017295.D

Acq: 23 Oct 2018 21:29


Tgt Ion:149 Resp: 832

Ion Ratio Lower Upper

149 100

91 43.4 51.3 76.9#



206 29.6 18.0 27.0#




Abundance Ion 149.00 (148.70 to 149.70): E

Ion 91.00 (90.70 to 91.70): BM0

Ion 206.00 (205.70 to 206.70): E

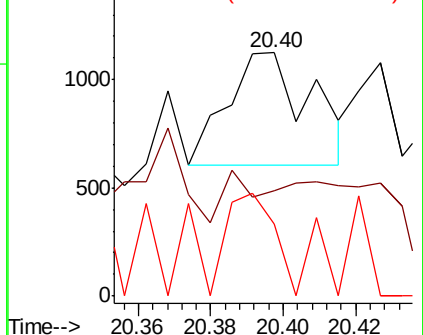


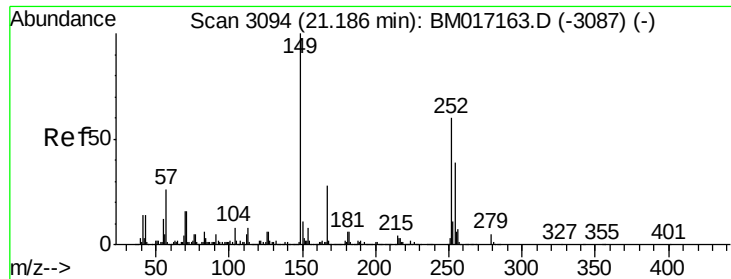




#84
 Bis(2-ethylhexyl)phthalate
 Concen: 5.482 ng
 RT: 21.17 min Scan# 3092
 Delta R.T. -0.01 min
 Lab File: BM017295.D
 Acq: 23 Oct 2018 21:29

Instrument :
 BNA_M
 ClientSampleID :

Tot Ion:149 Resp: 9614
 Ion Ratio Lower Upper
 149 100
 167 22.2 22.2 33.4#
 279 8.5 3.6 5.4#

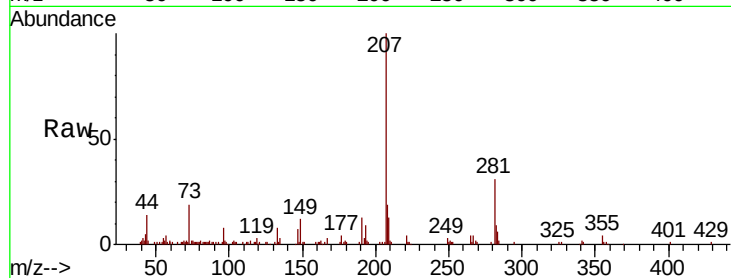


Abundance Ion 149.00 (148.70 to 149.70): E
 Ion 167.00 (166.70 to 167.70): E
 Ion 279.00 (278.70 to 279.70): E

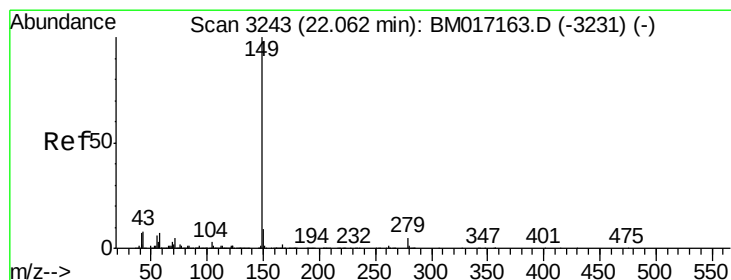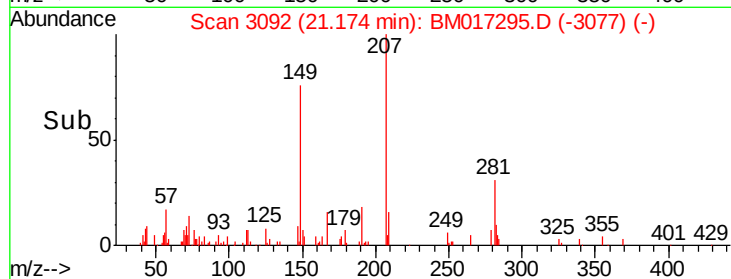
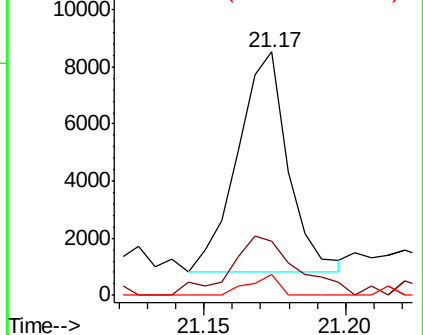



#85
 Di-n-octyl phthalate
 Concen: 5.583 ng
 RT: 22.04 min Scan# 3240
 Delta R.T. -0.02 min
 Lab File: BM017295.D
 Acq: 23 Oct 2018 21:29

Tgt Ion:149 Resp: 1049
 Ion Ratio Lower Upper
 149 100
 167 84.7 1.4 2.0#
 43 161.0 7.2 10.8#

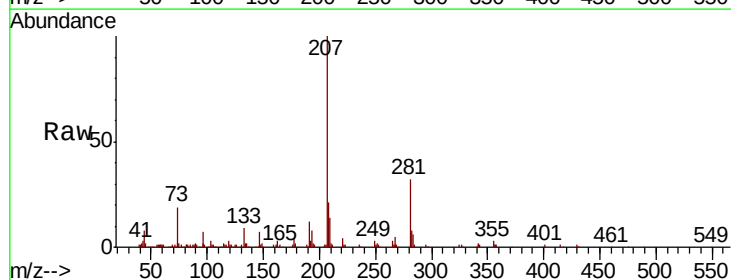

Abundance Ion 149.00 (148.70 to 149.70): E
 Ion 167.00 (166.70 to 167.70): E
 Ion 43.00 (42.70 to 43.70): BM

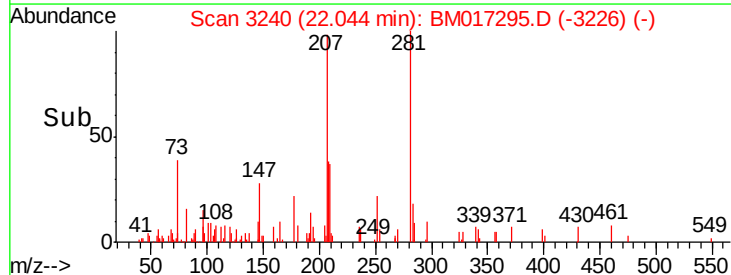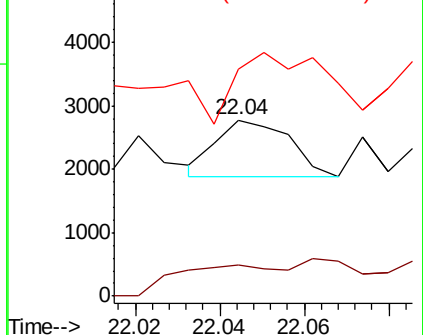

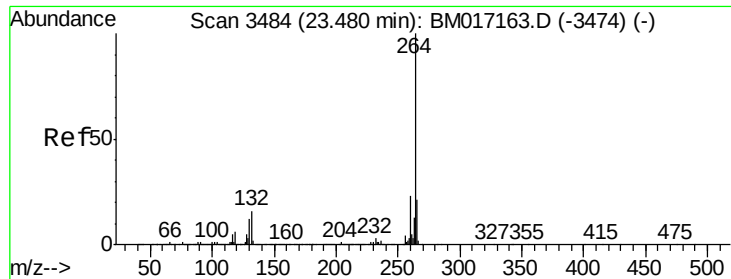

#87
Pervlene-d12
Concen: 20.000 ng
RT: 23.46 min Scan# 3480
Delta R.T. -0.02 min
Lab File: BM017295.D
Acq: 23 Oct 2018 21:29

Instrument :
BNA_M
ClientSampleId :

Tot Ion:264 Resp: 1279647

Ion	Ratio	Lower	Upper
264	100		
260	22.9	18.6	27.8
265	21.4	17.8	26.8

