

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102318\
 Data File : BM017296.D
 Acq On : 23 Oct 2018 22:05
 Operator : MJ/SJ
 Sample : J5606-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Oct 24 06:58:31 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM101718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 17 14:23:17 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	256358	20.00	ng	-0.02
21) Naphthalene-d8	10.43	136	984108	20.00	ng	-0.02
39) Acenaphthene-d10	14.30	164	560051	20.00	ng	-0.02
64) Phenanthrene-d10	17.05	188	1356100	20.00	ng	-0.02
76) Chrysene-d12	21.24	240	1558803	20.00	ng	-0.02
87) Perylene-d12	23.46	264	1389976	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.28	112	1419105	93.63	ng	-0.01
7) Phenol-d6	6.84	99	1709966	82.83	ng	-0.02
23) Nitrobenzene-d5	8.81	82	1314630	78.13	ng	-0.02
42) 2,4,6-Tribromophenol	15.80	330	922566	121.81	ng	-0.02
45) 2-Fluorobiphenyl	12.92	172	3094715	73.52	ng	-0.02
79) Terphenyl-d14	19.69	244	5369561	77.64	ng	-0.01
Target Compounds						
48) 2-Nitroaniline	13.32	65	109	5.697	ng	# 5
80) Butylbenzylphthalate	20.39	149	636	7.192	ng	# 81
84) Bis(2-ethylhexyl)phthalate	21.17	149	13277	5.541	ng	# 94
85) Di-n-octyl phthalate	22.05	149	3139	5.604	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102318\
Data File : BM017296.D
Acq On : 23 Oct 2018 22:05
Operator : MJ/SJ
Sample : J5606-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Oct 24 06:58:31 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM101718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 17 14:23:17 2018
Response via : Initial Calibration

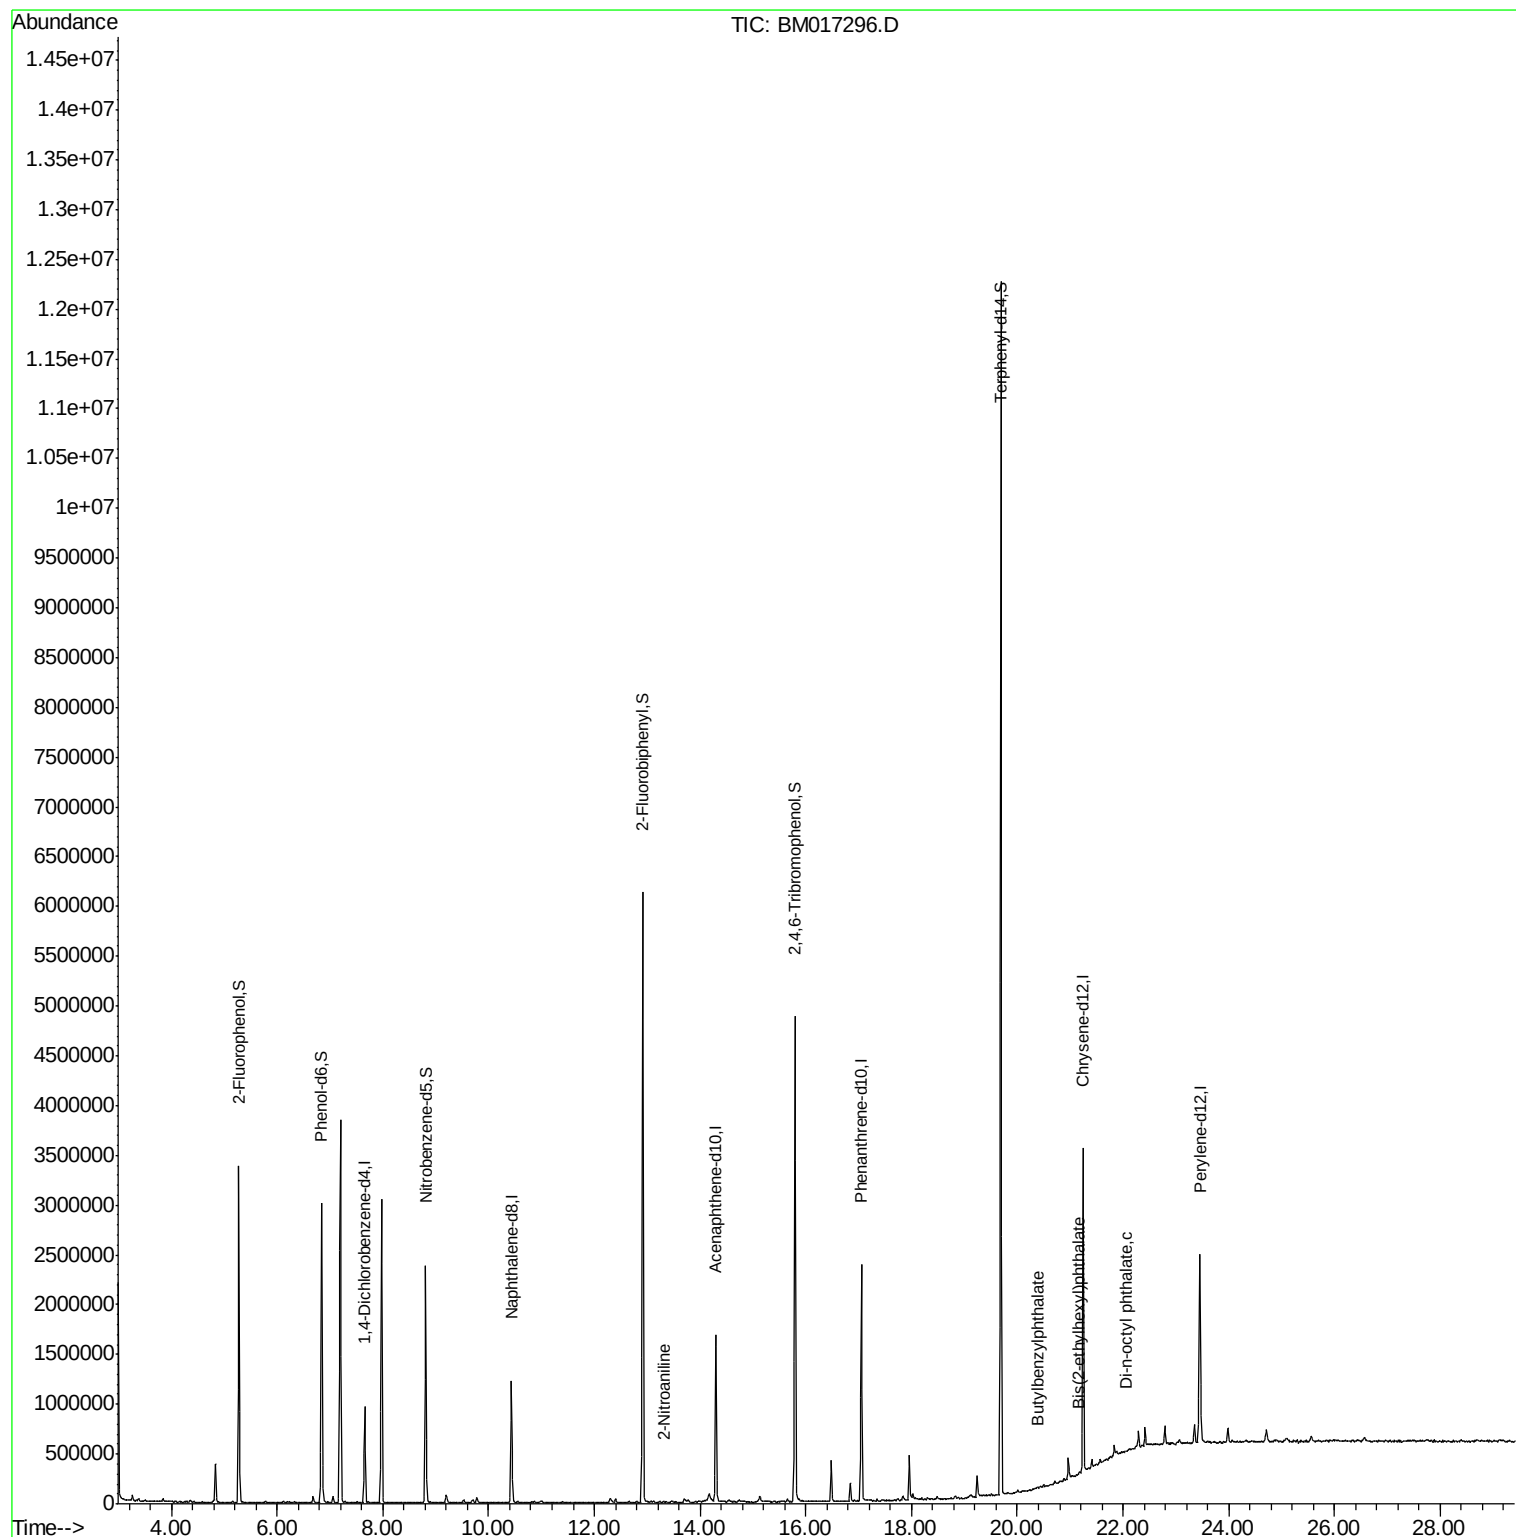

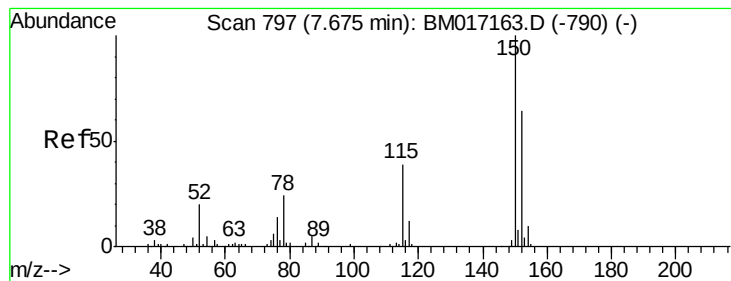


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.66 min Scan# 794
Delta R.T. -0.02 min
Lab File: BM017296.D
Acq: 23 Oct 2018 22:05

Instrument :
BNA_M
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	152.8	124.3	186.5
115	59.4	48.1	72.1



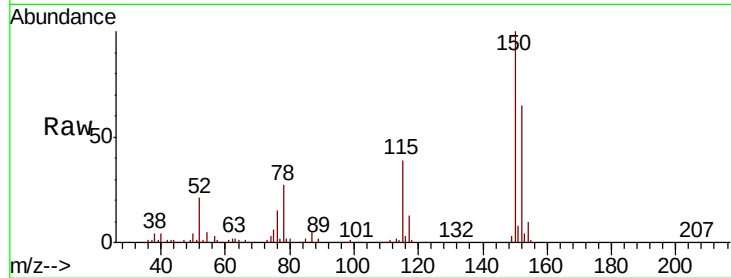


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

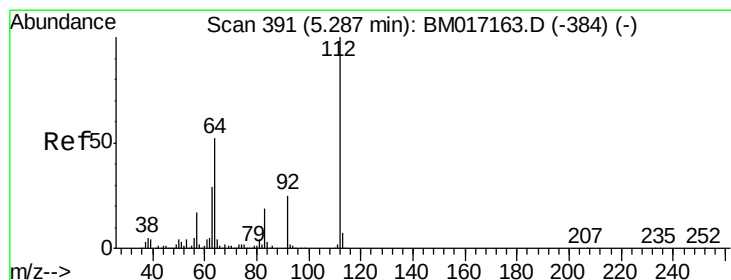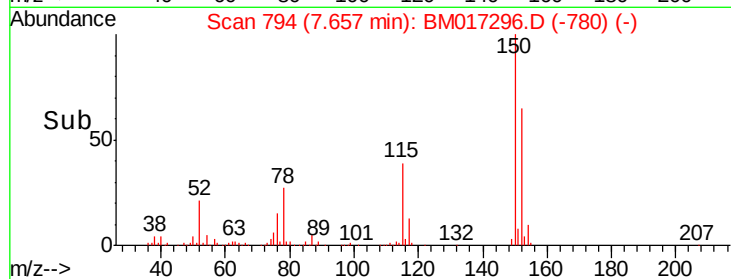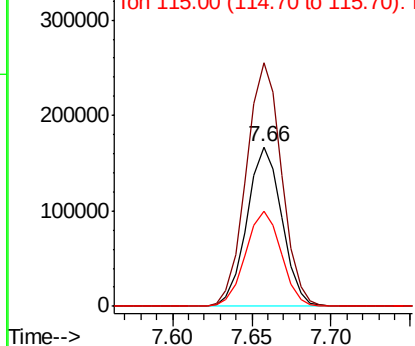

#5

2-Fluorophenol
Concen: 93.626 ng
RT: 5.28 min Scan# 389
Delta R.T. -0.01 min
Lab File: BM017296.D
Acq: 23 Oct 2018 22:05

Tgt Ion	Ratio	Lower	Upper
112	100		
64	59.3	41.7	62.5
63	30.6	23.0	34.4


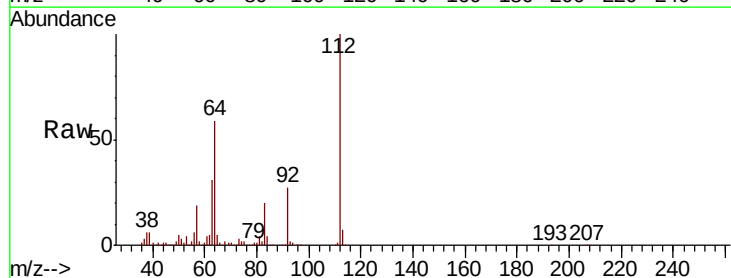



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 63.00 (62.70 to 63.70): BM0

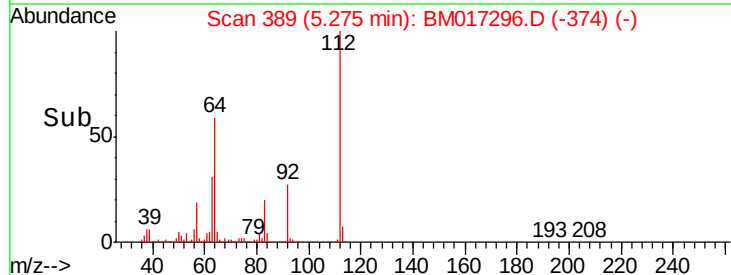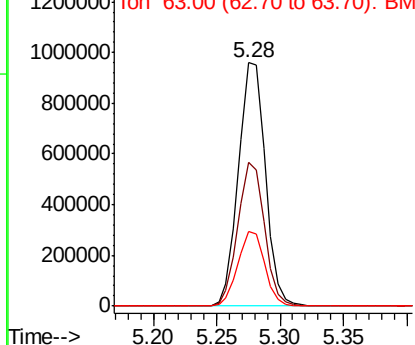

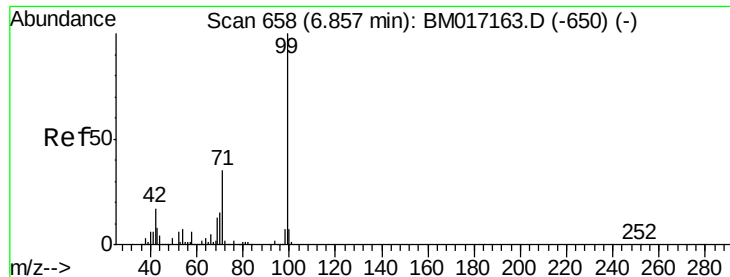

#7

Phenol-d6

Concen: 82.834 ng

RT: 6.84 min Scan# 655

Delta R.T. -0.02 min

Lab File: BM017296.D

Acq: 23 Oct 2018 22:05

Instrument :

BNA_M

ClientSampled :


Tot Ion: 99 Resp: 1709966

Ion Ratio Lower Upper

99 100

42 18.1 13.3 19.9




71 36.1 28.0 42.0

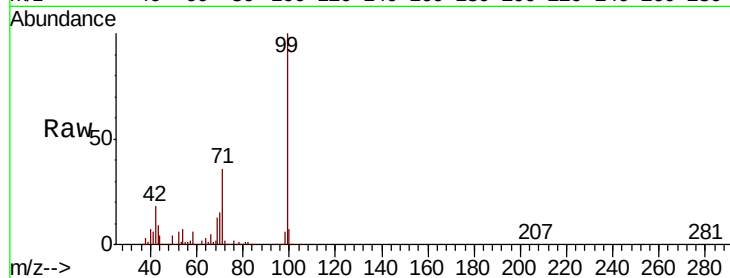

Abundance Ion 99.00 (98.70 to 99.70): BM017163.D (-650) (-)

Ion 42.00 (41.70 to 42.70): BM017163.D (-650) (-)

Ion 71.00 (70.70 to 71.70): BM017163.D (-650) (-)

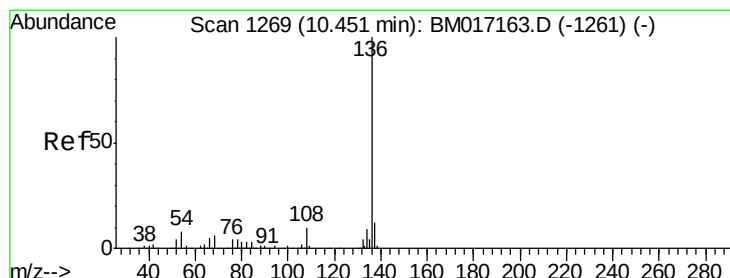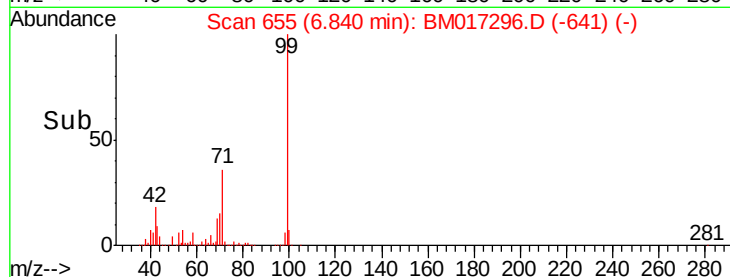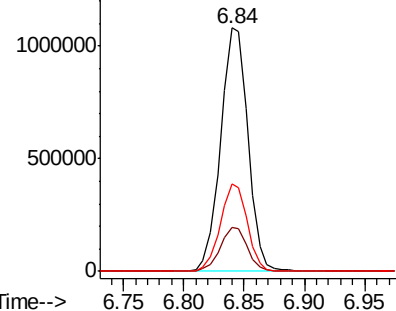

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.43 min Scan# 1266

Delta R.T. -0.02 min

Lab File: BM017296.D

Acq: 23 Oct 2018 22:05

Tgt Ion: 136 Resp: 984108


Ion Ratio Lower Upper

136 100

137 10.8 9.2 13.8

54 7.7 6.7 10.1

68 5.5 4.7 7.1


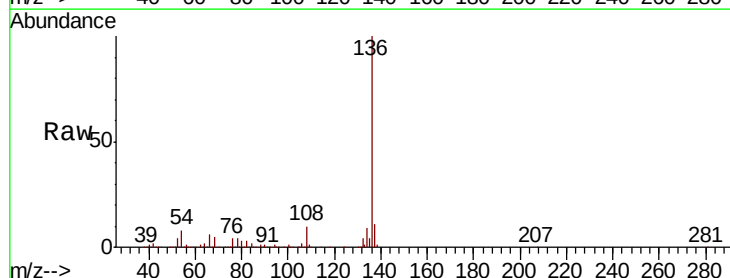



Abundance Ion 136.00 (135.70 to 136.70): BM017163.D (-1261) (-)

Ion 137.00 (136.70 to 137.70): BM017163.D (-1261) (-)

Ion 54.00 (53.70 to 54.70): BM017163.D (-1261) (-)

Ion 68.00 (67.70 to 68.70): BM017163.D (-1261) (-)

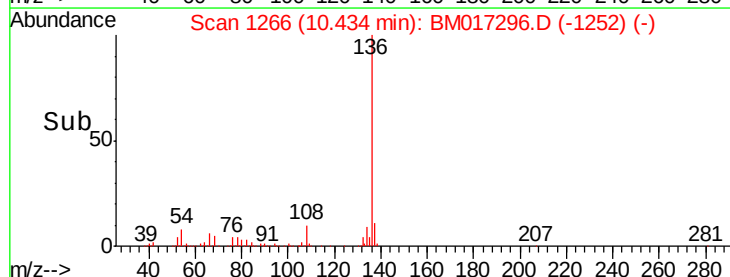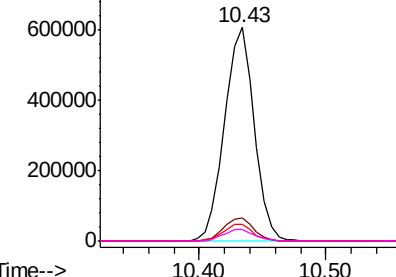




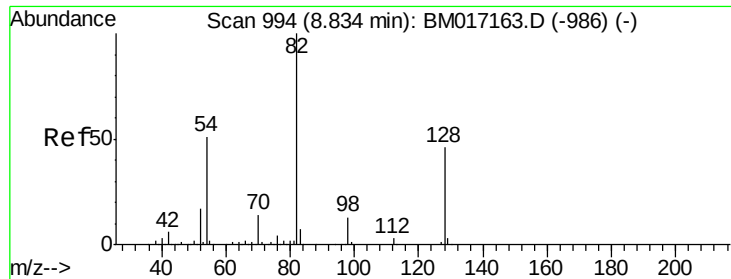


#23
 Nitrobenzene-d5
 Concen: 78.129 ng
 RT: 8.81 min Scan# 990
 Delta R.T. -0.02 min
 Lab File: BM017296.D
 Acq: 23 Oct 2018 22:05

Instrument :
 BNA_M
 ClientSampled :

Tot Ion: 82 Resp: 1314630




Ion	Ratio	Lower	Upper
82	100		
128	43.7	37.0	55.6
54	50.4	40.7	61.1

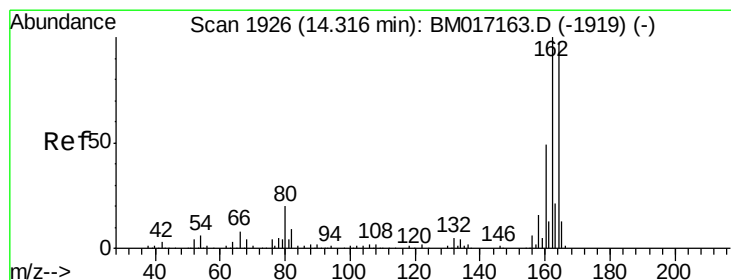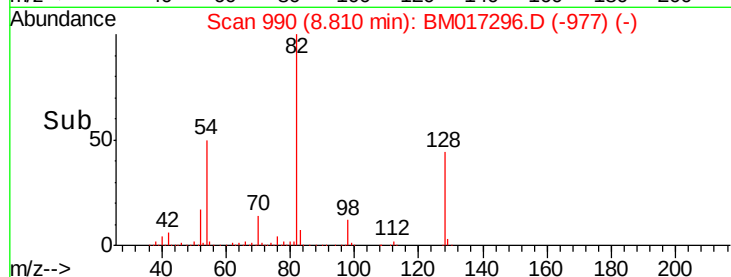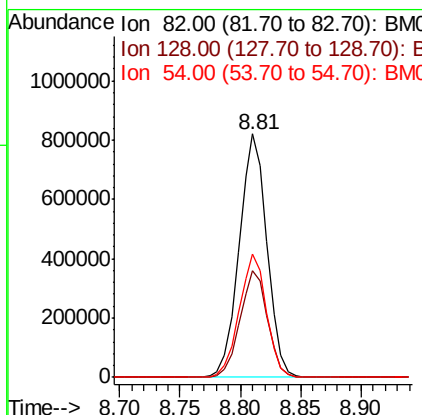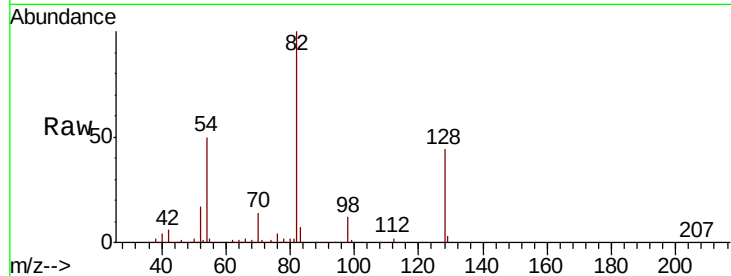


#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.30 min Scan# 1923
 Delta R.T. -0.02 min
 Lab File: BM017296.D
 Acq: 23 Oct 2018 22:05

Tgt Ion: 164 Resp: 560051

Ion	Ratio	Lower	Upper
164	100		
162	101.8	82.1	123.1
160	44.9	40.2	60.2

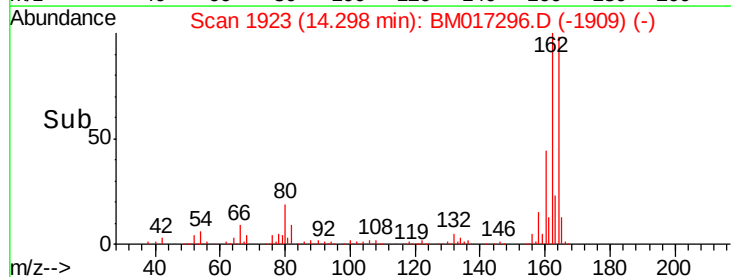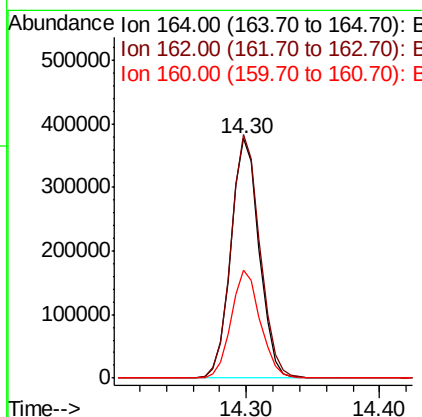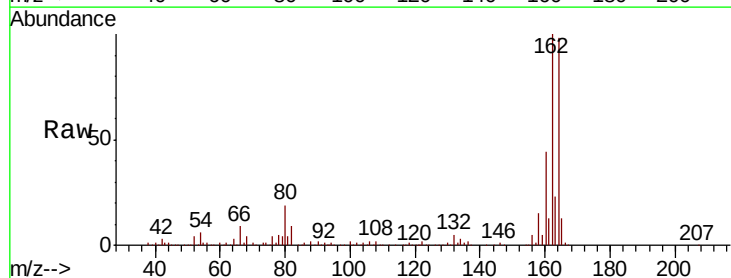

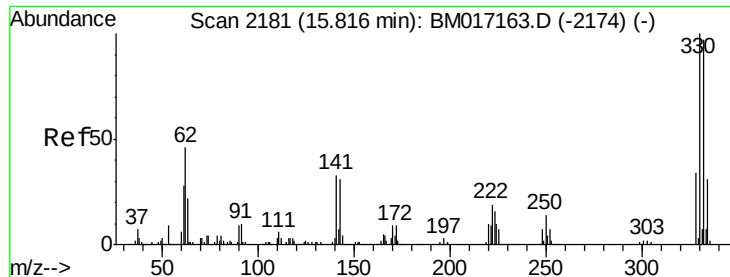

#42

2,4,6-Tribromophenol

Concen: 121.809 ng

RT: 15.80 min Scan# 2178

Delta R.T. -0.02 min

Lab File: BM017296.D

Acq: 23 Oct 2018 22:05

Instrument :

BNA_M

ClientSampleId :


Tot Ion:330 Resp: 922566

Ion Ratio Lower Upper

330 100

332 95.8 77.3 115.9

141 33.3 27.4 41.0



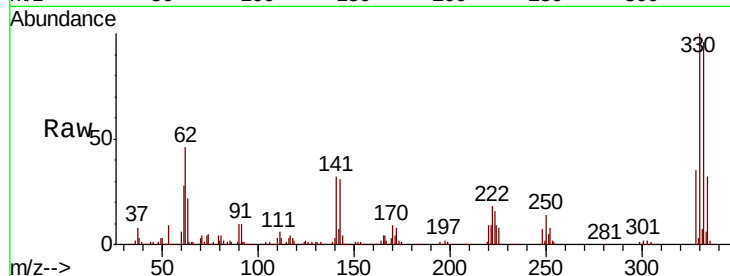


Abundance

Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

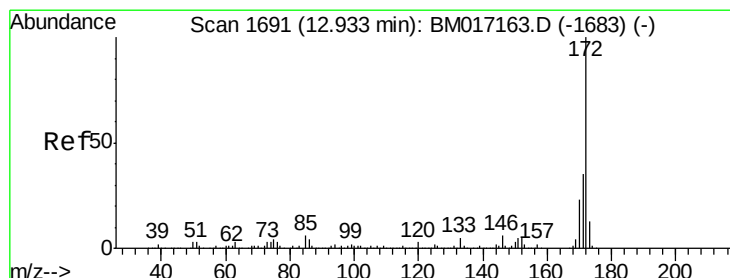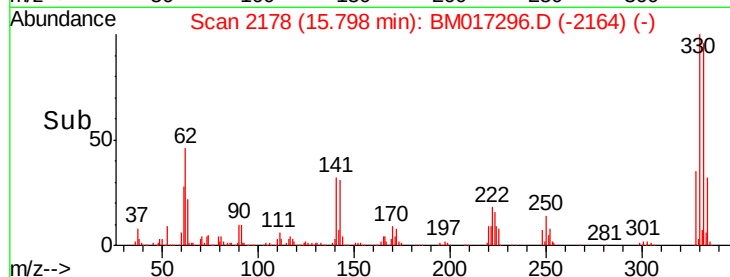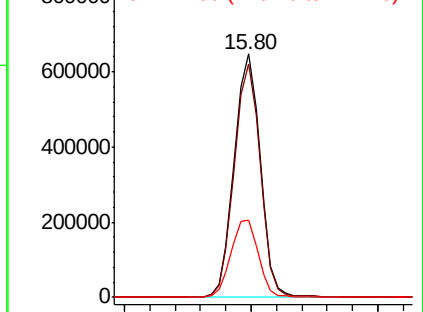

#45

2-Fluorobiphenyl

Concen: 73.523 ng

RT: 12.92 min Scan# 1688

Delta R.T. -0.02 min

Lab File: BM017296.D

Acq: 23 Oct 2018 22:05


Tgt Ion:172 Resp: 3094715

Ion Ratio Lower Upper

172 100

171 35.0 28.3 42.5

170 22.5 18.3 27.5


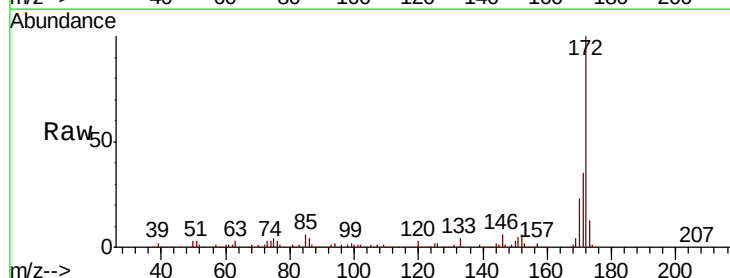



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

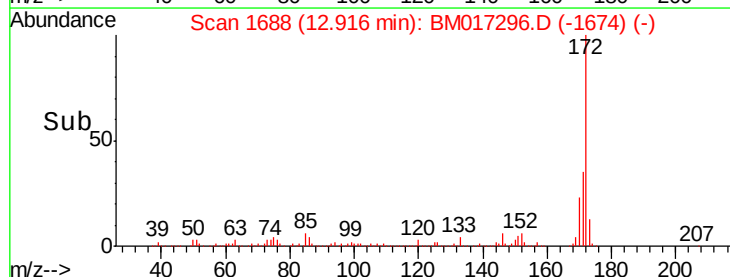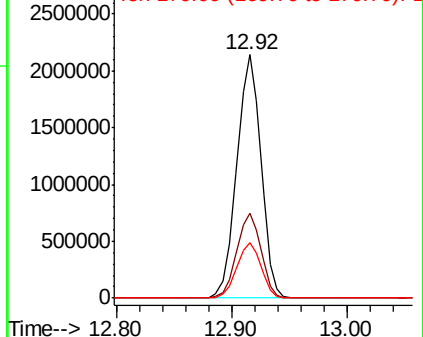


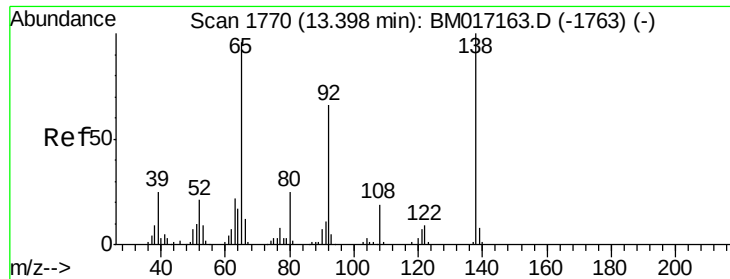




#48
 2-Nitroaniline
 Concen: 5.697 ng
 RT: 13.32 min Scan# 1756
 Delta R.T. -0.08 min
 Lab File: BM017296.D
 Acq: 23 Oct 2018 22:05

Instrument :
 BNA_M
 ClientSampled :

Tot Ion: 65 Resp: 109
 Ion Ratio Lower Upper
 65 100
 92 0.0 54.9 82.3#
 138 0.0 83.7 125.5#

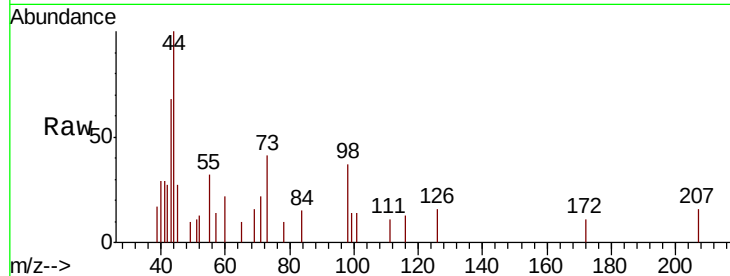


Abundance Ion 65.00 (64.70 to 65.70): BM0
 Ion 92.00 (91.70 to 92.70): BM0
 Ion 138.00 (137.70 to 138.70): E

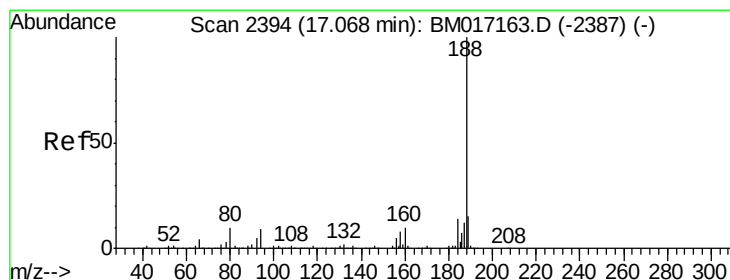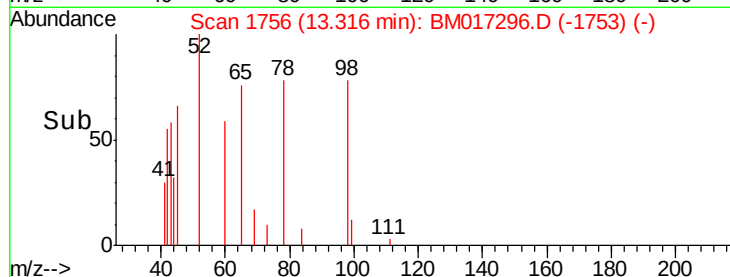
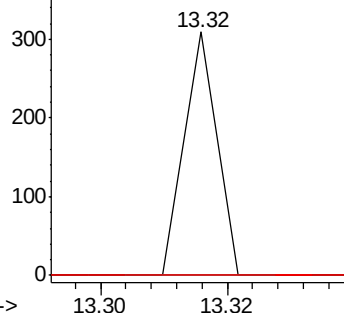



#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.05 min Scan# 2391
 Delta R.T. -0.02 min
 Lab File: BM017296.D
 Acq: 23 Oct 2018 22:05

Tgt Ion:188 Resp: 1356100
 Ion Ratio Lower Upper
 188 100
 94 9.0 7.0 10.4
 80 9.7 7.7 11.5

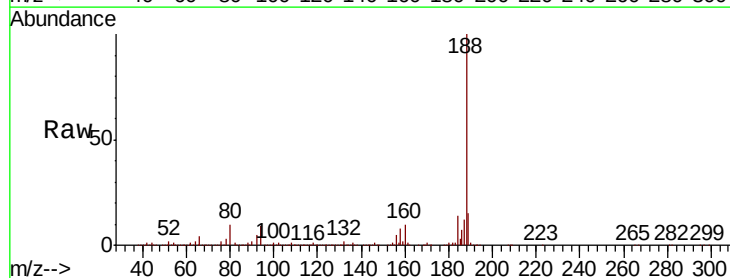

Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BM0
 Ion 80.00 (79.70 to 80.70): BM0

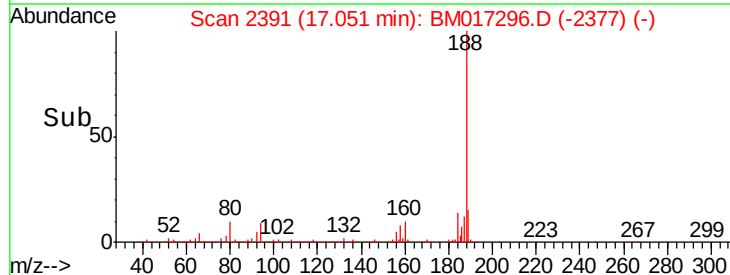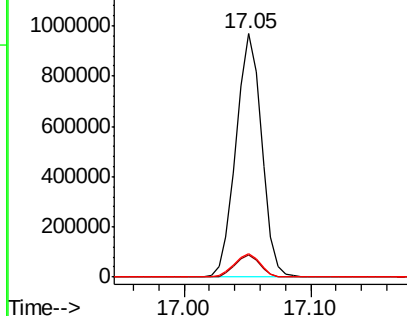

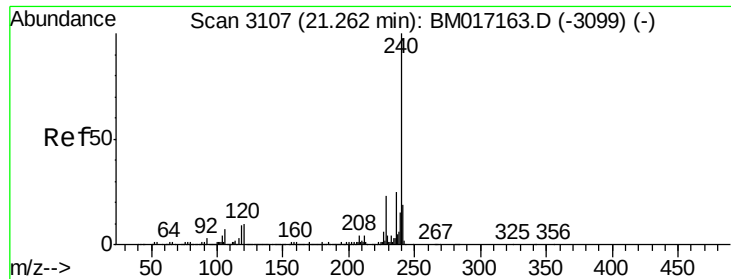

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.24 min Scan# 3104

Delta R.T. -0.02 min

Lab File: BM017296.D

Acq: 23 Oct 2018 22:05

Instrument :

BNA_M

ClientSampleId :


Tot Ion:240 Resp: 1558803

Ion Ratio Lower Upper

240 100

120 10.3 8.1 12.1




236 25.0 19.9 29.9

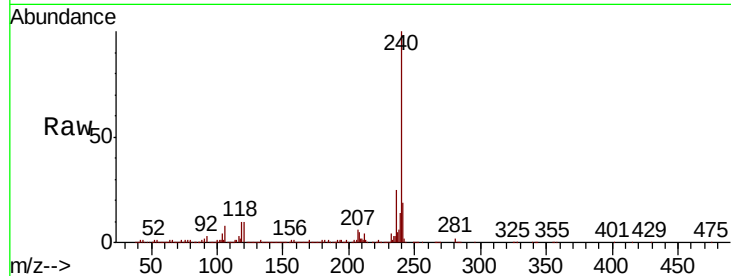

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

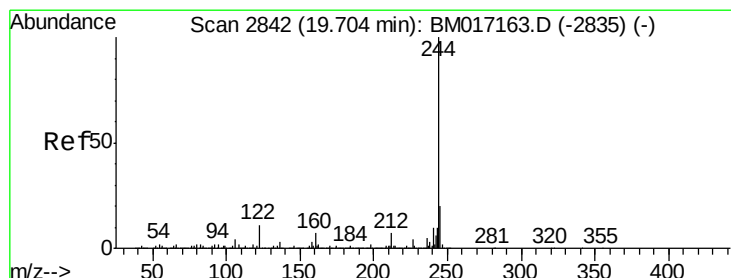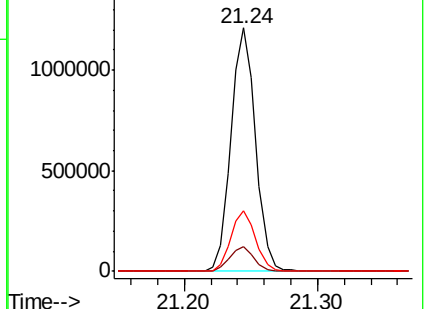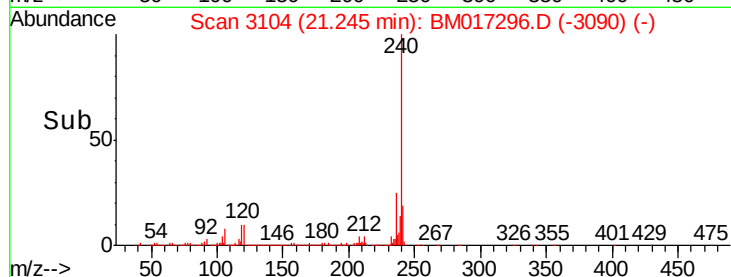

#79

Terphenyl-d14

Concen: 77.643 ng

RT: 19.69 min Scan# 2840

Delta R.T. -0.01 min

Lab File: BM017296.D

Acq: 23 Oct 2018 22:05


Tgt Ion:244 Resp: 5369561

Ion Ratio Lower Upper

244 100

212 7.2 5.5 8.3



122 10.2 8.4 12.6

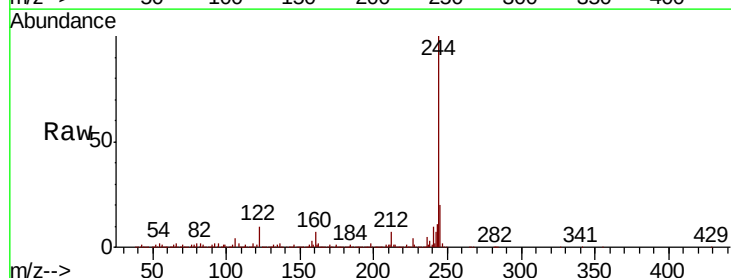


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E



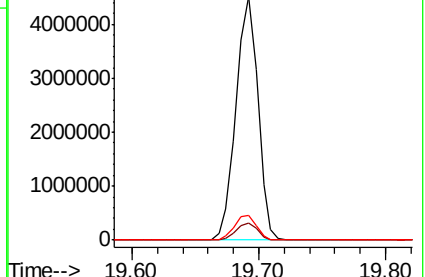
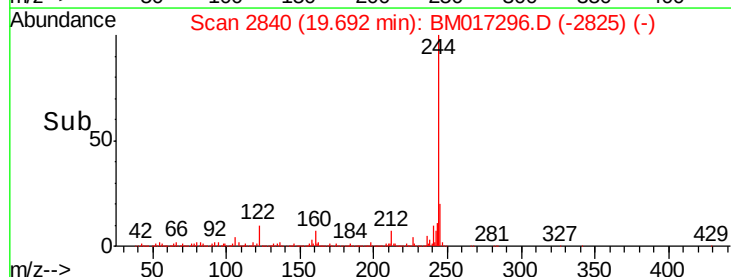


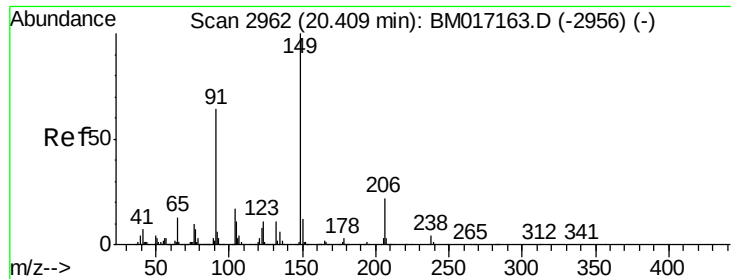

#80
 Butylbenzylphthalate
 Concen: 7.192 ng
 RT: 20.39 min Scan# 2959
 Delta R.T. -0.02 min
 Lab File: BM017296.D
 Acq: 23 Oct 2018 22:05




Instrument :
 BNA_M
 ClientSampled :


Tot Ion:149 Resp: 636
 Ion Ratio Lower Upper
 149 100
 91 71.0 51.3 76.9
 206 0.0 18.0 27.0#

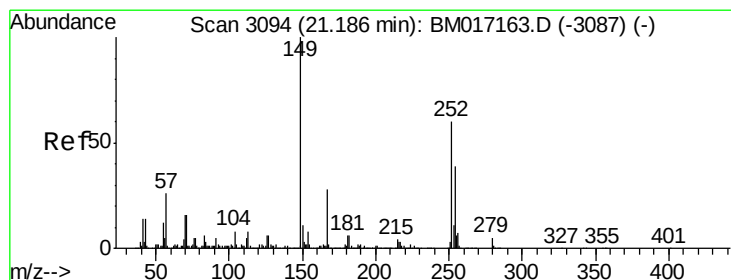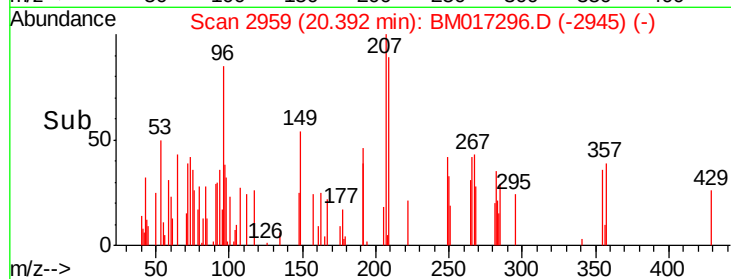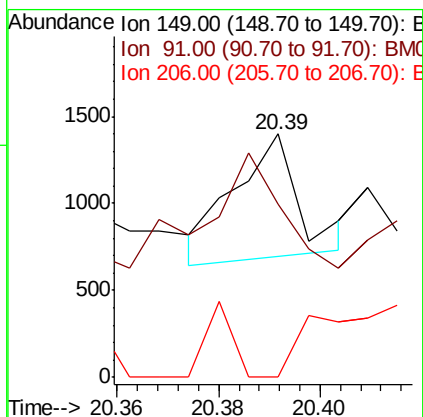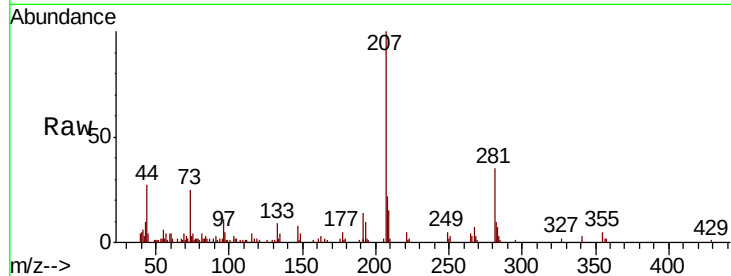

#84
 Bis(2-ethylhexyl)phthalate
 Concen: 5.541 ng
 RT: 21.17 min Scan# 3091
 Delta R.T. -0.02 min
 Lab File: BM017296.D
 Acq: 23 Oct 2018 22:05

Tgt Ion:149 Resp: 13277
 Ion Ratio Lower Upper
 149 100
 167 24.1 22.2 33.4
 279 4.9 3.6 5.4


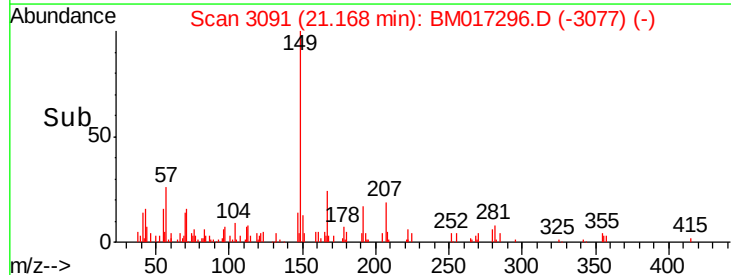
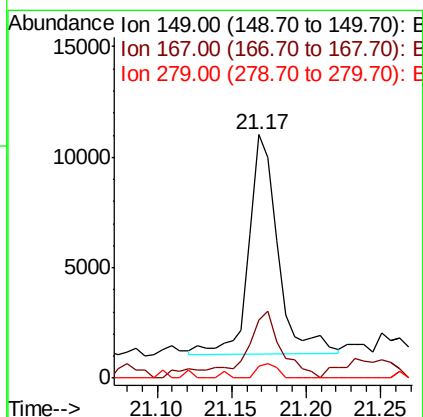
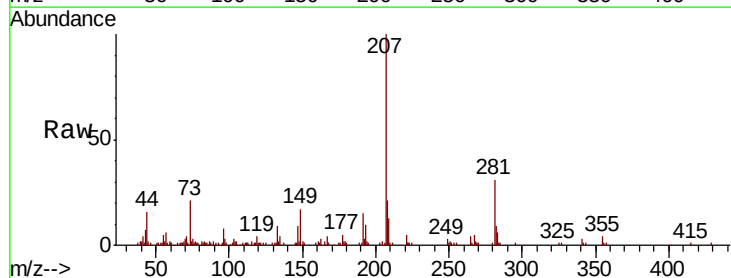


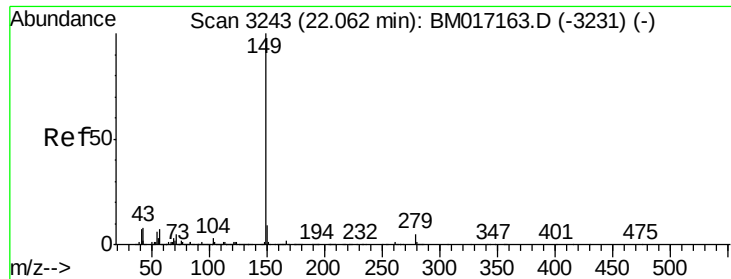

#85
Di-n-octyl phthalate
Concen: 5.604 ng
RT: 22.05 min Scan# 3241
Delta R.T. -0.01 min
Lab File: BM017296.D
Acq: 23 Oct 2018 22:05

Instrument :
BNA_M
ClientSampleId :

Tot Ion:149 Resp: 3139
Ion Ratio Lower Upper
149 100
167 12.5 1.4 2.0#
43 56.7 7.2 10.8#

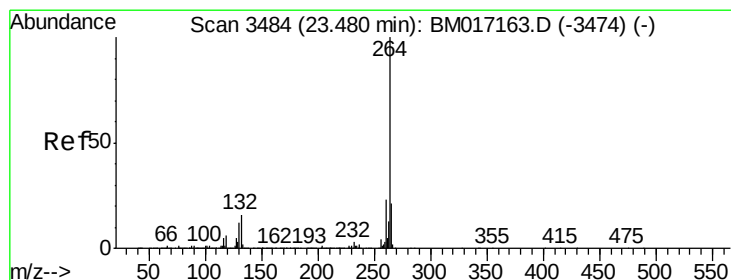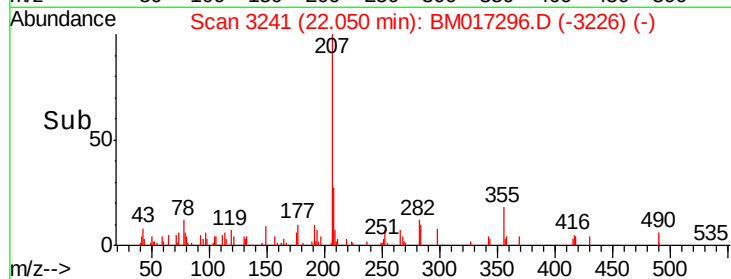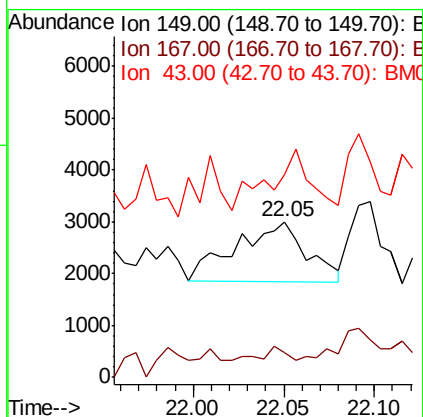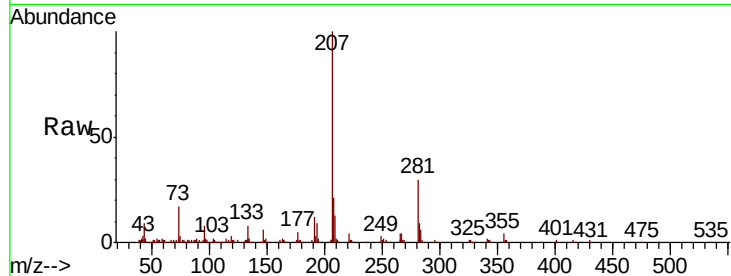

#87
Perylene-d12
Concen: 20.000 ng
RT: 23.46 min Scan# 3480
Delta R.T. -0.02 min
Lab File: BM017296.D
Acq: 23 Oct 2018 22:05

Tgt Ion:264 Resp: 1389976
Ion Ratio Lower Upper
264 100
260 22.8 18.6 27.8
265 21.9 17.8 26.8

