
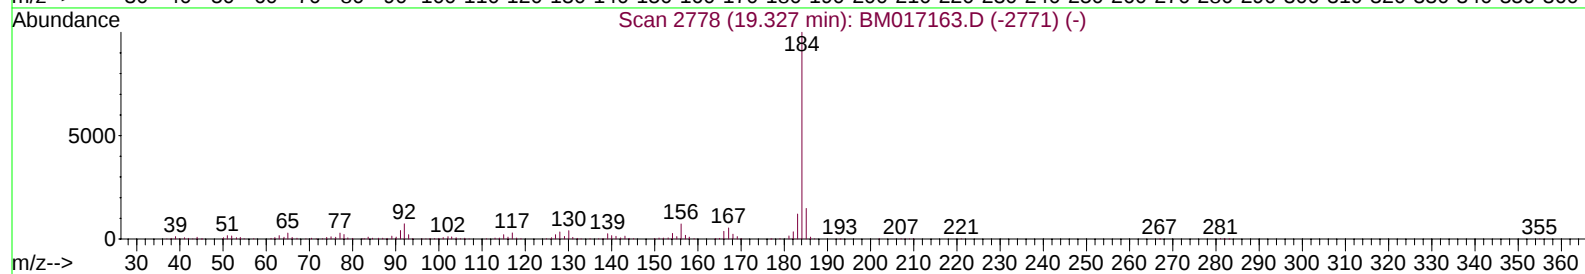
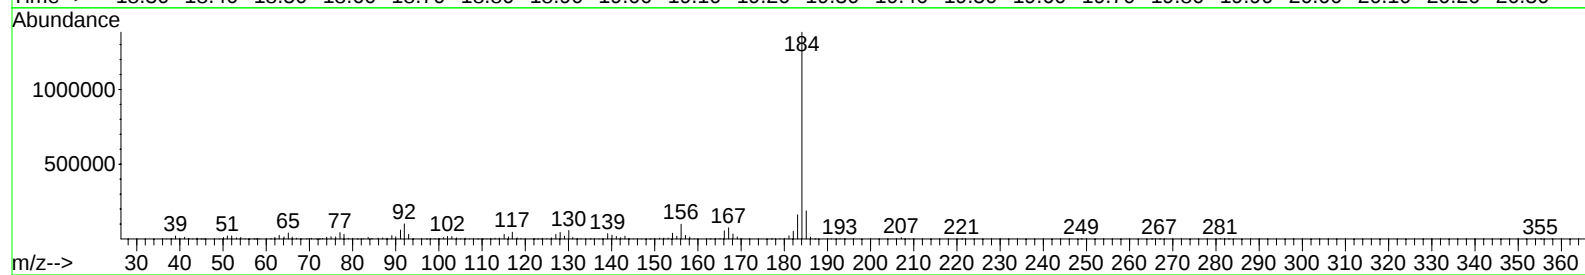


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM102318\
 Data File : BM017284.D
 Acq On : 23 Oct 2018 14:02
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 24 10:15:52 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM101718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 17 14:23:17 2018
 Response via : Initial Calibration

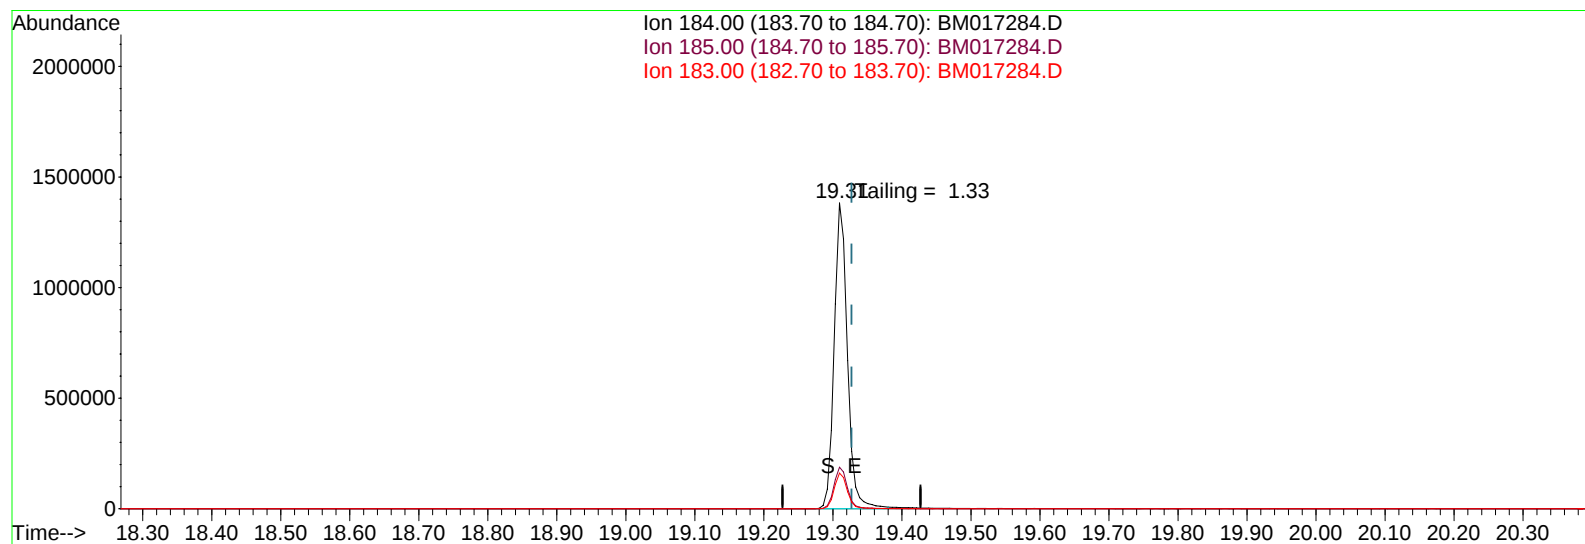

TIC: BM017284.D

(77) Benzidine




19.310min (-0.018) 26612.96ng

response 1832788

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	13.62
183.00	12.10	11.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM102318\
Data File : BM017284.D
Acq On : 23 Oct 2018 14:02
Operator : MJ/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 24 10:15:52 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM101718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 17 14:23:17 2018
Response via : Initial Calibration

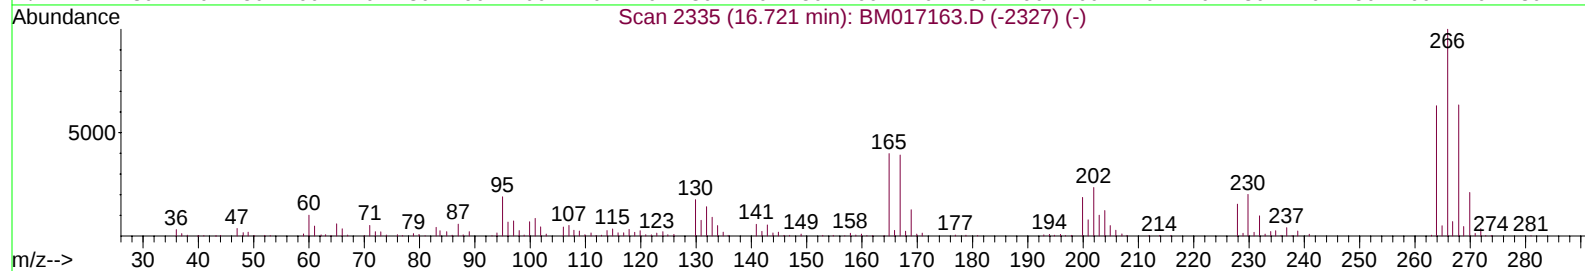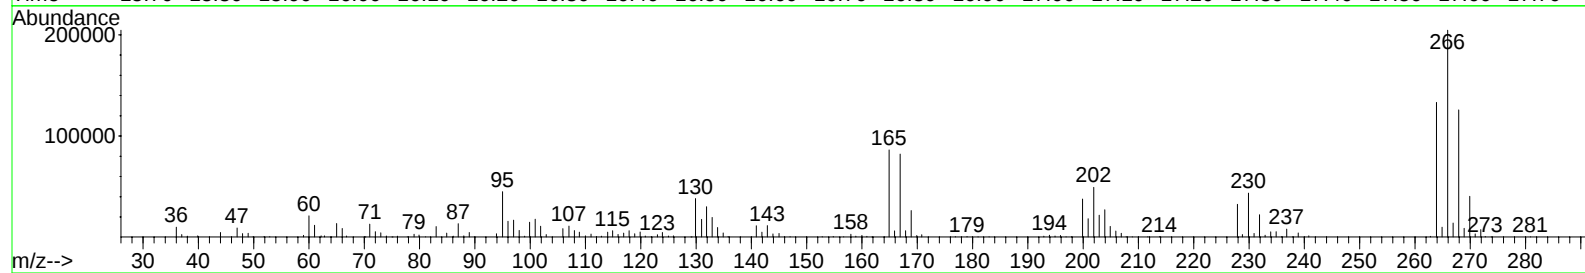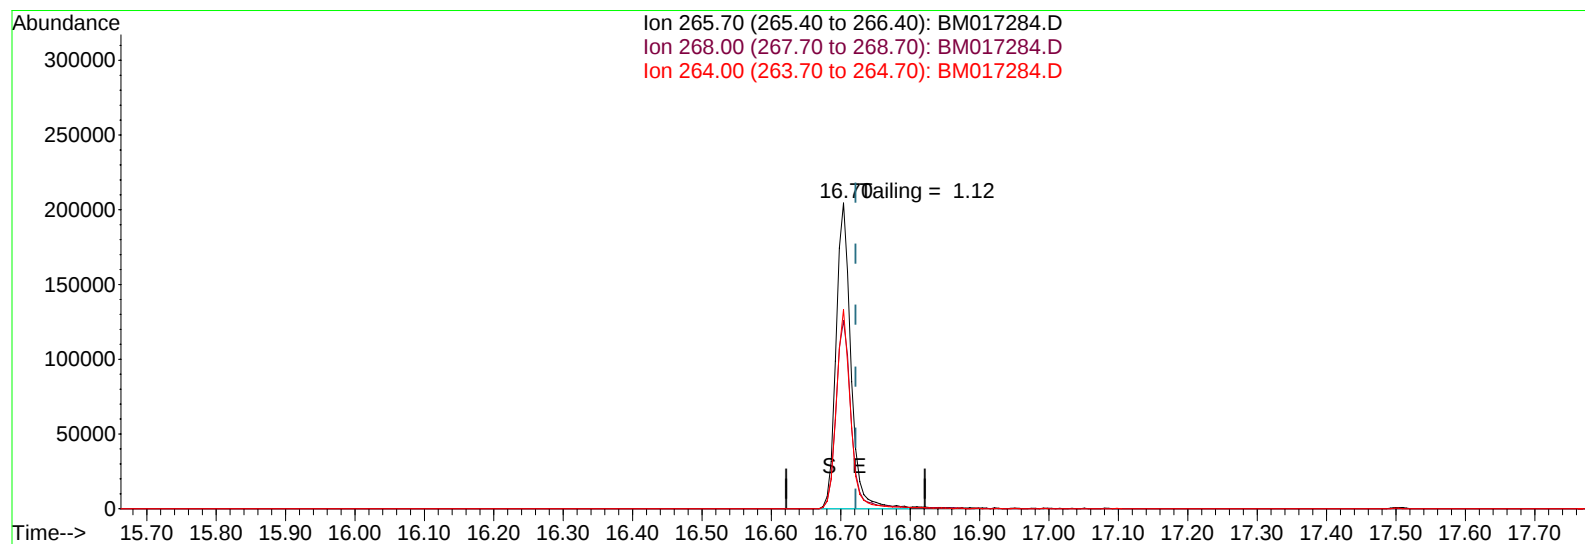

(70) Pentachlorophenol (C)

16.704min (-0.018) 15005.94ng

response 301815

Ion	Exp%	Act%
265.70	100	100
268.00	63.40	61.48
264.00	63.00	65.18
0.00	0.00	0.00