
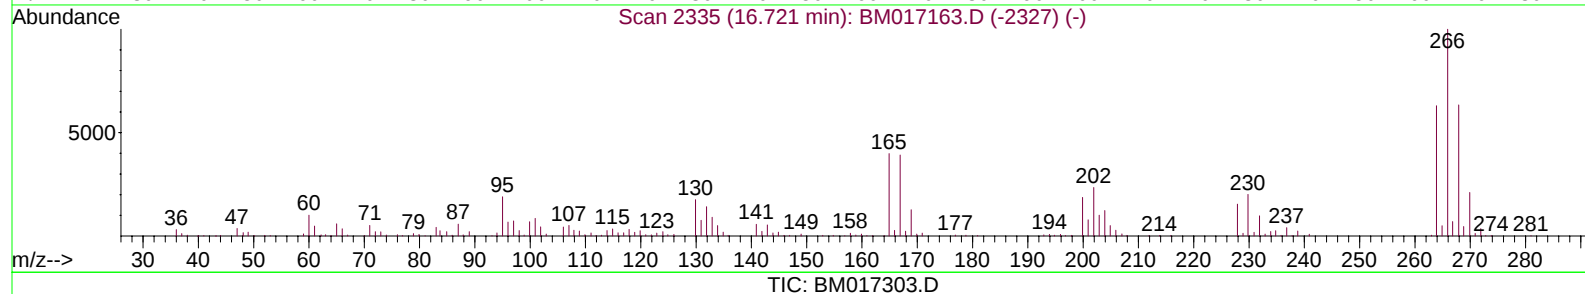
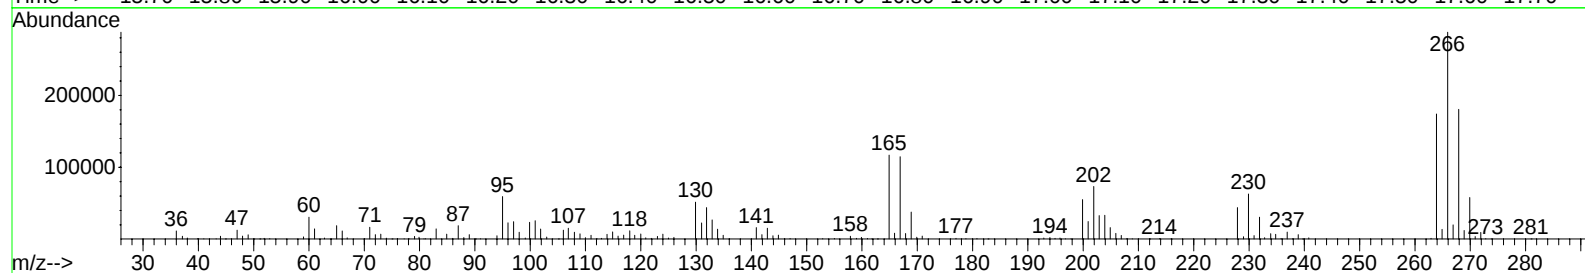


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM102318\
Data File : BM017303.D
Acq On : 24 Oct 2018 05:57
Operator : MJ/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 24 10:24:40 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM101718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 17 14:23:17 2018
Response via : Initial Calibration

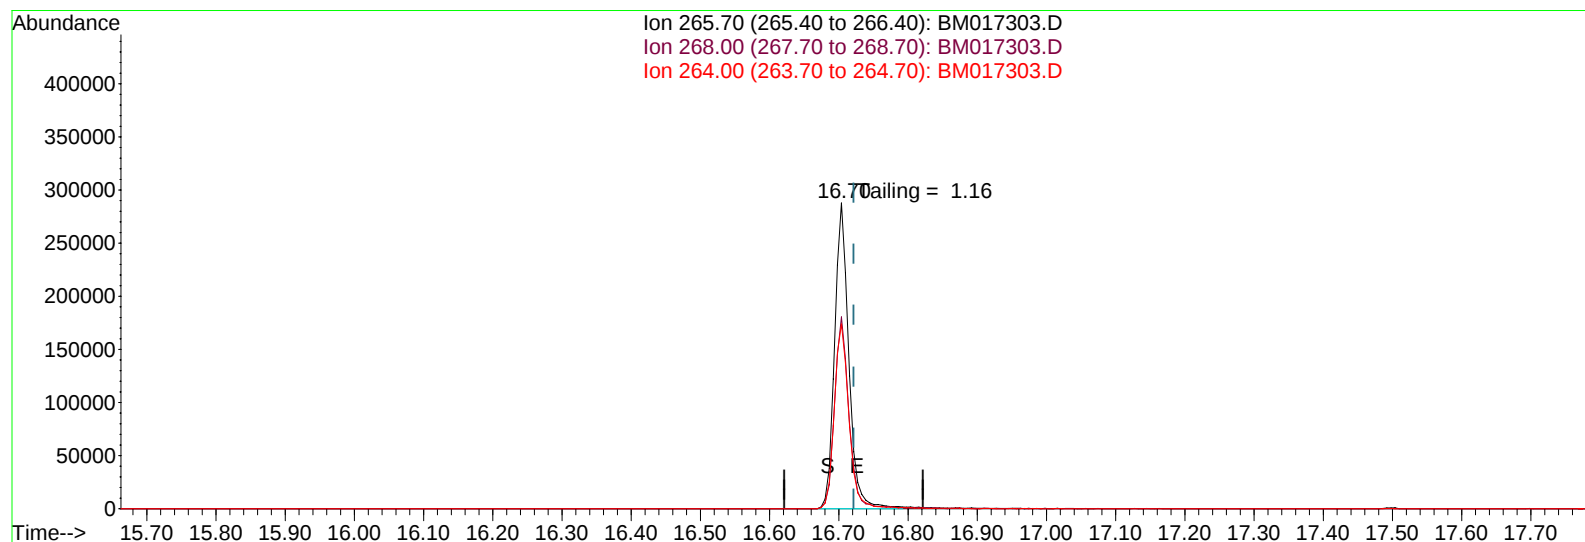

(70) Pentachlorophenol (C)




16.704min (-0.018) 65401.80ng

response 409143

Ion	Exp%	Act%
265.70	100	100
268.00	63.40	62.73
264.00	63.00	60.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM102318\
Data File : BM017303.D
Acq On : 24 Oct 2018 05:57
Operator : MJ/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 24 10:24:40 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM101718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 17 14:23:17 2018
Response via : Initial Calibration

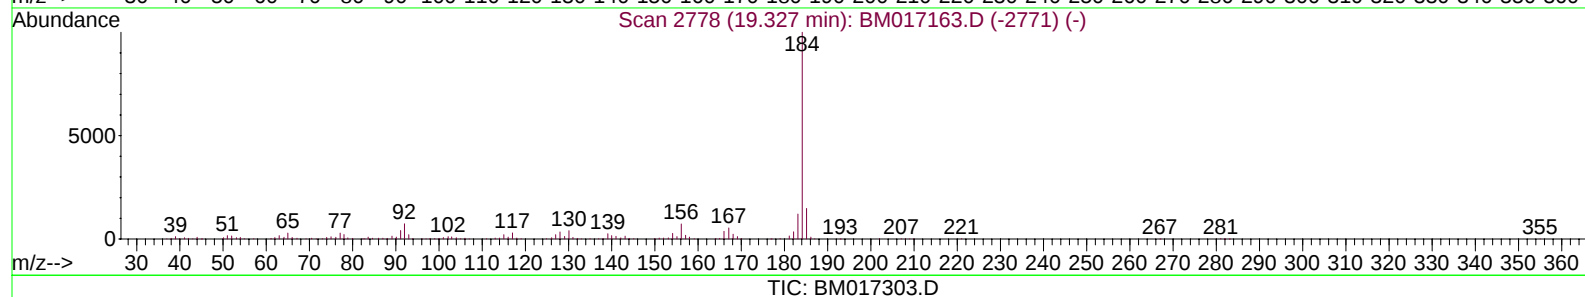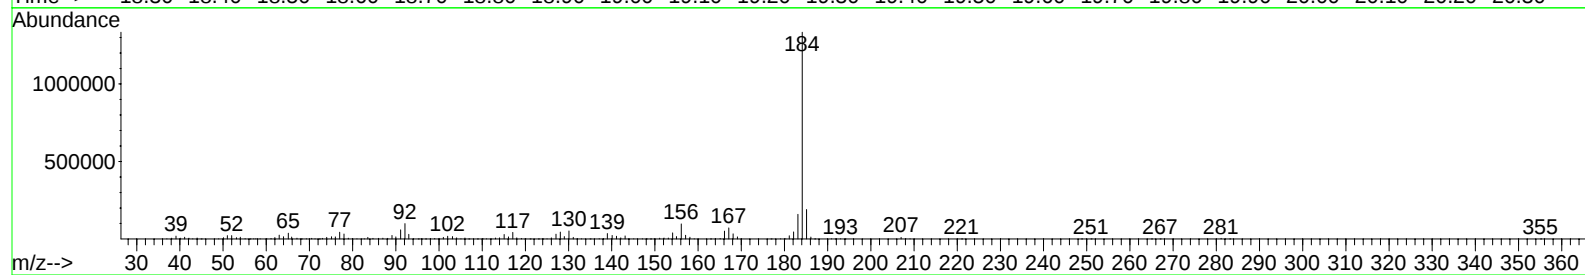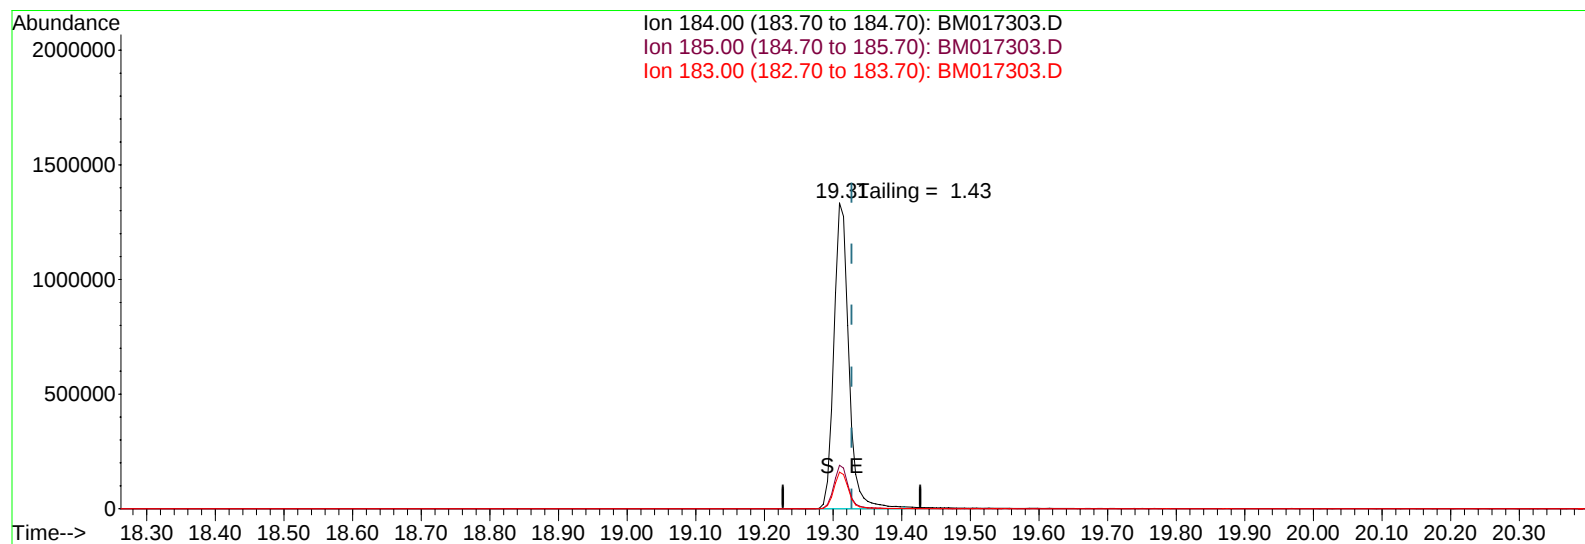

(77) Benzidine

19.309min (-0.018) 25114.03ng

response 2009753

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.24
183.00	12.10	11.97
0.00	0.00	0.00