


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM102318\
Data File : BM017284.D
Acq On : 23 Oct 2018 14:02
Operator : MJ/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM101718.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 17 14:23:17 2018

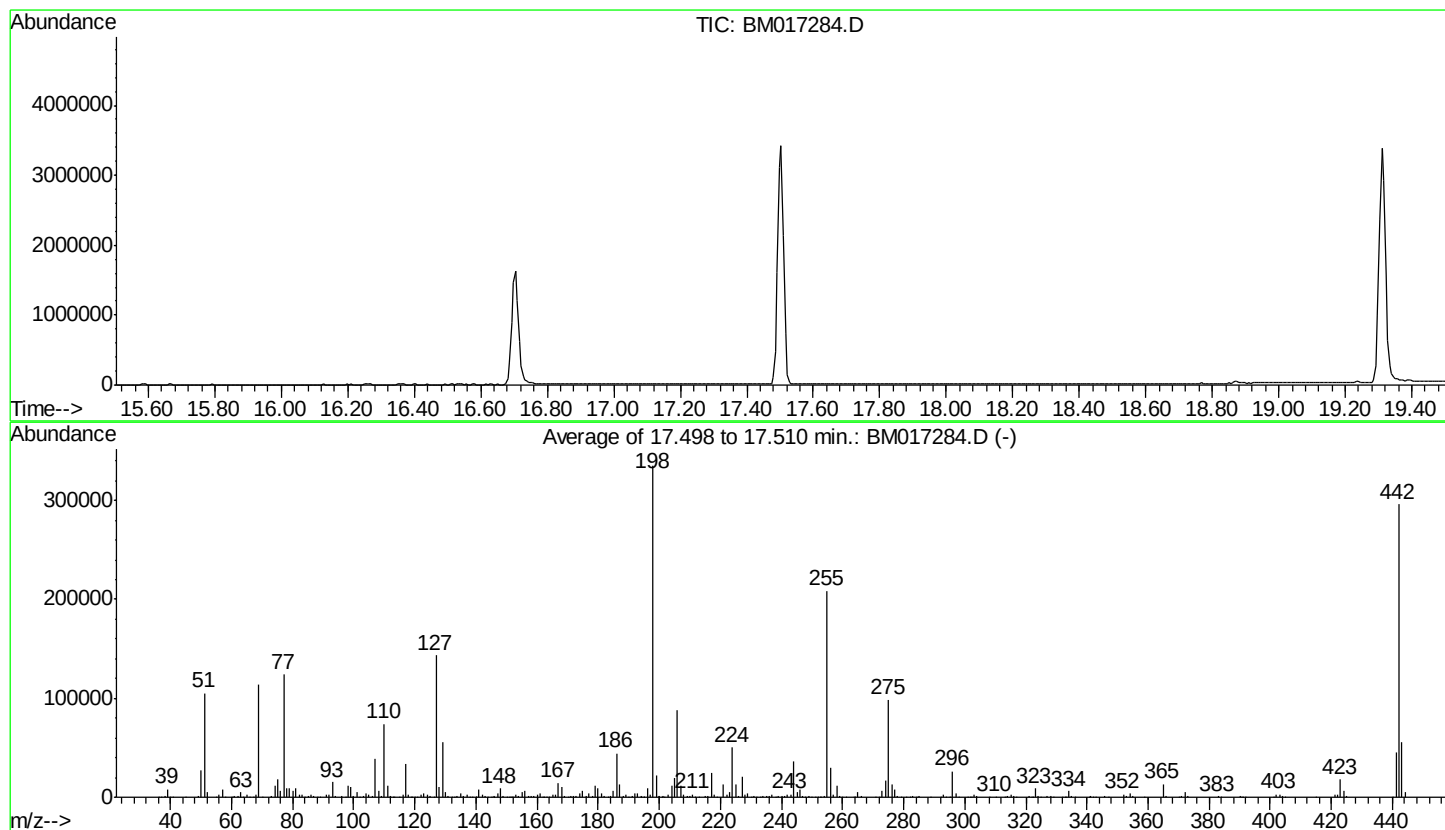

AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.3	104856	PASS
68	69	0.00	2	2.0	2244	PASS
69	198	0.00	100	34.0	113882	PASS
70	69	0.00	2	0.6	639	PASS
127	198	10	80	42.7	143170	PASS
197	198	0.00	2	0.6	2076	PASS
198	198	100	100	100.0	335168	PASS
199	198	5	9	6.8	22642	PASS
275	198	10	60	29.5	98773	PASS
365	198	1	100	3.9	13201	PASS
441	198	0.01	100	13.4	45026	PASS
442	198	50	100	88.4	296213	PASS
443	442	15	24	18.7	55258	PASS