


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM102318\
 Data File : BM017303.D
 Acq On : 24 Oct 2018 05:57
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM101718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 17 14:23:17 2018

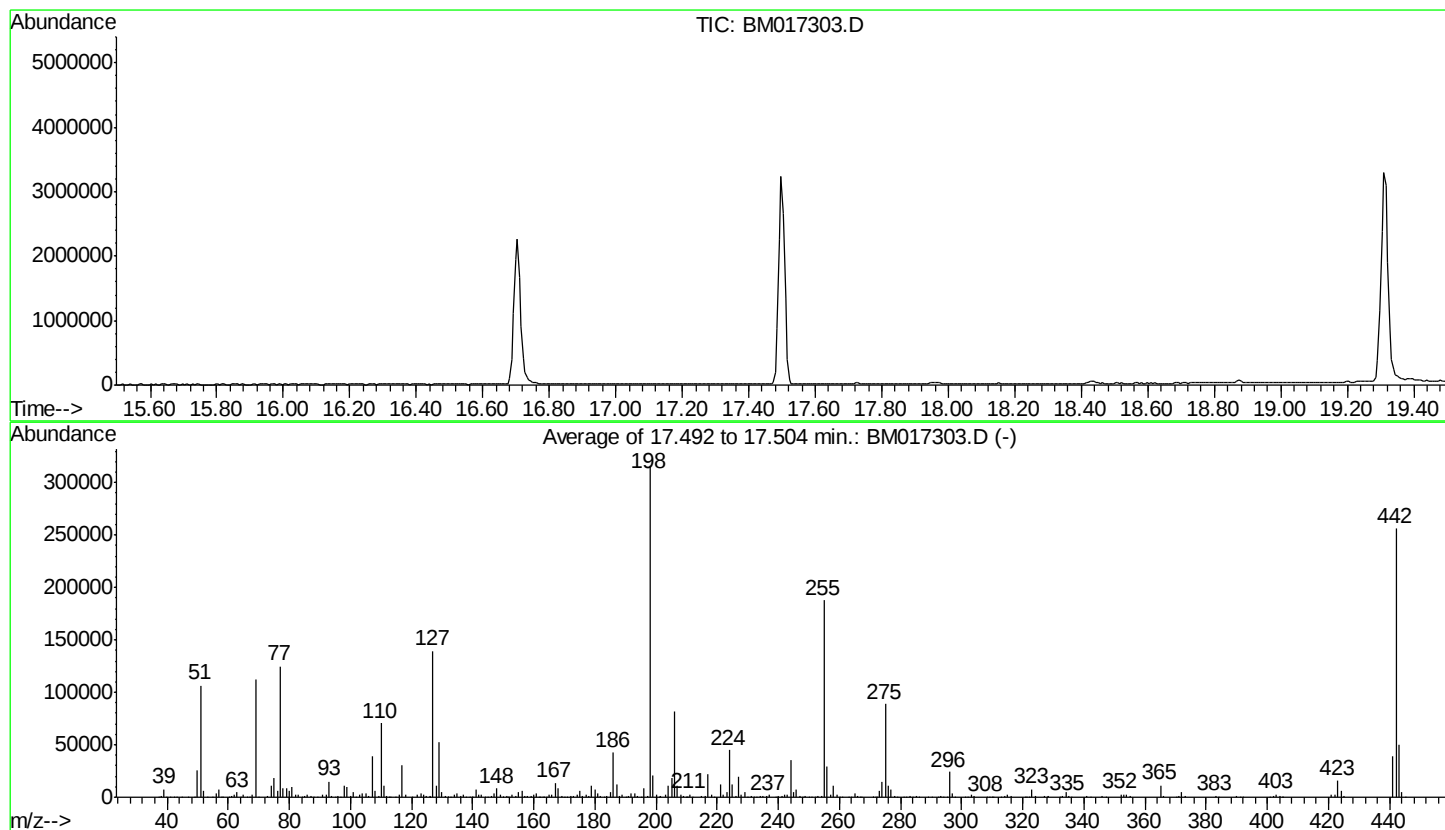

AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	106216	PASS
68	69	0.00	2	1.9	2176	PASS
69	198	0.00	100	35.5	112421	PASS
70	69	0.00	2	0.6	624	PASS
127	198	10	80	44.1	139552	PASS
197	198	0.00	2	0.6	1836	PASS
198	198	100	100	100.0	316245	PASS
199	198	5	9	6.5	20653	PASS
275	198	10	60	28.2	89042	PASS
365	198	1	100	3.6	11282	PASS
441	198	0.01	100	12.3	38888	PASS
442	198	50	100	81.0	256085	PASS
443	442	15	24	19.5	49885	PASS