

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102319\
 Data File : BM023350.D
 Acq On : 23 Oct 2019 20:11
 Operator : JU
 Sample : K5346-07
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Oct 24 02:58:10 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 23 18:47:16 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	613155	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	2803918	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	1761143	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	3333515	20.00	ng/ul	0.00
78) Chrysene-d12	21.23	240	2302032	20.00	ng/ul	0.00
86) Perylene-d12	23.43	264	2572054	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.16	96	53160	4.12	ng/uL	0.00
5) Phenol-d5	6.82	99	1138880	22.12	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	793194	26.28	ng/ul	0.00
9) 2-Chlorophenol-d4	7.17	132	992451	24.65	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	831030	19.87	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	551837	26.14	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	611471	26.11	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	1122194	24.38	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	851235	16.08	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	3763225	28.14	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	4239404	27.67	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	270384	11.67	ng/ul	0.00
58) Fluorene-d10	15.28	176	3164633	27.94	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	352445	16.98	ng/ul	0.00
71) Anthracene-d10	17.13	188	4611942	29.28	ng/ul	0.00
79) Pyrene-d10	19.43	212	4198885	33.17	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.30	264	3724270	28.42	ng/ul	0.01

Target Compounds

					Ovalue
6) Phenol	6.84	94	200653	3.784	ng/ul 99
28) Naphthalene	10.47	128	1462349	10.175	ng/ul 100
34) 2-Methylnaphthalene	12.09	142	212152	1.933	ng/ul 97
45) Dimethylphthalate	13.75	163	1255913	9.353	ng/ul 99
48) Acenaphthylene	14.00	152	1279816	8.059	ng/ul 100
50) Acenaphthene	14.35	153	166438	1.490	ng/ul 98
54) Dibenzofuran	14.69	168	286036	1.788	ng/ul 97
59) Fluorene	15.34	166	191324	1.467	ng/ul 96
70) Phenanthrene	17.07	178	1533469	8.232	ng/ul 100
72) Anthracene	17.16	178	2919547	15.468	ng/ul 99
75) Carbazole	17.43	167	268278	1.686	ng/ul 98
77) Fluoranthene	19.10	202	7860774	40.454	ng/ul 99
80) Pyrene	19.46	202	9349601	57.516	ng/ul 98
83) Benzo(a)anthracene	21.21	228	7570996	49.175	ng/ul 95
85) Chrysene	21.26	228	12223142	86.044	ng/ul 97
88) Benzo(b)fluoranthene	22.78	252	21879767	132.450	ng/ul 93
89) Benzo(k)fluoranthene	22.82	252	7061037	45.521	ng/ul 97
91) Benzo(a)pyrene	23.34	252	13355999	89.307	ng/ul 98
92) Indeno(1,2,3-cd)pyrene	25.64	276	10892853	67.269	ng/ul 98
93) Dibenz(a,h)anthracene	25.65	278	2912969	21.334	ng/ul# 86
94) Benzo(a,h,i)perylene	26.32	276	8166472	61.986	ng/ul 99

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102319\
Data File : BM023350.D
Acq On : 23 Oct 2019 20:11
Operator : JU
Sample : K5346-07
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Oct 24 02:58:10 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 23 18:47:16 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#)=qualifier out of range (m)=manual integration (+)=signals summed						

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102319\
Data File : BM023350.D
Acq On : 23 Oct 2019 20:11
Operator : JU
Sample : K5346-07
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Oct 24 02:58:10 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 23 18:47:16 2019
Response via : Initial Calibration

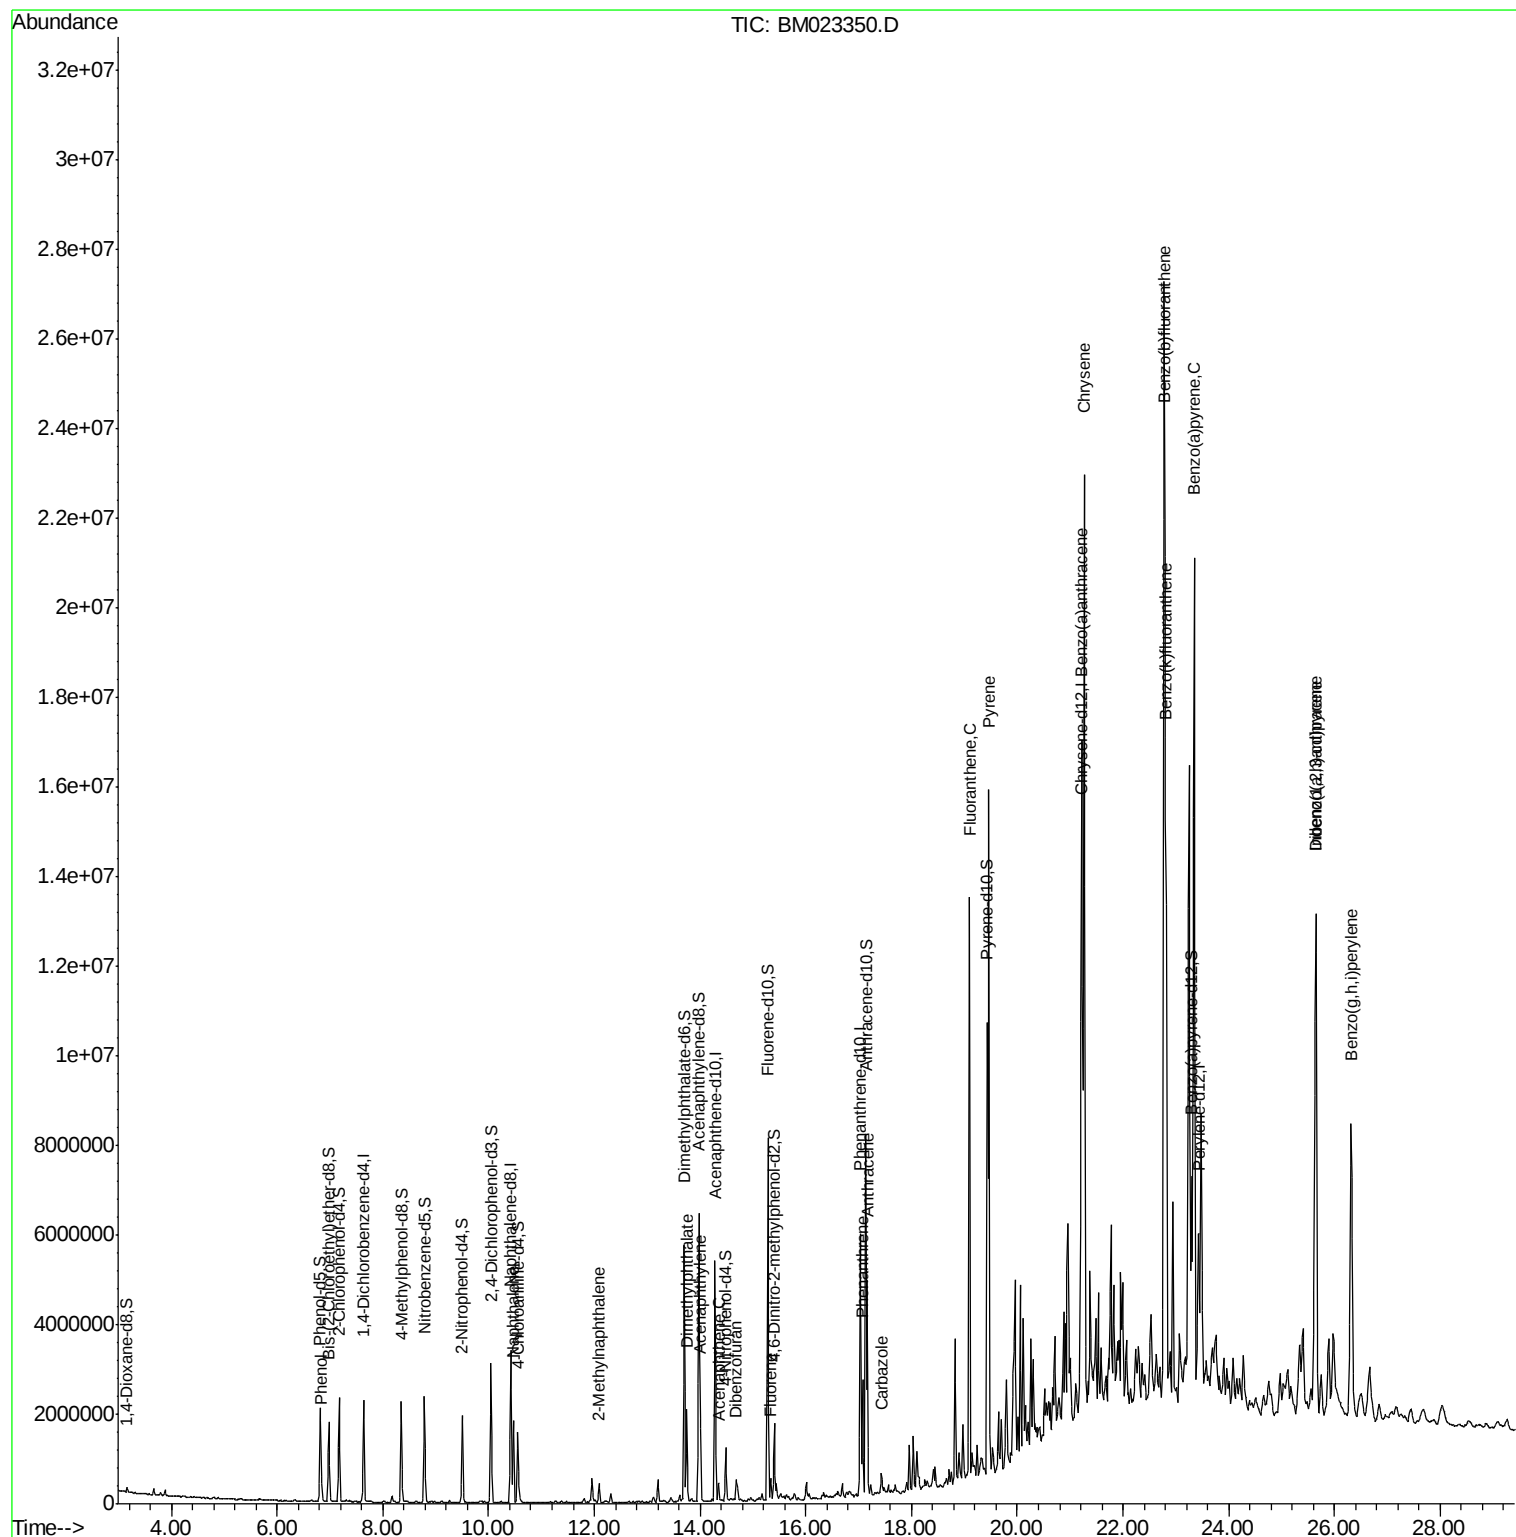

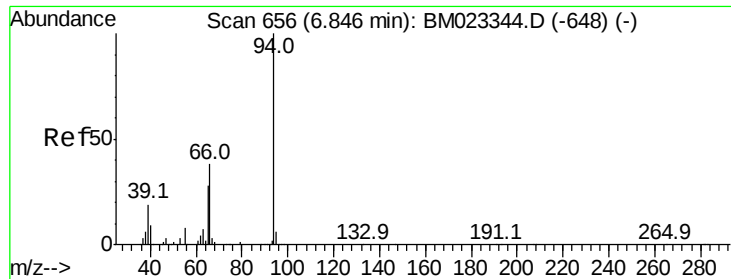





#6

Phenol

Concen: 3.784 ng/ul
 RT: 6.84 min Scan# 655
 Delta R.T. -0.01 min
 Lab File: BM023350.D
 Acq: 23 Oct 2019 20:11

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
94	100		
65	29.4	22.9	34.3
66	40.0	31.4	47.2


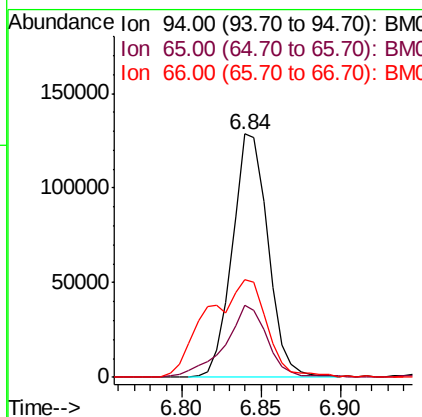
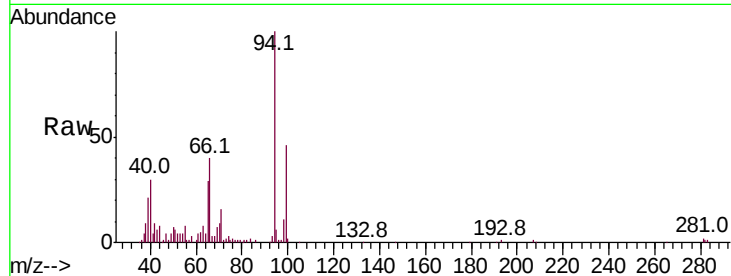



#28

Naphthalene

Concen: 10.175 ng/ul
 RT: 10.47 min Scan# 1272
 Delta R.T. -0.00 min
 Lab File: BM023350.D
 Acq: 23 Oct 2019 20:11

Tgt Ion	Ratio	Lower	Upper
128	100		
129	10.9	8.8	13.2
127	12.9	10.4	15.6

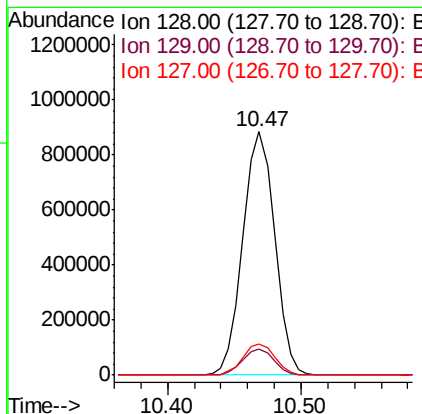

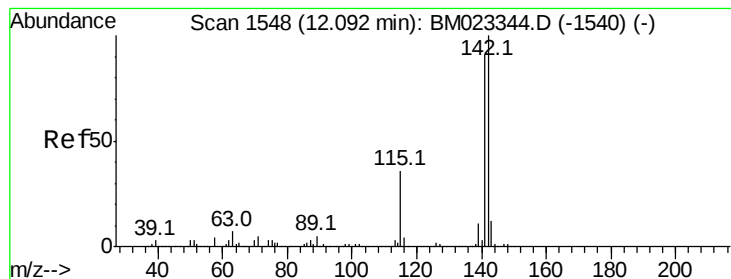

#34

2-Methylnaphthalene

Concen: 1.933 ng/ul

RT: 12.09 min Scan# 1548

Delta R.T. -0.00 min

Lab File: BM023350.D

Acq: 23 Oct 2019 20:11

Instrument :

BNA_M


ClientSampleId :

Tot Ion:142 Resp: 212152

Ion Ratio Lower Upper

142 100

141 87.5 72.4 108.6



Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

12.09



150000

100000

50000

0

Time-->

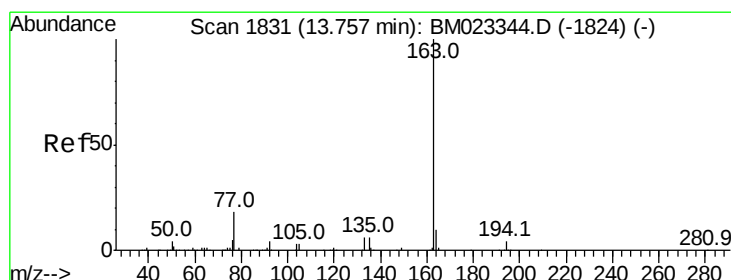

#45

Dimethylphthalate

Concen: 9.353 ng/ul

RT: 13.75 min Scan# 1830

Delta R.T. -0.01 min

Lab File: BM023350.D

Acq: 23 Oct 2019 20:11


Tgt Ion:163 Resp: 1255913

Ion Ratio Lower Upper

163 100

194 4.2 3.3 4.9

164 10.3 7.9 11.9

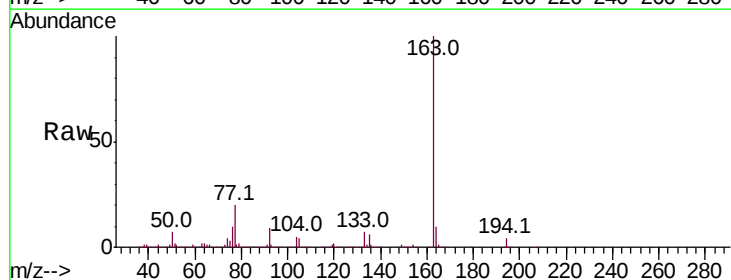

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

13.75

1200000

1000000

800000


600000


400000

200000

0

Time-->





#48

Acenaphthylene

Concen: 8.059 ng/ul

RT: 14.00 min Scan# 1873

Delta R.T. -0.00 min

Lab File: BM023350.D

Acq: 23 Oct 2019 20:11


Instrument :

BNA_M

ClientSampleId :

Tot Ion:152 Resp: 1279816




Ion	Ratio	Lower	Upper
152	100		
151	20.2	16.2	24.2
153	13.1	10.4	15.6



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

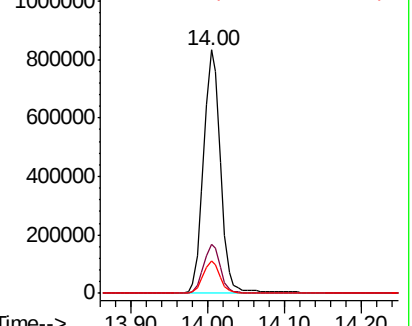

#50

Acenaphthene

Concen: 1.490 ng/ul

RT: 14.35 min Scan# 1932


Delta R.T. -0.00 min

Lab File: BM023350.D

Acq: 23 Oct 2019 20:11

Tgt Ion:153 Resp: 166438



Ion	Ratio	Lower	Upper
153	100		
152	51.0	37.9	56.9
154	88.3	70.6	106.0




Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

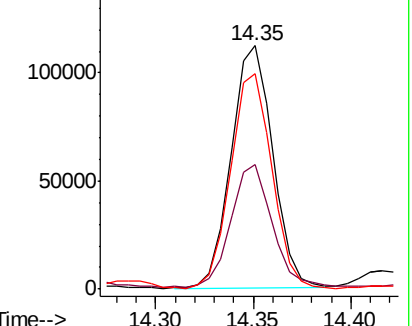



#54

Dibenzenofuran

Concen: 1.788 ng/ul

RT: 14.69 min Scan# 1989

Delta R.T. -0.01 min

Lab File: BM023350.D

Acq: 23 Oct 2019 20:11

Instrument :

BNA_M





ClientSampled :

Tot Ion:168 Resp: 286036

Ion Ratio Lower Upper

168 100

139 39.0 29.7 44.5

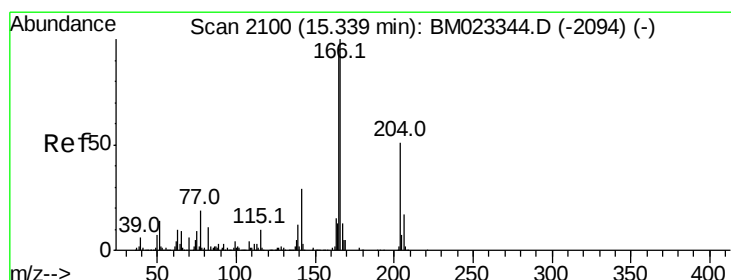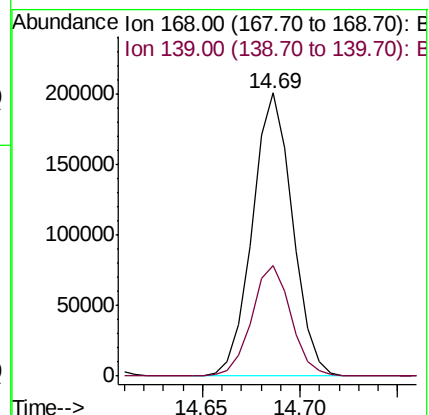

#59

Fluorene

Concen: 1.467 ng/ul

RT: 15.34 min Scan# 2100

Delta R.T. -0.00 min

Lab File: BM023350.D

Acq: 23 Oct 2019 20:11




Tgt Ion:166 Resp: 191324


Ion Ratio Lower Upper

166 100

165 92.7 77.8 116.6

167 13.8 10.8 16.2

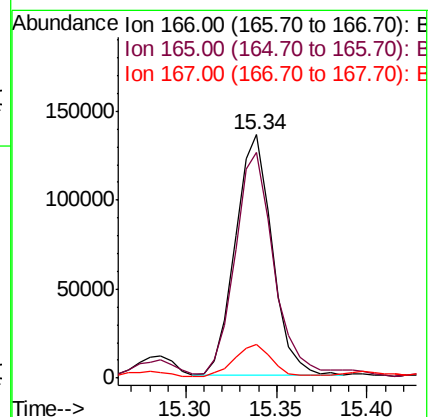

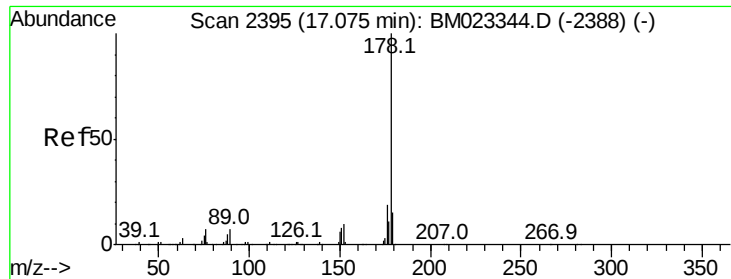

#70

Phenanthrene

Concen: 8.232 ng/ul

RT: 17.07 min Scan# 2395

Delta R.T. -0.00 min

Lab File: BM023350.D

Acq: 23 Oct 2019 20:11

Instrument :

BNA_M

ClientSampleId :


Tot Ion:178 Resp: 1533469

Ion Ratio Lower Upper




178 100

179 15.3 12.2 18.2

176 18.8 14.9 22.3

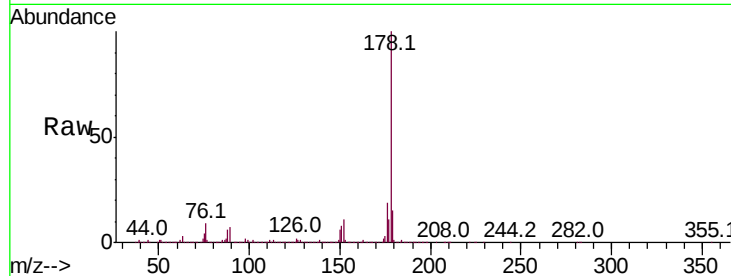

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

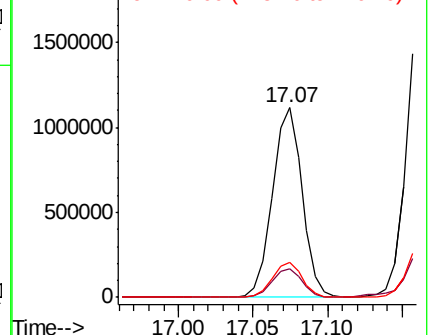

#72

Anthracene

Concen: 15.468 ng/ul

RT: 17.16 min Scan# 2410

Delta R.T. -0.01 min

Lab File: BM023350.D

Acq: 23 Oct 2019 20:11


Tgt Ion:178 Resp: 2919547

Ion Ratio Lower Upper



178 100


179 15.4 12.1 18.1

176 18.4 14.4 21.6



Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

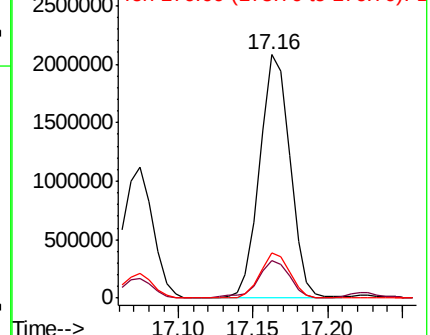




#75
 Carbazole
 Concen: 1.686 ng/ul
 RT: 17.43 min Scan# 2456
 Delta R.T. -0.00 min
 Lab File: BM023350.D
 Acq: 23 Oct 2019 20:11

Instrument :
 BNA_M
 ClientSampled :

Tot Ion	Ratio	Lower	Upper
167	100		
166	22.4	17.1	25.7
139	13.5	10.0	15.0



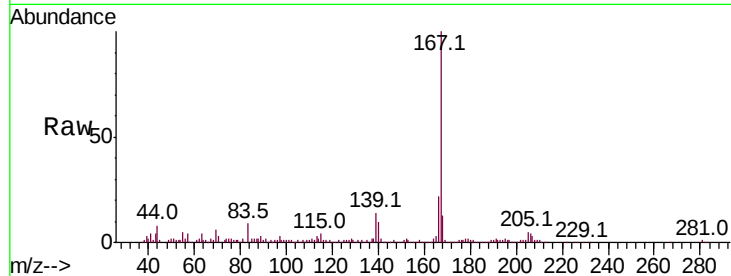


Abundance

Ion 167.00 (166.70 to 167.70): E


Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

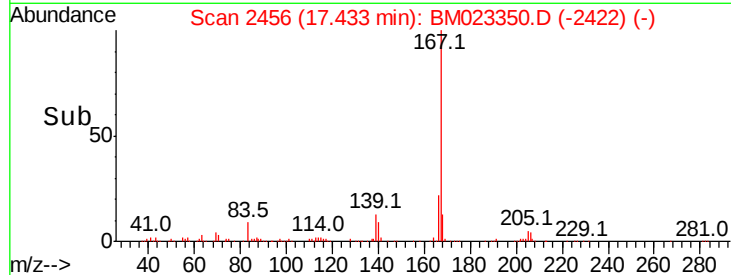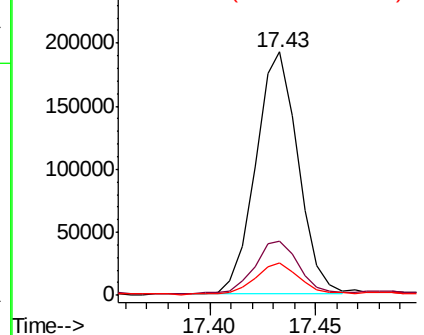

#77
 Fluoranthene
 Concen: 40.454 ng/ul
 RT: 19.10 min Scan# 2739
 Delta R.T. -0.00 min
 Lab File: BM023350.D
 Acq: 23 Oct 2019 20:11

Tgt Ion	Ratio	Lower	Upper
202	100		
101	9.8	8.1	12.1
100	7.5	6.2	9.2


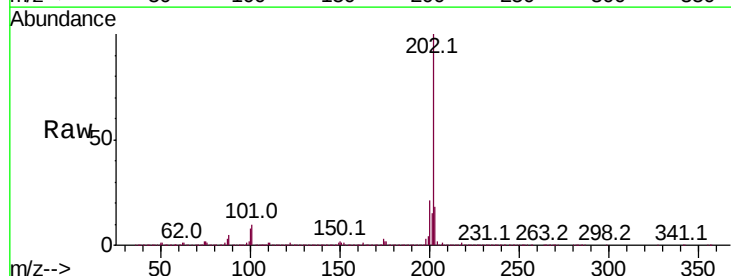



Abundance

Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

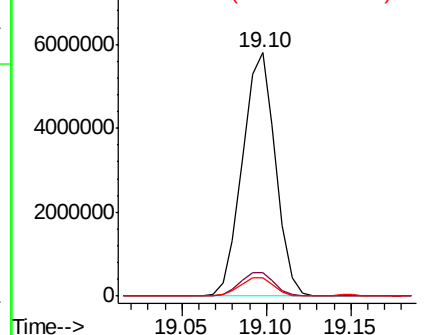







#80
Pvrene
Concen: 57.516 ng/ul
RT: 19.46 min Scan# 2801
Delta R.T. 0.01 min
Lab File: BM023350.D
Acq: 23 Oct 2019 20:11

Instrument :
BNA_M
ClientSampleId :

Tot Ion:202 Resp: 9349601
Ion Ratio Lower Upper
202 100
101 11.8 10.0 15.0
100 9.5 8.3 12.5

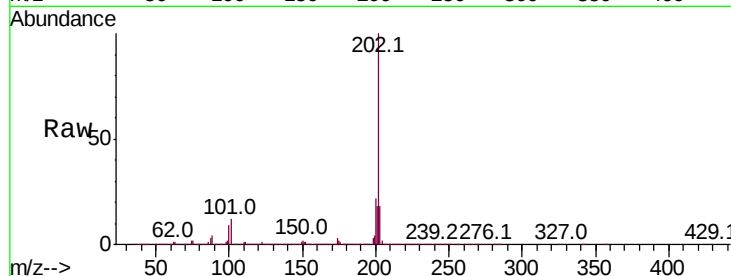


Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B


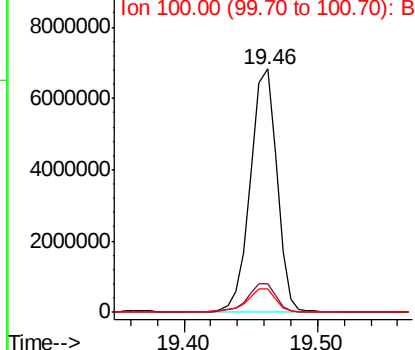



#83
Benzo(a)anthracene
Concen: 49.175 ng/ul
RT: 21.21 min Scan# 3098
Delta R.T. -0.00 min
Lab File: BM023350.D
Acq: 23 Oct 2019 20:11

Tgt Ion:228 Resp: 7570996
Ion Ratio Lower Upper
228 100
229 21.5 15.8 23.8
226 30.3 21.6 32.4



Abundance Ion 228.00 (227.70 to 228.70): E
Ion 229.00 (228.70 to 229.70): E
Ion 226.00 (225.70 to 226.70): E

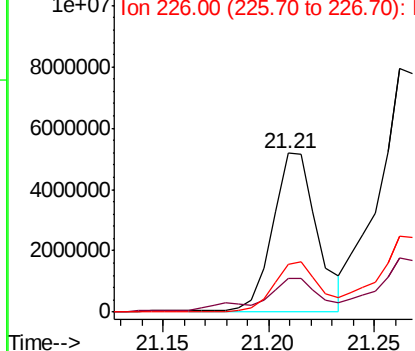

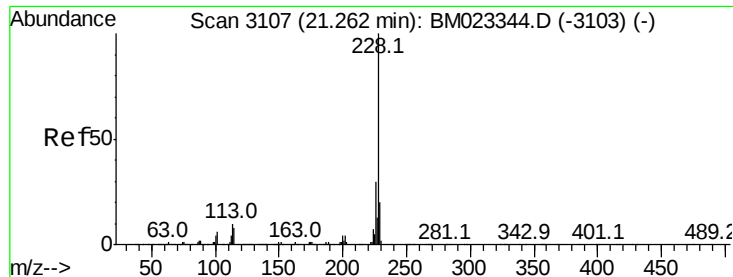

#85

Chrysene

Concen: 86.044 ng/ul

RT: 21.26 min Scan# 3107

Delta R.T. -0.00 min

Lab File: BM023350.D

Acq: 23 Oct 2019 20:11


Instrument :

BNA_M

ClientSampleId :

Tot Ion:228 Resp:12223142

Ion	Ratio	Lower	Upper
228	100		
226	31.5	24.0	36.0
229	22.1	16.0	24.0



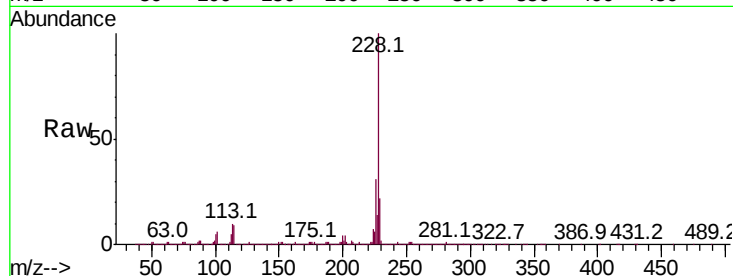


Abundance

Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

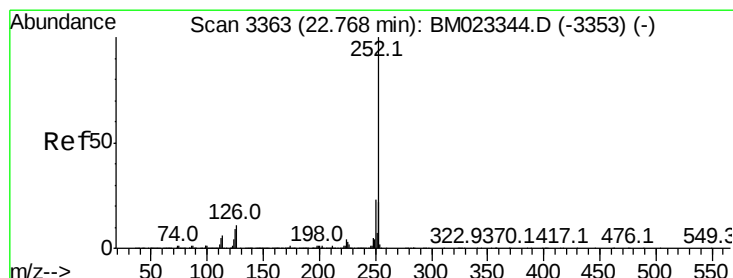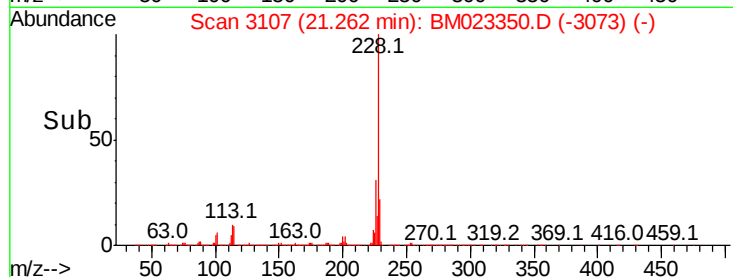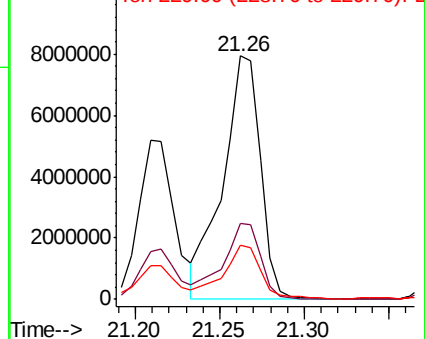

#88

Benzo(b)fluoranthene

Concen: 132.450 ng/ul

RT: 22.78 min Scan# 3365


Delta R.T. 0.01 min

Lab File: BM023350.D

Acq: 23 Oct 2019 20:11

Tgt Ion:252 Resp:21879767

Ion	Ratio	Lower	Upper
252	100		
253	25.9	17.5	26.3
125	9.8	7.1	10.7


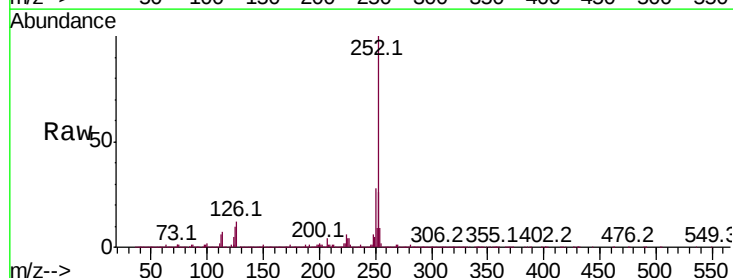



Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

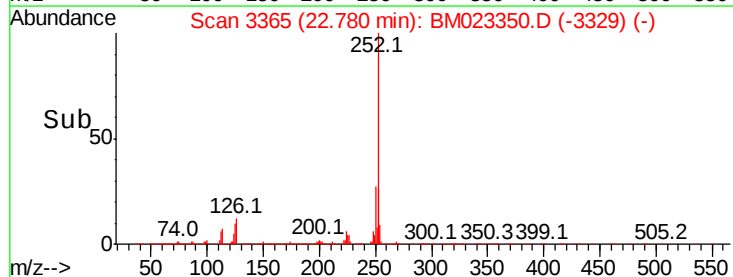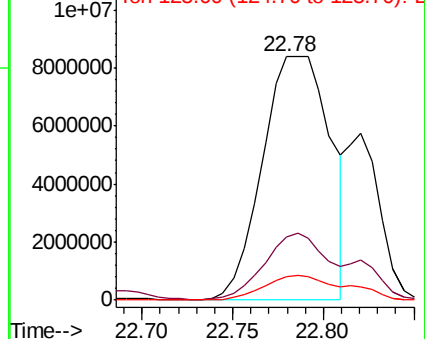

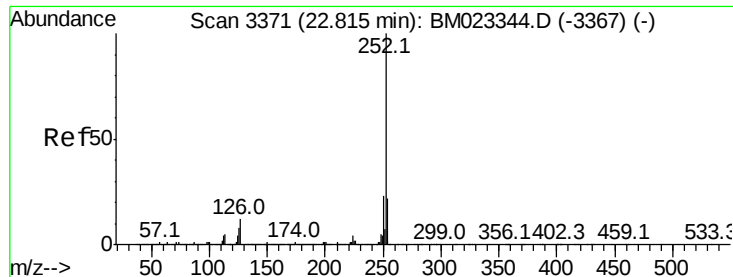

#89

Benzo(k)fluoranthene

Concen: 45.521 ng/ul

RT: 22.82 min Scan# 3372

Delta R.T. 0.01 min

Lab File: BM023350.D

Acq: 23 Oct 2019 20:11

Instrument :

BNA_M

ClientSampleId :


Tot Ion:252 Resp: 7061037

Ion Ratio Lower Upper




252 100

253 23.8 17.8 26.6

125 8.1 6.8 10.2

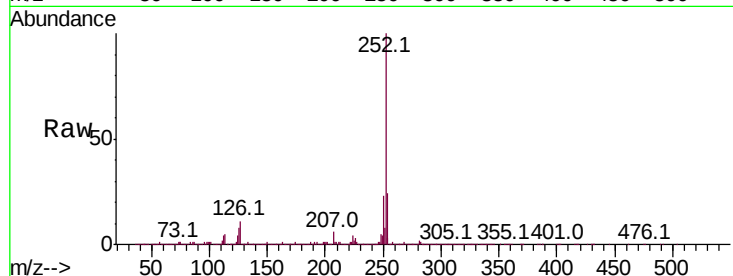

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

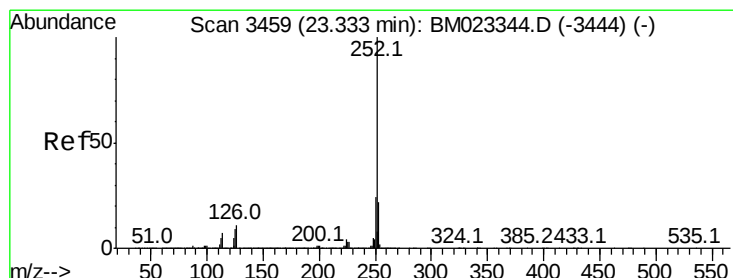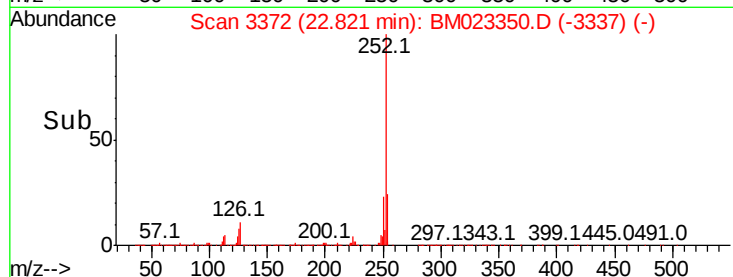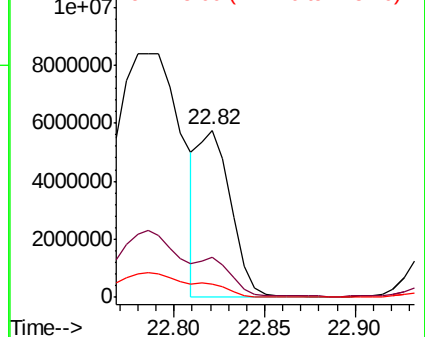

#91

Benzo(a)pyrene

Concen: 89.307 ng/ul

RT: 23.34 min Scan# 3461

Delta R.T. 0.01 min

Lab File: BM023350.D

Acq: 23 Oct 2019 20:11


Tgt Ion:252 Resp:13355999

Ion Ratio Lower Upper



252 100


253 23.3 17.7 26.5

125 8.8 7.5 11.3

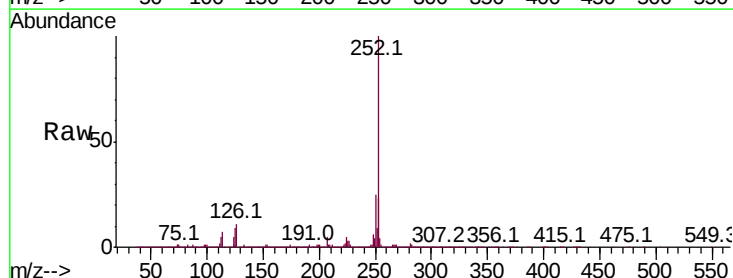

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

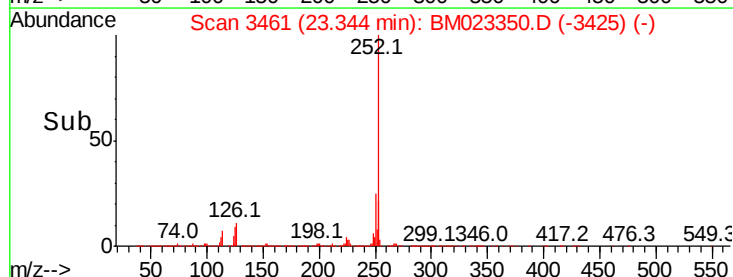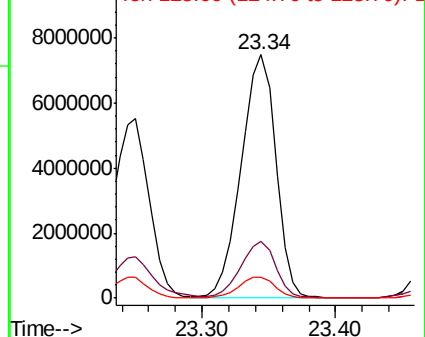

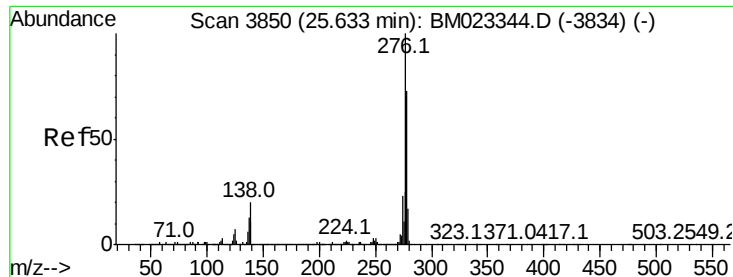


#92




Indeno(1,2,3-cd)pyrene
Concen: 67.269 ng/ul
RT: 25.64 min Scan# 3852
Delta R.T. 0.01 min
Lab File: BM023350.D
Acq: 23 Oct 2019 20:11

Instrument :
BNA_M
ClientSampled :

Tot Ion:276 Resp:10892853
Ion Ratio Lower Upper
276 100
138 17.5 15.7 23.5
277 24.9 20.2 30.2

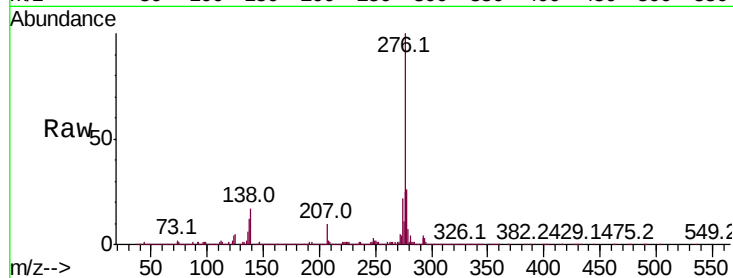


Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 277.00 (276.70 to 277.70): E

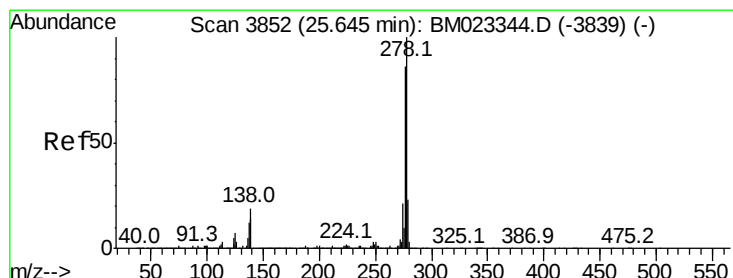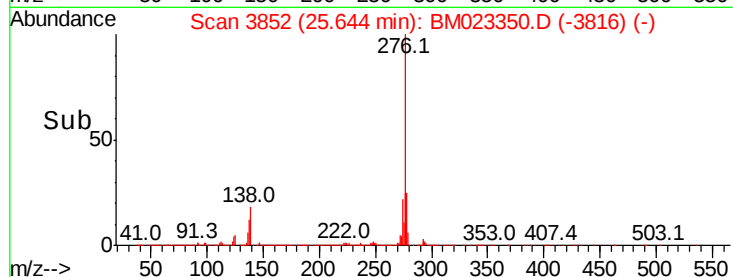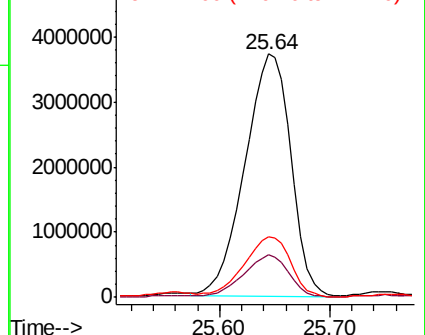



#93


Dibenzo(a,h)anthracene
Concen: 21.334 ng/ul
RT: 25.65 min Scan# 3853
Delta R.T. 0.01 min
Lab File: BM023350.D
Acq: 23 Oct 2019 20:11

Tgt Ion:278 Resp: 2912969
Ion Ratio Lower Upper
278 100
139 0.0 10.9 16.3#
279 24.8 18.7 28.1

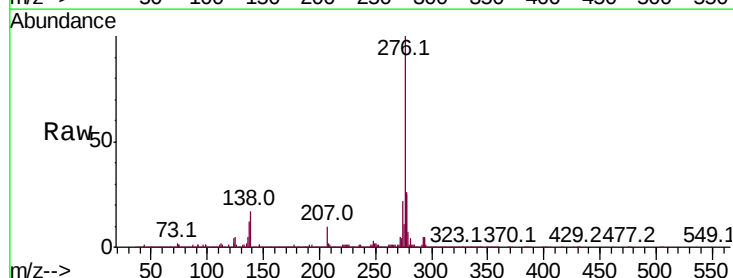

Abundance Ion 278.00 (277.70 to 278.70): E
Ion 139.00 (138.70 to 139.70): E
Ion 279.00 (278.70 to 279.70): E

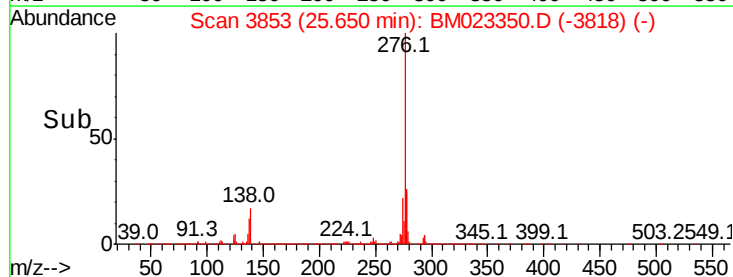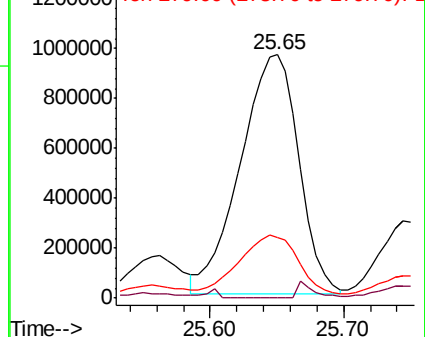



#94

Benzo(a,h,i)perylene

Concen: 61.986 ng/ul

RT: 26.32 min Scan# 3967

Delta R.T. 0.02 min

Lab File: BM023350.D

Acq: 23 Oct 2019 20:11

Instrument :

BNA_M

ClientSampleId :


Tot Ion:276 Resp: 8166472

Ion Ratio Lower Upper

276 100

138 17.1 14.4 21.6

277 23.6 19.0 28.6



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

