

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102319\
 Data File : BM023358.D
 Acq On : 24 Oct 2019 00:58
 Operator : JU
 Sample : K5378-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0011

Manual Integrations
 APPROVED

mohammad
 10/24/2019 5:03:04 PM

Quant Time: Oct 24 04:21:23 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 23 18:47:16 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	597745	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	2578851	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	1593270	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	2945938	20.00	ng/ul	0.00
78) Chrysene-d12	21.22	240	2468119	20.00	ng/ul	0.00
86) Perylene-d12	23.42	264	2716527	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.16	96	54075	4.30	ng/uL	0.00
5) Phenol-d5	6.82	99	932925	18.58	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	802375	27.27	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	944420	24.06	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	684381	16.78	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	540158	27.82	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	533662	24.78	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	976423	23.07	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	448369	9.21	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	3015299	24.92	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	3901824	28.15	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	107756	5.14	ng/ul	0.00
58) Fluorene-d10	15.28	176	2800790	27.33	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	291233	15.88	ng/ul	0.00
71) Anthracene-d10	17.13	188	3849966	27.65	ng/ul	0.00
79) Pyrene-d10	19.43	212	4001817	29.48	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.28	264	3938376	28.46	ng/ul	0.00

Target Compounds

					Ovalue
6) Phenol	6.84	94	142914	2.764	ng/ul 99
45) Dimethylphthalate	13.75	163	1111072	9.146	ng/ul 100
70) Phenanthrene	17.07	178	943753	5.733	ng/ul 99
77) Fluoranthene	19.09	202	2637143	15.357	ng/ul 100
80) Pyrene	19.46	202	1991274	11.425	ng/ul 99
83) Benzo(a)anthracene	21.20	228	1227070	7.434	ng/ul 100
85) Chrysene	21.26	228	1180015	7.748	ng/ul 99
88) Benzo(b)fluoranthene	22.76	252	1530179	8.770	ng/ul 99
89) Benzo(k)fluoranthene	22.80	252	466017m	2.845	ng/ul
91) Benzo(a)pyrene	23.32	252	784972	4.970	ng/ul 99
92) Indeno(1,2,3-cd)pyrene	25.62	276	659956	3.859	ng/ul 97
93) Dibenzo(a,h)anthracene	25.62	278	194291	1.347	ng/ul 96
94) Benzo(g,h,i)perylene	26.28	276	520844	3.743	ng/ul 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102319\
Data File : BM023358.D
Acq On : 24 Oct 2019 00:58
Operator : JU
Sample : K5378-03
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0011

Manual Integrations
APPROVED

mohammad
10/24/2019 5:03:04 PM

Quant Time: Oct 24 04:21:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 23 18:47:16 2019
Response via : Initial Calibration

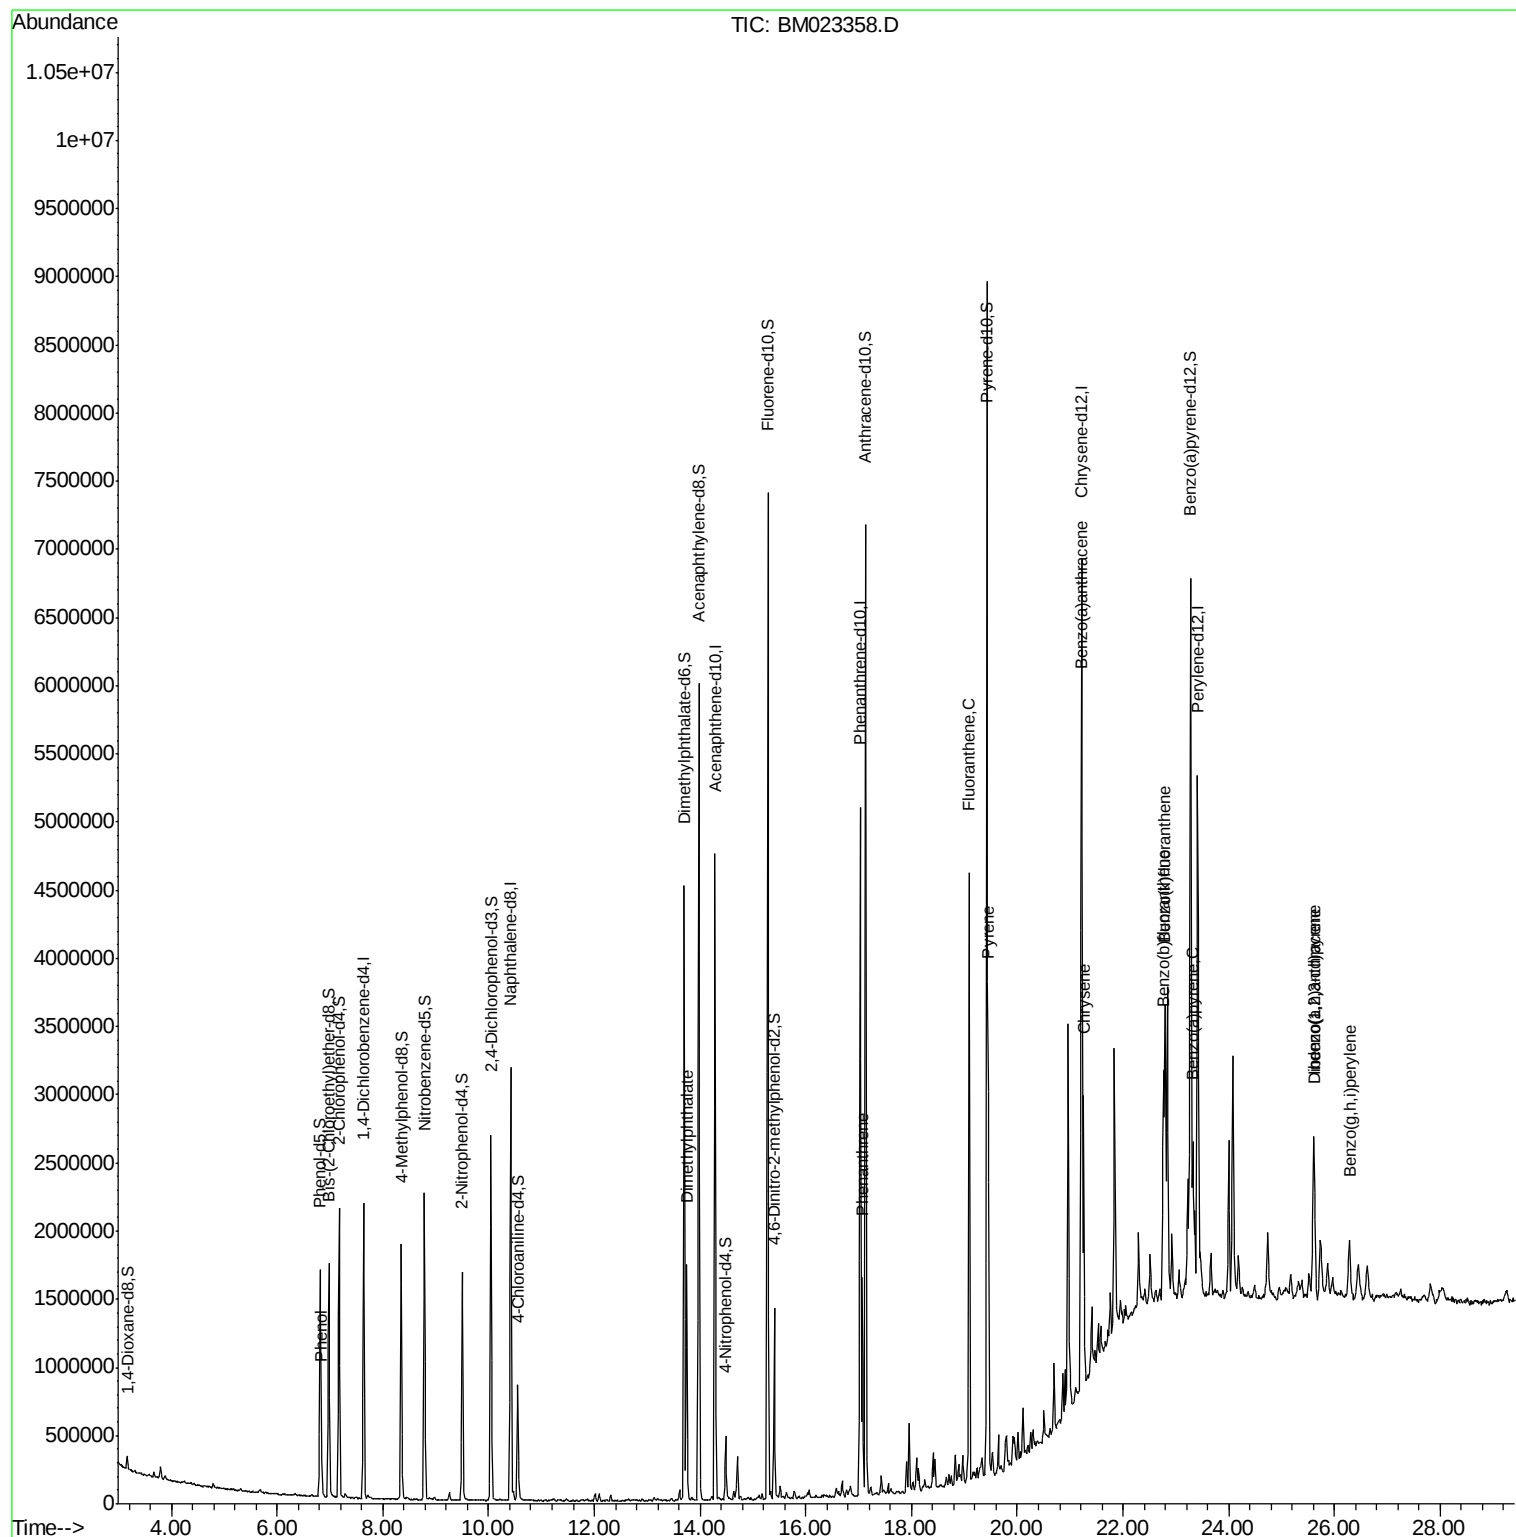

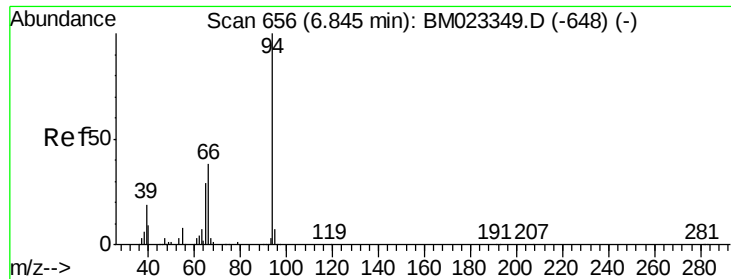

#6

Phenol





Concen: 2.764 ng/ul
 RT: 6.84 min Scan# 655
 Delta R.T. -0.01 min
 Lab File: BM023358.D
 Acq: 24 Oct 2019 00:58

Instrument :
 BNA_M
 ClientSampleId :
 C0011

Tot Ion	Ratio	Lower	Upper
94	100		
65	28.9	22.9	34.3
66	38.8	31.4	47.2

Manual Integrations
 APPROVED

mohammad
 10/24/2019 5:03:04 PM

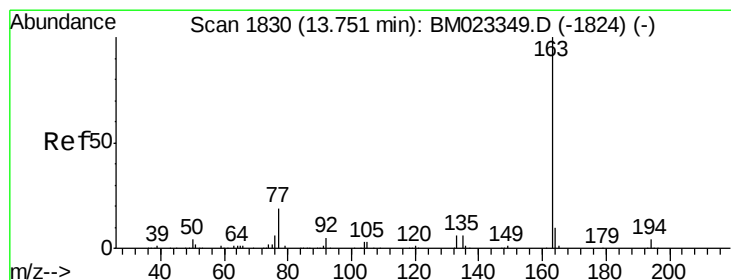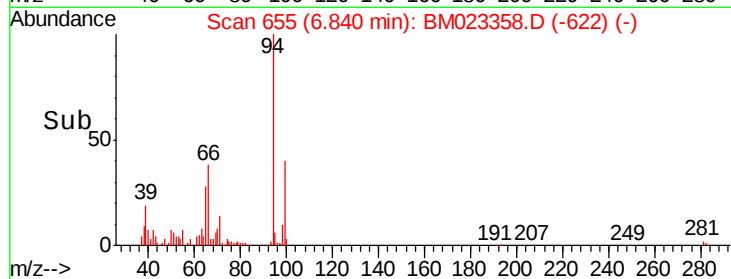
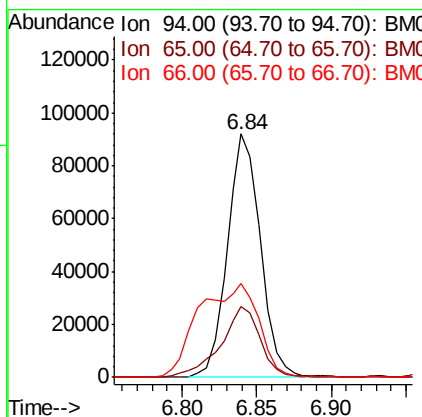
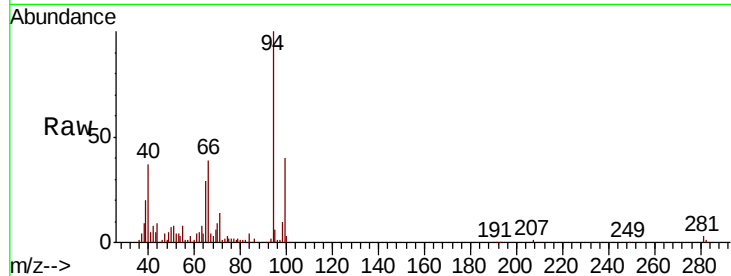



#45

Dimethylphthalate

Concen: 9.146 ng/ul
 RT: 13.75 min Scan# 1830
 Delta R.T. -0.01 min
 Lab File: BM023358.D
 Acq: 24 Oct 2019 00:58

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.1	3.3	4.9
164	10.0	7.9	11.9

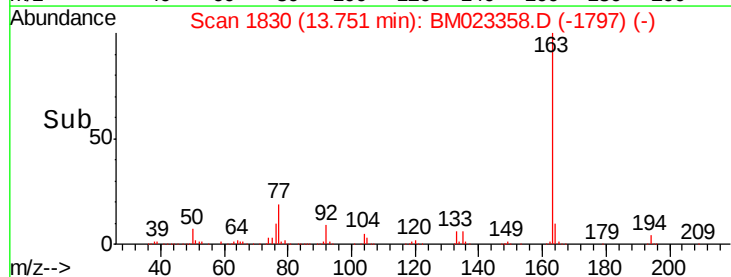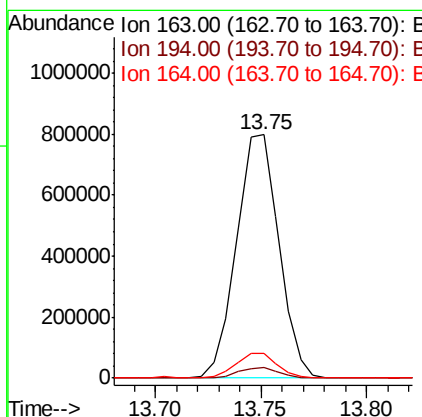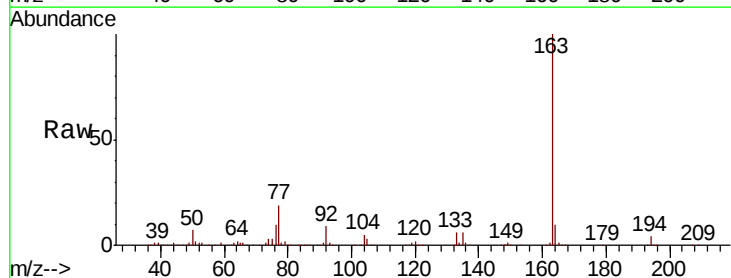

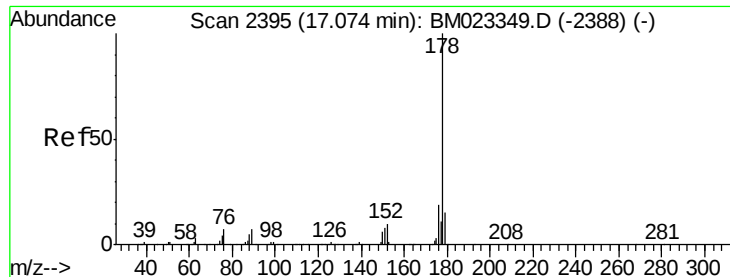





#70
Phenanthrene
Concen: 5.733 ng/ul
RT: 17.07 min Scan# 2394
Delta R.T. -0.01 min
Lab File: BM023358.D
Acq: 24 Oct 2019 00:58

Instrument :
BNA_M
ClientSampleId :
C0011

Tot Ion	Ratio	Lower	Upper
178	100		
179	15.6	12.2	18.2
176	19.4	14.9	22.3




Manual Integrations
APPROVED


mohammad
10/24/2019 5:03:04 PM

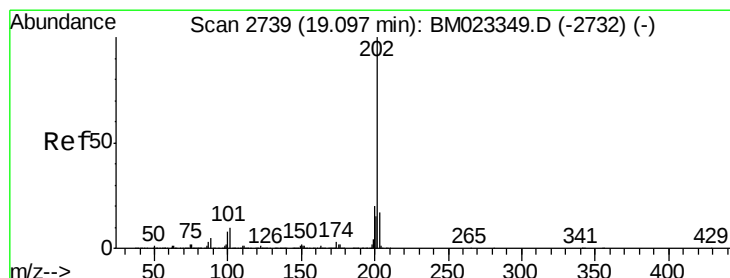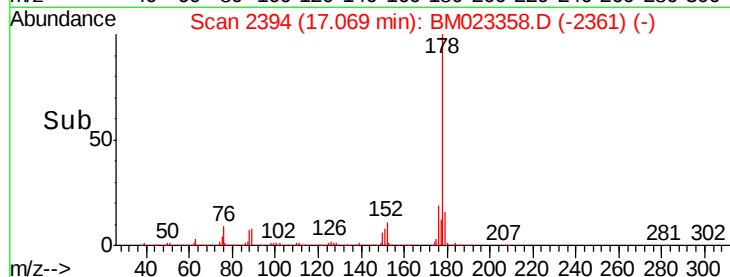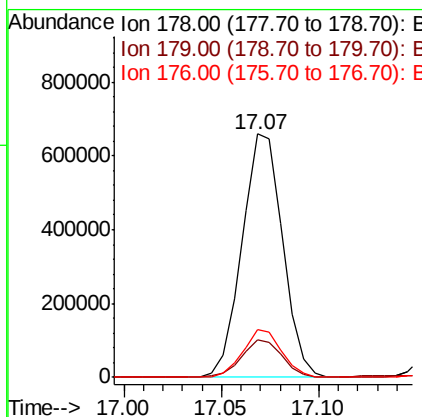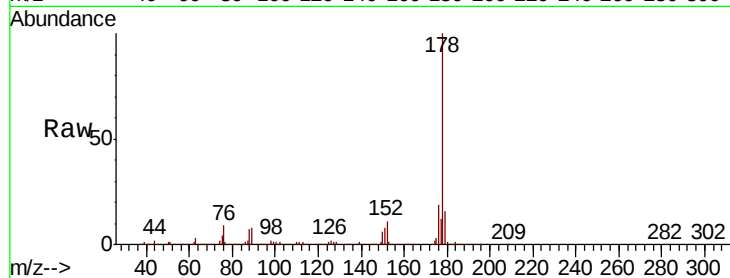

#77
Fluoranthene
Concen: 15.357 ng/ul
RT: 19.09 min Scan# 2738
Delta R.T. -0.01 min
Lab File: BM023358.D
Acq: 24 Oct 2019 00:58

Tgt Ion	Ratio	Lower	Upper
202	100		
101	10.0	8.1	12.1
100	7.8	6.2	9.2

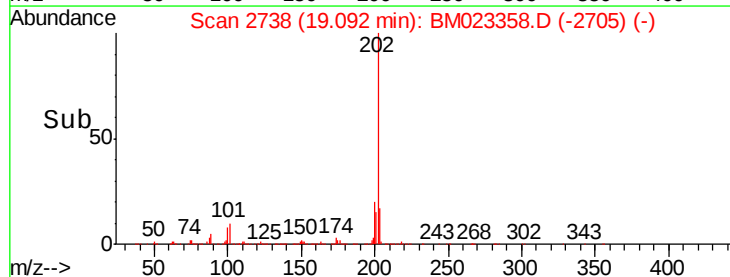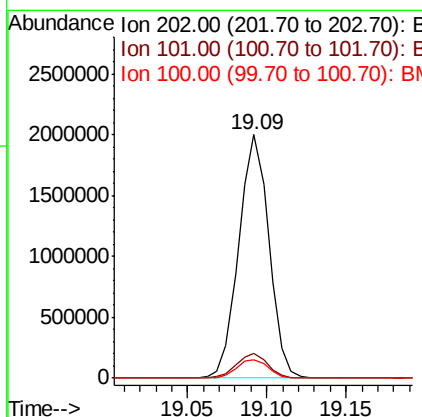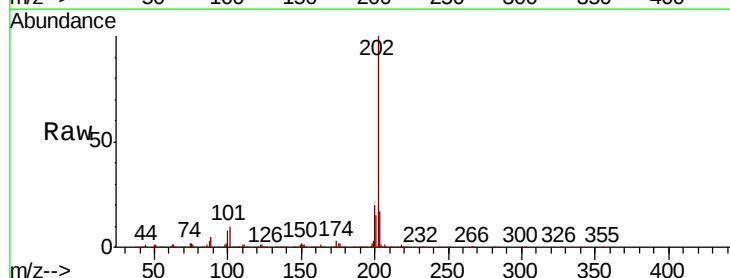

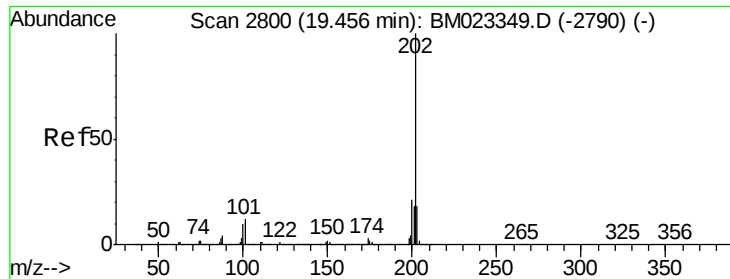


#80
Pvrene
Concen: 11.425 ng/ul
RT: 19.46 min Scan# 2800
Delta R.T. -0.00 min
Lab File: BM023358.D
Acq: 24 Oct 2019 00:58

Instrument :
BNA_M
ClientSampleId :
C0011




Tot Ion	Ratio	Lower	Upper
202	100		
101	12.2	10.0	15.0
100	9.8	8.3	12.5

Manual Integrations
APPROVED

mohammad
10/24/2019 5:03:04 PM

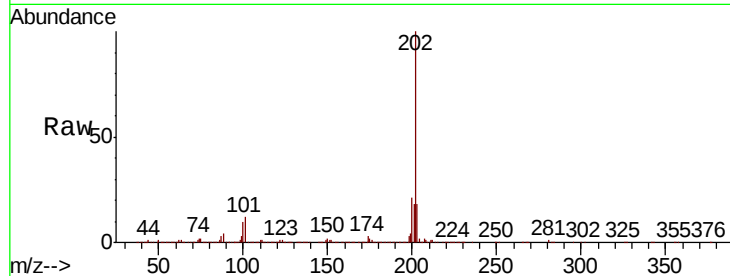


Abundance Ion 202.00 (201.70 to 202.70): E
2000000
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

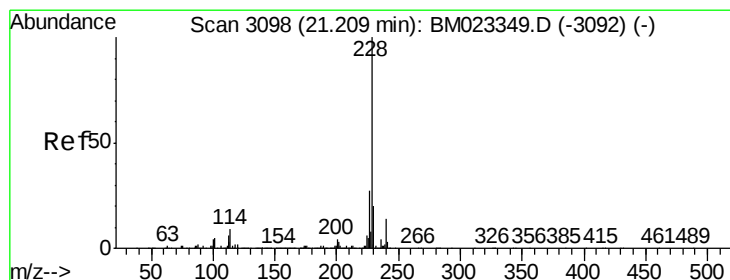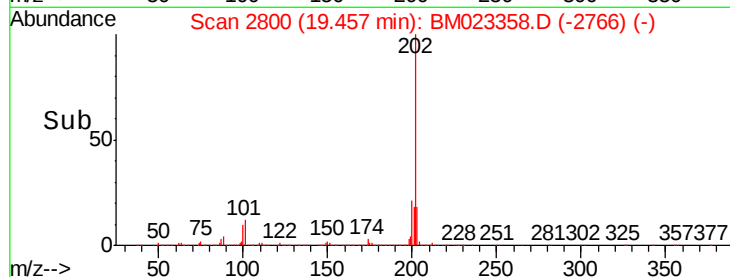
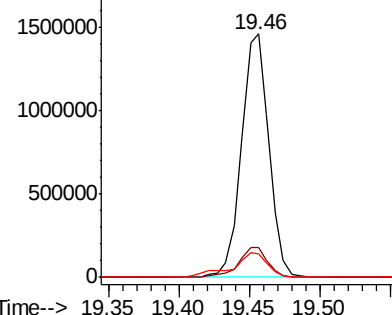



#83
Benzo(a)anthracene
Concen: 7.434 ng/ul
RT: 21.20 min Scan# 3097
Delta R.T. -0.01 min
Lab File: BM023358.D
Acq: 24 Oct 2019 00:58

Tgt Ion	Ratio	Lower	Upper
228	100		
229	19.8	15.8	23.8
226	27.1	21.6	32.4

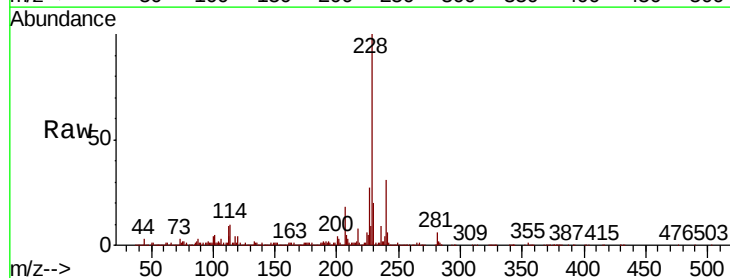

Abundance Ion 228.00 (227.70 to 228.70): E
1200000
Ion 229.00 (228.70 to 229.70): E
Ion 226.00 (225.70 to 226.70): E

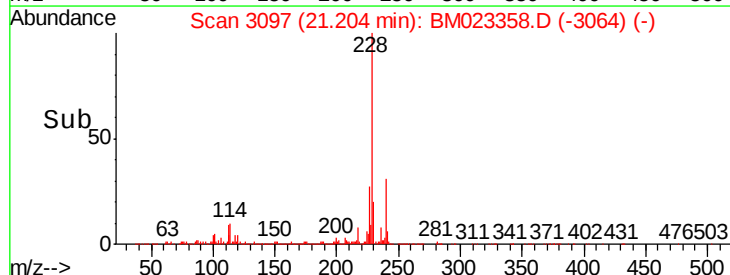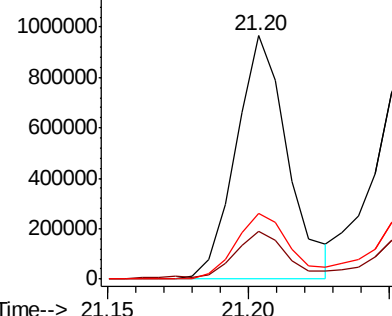

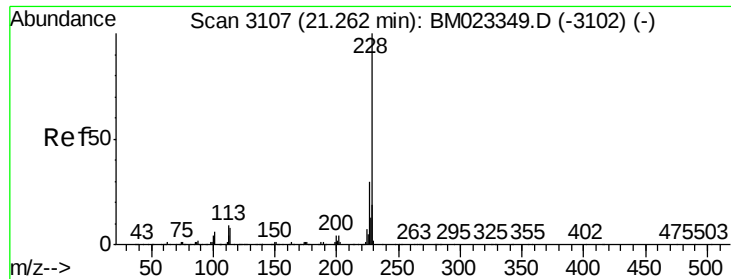





#85
Chrysene
Concen: 7.748 ng/ul
RT: 21.26 min Scan# 3106
Delta R.T. -0.01 min
Lab File: BM023358.D
Acq: 24 Oct 2019 00:58

Instrument :
BNA_M
ClientSampleId :
C0011

Tot Ion	Ratio	Lower	Upper
228	100		
226	29.9	24.0	36.0
229	20.9	16.0	24.0




Manual Integrations
APPROVED


mohammad
10/24/2019 5:03:04 PM

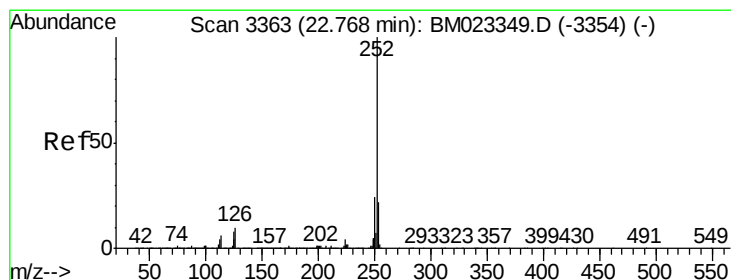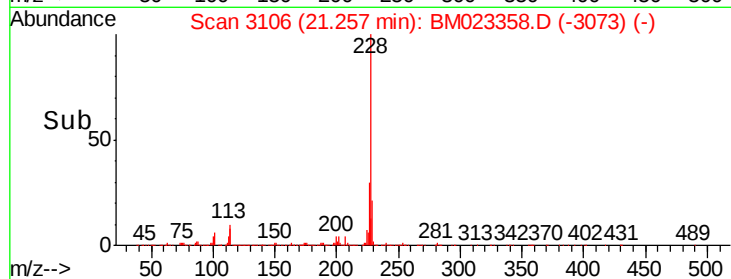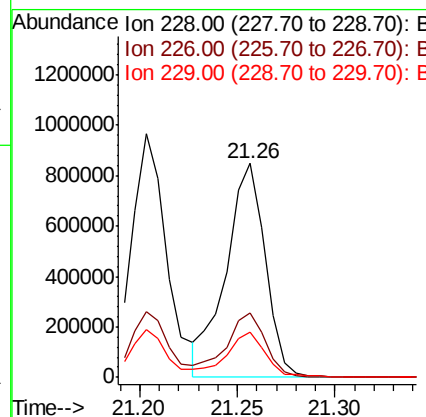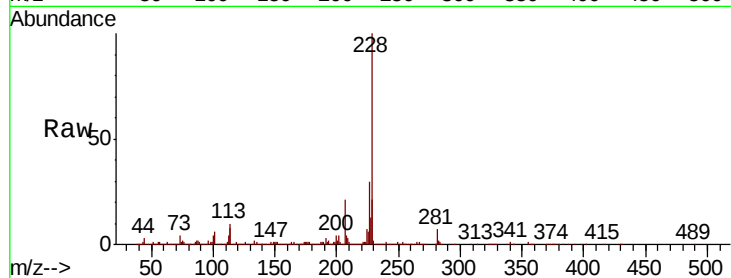

#88
Benzo(b)fluoranthene
Concen: 8.770 ng/ul
RT: 22.76 min Scan# 3362
Delta R.T. -0.01 min
Lab File: BM023358.D
Acq: 24 Oct 2019 00:58

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.0	17.5	26.3
125	9.6	7.1	10.7

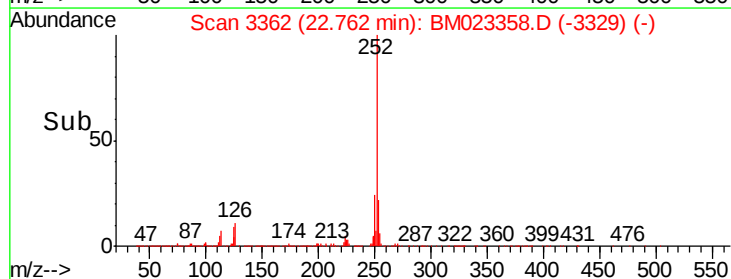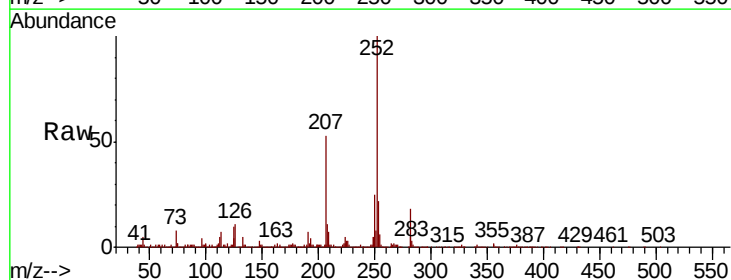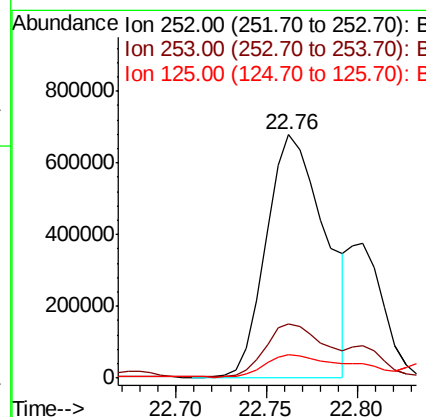

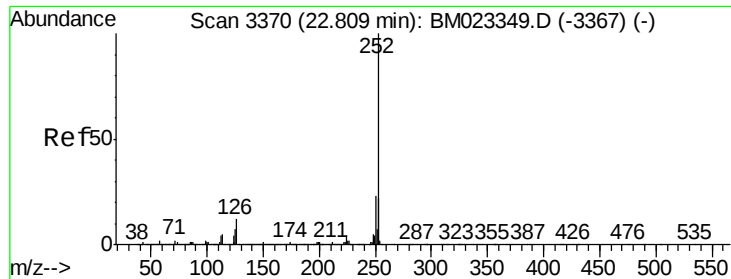





#89
Benzo(k)fluoranthene
Concen: 2.845 ng/ul m
RT: 22.80 min Scan# 3369
Delta R.T. -0.01 min
Lab File: BM023358.D
Acq: 24 Oct 2019 00:58

Instrument :
BNA_M
ClientSampleId :
C0011

Tot Ion	Ratio	Lower	Upper
252	100		
253	23.7	17.8	26.6
125	10.4	6.8	10.2




Manual Integrations
APPROVED


mohammad
10/24/2019 5:03:04 PM

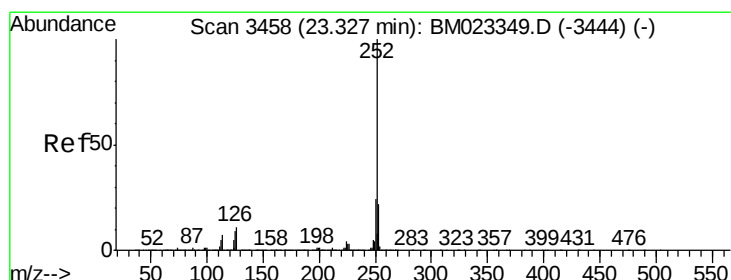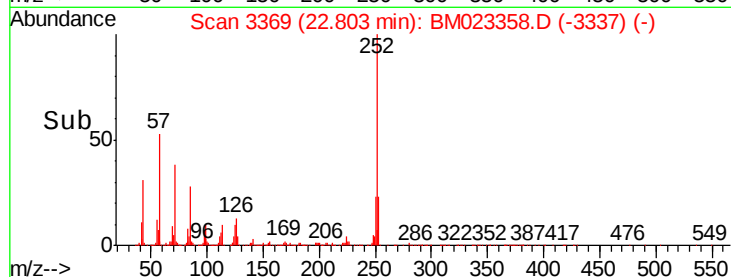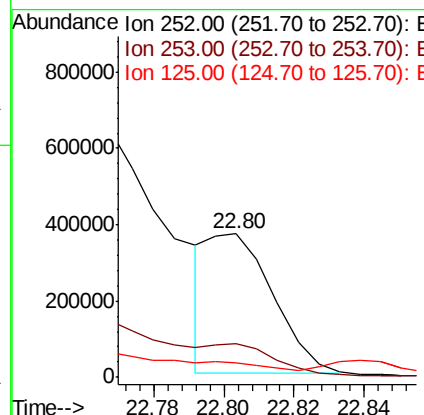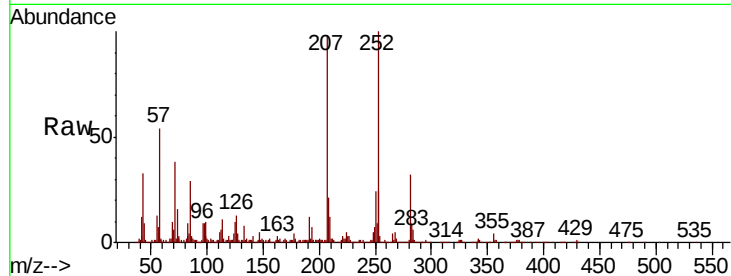

#91
Benzo(a)pyrene
Concen: 4.970 ng/ul
RT: 23.32 min Scan# 3457
Delta R.T. -0.01 min
Lab File: BM023358.D
Acq: 24 Oct 2019 00:58

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.4	17.7	26.5
125	10.2	7.5	11.3

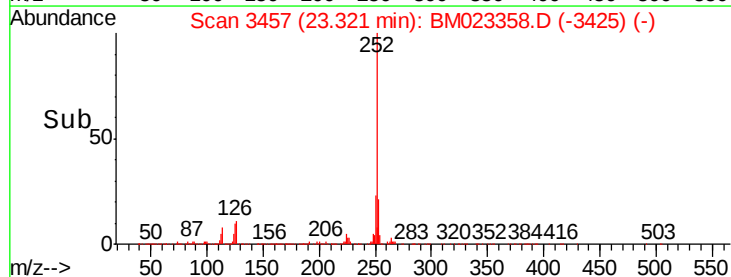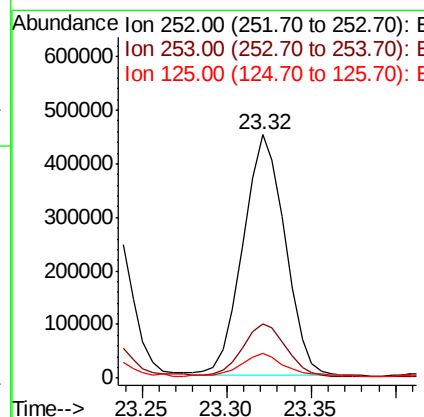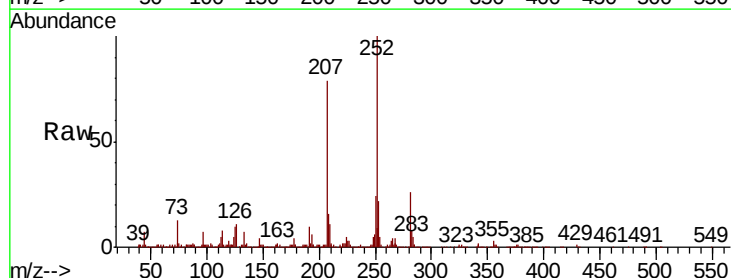

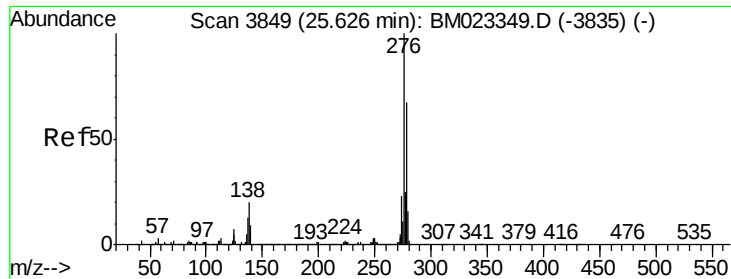

#92





Indeno(1,2,3-cd)pyrene
Concen: 3.859 ng/ul
RT: 25.62 min Scan# 3847
Delta R.T. -0.02 min
Lab File: BM023358.D
Acq: 24 Oct 2019 00:58

Instrument :
BNA_M
ClientSampleId :
C0011

Tot Ion	Ratio	Lower	Upper
276	100		
138	17.0	15.7	23.5
277	24.9	20.2	30.2

Manual Integrations
APPROVED




mohammad
10/24/2019 5:03:04 PM

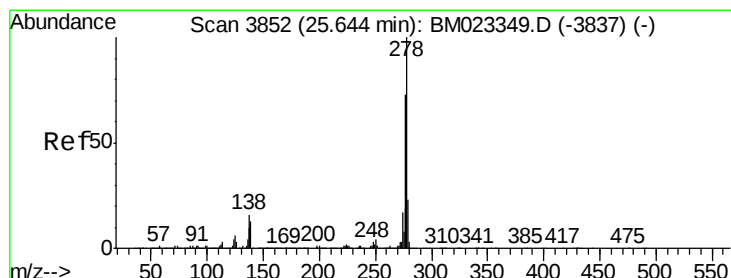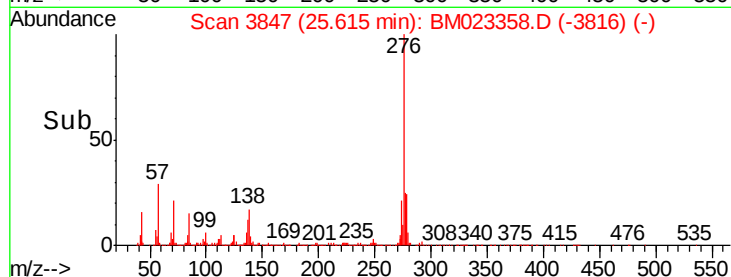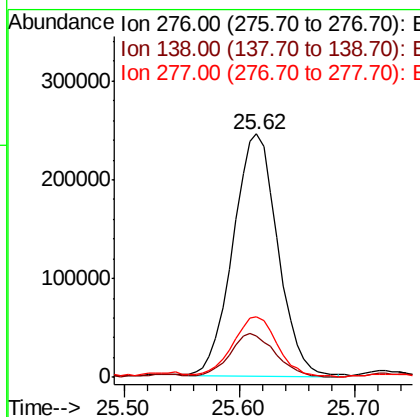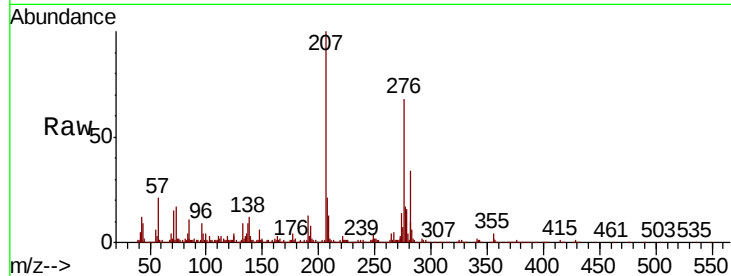


#93

Dibenzo(a,h)anthracene
Concen: 1.347 ng/ul
RT: 25.62 min Scan# 3848
Delta R.T. -0.02 min
Lab File: BM023358.D
Acq: 24 Oct 2019 00:58

Tgt Ion	Ratio	Lower	Upper
278	100		
139	15.3	10.9	16.3
279	25.0	18.7	28.1

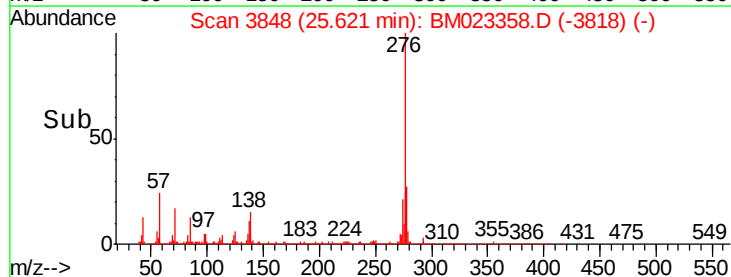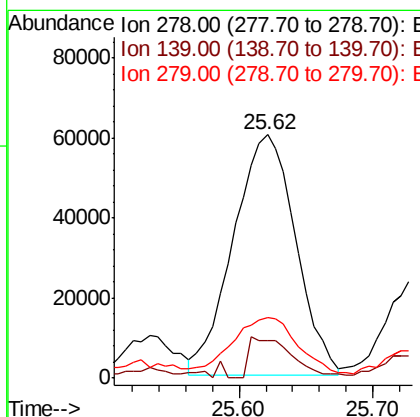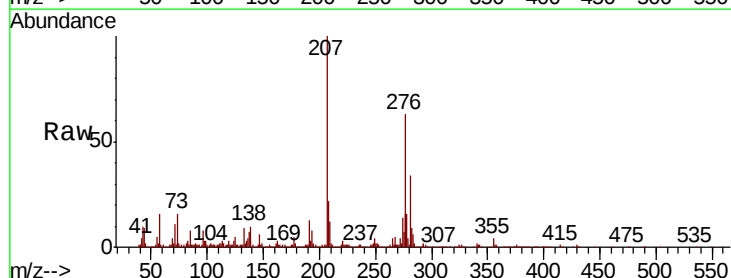

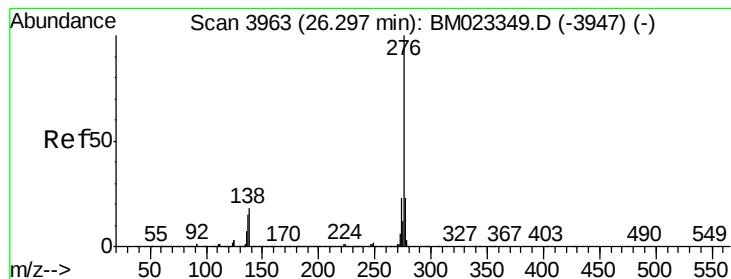

#94

Benzo(a,h,i)perylene

Concen: 3.743 ng/ul

RT: 26.28 min Scan# 3960

Delta R.T. -0.02 min

Lab File: BM023358.D

Acq: 24 Oct 2019 00:58

Instrument :

BNA_M

ClientSampleId :

C0011

Tot Ion:	276	Resp:	520844
Ion Ratio	Lower	Upper	
276	100		
138	18.1	14.4	21.6
277	23.4	19.0	28.6

Manual Integrations
APPROVED

mohammad
10/24/2019 5:03:04 PM

