
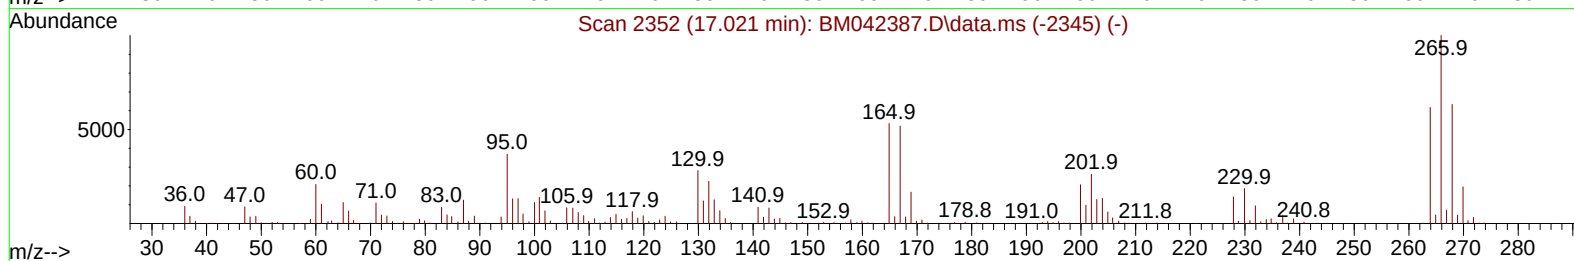
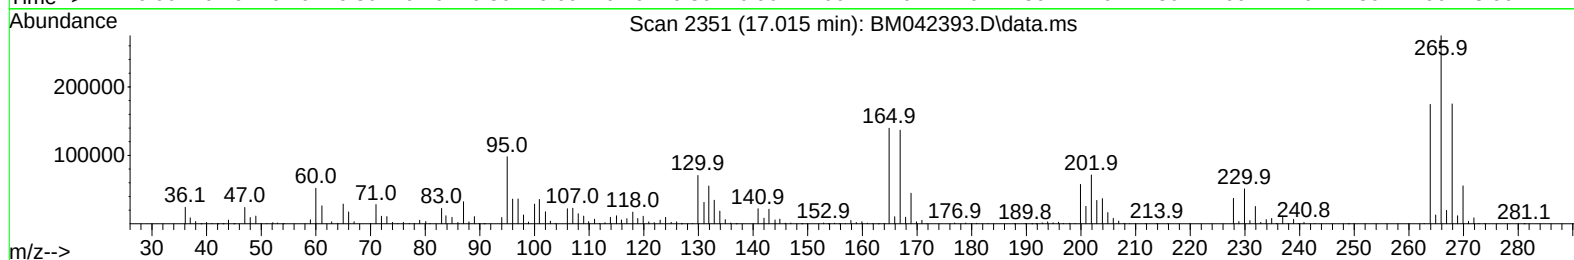


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102323\
Data File : BM042393.D
Acq On : 23 Oct 2023 08:47
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 23 09:34:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 21 02:32:53 2023
Response via : Initial Calibration

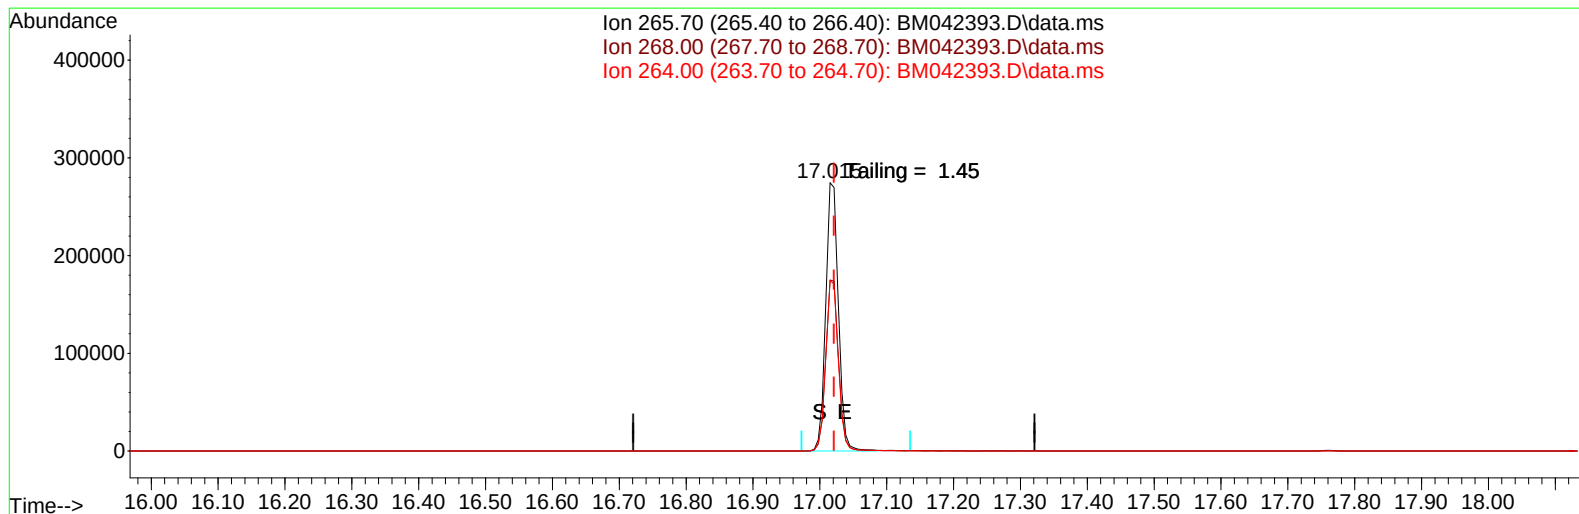

TIC: BM042393.D\data.ms

(70) Pentachlorophenol (C)




17.015min (-0.006) 0.00 ng m

response 362086

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	63.77
264.00	61.70	63.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102323\
Data File : BM042393.D
Acq On : 23 Oct 2023 08:47
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 23 09:34:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 21 02:32:53 2023
Response via : Initial Calibration

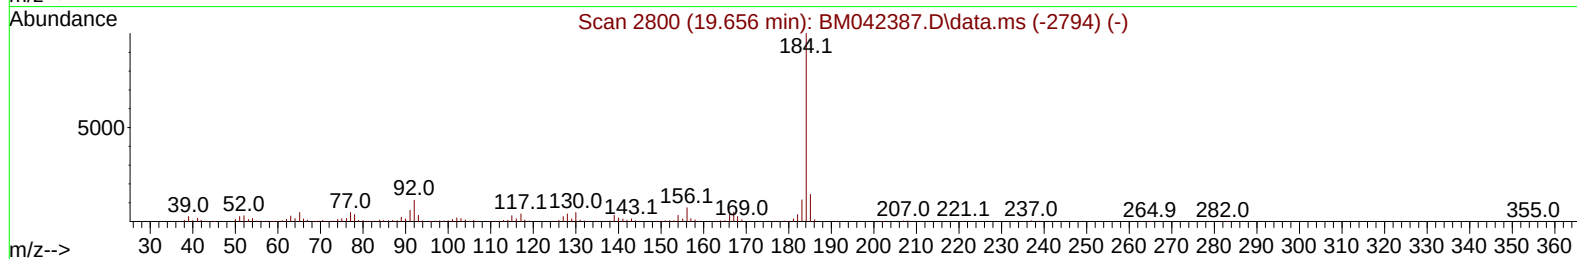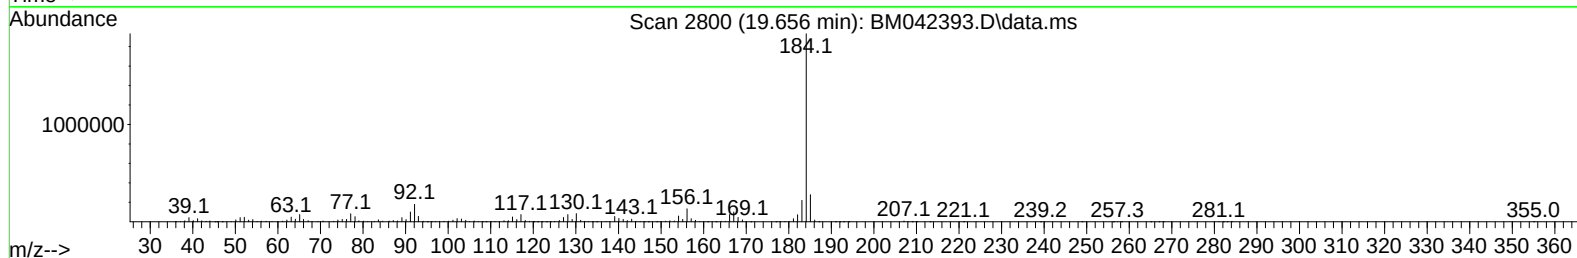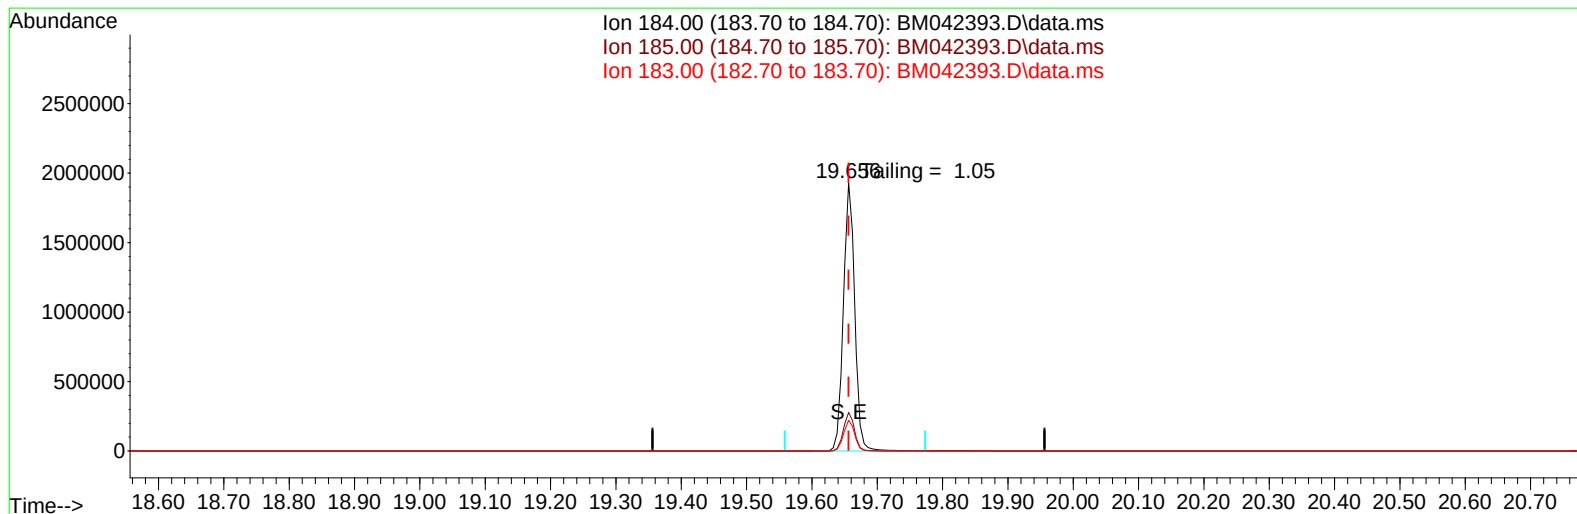

TIC: BM042393.D\data.ms

(77) Benzidine

19.656min (-0.000) 0.00 ng m

response 2327562

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.40
183.00	11.50	11.44
0.00	0.00	0.00