

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102323\
 Data File : BM042408.D
 Acq On : 23 Oct 2023 18:46
 Operator : MA/JU
 Sample : 04957-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MH-H

Quant Time: Oct 23 19:16:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 21 02:32:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.998	152	142313	20.000	ng	0.00
21) Naphthalene-d8	10.816	136	536322	20.000	ng	0.00
39) Acenaphthene-d10	14.639	164	271564	20.000	ng	0.00
64) Phenanthrene-d10	17.392	188	562605	20.000	ng	0.00
76) Chrysene-d12	21.574	240	577587	20.000	ng	0.00
86) Perylene-d12	24.039	264	660594	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.522	112	752320	74.713	ng	0.00
7) Phenol-d6	7.146	99	631182	46.774	ng	0.00
23) Nitrobenzene-d5	9.192	82	1196931	98.687	ng	0.00
42) 2,4,6-Tribromophenol	16.133	330	423303	140.353	ng	0.00
45) 2-Fluorobiphenyl	13.263	172	2005267	99.436	ng	0.00
79) Terphenyl-d14	20.003	244	3128583	96.064	ng	0.00
Target Compounds						
74) Di-n-butylphthalate	18.333	149	6060	2.976	ng	# 93
84) Bis(2-ethylhexyl)phtha...	21.439	149	6068	3.585	ng	# 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102323\
Data File : BM042408.D
Acq On : 23 Oct 2023 18:46
Operator : MA/JU
Sample : 04957-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MH-H

Quant Time: Oct 23 19:16:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 21 02:32:53 2023
Response via : Initial Calibration




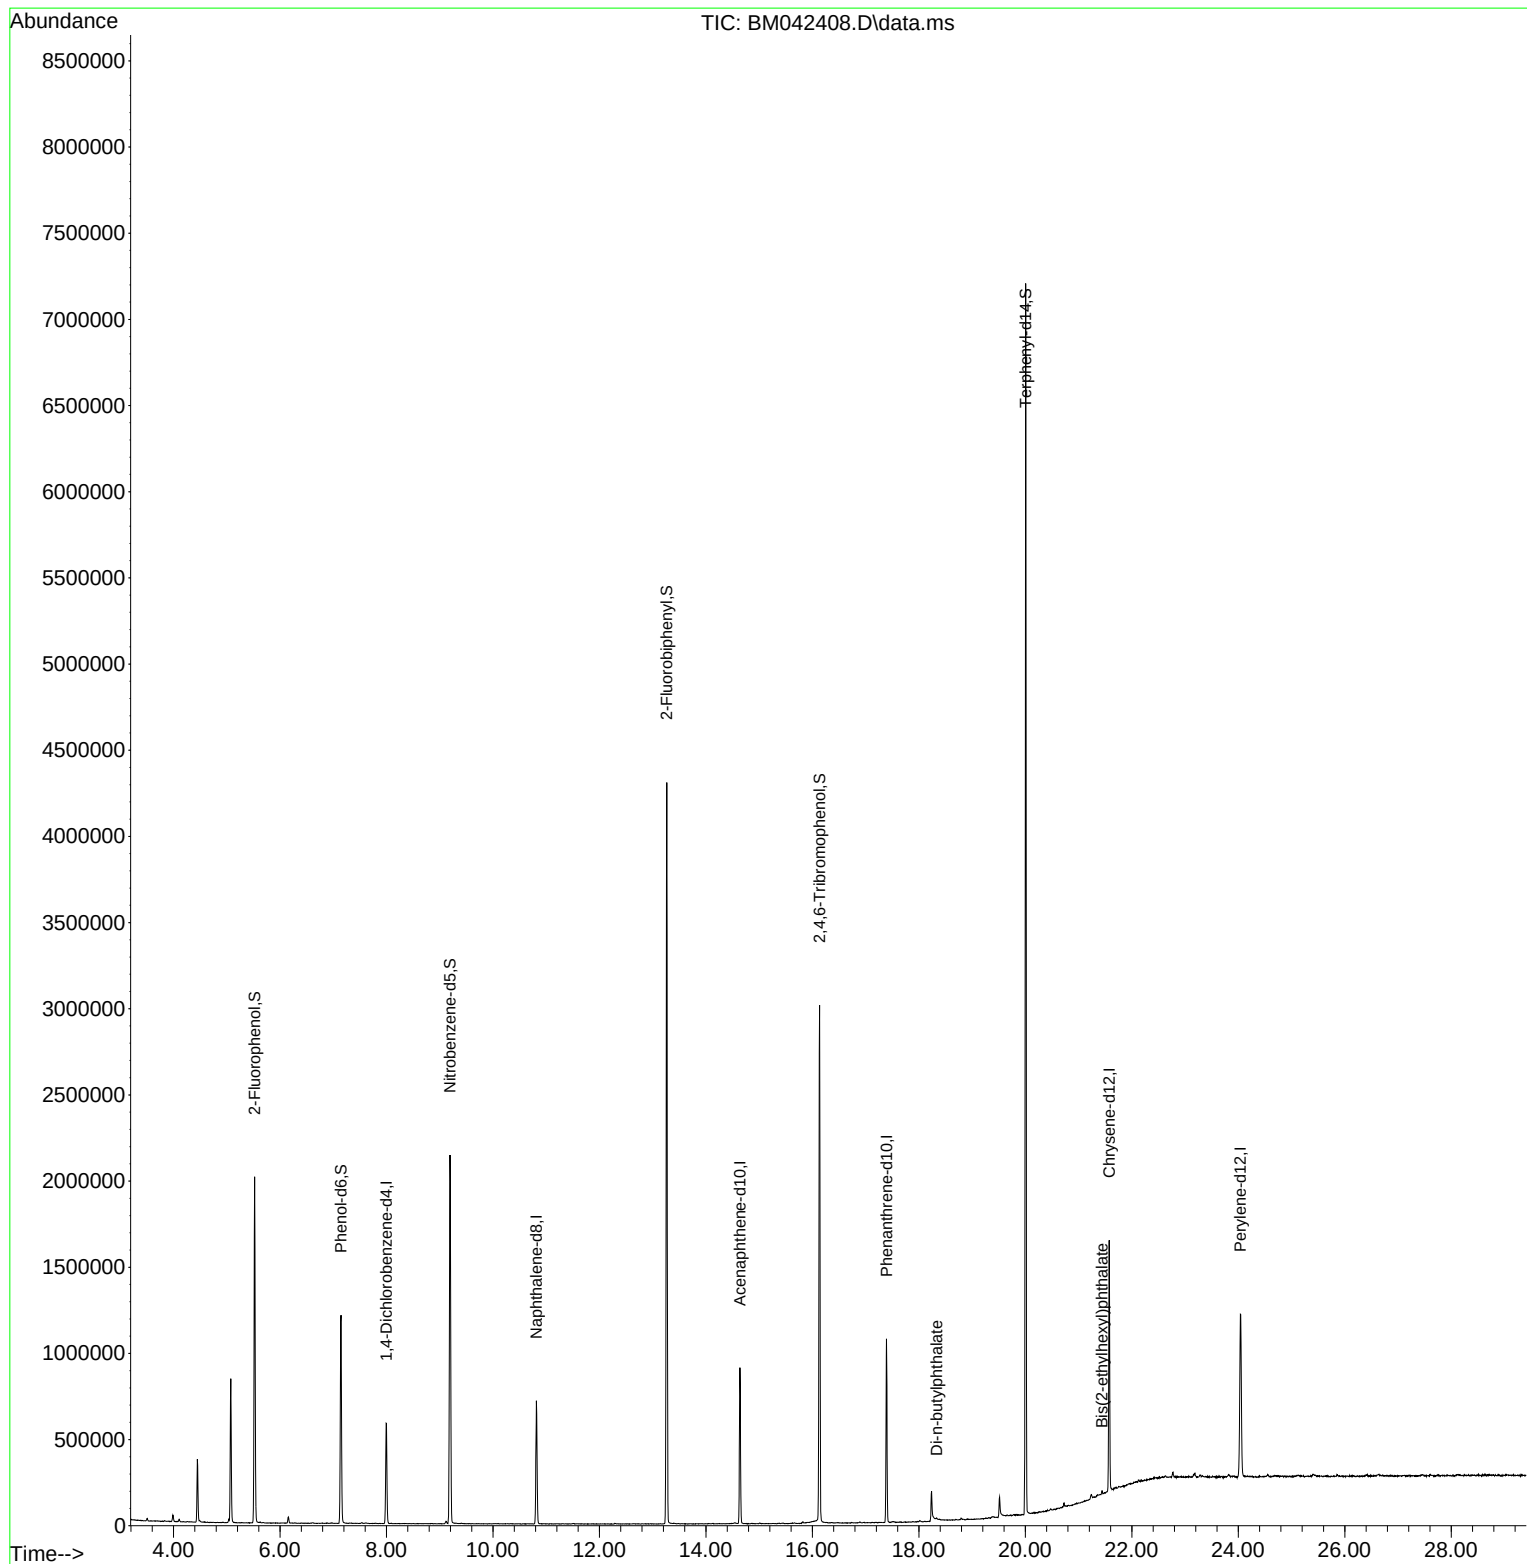




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 7.998 min Scan# 81
 Delta R.T. 0.000 min
 Lab File: BM042408.D
 Acq: 23 Oct 2023 18:46




Instrument :
 BNA_M
 ClientSampleId :
 MH-H


Tgt Ion:152 Resp: 142313
 Ion Ratio Lower Upper
 152 100
 150 155.5 126.2 189.4
 115 61.0 51.9 77.9

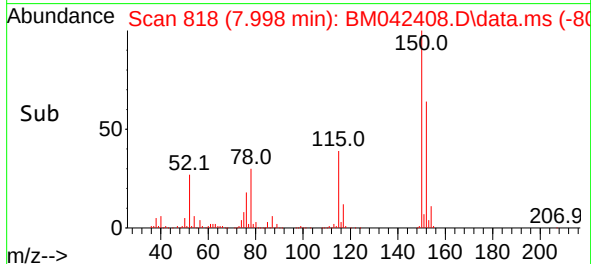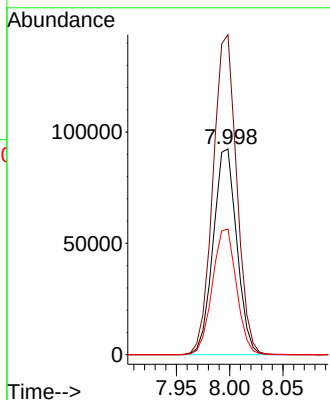

#5
 2-Fluorophenol
 Concen: 74.713 ng
 RT: 5.522 min Scan# 397
 Delta R.T. 0.000 min
 Lab File: BM042408.D
 Acq: 23 Oct 2023 18:46

Tgt Ion:112 Resp: 752320
 Ion Ratio Lower Upper
 112 100
 64 64.9 52.7 79.1
 63 33.8 28.3 42.5


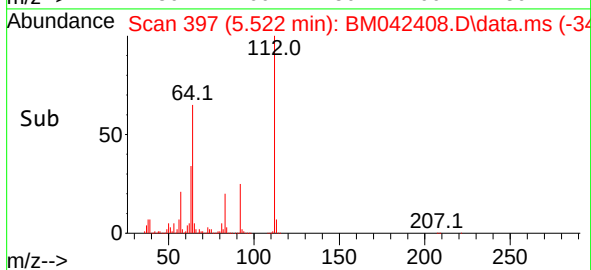
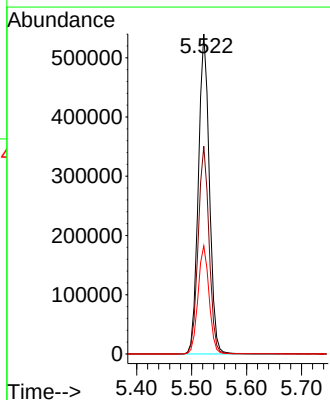
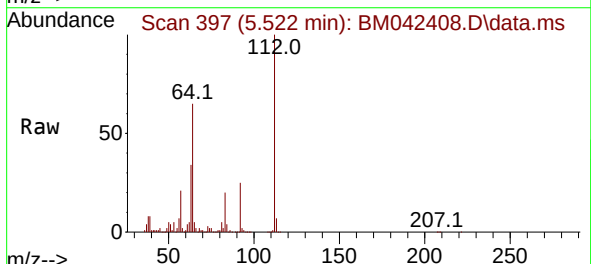




#7
Phenol-d6
Concen: 46.774 ng
RT: 7.146 min Scan# 61
Delta R.T. -0.006 min
Lab File: BM042408.D
Acq: 23 Oct 2023 18:46




Instrument :
BNA_M
ClientSampleId :
MH-H


Tgt Ion: 99 Resp: 631182
Ion Ratio Lower Upper
99 100
42 21.6 18.5 27.7
71 33.4 27.7 41.5

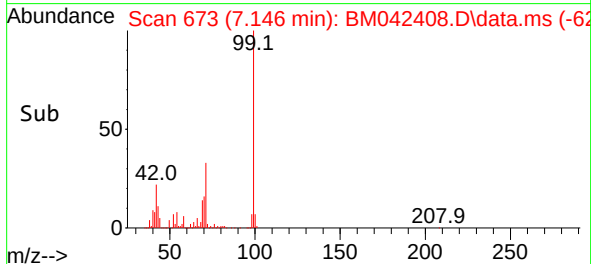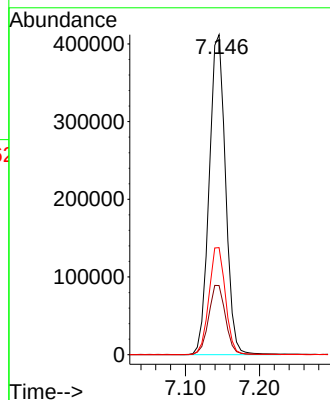

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.816 min Scan# 1297
Delta R.T. -0.006 min
Lab File: BM042408.D
Acq: 23 Oct 2023 18:46

Tgt Ion: 136 Resp: 536322
Ion Ratio Lower Upper
136 100
137 10.8 8.5 12.7
54 10.4 8.6 12.8
68 7.8 6.4 9.6


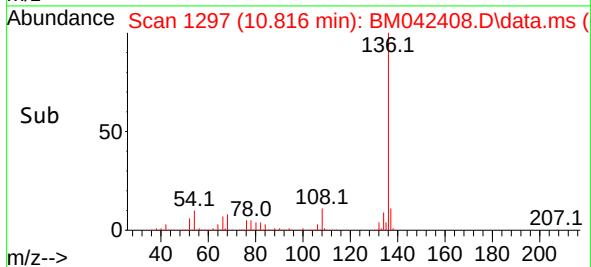
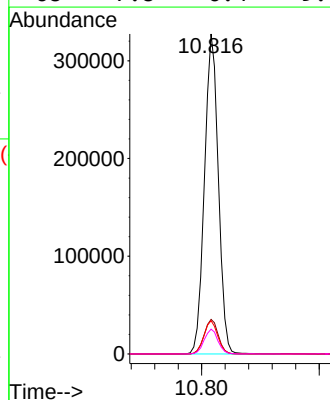
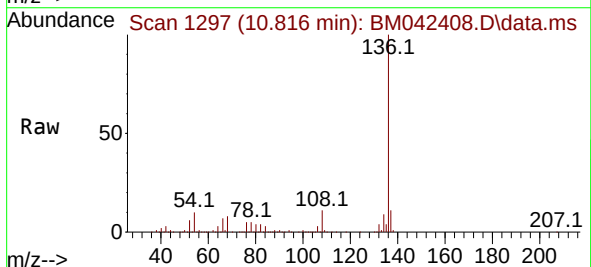




#23
Nitrobenzene-d5
Concen: 98.687 ng
RT: 9.192 min Scan# 1021
Delta R.T. -0.006 min
Lab File: BM042408.D
Acq: 23 Oct 2023 18:46




Instrument :
BNA_M
ClientSampleId :
MH-H


Tgt Ion: 82 Resp: 1196931
Ion Ratio Lower Upper
82 100
128 37.0 29.0 43.6
54 54.6 43.7 65.5

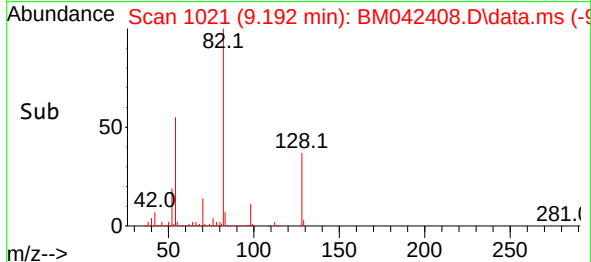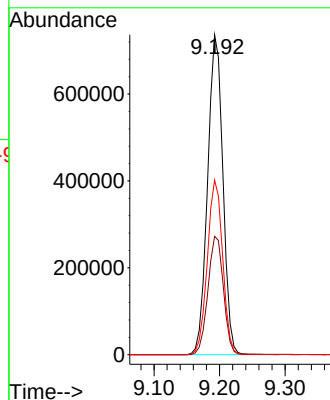

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.639 min Scan# 1947
Delta R.T. -0.006 min
Lab File: BM042408.D
Acq: 23 Oct 2023 18:46

Tgt Ion: 164 Resp: 271564
Ion Ratio Lower Upper
164 100
162 102.8 83.0 124.4
160 47.1 37.0 55.4


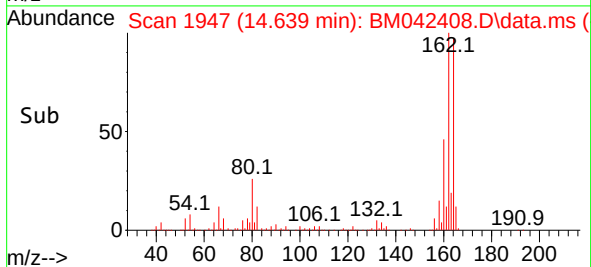
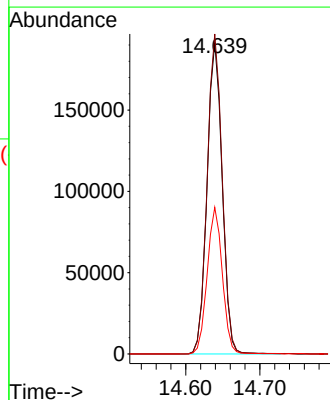
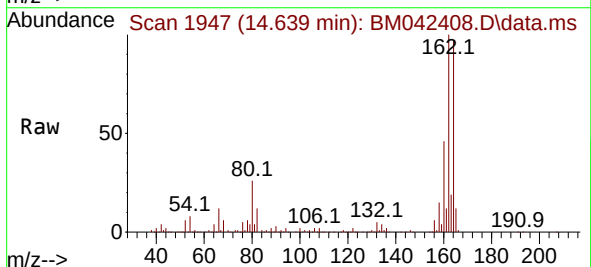




#42
2,4,6-Tribromophenol
Concen: 140.353 ng
RT: 16.133 min Scan# 21
Delta R.T. -0.006 min
Lab File: BM042408.D
Acq: 23 Oct 2023 18:46




Instrument :
BNA_M
ClientSampleId :
MH-H


Tgt Ion:330 Resp: 423303
Ion Ratio Lower Upper
330 100
332 97.4 77.6 116.4
141 41.9 38.0 57.0

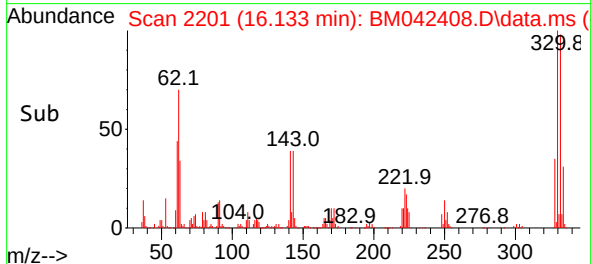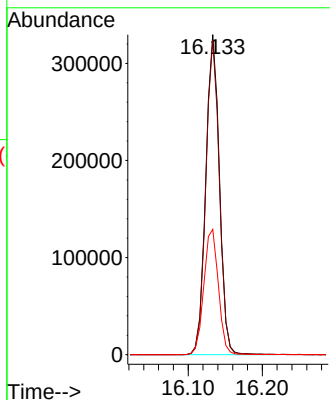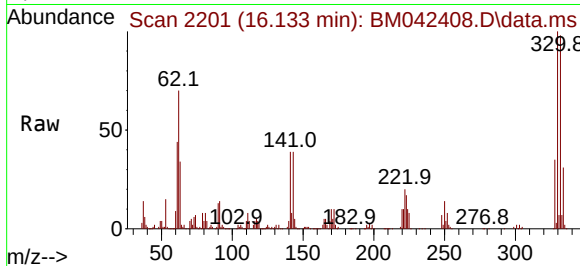

#45
2-Fluorobiphenyl
Concen: 99.436 ng
RT: 13.263 min Scan# 1713
Delta R.T. -0.006 min
Lab File: BM042408.D
Acq: 23 Oct 2023 18:46

Tgt Ion:172 Resp: 2005267
Ion Ratio Lower Upper
172 100
171 34.7 28.1 42.1
170 23.5 18.9 28.3

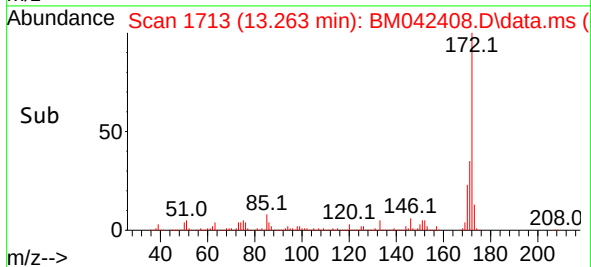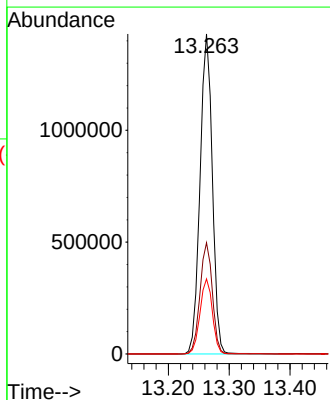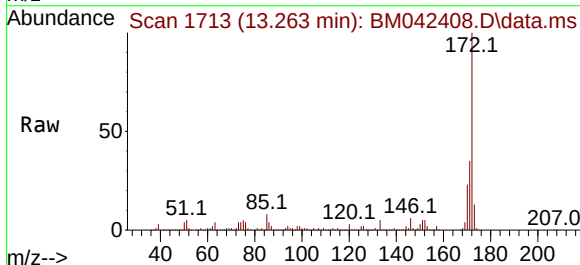



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.392 min Scan# 2416

Delta R.T. -0.006 min

Lab File: BM042408.D

Acq: 23 Oct 2023 18:46

Instrument :

BNA_M

ClientSampleId :

MH-H





Tgt Ion:188 Resp: 562605

Ion Ratio Lower Upper

188 100

94 11.3 9.4 14.0

80 13.6 10.7 16.1

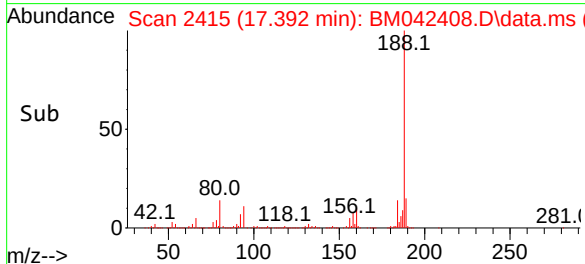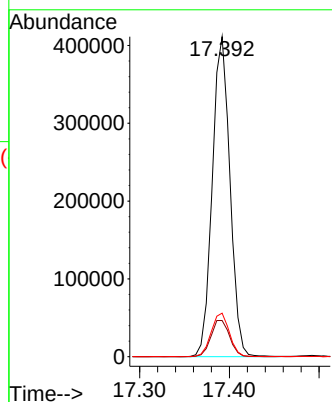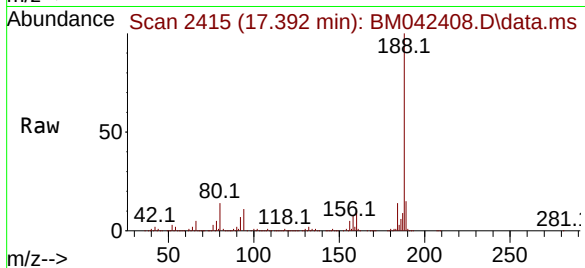

#74

Di-n-butylphthalate

Concen: 2.976 ng

RT: 18.333 min Scan# 2575

Delta R.T. -0.006 min

Lab File: BM042408.D

Acq: 23 Oct 2023 18:46




Tgt Ion:149 Resp: 6060


Ion Ratio Lower Upper

149 100

150 10.6 7.4 11.0

104 9.5 4.6 7.0#

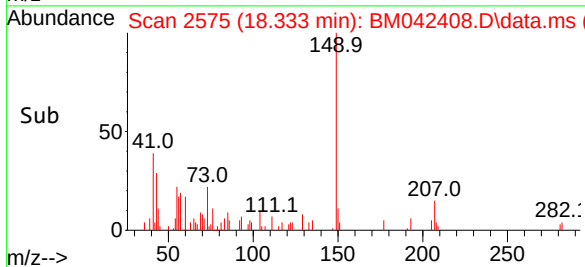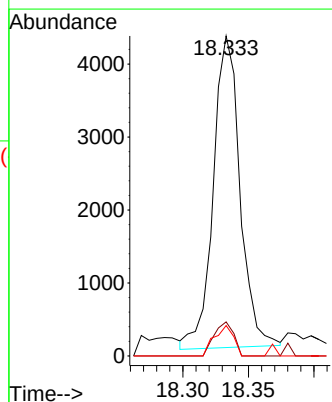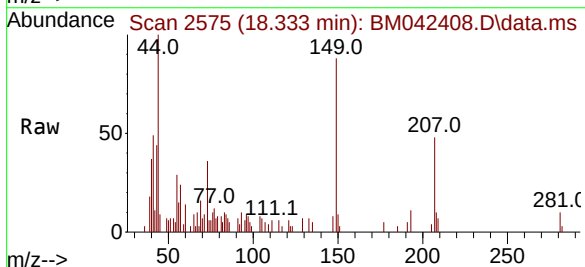



#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.574 min Scan# 31

Delta R.T. -0.006 min

Lab File: BM042408.D

Acq: 23 Oct 2023 18:46

Instrument :

BNA_M

ClientSampleId :

MH-H





Tgt Ion:240 Resp: 577587

Ion Ratio Lower Upper

240 100

120 14.1 10.7 16.1

236 25.8 20.7 31.1

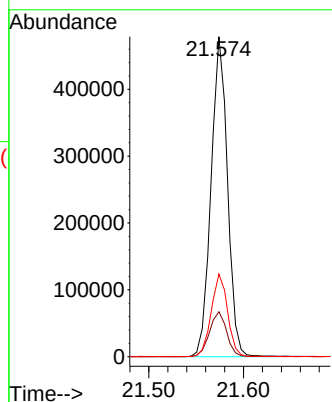

#79

Terphenyl-d14

Concen: 96.064 ng

RT: 20.003 min Scan# 2859

Delta R.T. -0.006 min

Lab File: BM042408.D

Acq: 23 Oct 2023 18:46




Tgt Ion:244 Resp: 3128583


Ion Ratio Lower Upper

244 100

212 7.0 5.6 8.4

122 11.3 8.8 13.2


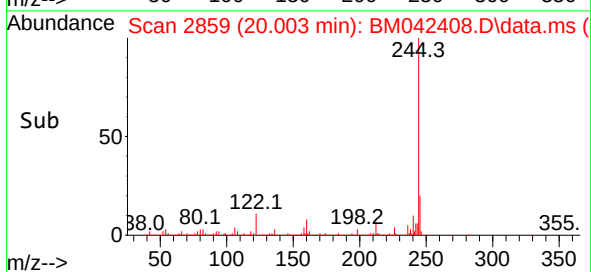
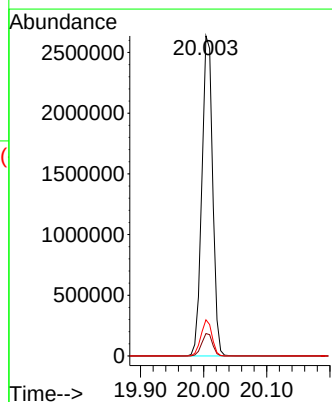





#84
 Bis(2-ethylhexyl)phthalate
 Concen: 3.585 ng
 RT: 21.439 min Scan# 3103
 Delta R.T. -0.006 min
 Lab File: BM042408.D
 Acq: 23 Oct 2023 18:46

Instrument :
 BNA_M
 ClientSampleId :
 MH-H

Tgt Ion:149 Resp: 6068
 Ion Ratio Lower Upper
 149 100
 167 20.8 20.9 31.3#
 279 4.4 2.7 4.1#

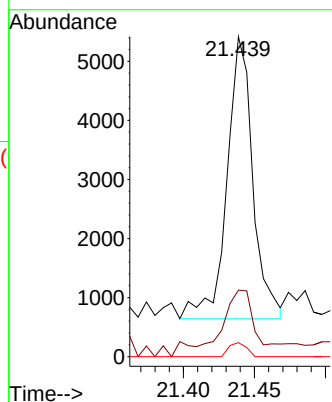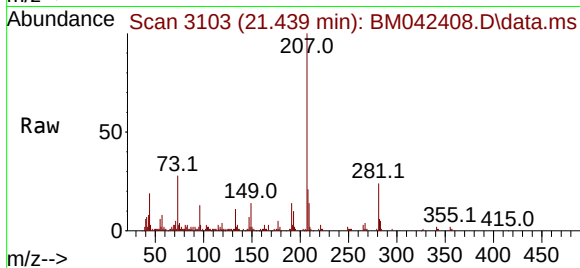

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.039 min Scan# 3545
 Delta R.T. -0.006 min
 Lab File: BM042408.D
 Acq: 23 Oct 2023 18:46

Tgt Ion:264 Resp: 660594
 Ion Ratio Lower Upper
 264 100
 260 23.4 18.6 27.8
 265 21.7 17.8 26.8

