


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102323\
 Data File : BM042393.D
 Acq On : 23 Oct 2023 08:47
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Oct 21 02:32:53 2023

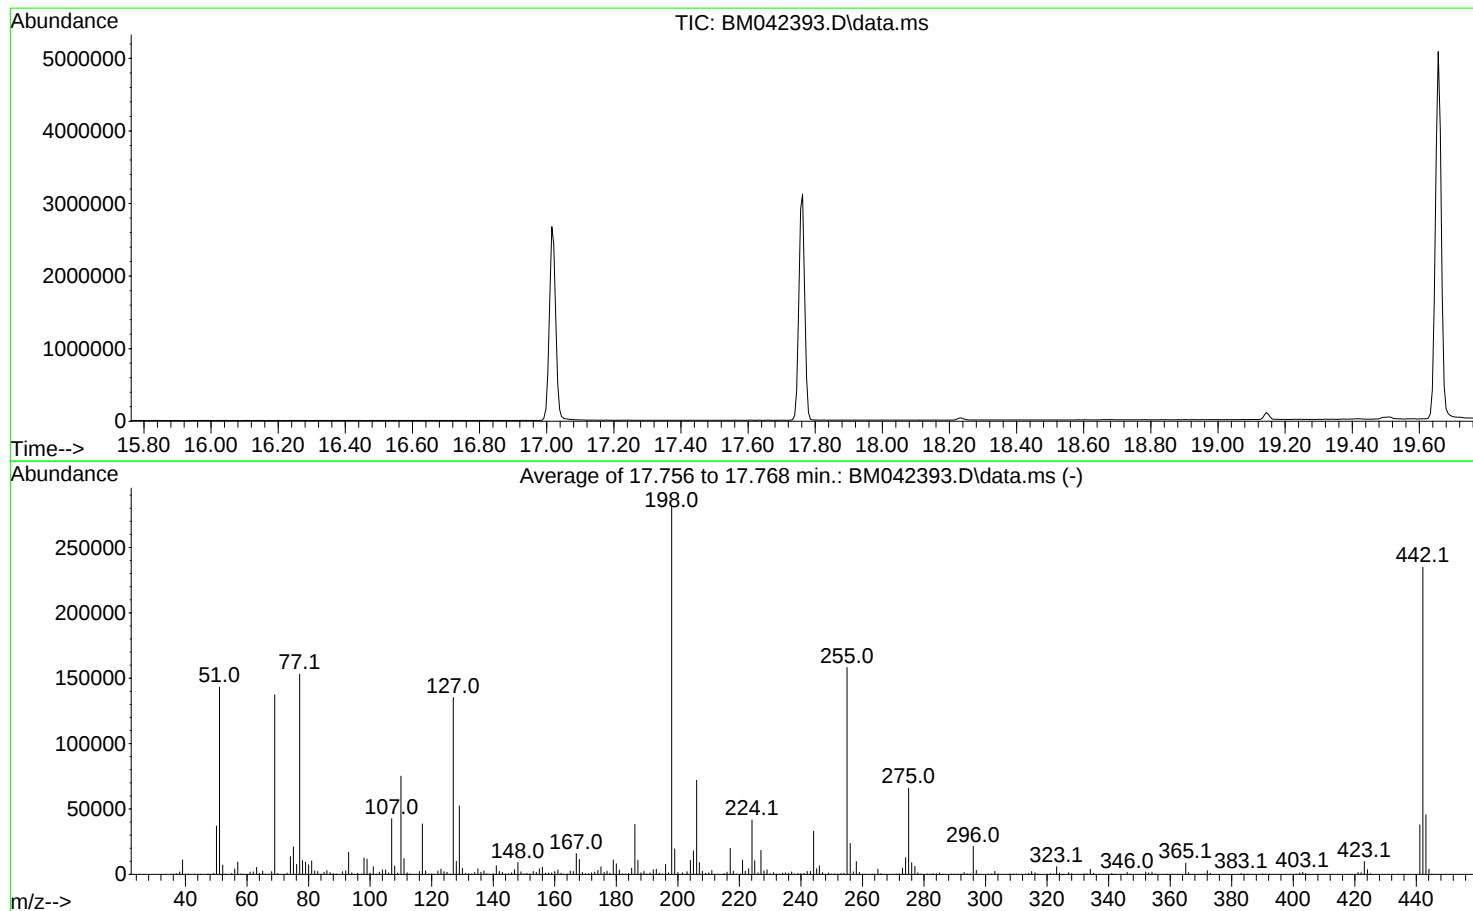




AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.9	143184	PASS
68	69	0.00	2	1.5	2061	PASS
69	198	0.00	100	48.8	137245	PASS
70	69	0.00	2	0.5	701	PASS
127	198	10	80	48.1	135251	PASS
197	198	0.00	2	0.4	1175	PASS
198	198	100	100	100.0	281323	PASS
199	198	5	9	6.9	19411	PASS
275	198	10	60	23.4	65915	PASS
365	198	1	100	3.0	8561	PASS
441	198	0.01	100	13.5	37840	PASS
442	442	50	100	100.0	234880	PASS
443	442	15	24	19.4	45539	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102323\
Data File : BM042393.D
Acq On : 23 Oct 2023 08:47
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Oct 23 09:34:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 21 02:32:53 2023
Response via : Initial Calibration

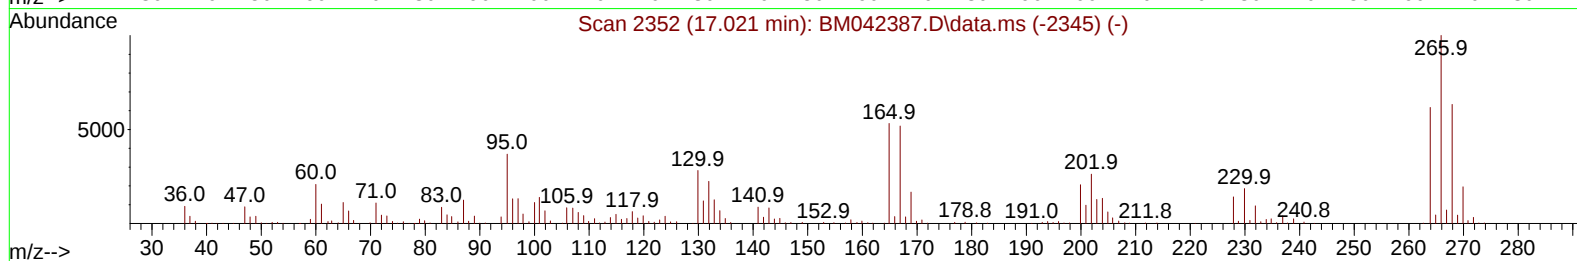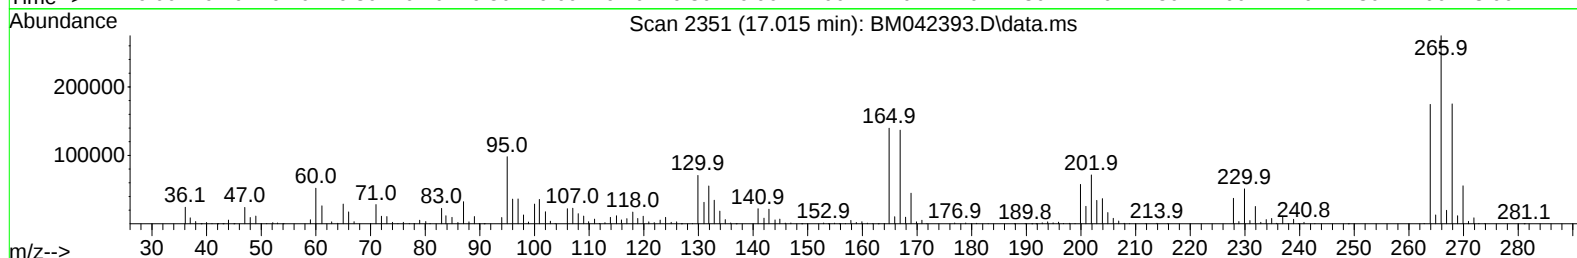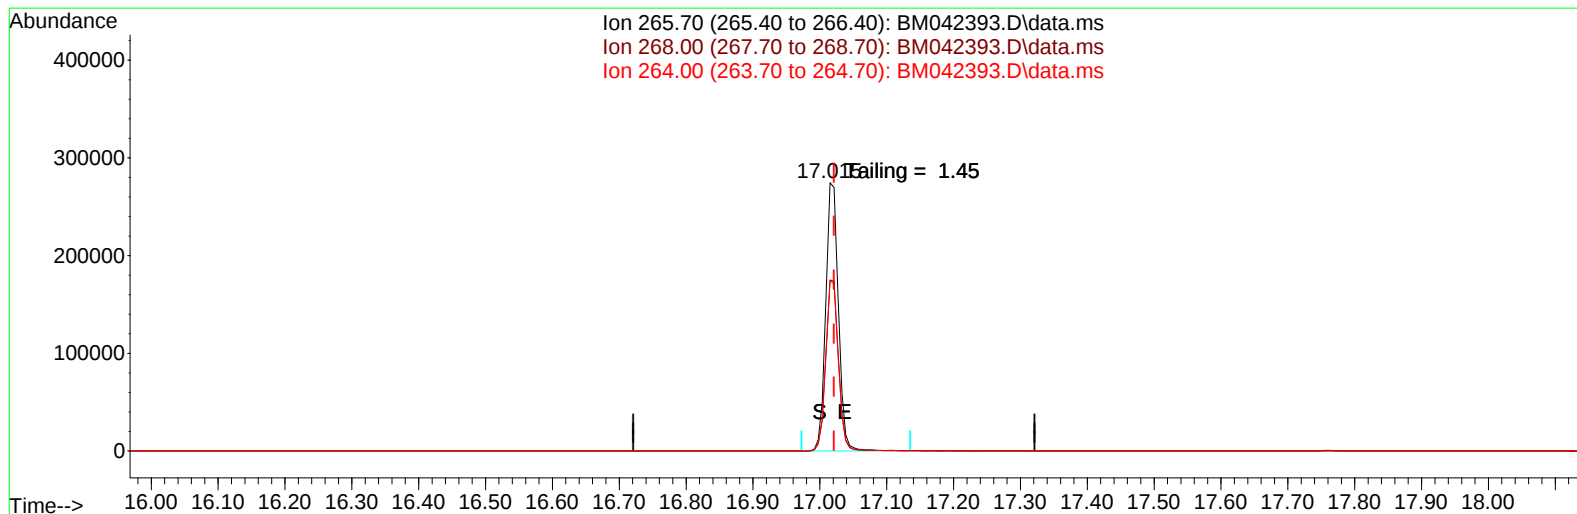

TIC: BM042393.D\data.ms

(70) Pentachlorophenol (C)

17.015min (-0.006) 0.00 ng m




response 362086

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	63.77
264.00	61.70	63.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102323\
Data File : BM042393.D
Acq On : 23 Oct 2023 08:47
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Oct 23 09:34:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 21 02:32:53 2023
Response via : Initial Calibration

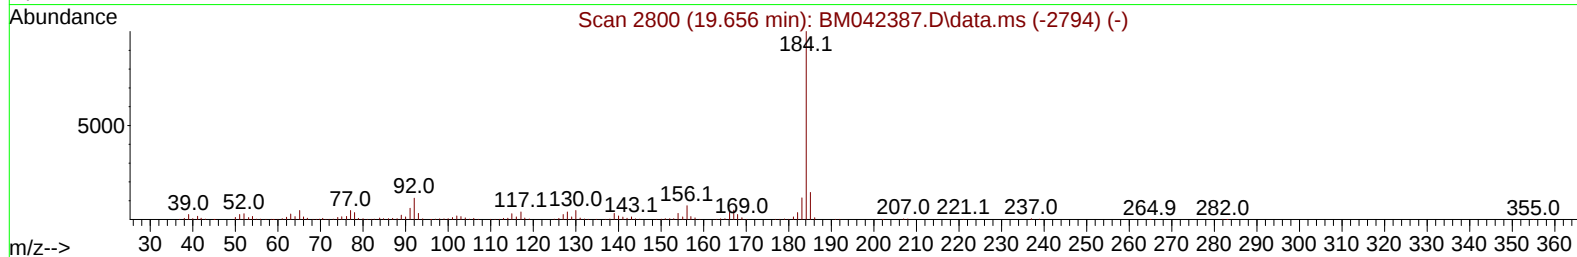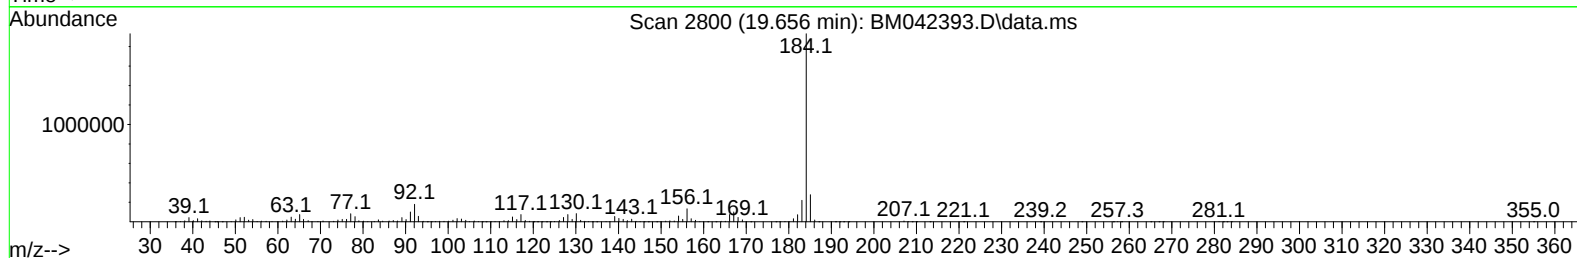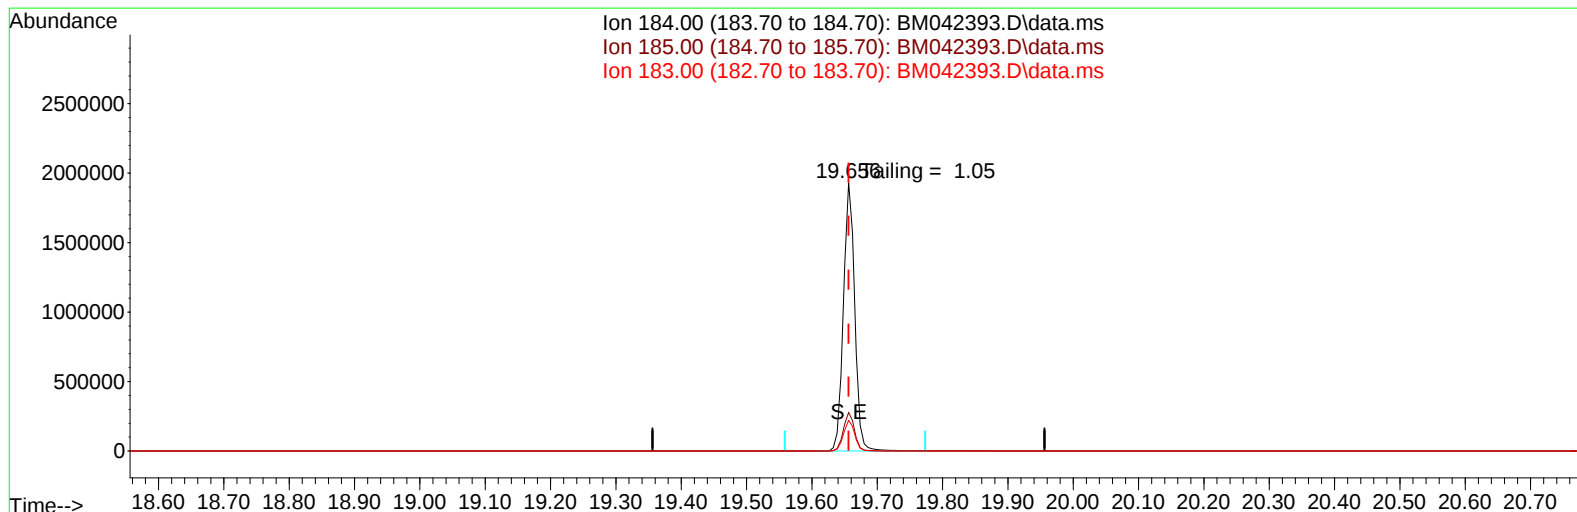

TIC: BM042393.D\data.ms

(77) Benzidine

19.656min (-0.000) 0.00 ng m

response 2327562

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.40
183.00	11.50	11.44
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/23/2023	BNA_M	<u>BM042393.D</u>
Compound Name	Response	Retention Time
DDT	1038833	20.844
DDD	8236	20.456
DDE	114	19.897
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8350	1047183	0.80

Instrument :
BNA_M
ClientSampleId :
DFTPP