

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM102418\
 Data File : BM017326.D
 Acq On : 24 Oct 2018 20:29
 Operator : MJ/SJ
 Sample : J5598-15
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AE3

Manual Integrations
 APPROVED

Sohil
 10/25/2018 3:34:06 PM

Quant Time: Oct 25 02:25:50 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 25 01:24:17 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	265086	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1203665	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.30	164	727068	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.05	188	1740080	20.00	ng/ul	0.00
78) Chrysene-d12	21.24	240	2132557	20.00	ng/ul	0.00
86) Perylene-d12	23.45	264	2374602	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	17837m	3.10	ng/uL	0.00
5) Phenol-d5	6.83	99	401636	16.59	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	261487	18.52	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	339241	18.07	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	344601	18.00	ng/ul	0.00
19) Nitrobenzene-d5	8.81	128	172091	18.29	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	191176	18.12	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	344791	17.60	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	446743	27.93	ng/ul	0.00
44) Dimethylphthalate-d6	13.72	166	1325044	21.25	ng/ul	0.00
47) Acenaphthylene-d8	13.99	160	1502667	19.85	ng/ul	0.00
52) 4-Nitrophenol-d4	14.53	143	158058	13.57	ng/ul	0.00
58) Fluorene-d10	15.30	176	1132713	20.92	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.42	200	174391	14.38	ng/ul	0.00
71) Anthracene-d10	17.14	188	1905796	22.13	ng/ul	0.00
79) Pyrene-d10	19.45	212	2315847	23.44	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.32	264	2944623	23.48	ng/ul	0.00

Target Compounds

					Qvalue
6) Phenol	6.86	94	92628	3.852	ng/ul 97
45) Dimethylphthalate	13.76	163	177846	2.944	ng/ul 100
77) Fluoranthene	19.11	202	598329	5.224	ng/ul 100
80) Pyrene	19.47	202	788106	6.364	ng/ul 99
83) Benzo(a)anthracene	21.23	228	455382	3.489	ng/ul 97
85) Chrysene	21.28	228	713189	5.747	ng/ul 99
88) Benzo(b)fluoranthene	22.79	252	1151735	8.286	ng/ul# 98
89) Benzo(k)fluoranthene	22.83	252	356023m	2.622	ng/ul
91) Benzo(a)pyrene	23.36	252	387520	2.854	ng/ul 97
92) Indeno(1,2,3-cd)pyrene	25.65	276	315673	1.911	ng/ul 95
94) Benzo(g,h,i)perylene	26.33	276	238048	1.696	ng/ul 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM102418\
Data File : BM017326.D
Acq On : 24 Oct 2018 20:29
Operator : MJ/SJ
Sample : J5598-15
Misc :
ALS Vial : 18 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
C0AE3

Manual Integrations
APPROVED

Sohil
10/25/2018 3:34:06 PM

Quant Time: Oct 25 02:25:50 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 25 01:24:17 2018
Response via : Initial Calibration

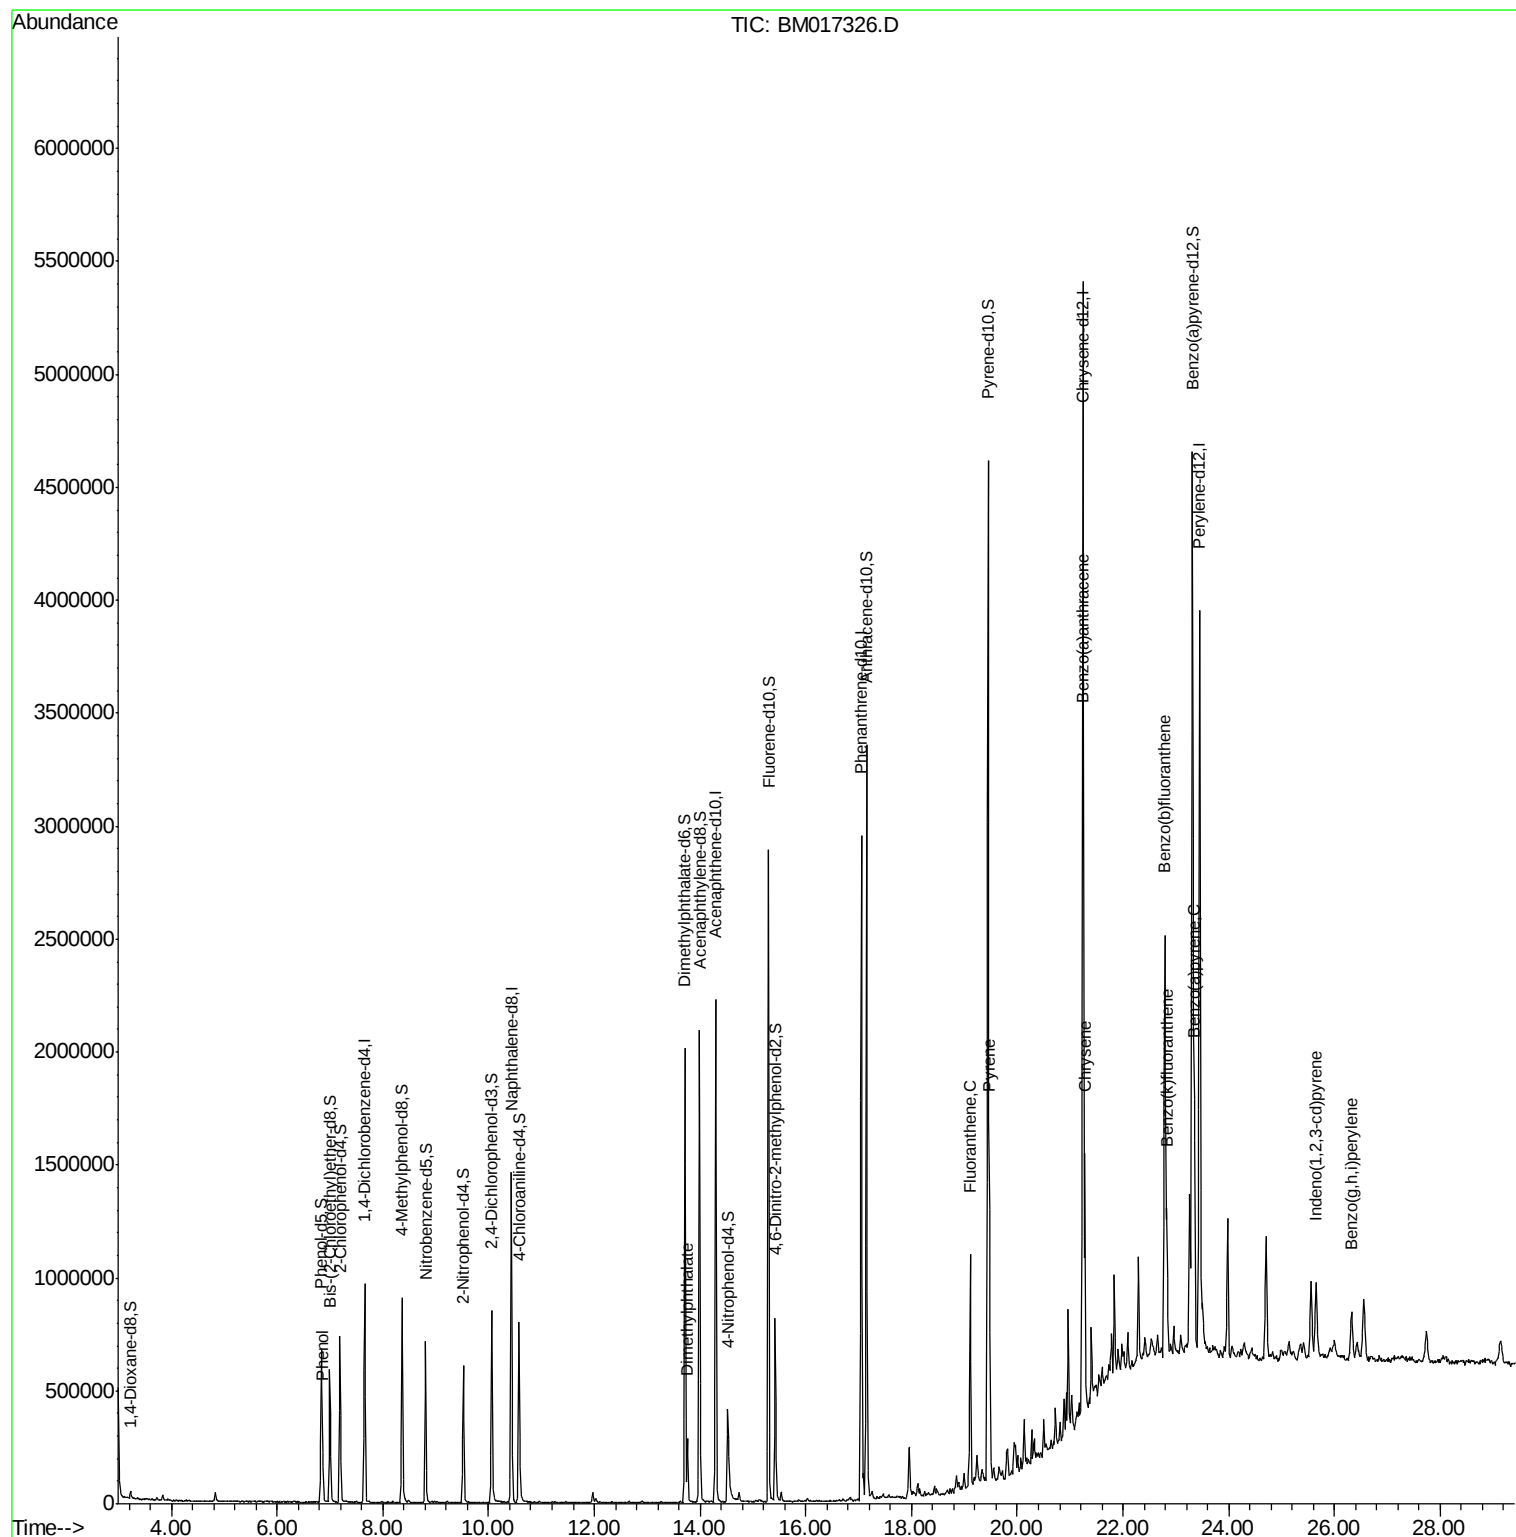

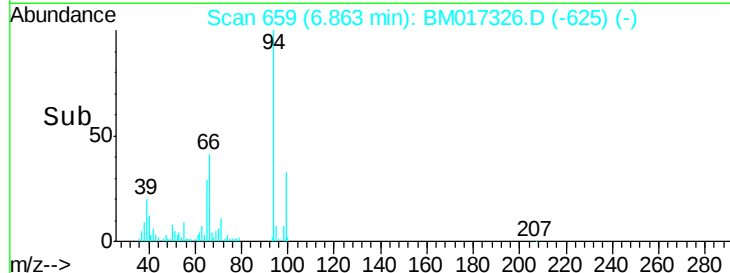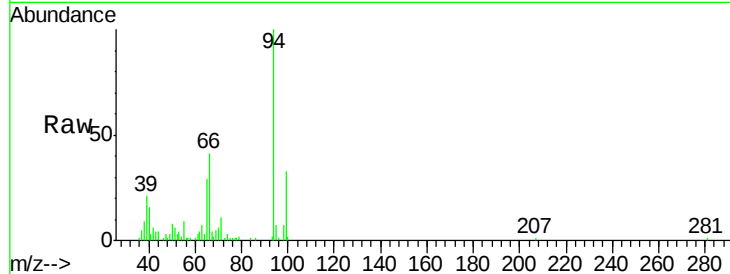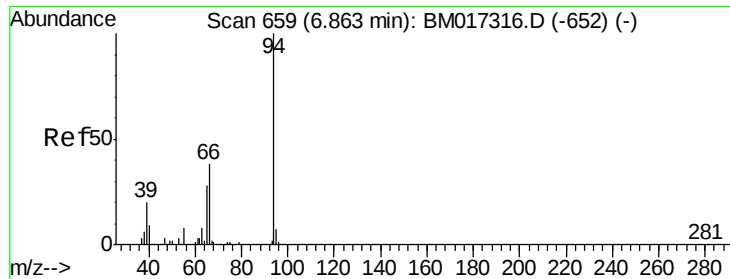





#6
Phenol
Concen: 3.852 ng/ul
RT: 6.86 min Scan# 659
Delta R.T. 0.00 min
Lab File: BM017326.D
Acq: 24 Oct 2018 20:29

Tgt Ion	Ratio	Lower	Upper
94	100		
65	29.3	24.0	36.0
66	41.4	31.1	46.7

Instrument :
BNA_M
ClientSampleId :
C0AE3


Manual Integrations
APPROVED


Sohil
10/25/2018 3:34:06 PM

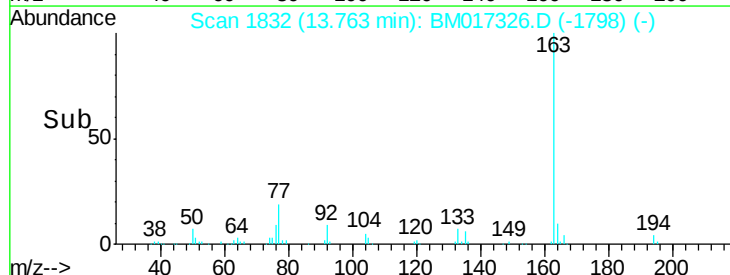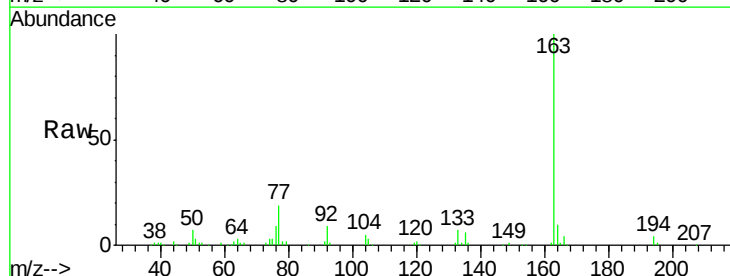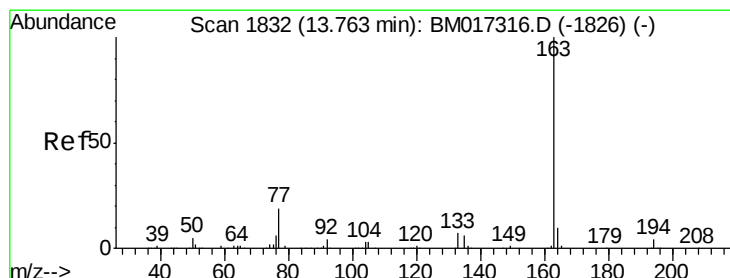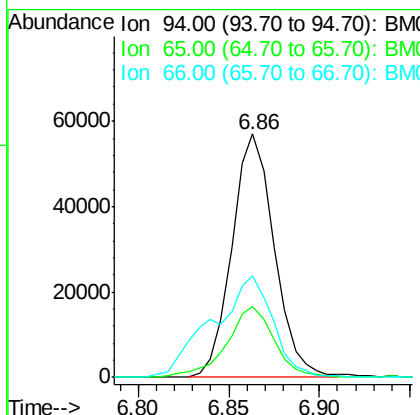

#45
Dimethylphthalate
Concen: 2.944 ng/ul
RT: 13.76 min Scan# 1832
Delta R.T. 0.00 min
Lab File: BM017326.D
Acq: 24 Oct 2018 20:29

Tgt Ion	Ratio	Lower	Upper
163	100		
194	3.8	3.2	4.8
164	10.1	8.1	12.1

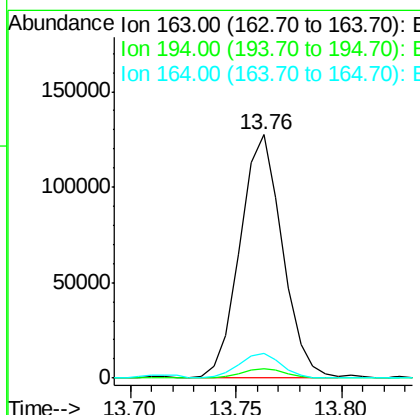

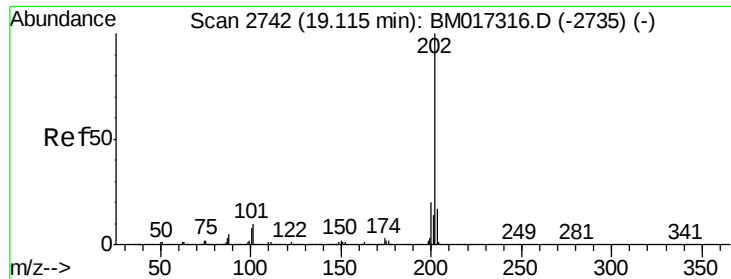





#77
Fluoranthene
 Concen: 5.224 ng/ul
 RT: 19.11 min Scan# 2741
 Delta R.T. -0.01 min
 Lab File: BM017326.D
 Acq: 24 Oct 2018 20:29

Instrument :
 BNA_M
 ClientSampleId :
 C0AE3

Tgt Ion	Ratio	Resp Lower	Resp Upper
202	100		
101	10.6	8.2	12.4
100	7.9	6.3	9.5




Manual Integrations
 APPROVED


Sohil
 10/25/2018 3:34:06 PM

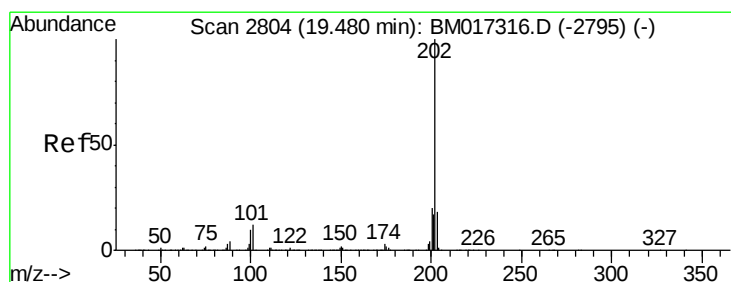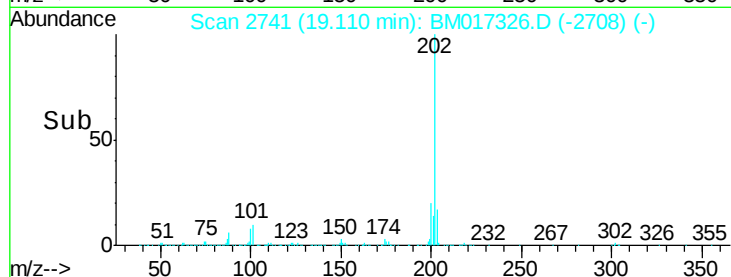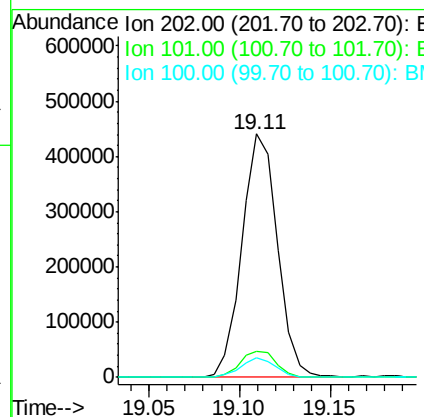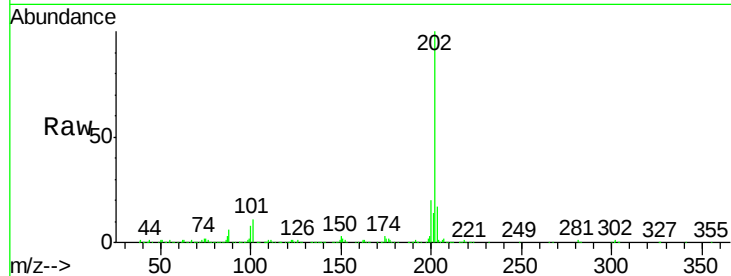

#80
Pyrene
 Concen: 6.364 ng/ul
 RT: 19.47 min Scan# 2803
 Delta R.T. -0.01 min
 Lab File: BM017326.D
 Acq: 24 Oct 2018 20:29

Tgt Ion	Ratio	Resp Lower	Resp Upper
202	100		
101	12.3	9.5	14.3
100	10.2	8.1	12.1

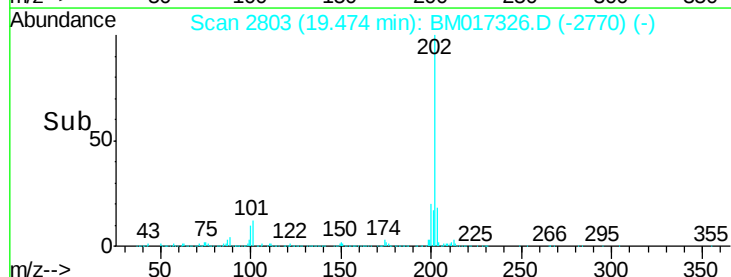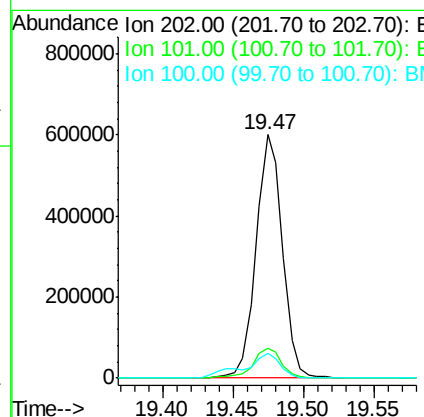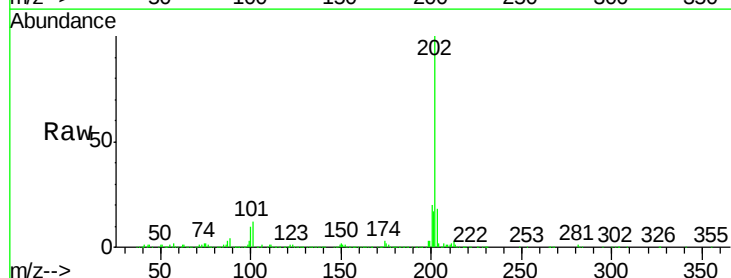

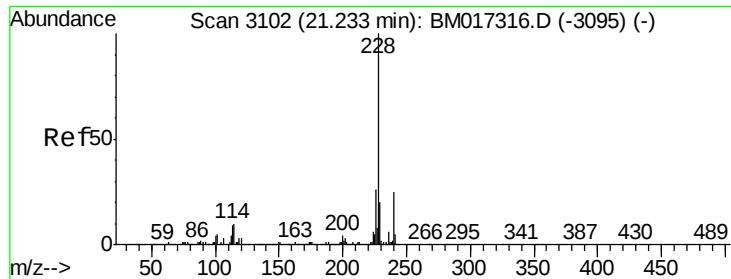





#83
Benzo(a)anthracene
Concen: 3.489 ng/ul
RT: 21.23 min Scan# 3101
Delta R.T. -0.01 min
Lab File: BM017326.D
Acq: 24 Oct 2018 20:29

Instrument :
BNA_M
ClientSampled :
C0AE3

Tgt Ion	Ratio	Lower	Upper
228	100		
229	20.5	15.6	23.4
226	27.8	20.8	31.2




Manual Integrations
APPROVED


Sohil
10/25/2018 3:34:06 PM

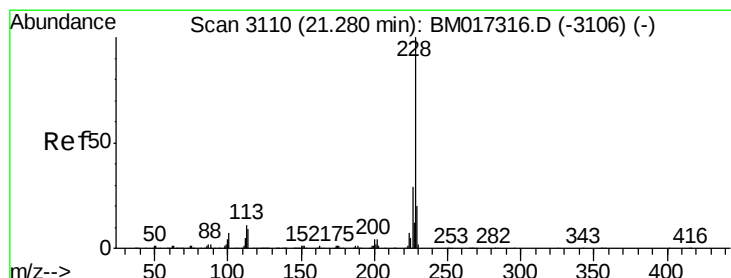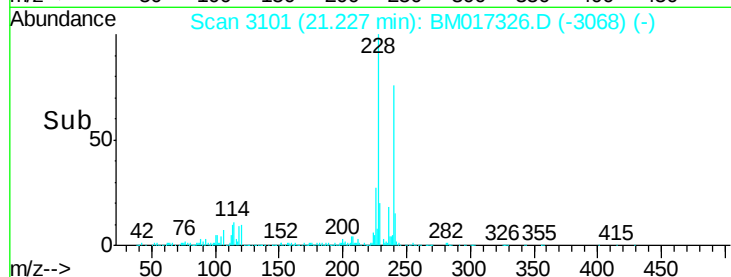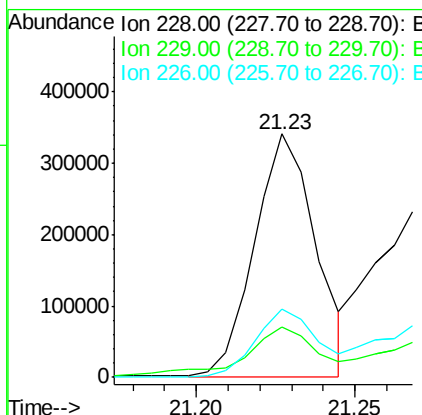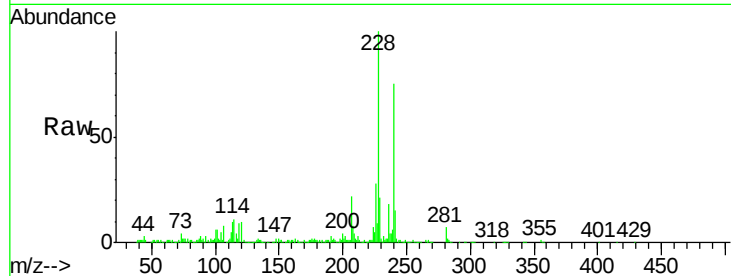

#85
Chrysene
Concen: 5.747 ng/ul
RT: 21.28 min Scan# 3110
Delta R.T. 0.00 min
Lab File: BM017326.D
Acq: 24 Oct 2018 20:29

Tgt Ion	Ratio	Lower	Upper
228	100		
226	29.2	23.3	34.9
229	20.6	15.6	23.4

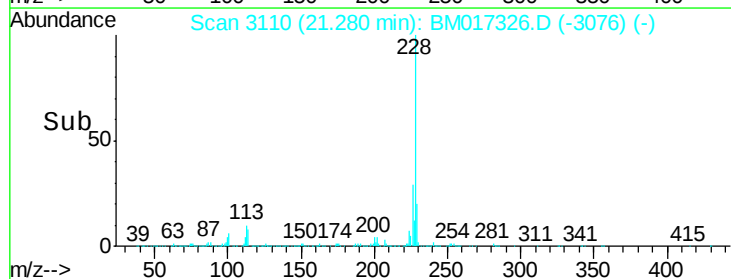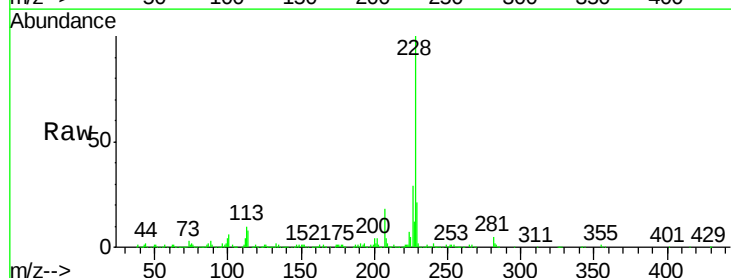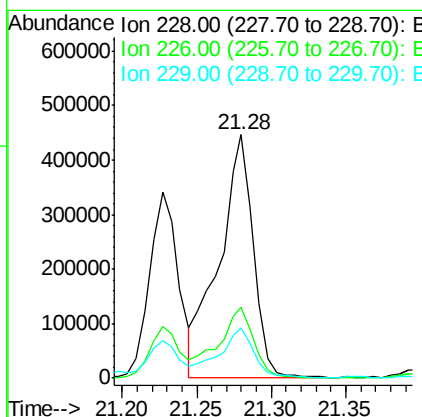

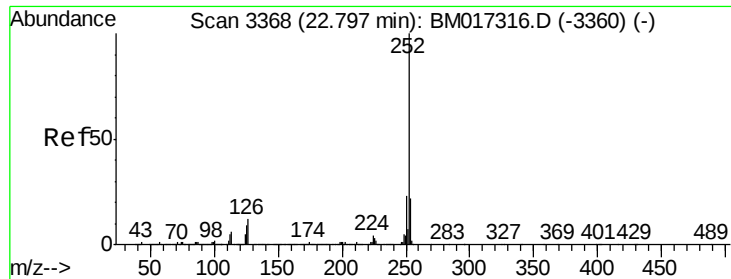





#88
Benzo(b)fluoranthene
Concen: 8.286 ng/ul
RT: 22.79 min Scan# 3367
Delta R.T. -0.01 min
Lab File: BM017326.D
Acq: 24 Oct 2018 20:29

Instrument :
BNA_M
ClientSampleId :
C0AE3

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.3	17.6	26.4
125	11.3	7.2	10.8




Manual Integrations
APPROVED


Sohil
10/25/2018 3:34:06 PM

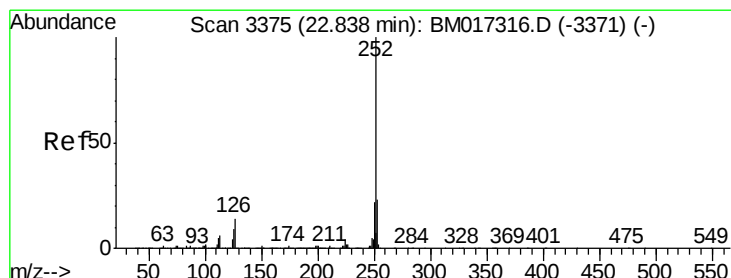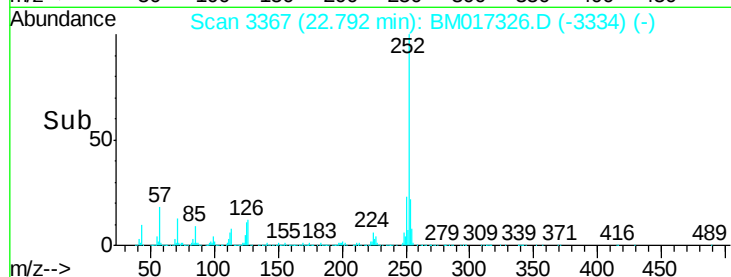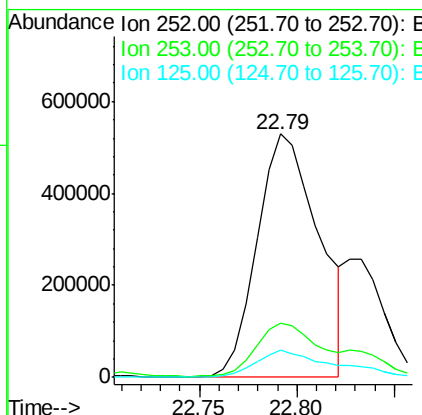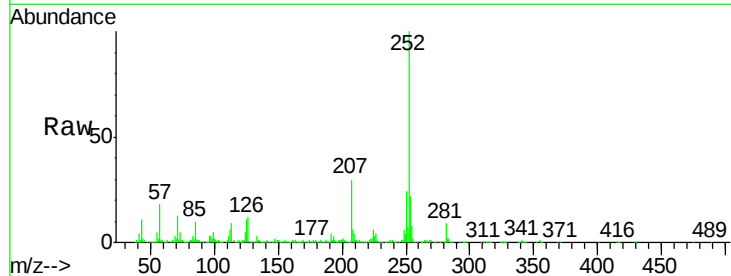

#89
Benzo(k)fluoranthene
Concen: 2.622 ng/ul m
RT: 22.83 min Scan# 3374
Delta R.T. -0.01 min
Lab File: BM017326.D
Acq: 24 Oct 2018 20:29

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.2	17.7	26.5
125	9.2	7.8	11.6

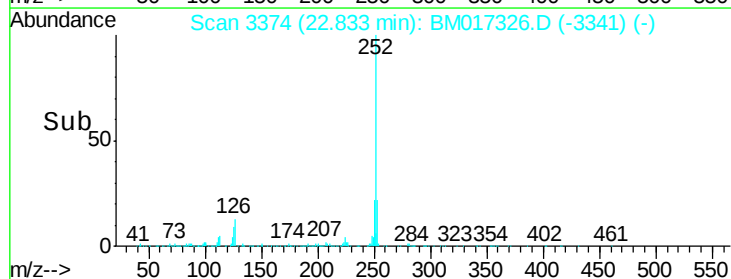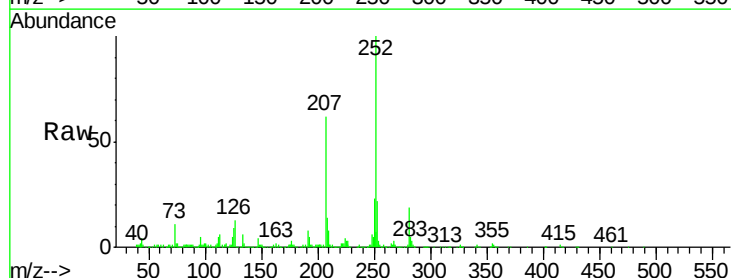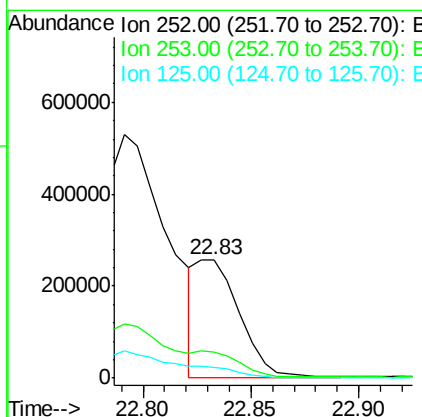

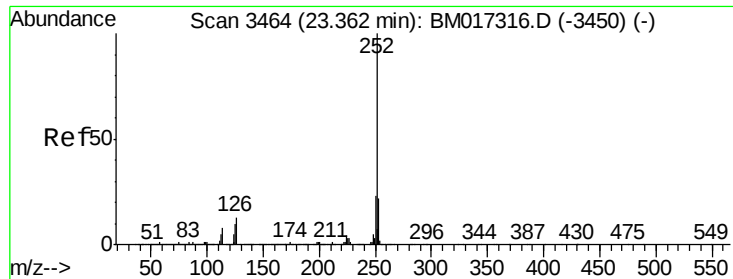





#91
Benzo(a)pyrene
Concen: 2.854 ng/ul
RT: 23.36 min Scan# 3463
Delta R.T. -0.01 min
Lab File: BM017326.D
Acq: 24 Oct 2018 20:29

Instrument :
BNA_M
ClientSampleId :
C0AE3

Tgt Ion	Ratio	Resp Lower	Resp Upper
252	100		
253	23.4	17.6	26.4
125	12.0	8.3	12.5




Manual Integrations
APPROVED


Sohil
10/25/2018 3:34:06 PM

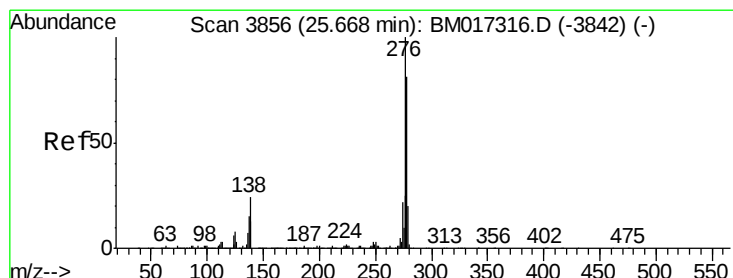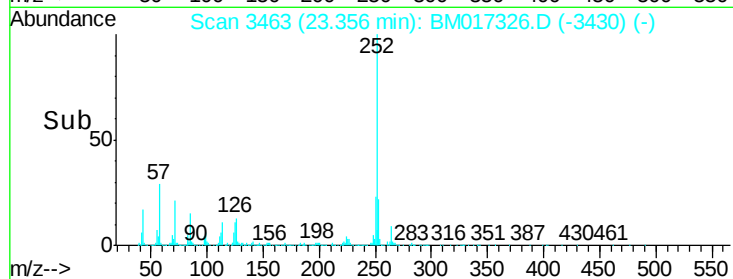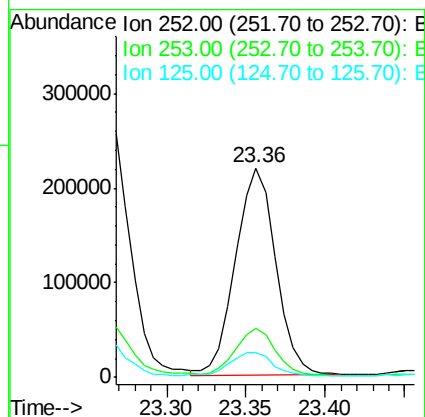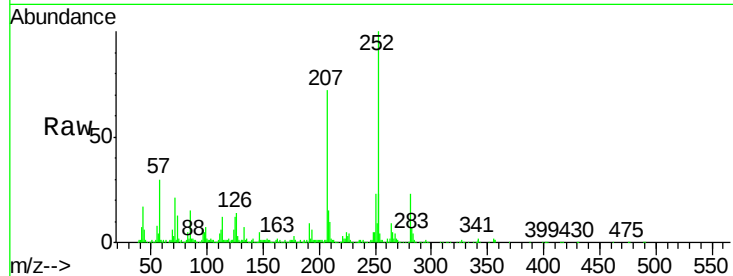

#92
Indeno(1,2,3-cd)pyrene
Concen: 1.911 ng/ul
RT: 25.65 min Scan# 3853
Delta R.T. -0.02 min
Lab File: BM017326.D
Acq: 24 Oct 2018 20:29

Tgt Ion	Ratio	Resp Lower	Resp Upper
276	100		
138	18.4	18.1	27.1
277	23.4	19.6	29.4

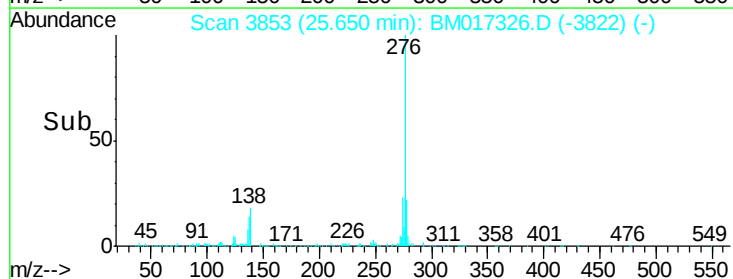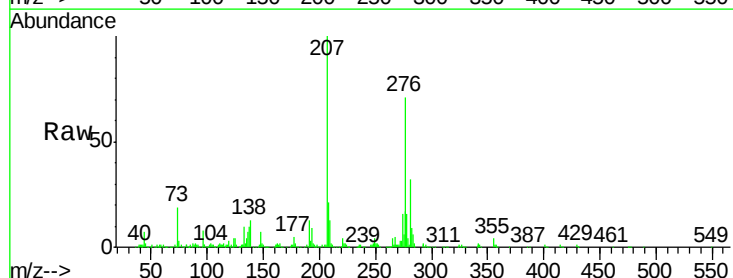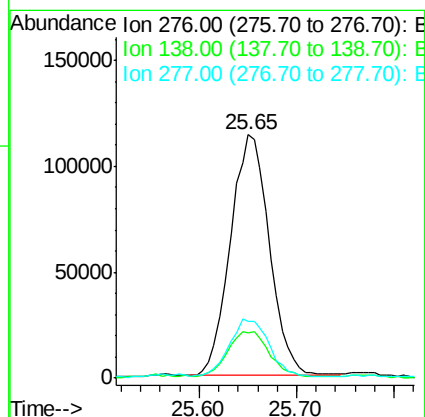

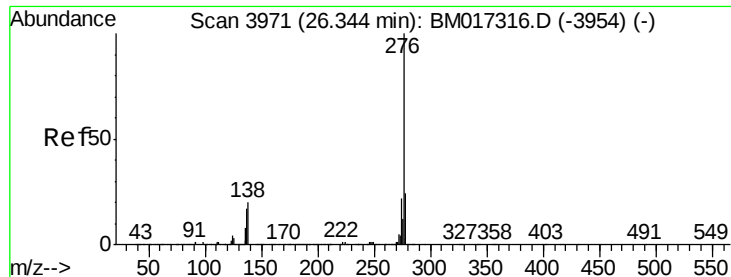

#94

Benzo(g,h,i)perylene

Concen: 1.696 ng/ul

RT: 26.33 min Scan# 3968

Delta R.T. -0.02 min

Lab File: BM017326.D


Acq: 24 Oct 2018 20:29

Instrument :

BNA_M

ClientSampleId :

C0AE3

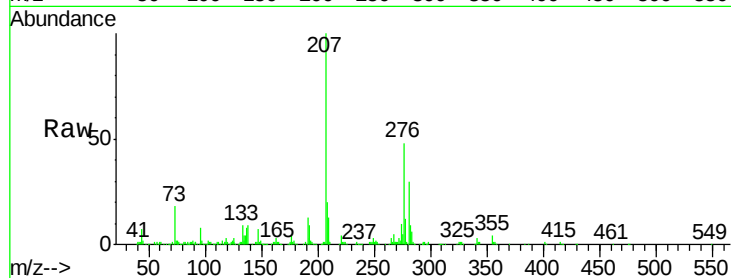

Tgt Ion: 276 Resp: 238048

Ion Ratio Lower Upper

276 100

138 19.3 16.6 25.0

277 24.0 18.9 28.3

Manual Integrations

APPROVED

Sohil

10/25/2018 3:34:06 PM

