

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102419\
 Data File : BM023396.D
 Acq On : 25 Oct 2019 05:25
 Operator : JU
 Sample : K5403-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Oct 25 11:52:53 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 23 18:47:16 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	618031	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	2382625	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	1280179	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	2049199	20.00	ng/ul	0.00
78) Chrysene-d12	21.23	240	1766303	20.00	ng/ul	0.00
86) Perylene-d12	23.43	264	2318122	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	551	0.04	ng/uL	0.00
5) Phenol-d5	6.66	99	365	0.01	ng/ul	-0.16
7) Bis-(2-Chloroethyl)ether-d	6.97	67	465	0.02	ng/ul	-0.01
9) 2-Chlorophenol-d4	0.00	132	0	0.00	ng/ul	
13) 4-Methylphenol-d8	8.32	113	114	0.00	ng/ul	-0.03
19) Nitrobenzene-d5	8.80	128	238	0.01	ng/ul	0.02
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul	
29) 4-Chloroaniline-d4	10.54	131	1614	0.04	ng/ul	-0.02
44) Dimethylphthalate-d6	13.62	166	460	0.00	ng/ul	-0.09
47) Acenaphthylene-d8	0.00	160	0	0.00	ng/ul	
52) 4-Nitrophenol-d4	14.49	143	140	0.01	ng/ul	0.00
58) Fluorene-d10	15.28	176	3182	0.04	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.42	200	121	0.01	ng/ul	0.01
71) Anthracene-d10	17.03	188	2051019	21.18	ng/ul	-0.10
79) Pyrene-d10	19.43	212	2744	0.03	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.43	264	2308899	19.55	ng/ul	0.14

Target Compounds


					Ovalue	
70) Phenanthrene	17.07	178	756170	6.603	ng/ul	99
72) Anthracene	17.07	178	756170	6.517	ng/ul	98
77) Fluoranthene	19.10	202	1197820	10.028	ng/ul	100
80) Pyrene	19.46	202	303546	2.434	ng/ul	98
83) Benzo(a)anthracene	21.21	228	357564	3.027	ng/ul	97
85) Chrysene	21.26	228	518984	4.761	ng/ul	99
88) Benzo(b)fluoranthene	22.77	252	464258	3.118	ng/ul#	83
89) Benzo(k)fluoranthene	22.77	252	464258	3.321	ng/ul#	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102419\
Data File : BM023396.D
Acq On : 25 Oct 2019 05:25
Operator : JU
Sample : K5403-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Oct 25 11:52:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 23 18:47:16 2019
Response via : Initial Calibration

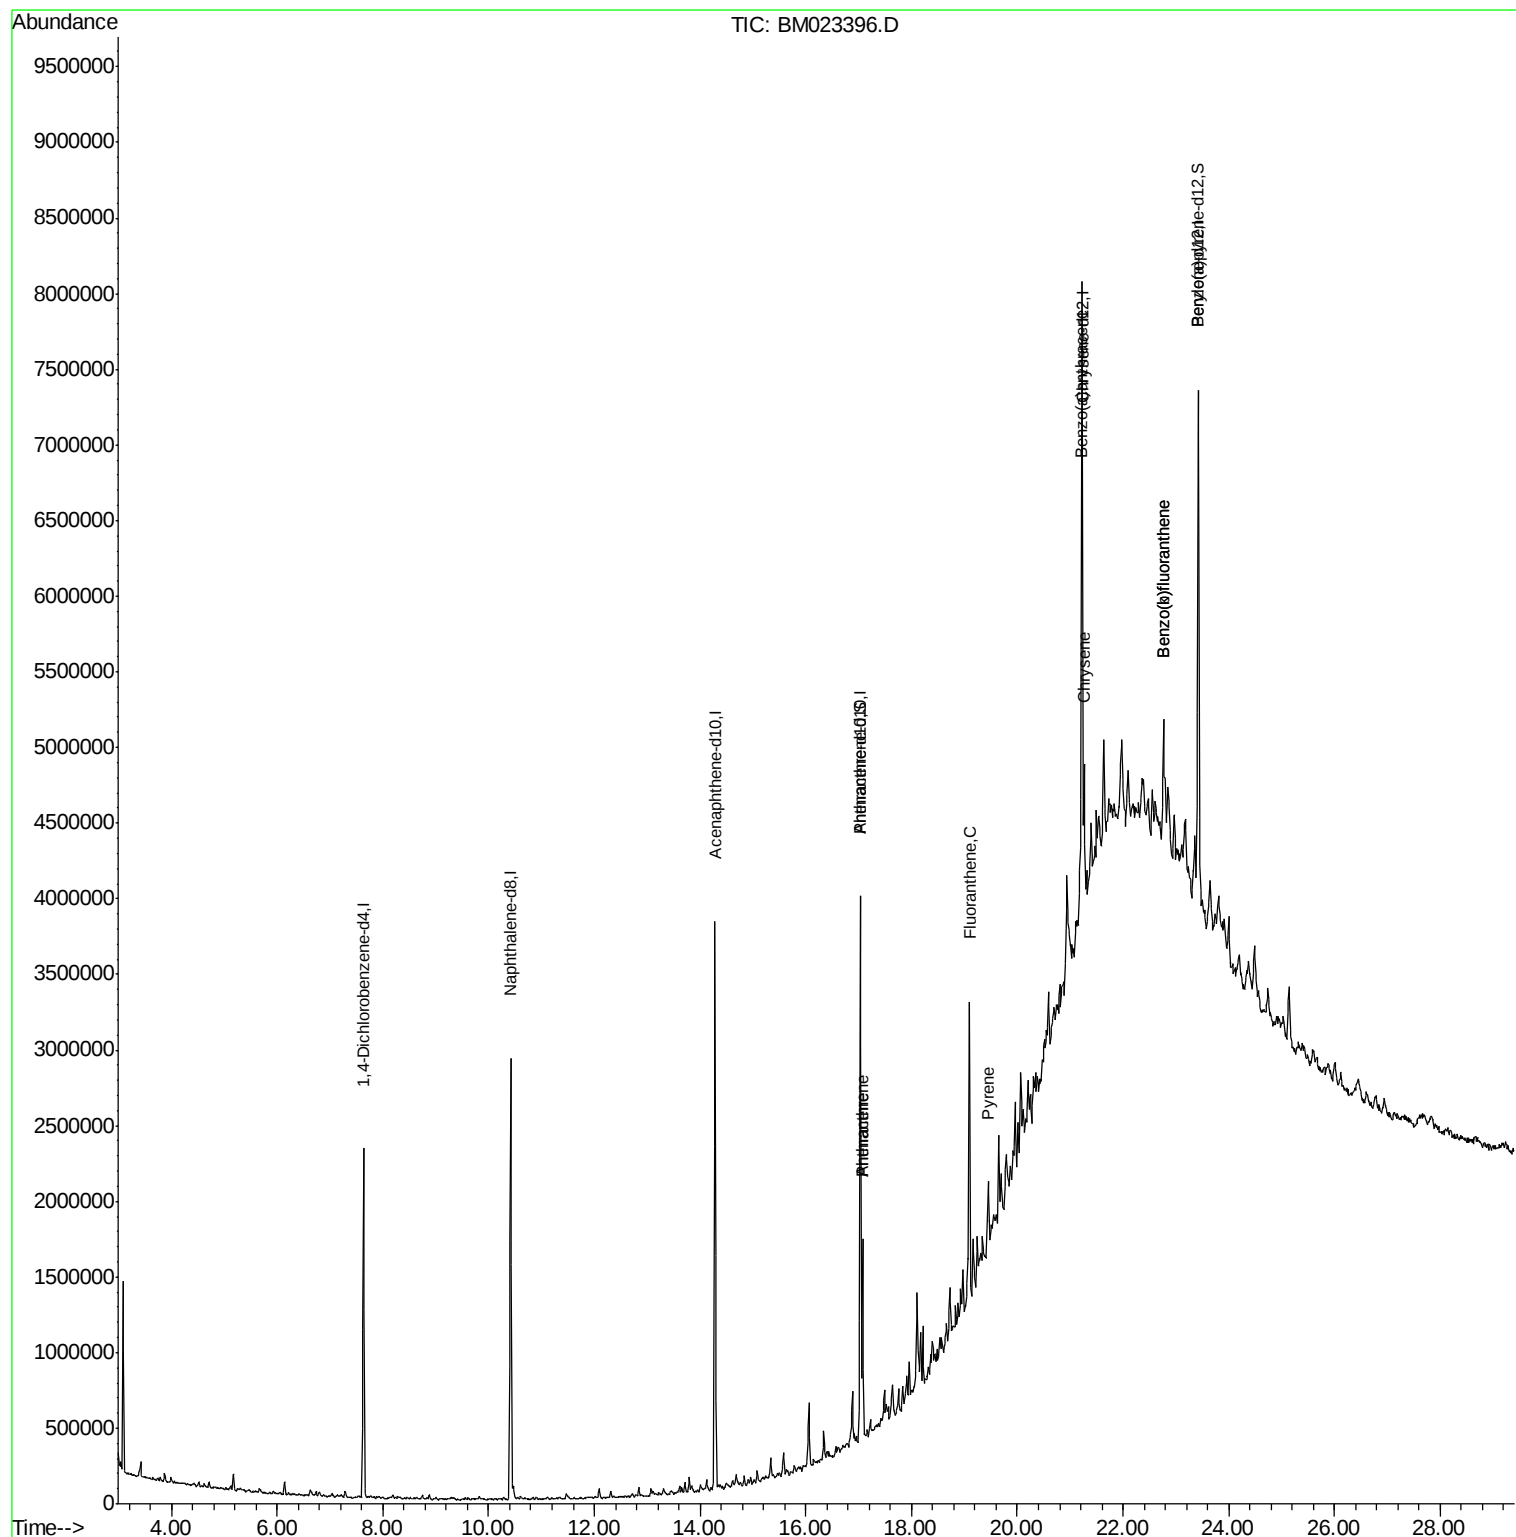

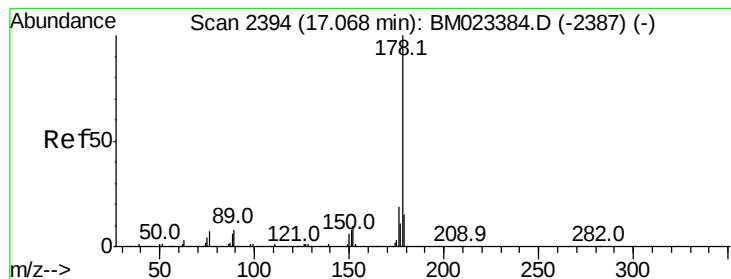

#70

Phenanthrene

Concen: 6.603 ng/ul

RT: 17.07 min Scan# 2395

Delta R.T. -0.00 min

Lab File: BM023396.D

Acq: 25 Oct 2019 05:25

Instrument :

BNA_M

ClientSampleId :


Tot Ion:178 Resp: 756170

Ion Ratio Lower Upper




178 100

179 15.4 12.2 18.2

176 19.2 14.9 22.3

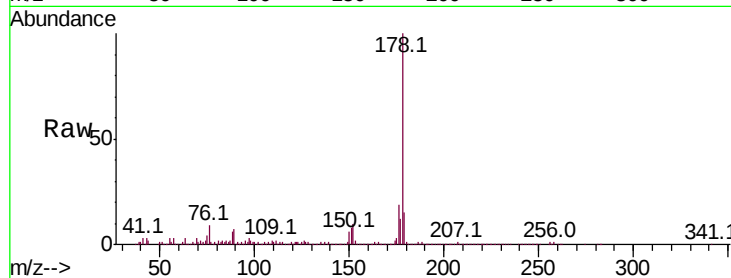

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

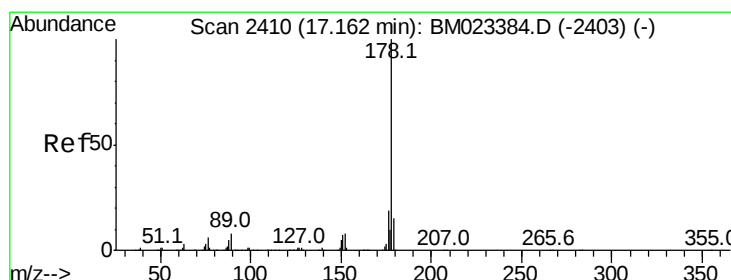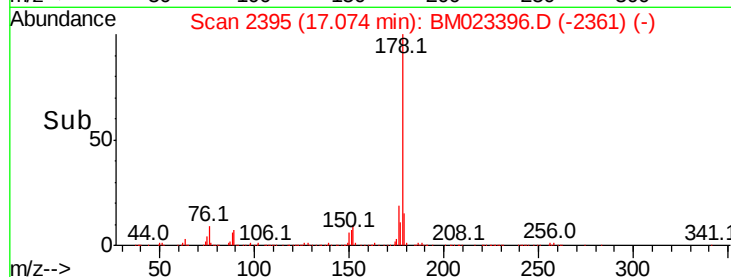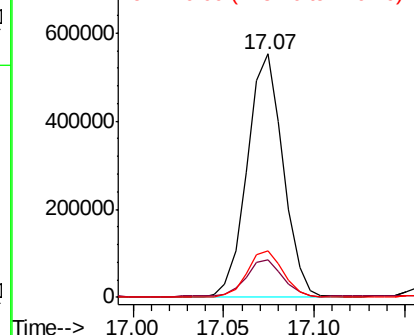

#72

Anthracene

Concen: 6.517 ng/ul

RT: 17.07 min Scan# 2395

Delta R.T. -0.09 min

Lab File: BM023396.D

Acq: 25 Oct 2019 05:25


Tgt Ion:178 Resp: 756170

Ion Ratio Lower Upper



178 100


179 15.4 12.1 18.1

176 19.2 14.4 21.6

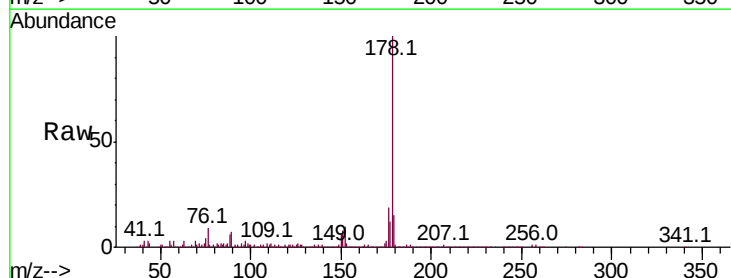

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

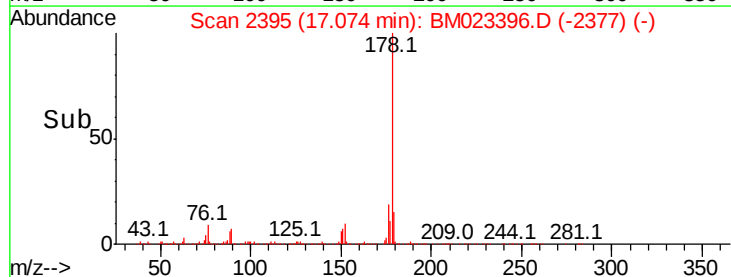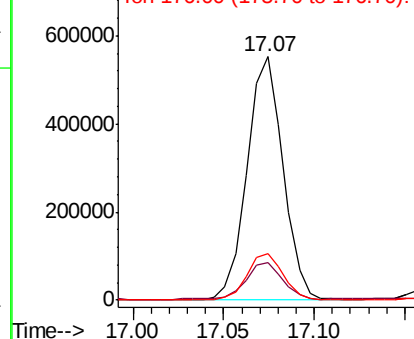

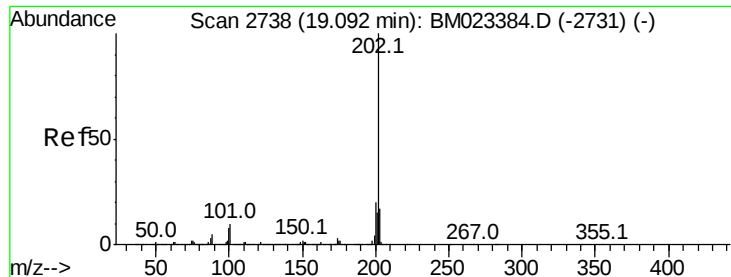


#77
Fluoranthene
 Concen: 10.028 ng/ul
 RT: 19.10 min Scan# 2739
 Delta R.T. -0.00 min
 Lab File: BM023396.D
 Acq: 25 Oct 2019 05:25




Instrument :
 BNA_M
 ClientSampleId :

Tot Ion:202 Resp: 1197820

Ion	Ratio	Lower	Upper
202	100		
101	10.0	8.1	12.1
100	7.9	6.2	9.2

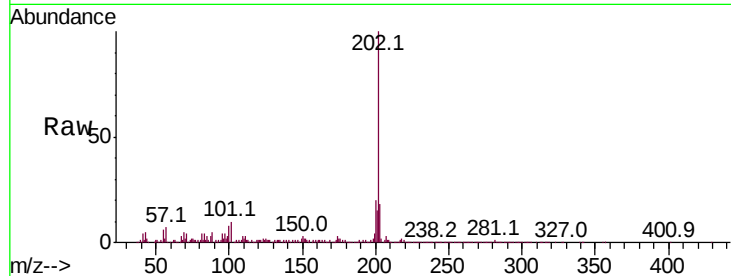


Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B

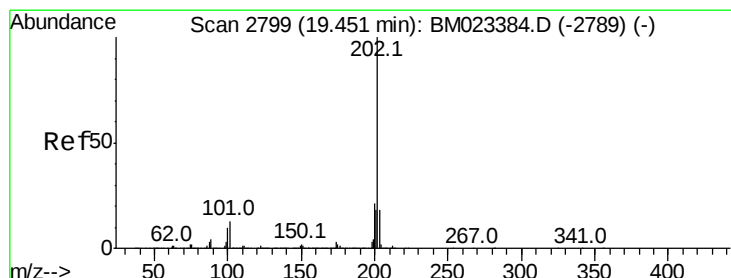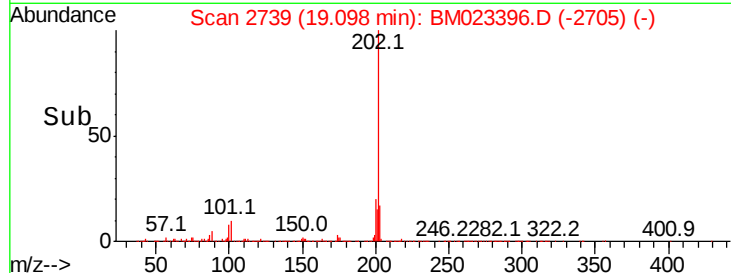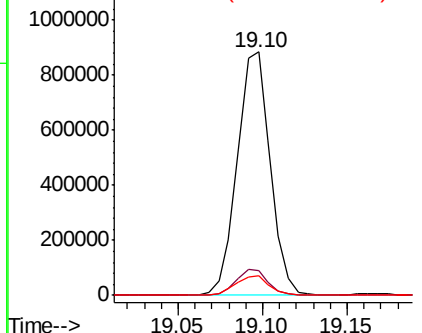



#80
Pyrene
 Concen: 2.434 ng/ul
 RT: 19.46 min Scan# 2800
 Delta R.T. -0.00 min
 Lab File: BM023396.D
 Acq: 25 Oct 2019 05:25


Tgt Ion:202 Resp: 303546

Ion	Ratio	Lower	Upper
202	100		
101	11.8	10.0	15.0
100	9.7	8.3	12.5

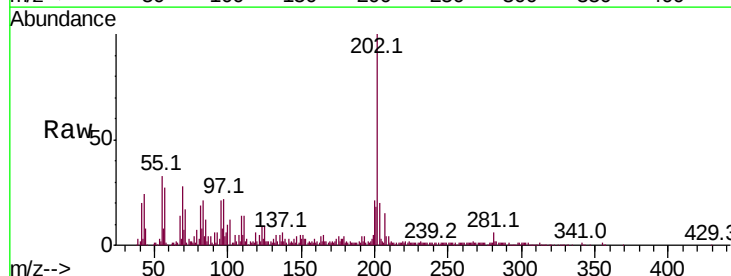

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B

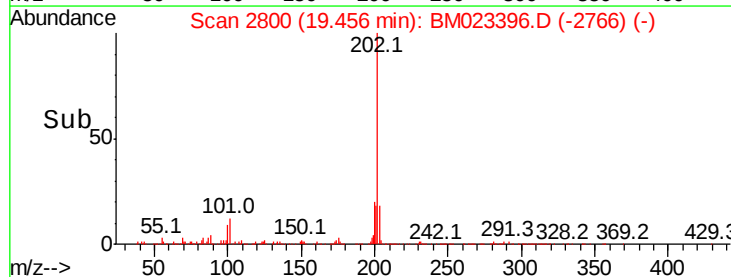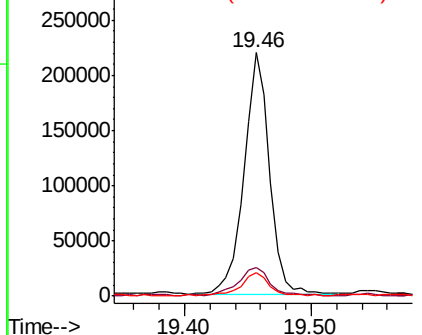

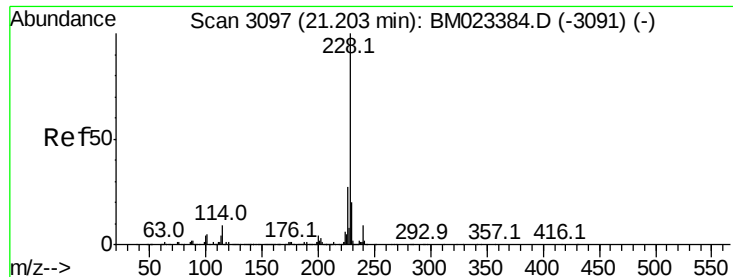

#83

Benzo(a)anthracene

Concen: 3.027 ng/ul

RT: 21.21 min Scan# 3098

Delta R.T. -0.00 min

Lab File: BM023396.D

Acq: 25 Oct 2019 05:25

Instrument :

BNA_M

ClientSampleId :


Tot Ion:228 Resp: 357564

Ion Ratio Lower Upper

228 100

229 21.4 15.8 23.8




226 28.5 21.6 32.4

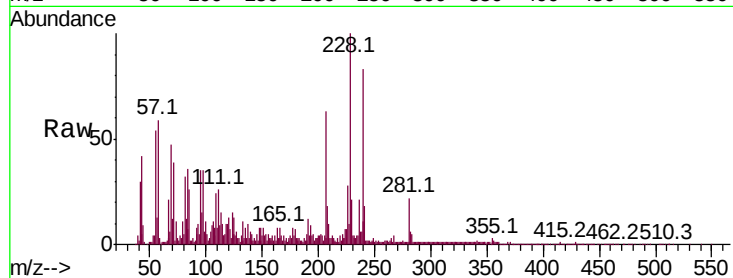

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

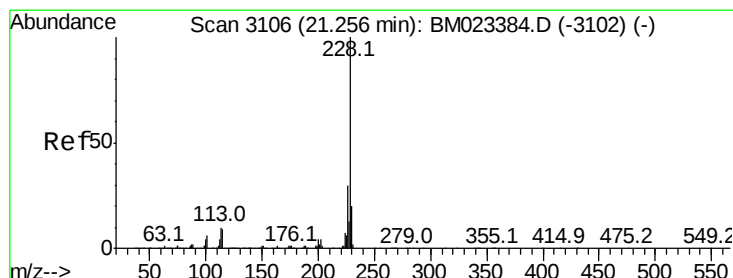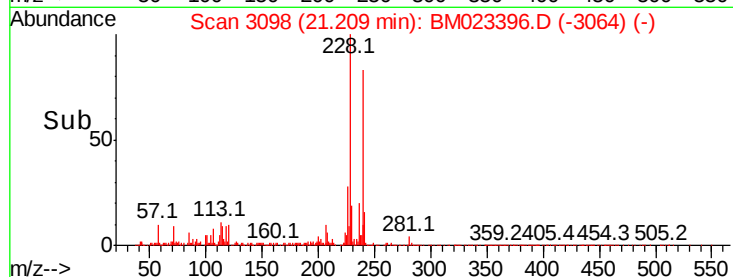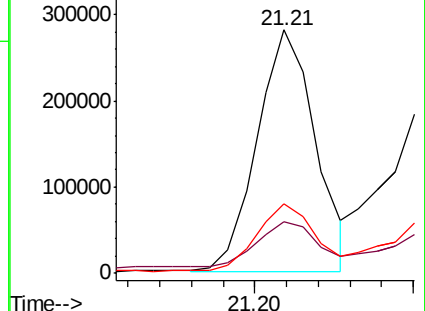

#85

Chrysene

Concen: 4.761 ng/ul

RT: 21.26 min Scan# 3107

Delta R.T. -0.00 min

Lab File: BM023396.D

Acq: 25 Oct 2019 05:25


Tgt Ion:228 Resp: 518984

Ion Ratio Lower Upper

228 100

226 29.5 24.0 36.0



229 20.3 16.0 24.0

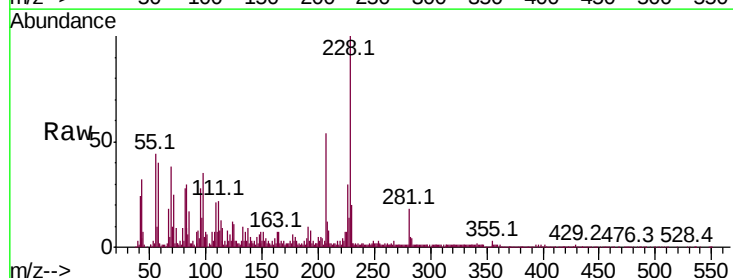


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

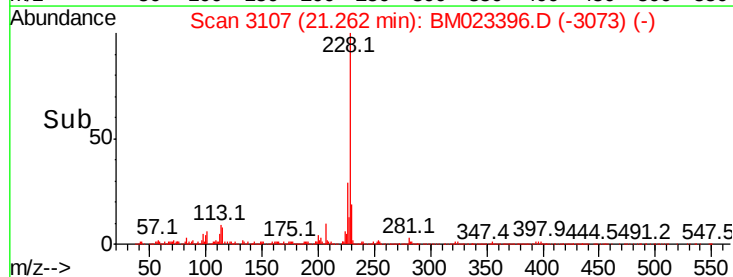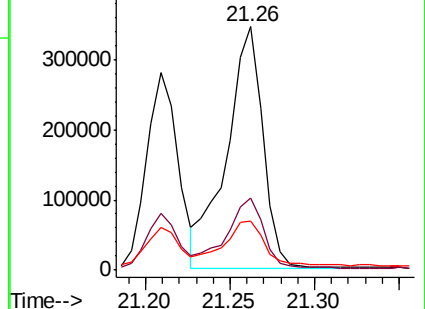

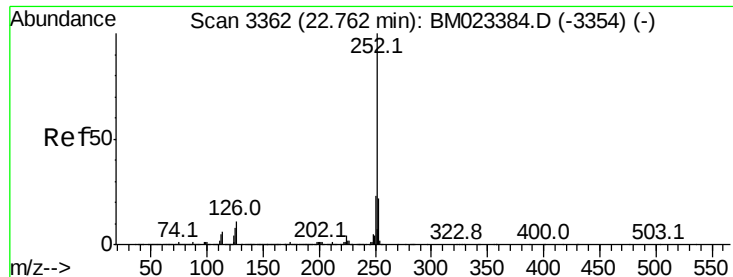

#88

Benzo(b)fluoranthene

Concen: 3.118 ng/ul

RT: 22.77 min Scan# 3364

Delta R.T. 0.01 min

Lab File: BM023396.D





Acq: 25 Oct 2019 05:25

Instrument :

BNA_M

ClientSampleId :

Tot Ion:252	Resp:	464258
Ion Ratio	Lower	Upper
252	100	
253	25.6	17.5 26.3
125	23.6	7.1 10.7#

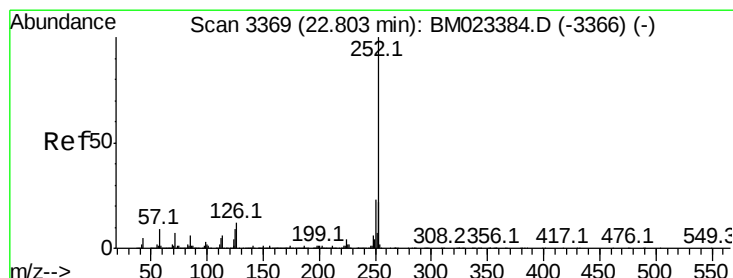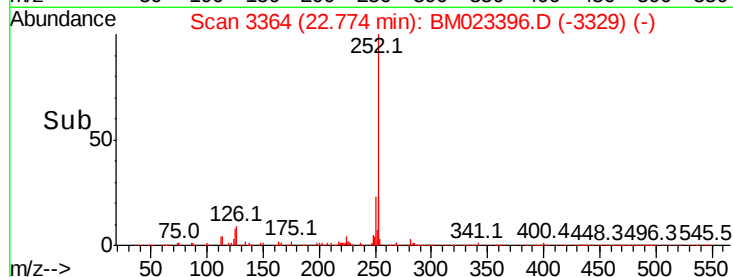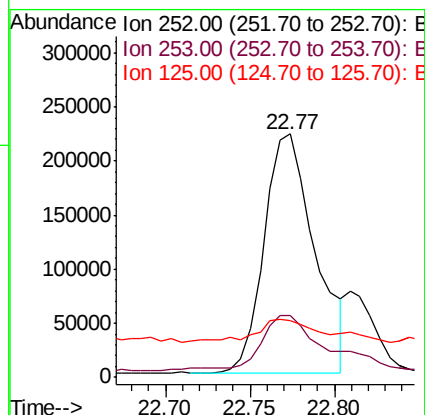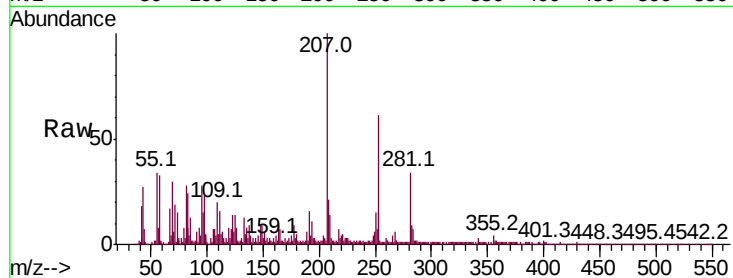

#89

Benzo(k)fluoranthene

Concen: 3.321 ng/ul

RT: 22.77 min Scan# 3364

Delta R.T. -0.04 min

Lab File: BM023396.D

Acq: 25 Oct 2019 05:25

Tgt Ion:252	Resp:	464258
Ion Ratio	Lower	Upper
252	100	
253	25.6	17.8 26.6
125	23.6	6.8 10.2#

