

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102419\
 Data File : BM023389.D
 Acq On : 24 Oct 2019 21:04
 Operator : JU
 Sample : K5346-08DL 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ETOM1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.828	647	653	669	rVB2	285780	545381	3.14%	0.598%
2	6.987	674	680	688	rBV	214543	352454	2.03%	0.386%
3	7.181	707	713	721	rVB	326841	515099	2.97%	0.564%
4	7.645	785	792	803	rBV	1916814	3023928	17.43%	3.313%
5	8.181	877	883	892	rBV2	34154	73209	0.42%	0.080%
6	8.357	907	913	923	rBV	307789	513945	2.96%	0.563%
7	8.792	981	987	994	rBV	265039	454022	2.62%	0.497%
8	9.516	1104	1110	1117	rBV	202541	336427	1.94%	0.369%
9	9.934	1176	1181	1186	rBV9	9986	20161	0.12%	0.022%
10	10.057	1194	1202	1209	rBV	344360	596245	3.44%	0.653%
11	10.428	1257	1265	1270	rBV	2365611	3948078	22.76%	4.325%
12	10.475	1270	1273	1280	rVB	117481	191347	1.10%	0.210%
13	10.563	1280	1288	1301	rBV2	232617	460798	2.66%	0.505%
14	12.092	1543	1548	1555	rBV	32466	62132	0.36%	0.068%
15	12.322	1583	1587	1592	rVB5	14166	21770	0.13%	0.024%
16	13.127	1719	1724	1729	rBV6	11459	18068	0.10%	0.020%
17	13.710	1817	1823	1827	rVV	643504	915077	5.27%	1.003%
18	13.757	1827	1831	1839	rVB	202421	292162	1.68%	0.320%
19	13.980	1862	1869	1872	rBV2	718167	1140574	6.57%	1.250%
20	14.010	1872	1874	1888	rVB	485987	713406	4.11%	0.782%
21	14.292	1916	1922	1929	rBV	3392708	5003859	28.84%	5.482%
22	14.357	1929	1933	1938	rVB	53662	79330	0.46%	0.087%
23	14.510	1952	1959	1964	rBV	113026	195340	1.13%	0.214%
24	14.651	1979	1983	1986	rBV4	19953	29911	0.17%	0.033%
25	14.692	1986	1990	1992	rVV	45991	67919	0.39%	0.074%
26	14.721	1992	1995	2002	rVB5	60407	97676	0.56%	0.107%
27	14.968	2032	2037	2044	rVB9	18781	39198	0.23%	0.043%
28	15.186	2066	2074	2078	rBV5	31348	72199	0.42%	0.079%
29	15.292	2085	2092	2097	rBV	984302	1446147	8.34%	1.584%
30	15.345	2097	2101	2109	rVV	100442	173671	1.00%	0.190%
31	15.427	2111	2115	2122	rVV7	26108	40901	0.24%	0.045%
32	15.539	2130	2134	2139	rBV6	20866	46092	0.27%	0.050%
33	15.645	2147	2152	2155	rBV7	15776	33451	0.19%	0.037%
34	16.021	2211	2216	2222	rBV4	57525	105314	0.61%	0.115%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102419\
 Data File : BM023389.D
 Acq On : 24 Oct 2019 21:04
 Operator : JU
 Sample : K5346-08DL 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ETOM1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
 Title : SVOA CALIBRATION

35	16.357	2269	2273	2277	rBV5	24728	33324	0.19%	0.037%
36	16.621	2316	2318	2322	rVB4	29482	29336	0.17%	0.032%
37	16.698	2328	2331	2336	rBV4	40946	71247	0.41%	0.078%
38	16.821	2350	2352	2356	rBV5	24995	28864	0.17%	0.032%
39	17.039	2383	2389	2394	rBV2	3816212	5560945	32.06%	6.092%
40	17.080	2394	2396	2401	rVV	422228	516441	2.98%	0.566%
41	17.139	2401	2406	2409	rVV2	1125726	1654645	9.54%	1.813%
42	17.174	2409	2412	2418	rVB	1313836	1744447	10.06%	1.911%
43	17.445	2455	2458	2462	rVB	95382	118920	0.69%	0.130%
44	18.045	2556	2560	2565	rBV	276565	394017	2.27%	0.432%
45	19.104	2736	2740	2747	rBV	1477106	1918881	11.06%	2.102%
46	19.439	2793	2797	2799	rBV2	1531459	2070099	11.93%	2.268%
47	19.468	2799	2802	2811	rVB	2119977	2860008	16.49%	3.133%
48	20.068	2901	2904	2909	rBV	822689	987101	5.69%	1.081%
49	21.233	3097	3102	3106	rBV2	5515530	10680651	61.57%	11.701%
50	21.274	3106	3109	3117	rVB	4650880	6022509	34.72%	6.598%
51	22.791	3362	3367	3379	rVB	6208124	17347860	100.00%	19.006%
52	23.256	3442	3446	3451	rBV	2825274	4325358	24.93%	4.739%
53	23.350	3458	3462	3470	rVB	4116873	8077103	46.56%	8.849%
54	23.444	3474	3478	3483	rVV	3165902	5209076	30.03%	5.707%


Sum of corrected areas: 91276123

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102419\
Data File : BM023389.D
Acq On : 24 Oct 2019 21:04
Operator : JU
Sample : K5346-08DL 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ETOM1DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

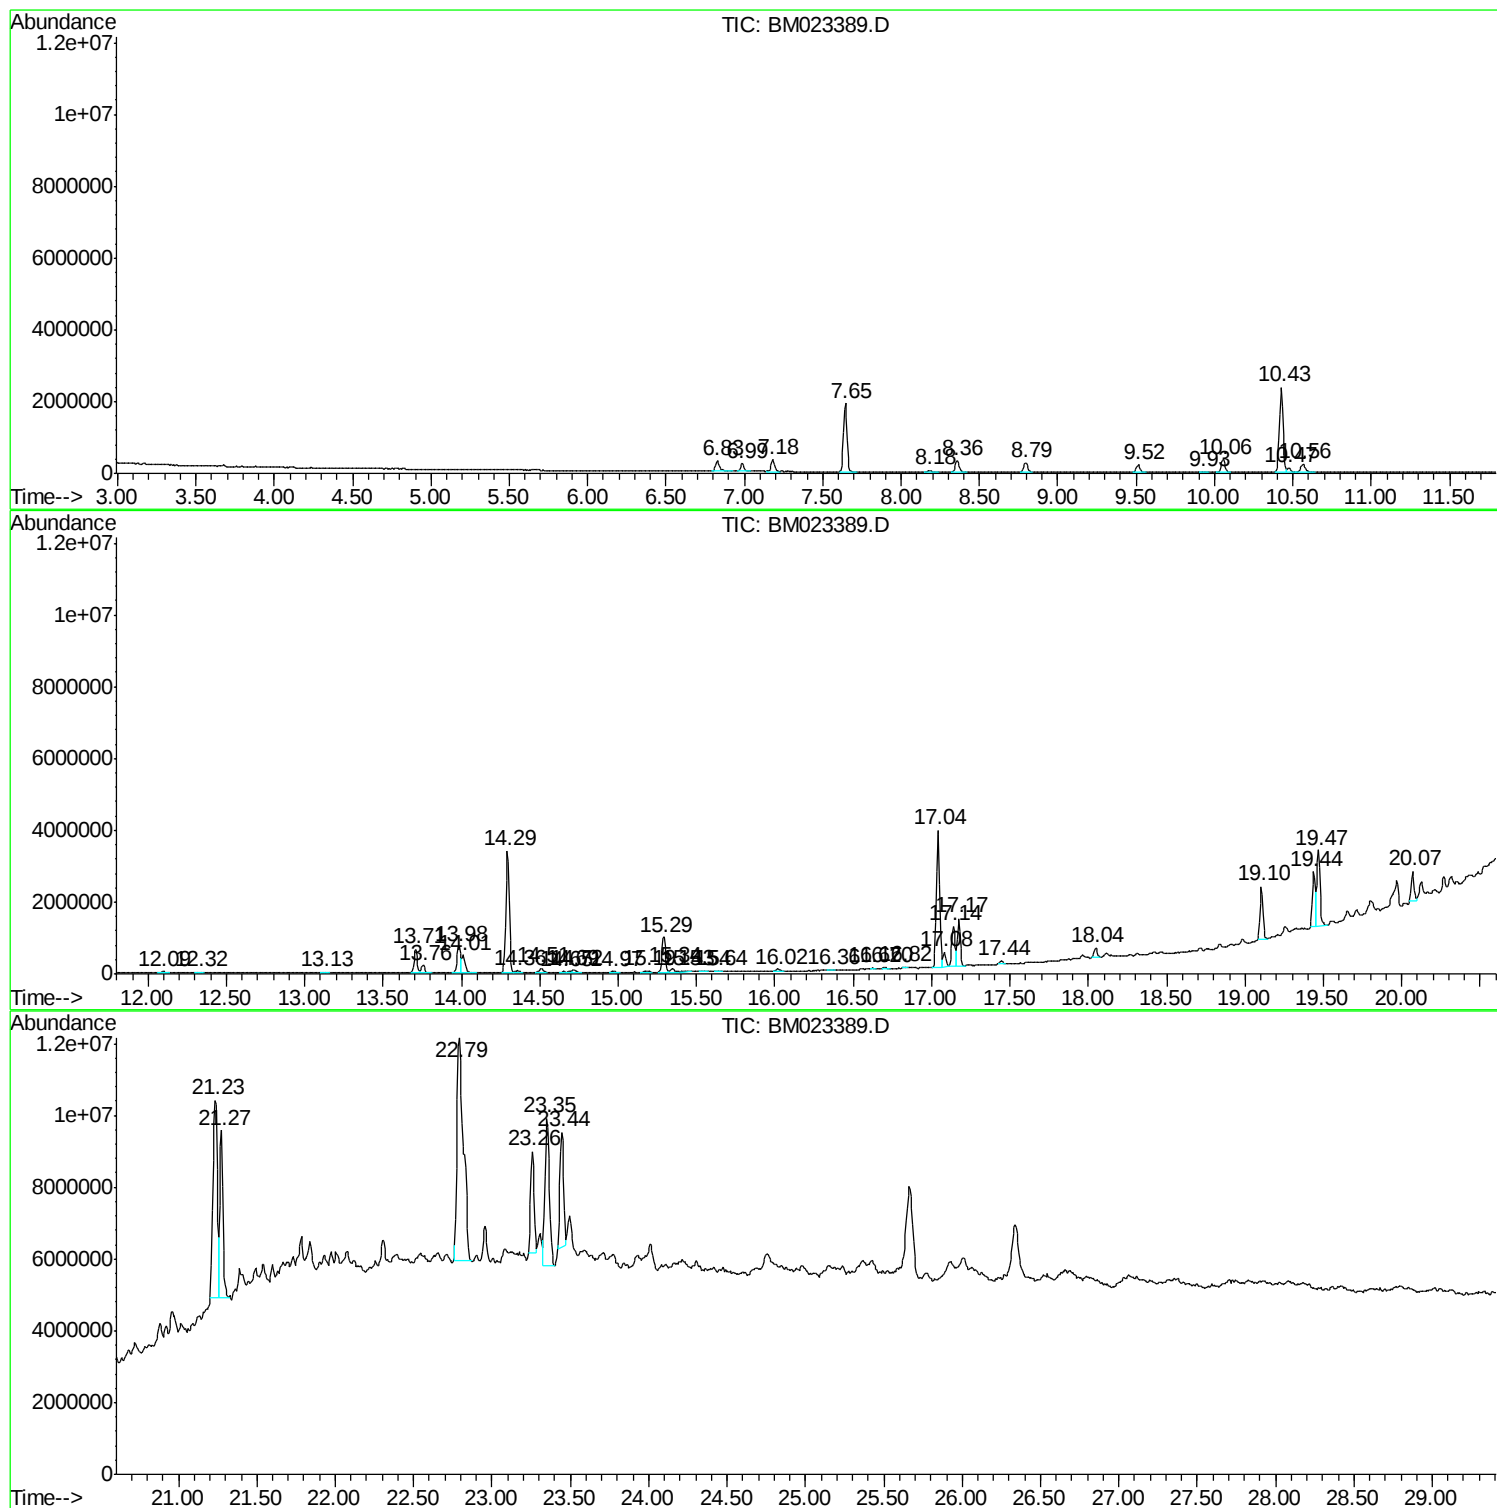

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM102419\
Data File : BM023389.D
Acq On : 24 Oct 2019 21:04
Operator : JU
Sample : K5346-08DL 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ETOM1DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM102419\
Data File : BM023389.D
Acq On : 24 Oct 2019 21:04
Operator : JU
Sample : K5346-08DL 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ETOM1DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc