
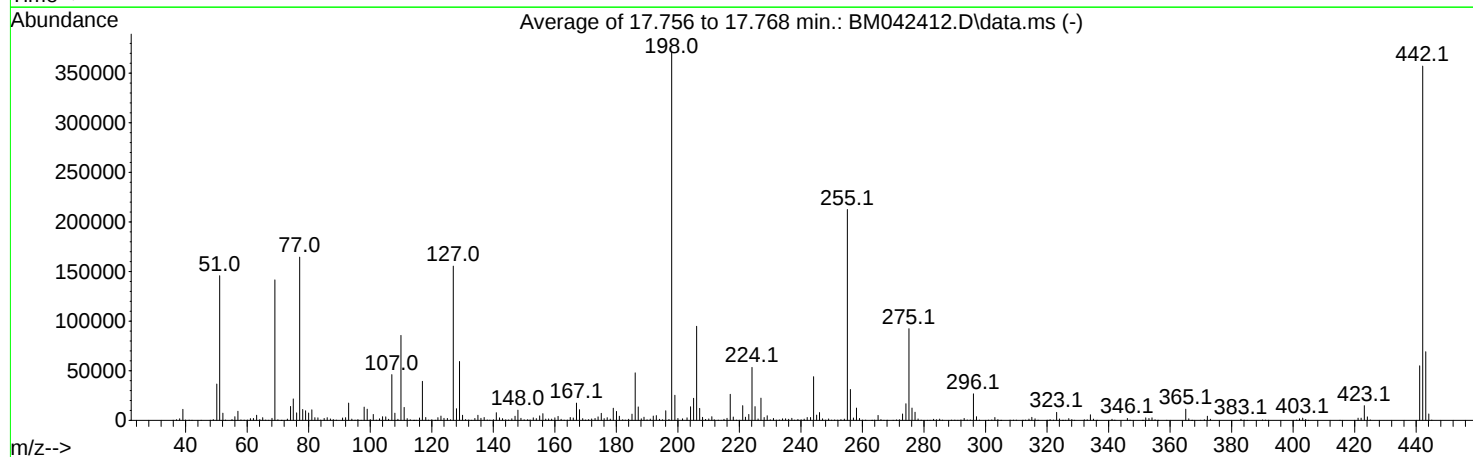


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102423\
Data File : BM042412.D
Acq On : 24 Oct 2023 10:33
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Oct 21 02:32:53 2023

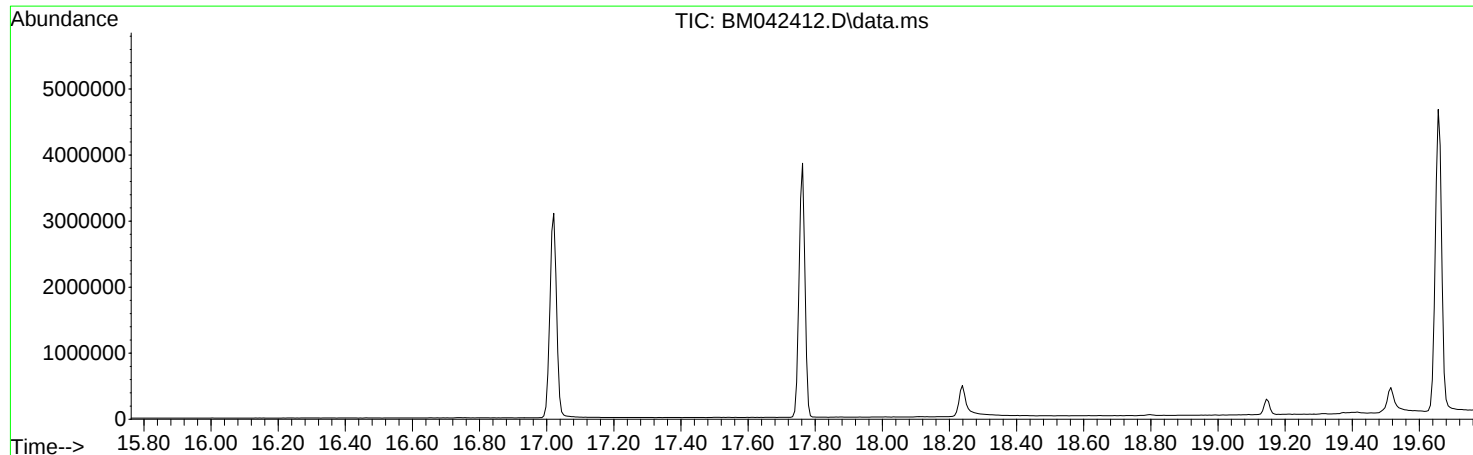




AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.3	145776	PASS
68	69	0.00	2	1.5	2107	PASS
69	198	0.00	100	38.2	141659	PASS
70	69	0.00	2	0.4	614	PASS
127	198	10	80	41.9	155429	PASS
197	198	0.00	2	0.3	987	PASS
198	198	100	100	100.0	370795	PASS
199	198	5	9	6.8	25299	PASS
275	198	10	60	24.9	92379	PASS
365	198	1	100	3.1	11366	PASS
441	198	0.01	100	14.8	54936	PASS
442	442	50	100	100.0	357163	PASS
443	442	15	24	19.4	69171	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102423\
Data File : BM042412.D
Acq On : 24 Oct 2023 10:33
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Oct 24 20:52:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 21 02:32:53 2023
Response via : Initial Calibration

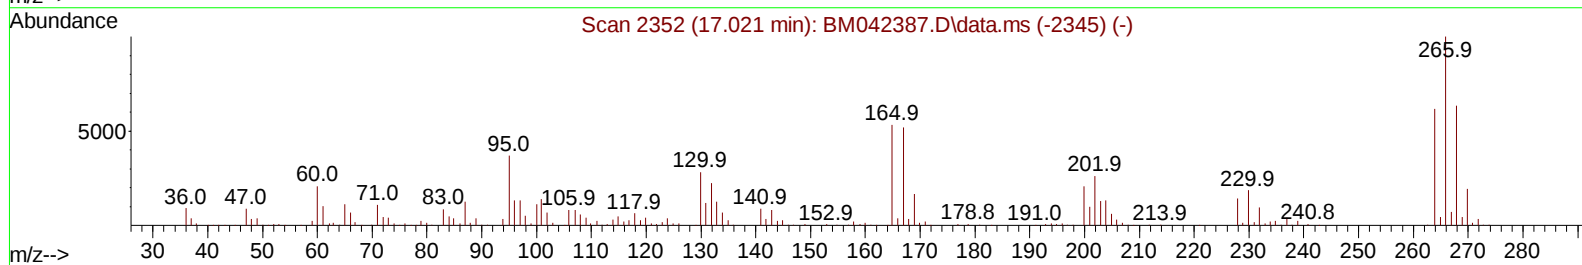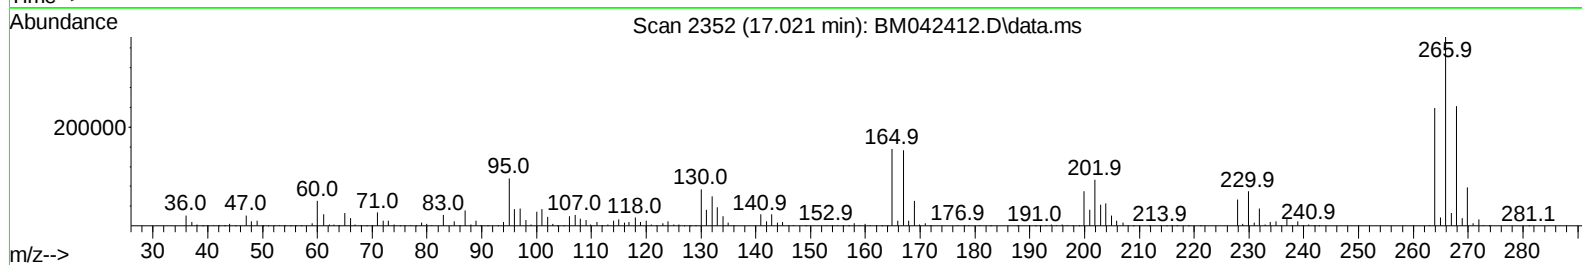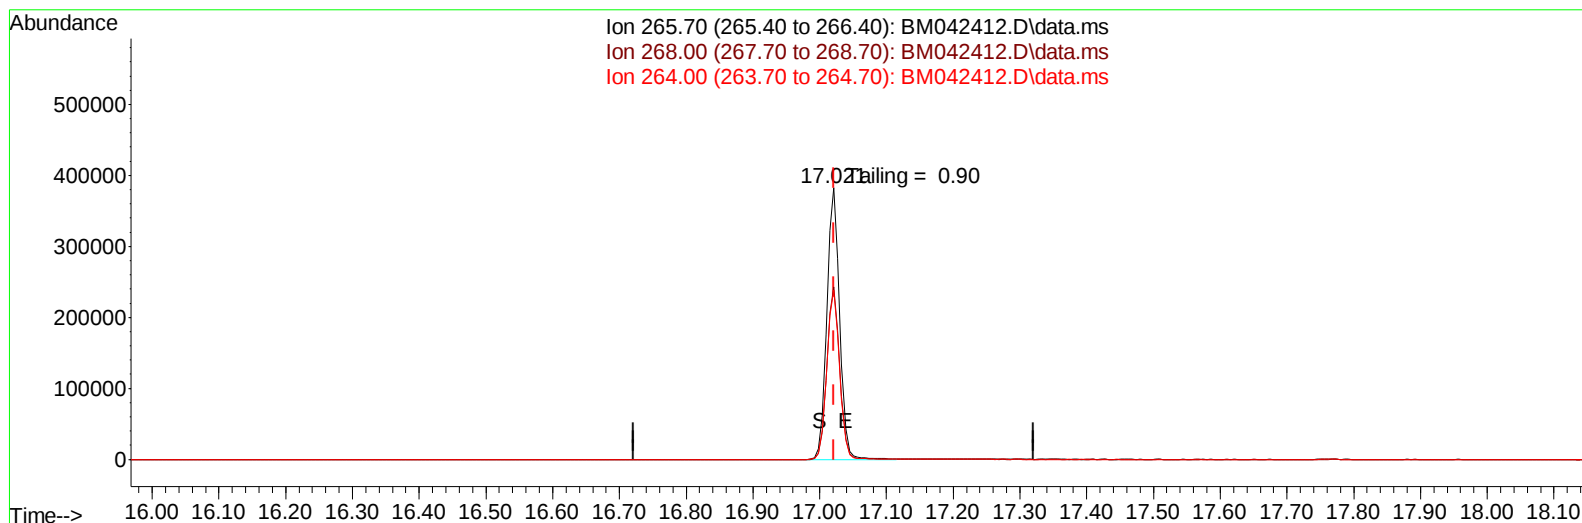

TIC: BM042412.D\data.ms

(70) Pentachlorophenol (C)

17.021min (+ 0.000) 0.00 ng




response 513925

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	63.51
264.00	61.70	62.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102423\
Data File : BM042412.D
Acq On : 24 Oct 2023 10:33
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Oct 24 20:52:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 21 02:32:53 2023
Response via : Initial Calibration

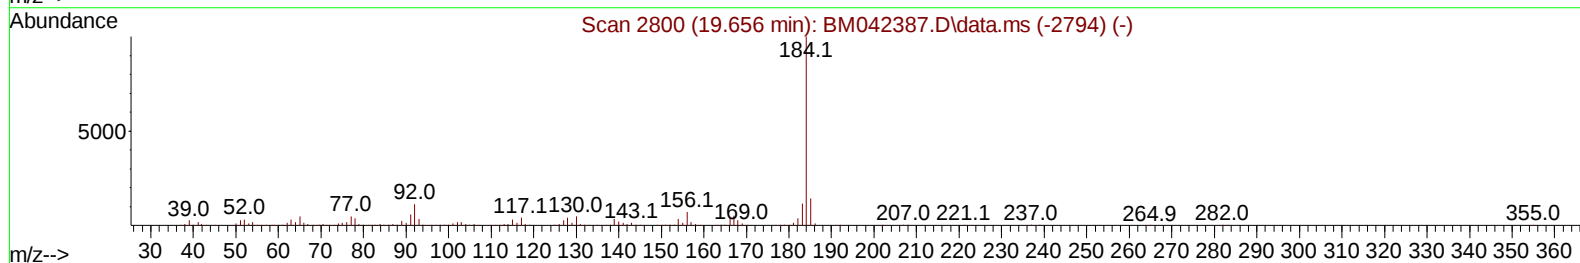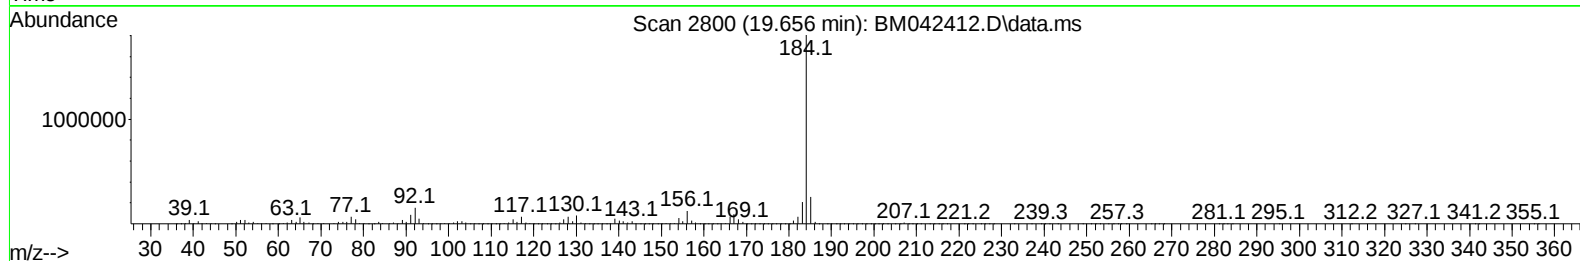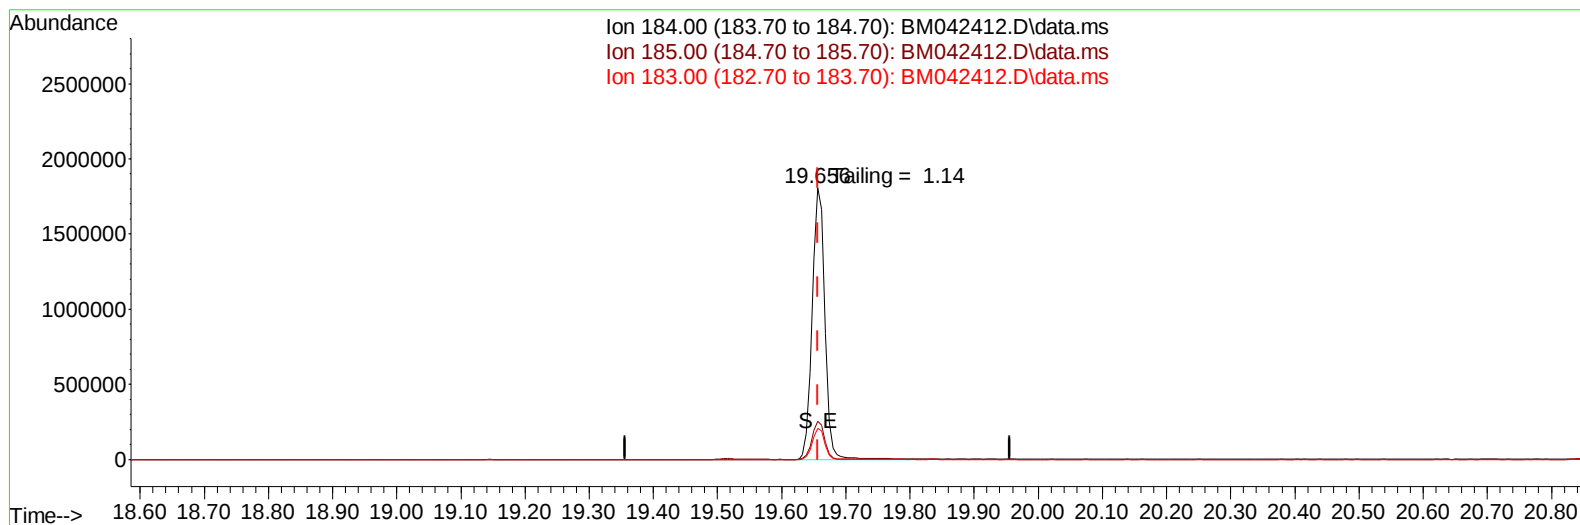

TIC: BM042412.D\data.ms

(77) Benzidine

19.656min (-0.000) 239771.26 ng

response 2455424

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.13
183.00	11.50	11.42
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/24/2023	BNA_M	<u>BM042412.D</u>
Compound Name	Response	Retention Time
DDT	1299280	20.85
DDD	18029	20.456
DDE	550	19.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18579	1317859	1.41

Instrument :
BNA_M
ClientSampleId :
DFTPP