
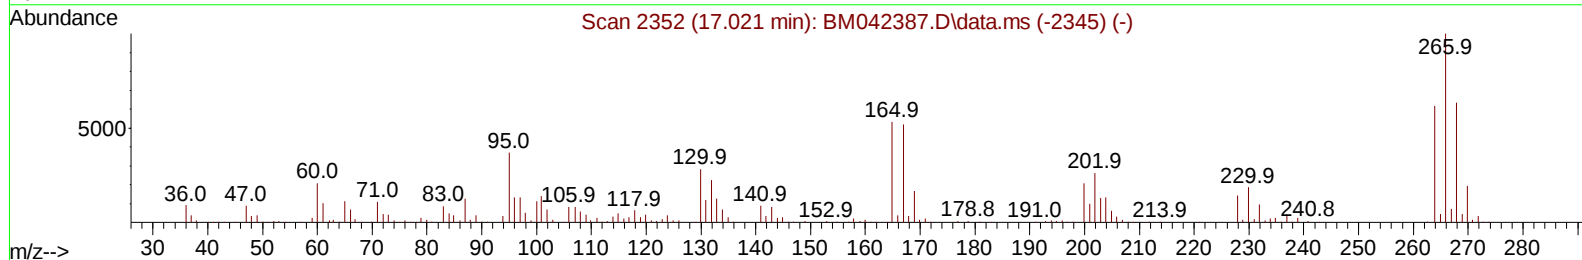
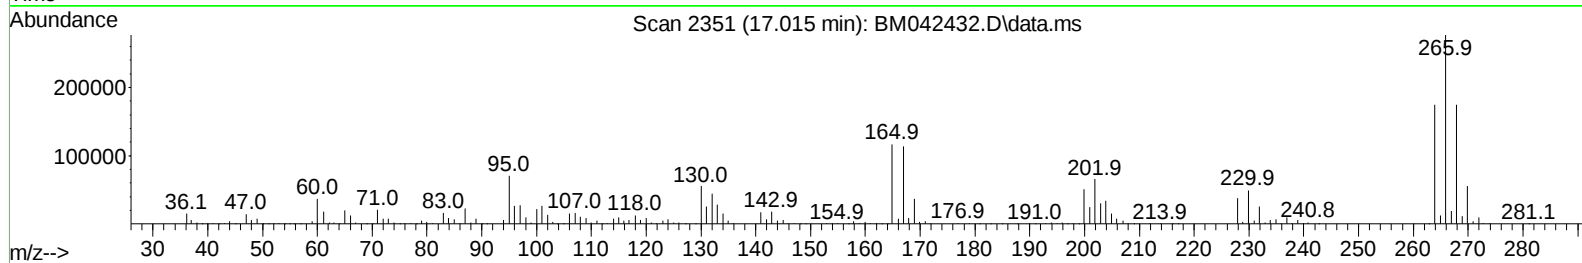


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102523\
Data File : BM042432.D
Acq On : 25 Oct 2023 11:30
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 25 20:30:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 21 02:32:53 2023
Response via : Initial Calibration

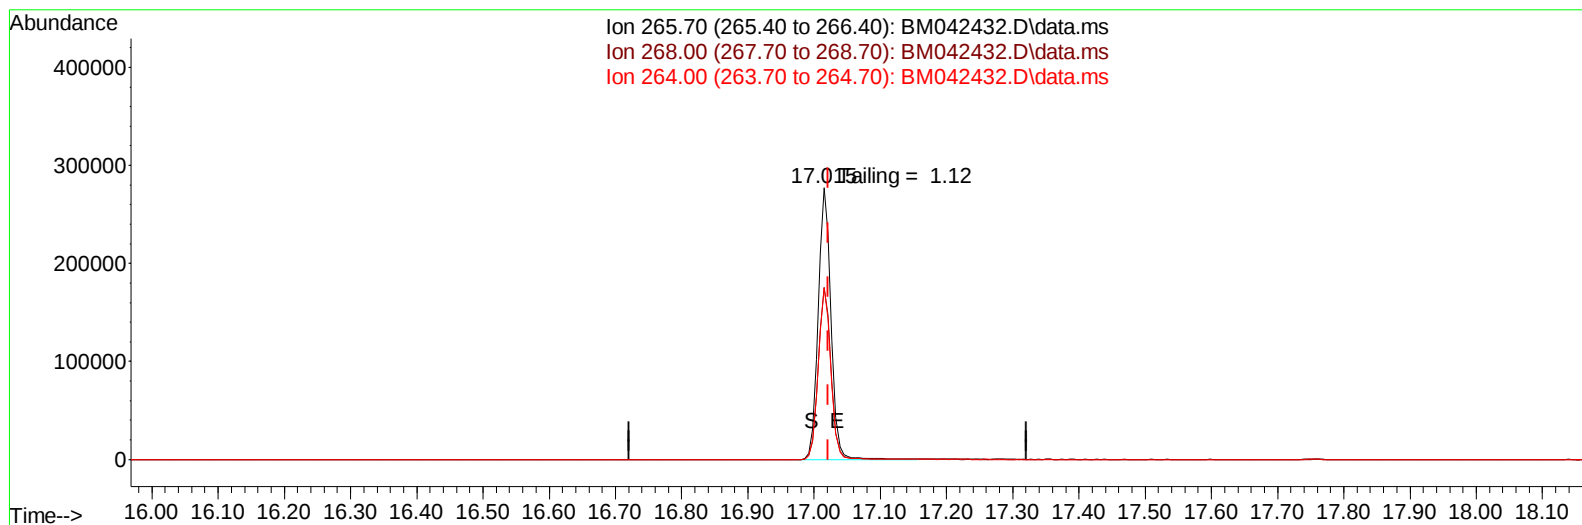

TIC: BM042432.D\data.ms

(70) Pentachlorophenol (C)




17.015min (-0.006) 16983.07 ng

response 373793

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	63.22
264.00	61.70	63.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102523\
Data File : BM042432.D
Acq On : 25 Oct 2023 11:30
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 25 20:30:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 21 02:32:53 2023
Response via : Initial Calibration

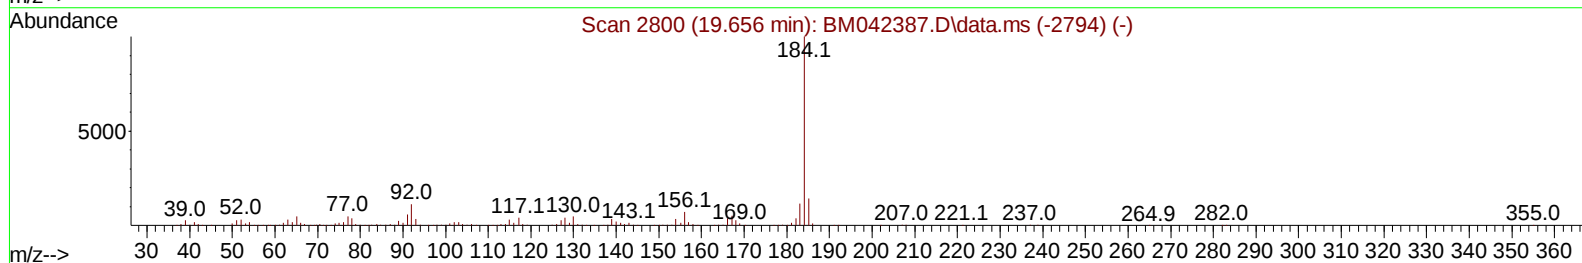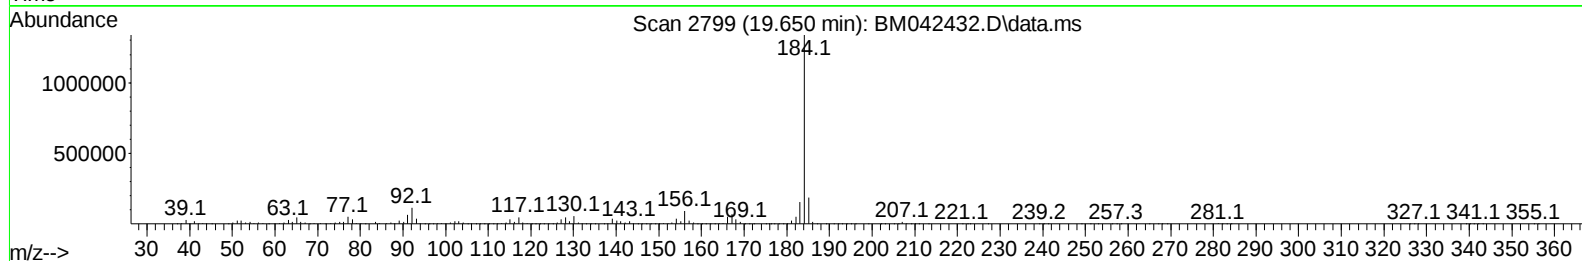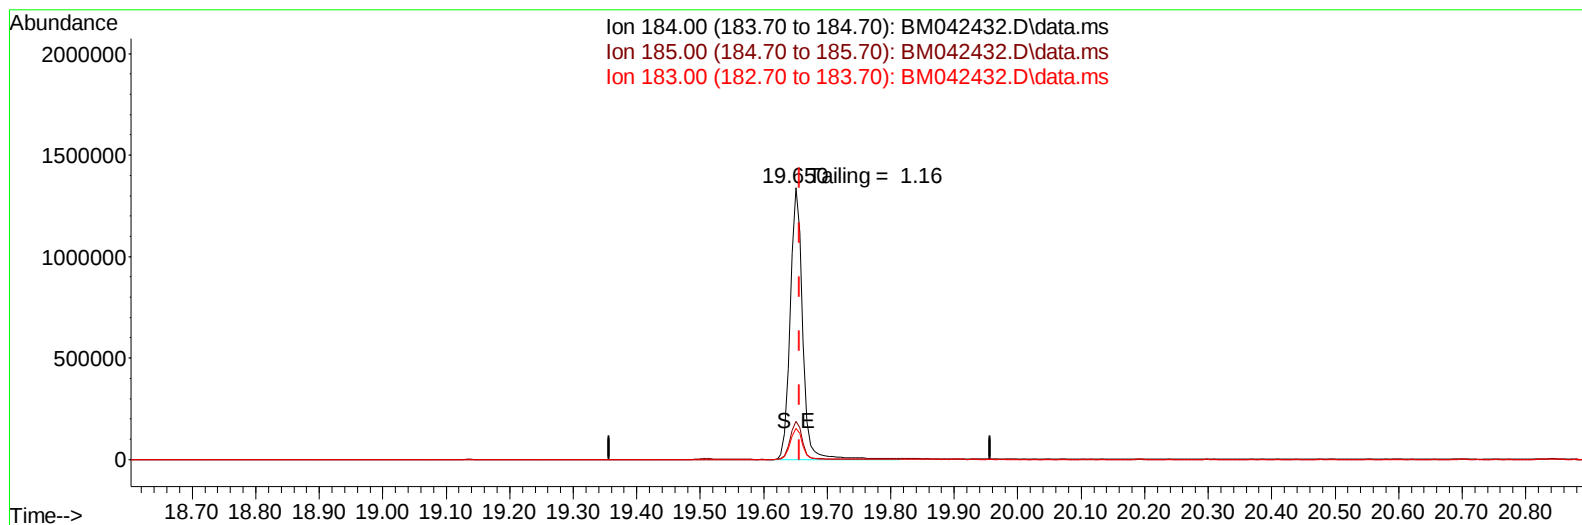

TIC: BM042432.D\data.ms

(77) Benzidine**19.650min (-0.006) 26820.11 ng****response 1840742**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.07
183.00	11.50	11.43
0.00	0.00	0.00