

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102618\
 Data File : BM017358.D
 Acq On : 26 Oct 2018 21:10
 Operator : MJ/SJ
 Sample : J5204-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Oct 27 01:50:09 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM101718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 17 14:23:17 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	231945	20.00	ng	-0.02
21) Naphthalene-d8	10.43	136	976964	20.00	ng	-0.02
39) Acenaphthene-d10	14.29	164	617407	20.00	ng	-0.02
64) Phenanthrene-d10	17.05	188	1594880	20.00	ng	-0.02
76) Chrysene-d12	21.24	240	1850019	20.00	ng	-0.02
87) Perylene-d12	23.46	264	1676969	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.28	112	1591479	116.05	ng	-0.01
7) Phenol-d6	6.84	99	2011689	107.71	ng	-0.02
23) Nitrobenzene-d5	8.80	82	1460331	87.42	ng	-0.03
42) 2,4,6-Tribromophenol	15.79	330	1180317	141.36	ng	-0.02
45) 2-Fluorobiphenyl	12.91	172	3641909	78.48	ng	-0.02
79) Terphenyl-d14	19.69	244	6846793	83.42	ng	-0.02
Target Compounds						
80) Butylbenzylphthalate	20.40	149	177	7.180	ng	# 77
84) Bis(2-ethylhexyl)phthalate	21.17	149	2260	5.341	ng	# 92
85) Di-n-octyl phthalate	22.04	149	1393	5.584	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102618\
Data File : BM017358.D
Acq On : 26 Oct 2018 21:10
Operator : MJ/SJ
Sample : J5204-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Oct 27 01:50:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM101718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 17 14:23:17 2018
Response via : Initial Calibration

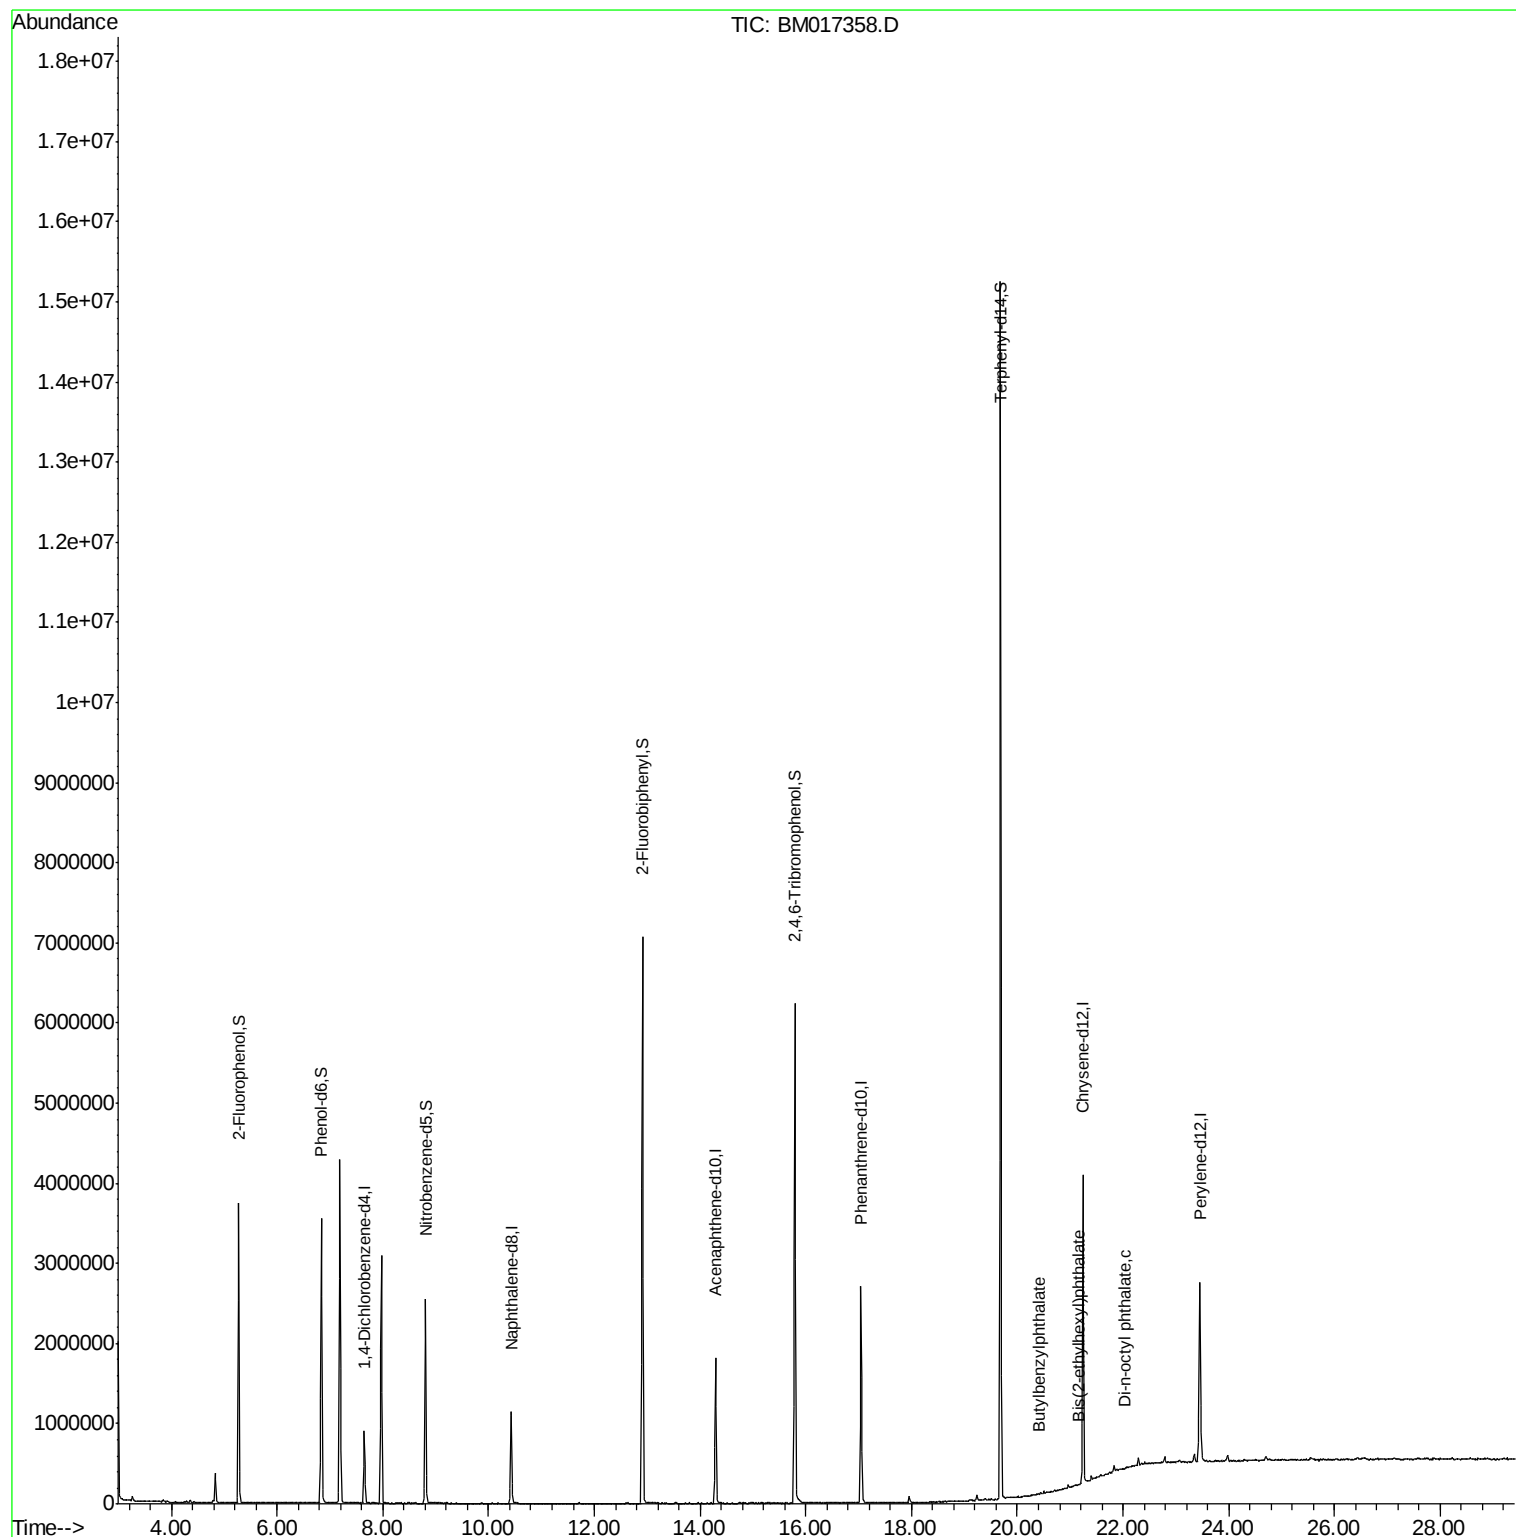

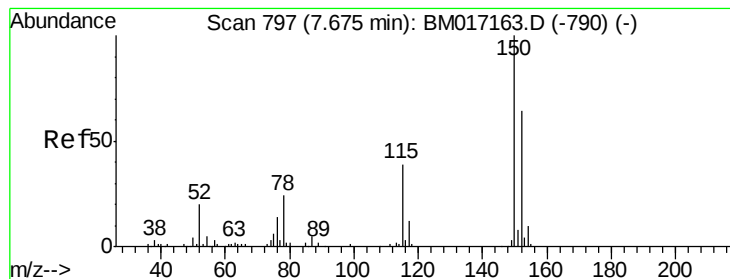


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.65 min Scan# 793
Delta R.T. -0.02 min
Lab File: BM017358.D
Acq: 26 Oct 2018 21:10

Instrument :
BNA_M
ClientSampleId :

Tot Ion:152 Resp: 231945
Ion Ratio Lower Upper
152 100
150 155.8 124.3 186.5
115 59.4 48.1 72.1

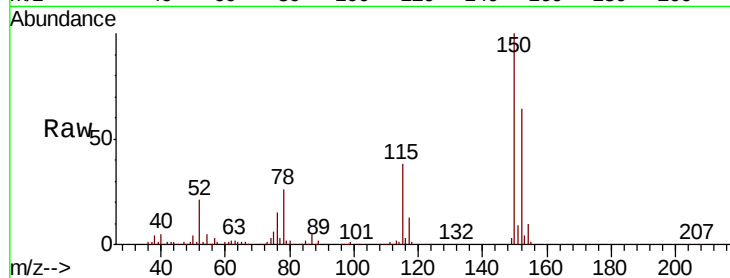


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

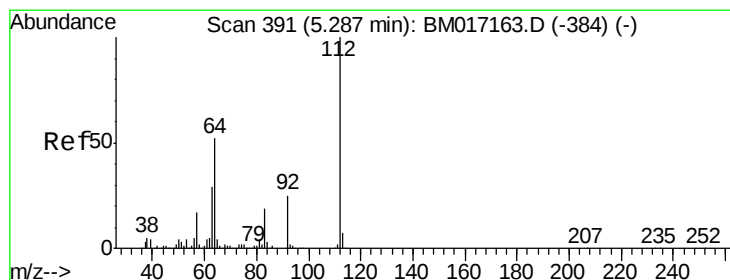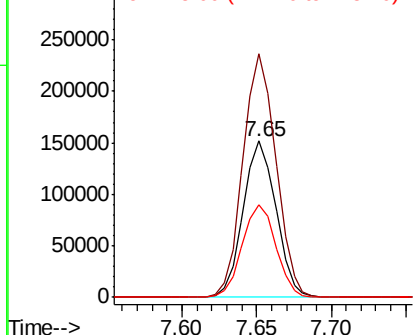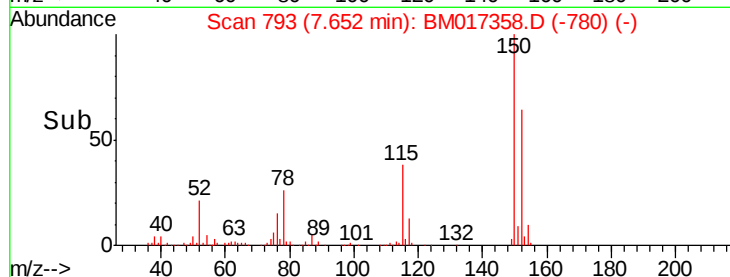



#5


2-Fluorophenol
Concen: 116.050 ng
RT: 5.28 min Scan# 389
Delta R.T. -0.01 min
Lab File: BM017358.D
Acq: 26 Oct 2018 21:10

Tgt Ion:112 Resp: 1591479
Ion Ratio Lower Upper
112 100
64 56.4 41.7 62.5
63 29.6 23.0 34.4

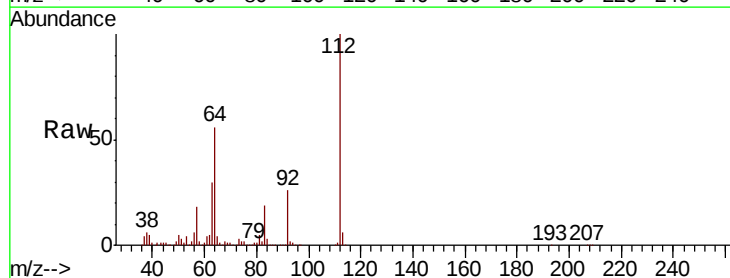

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

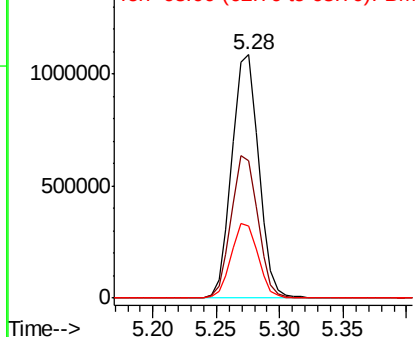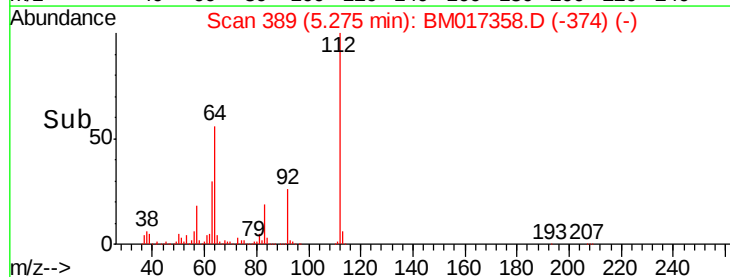

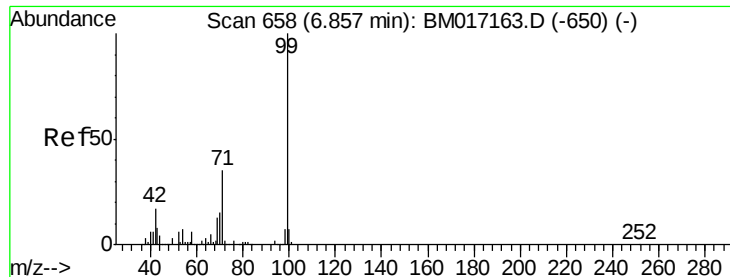

#7

Phenol-d6

Concen: 107.708 ng

RT: 6.84 min Scan# 655

Delta R.T. -0.02 min

Lab File: BM017358.D

Acq: 26 Oct 2018 21:10


Instrument :

BNA_M

ClientSampleId :

Tot Ion: 99 Resp: 2011689

Ion	Ratio	Lower	Upper
99	100		
42	18.1	13.3	19.9
71	35.4	28.0	42.0


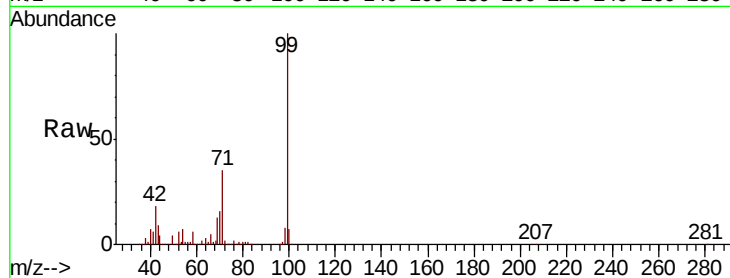


Abundance

Ion 99.00 (98.70 to 99.70): BM017163.D (-650) (-)

Ion 42.00 (41.70 to 42.70): BM017163.D (-650) (-)

Ion 71.00 (70.70 to 71.70): BM017163.D (-650) (-)

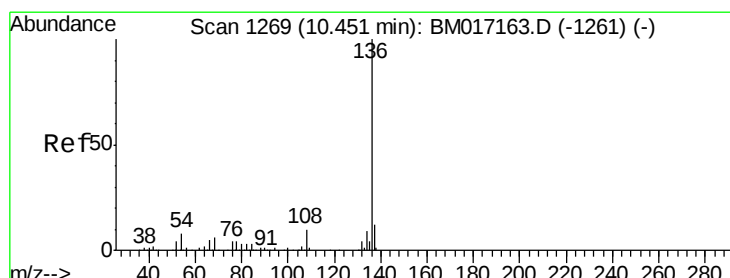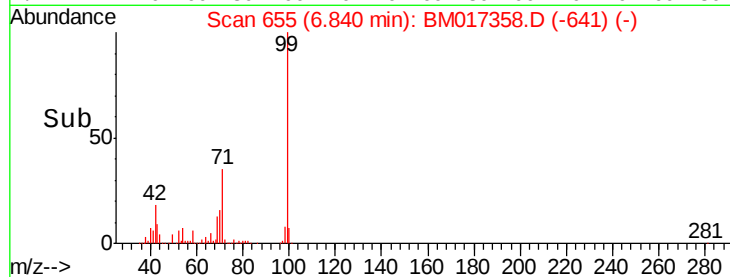

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.43 min Scan# 1265


Delta R.T. -0.02 min

Lab File: BM017358.D

Acq: 26 Oct 2018 21:10

Tgt Ion: 136 Resp: 976964

Ion	Ratio	Lower	Upper
136	100		
137	10.4	9.2	13.8
54	7.9	6.7	10.1
68	5.8	4.7	7.1

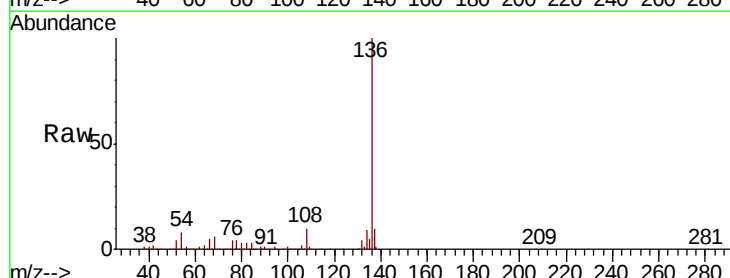


Abundance


Ion 136.00 (135.70 to 136.70): BM017163.D (-1261) (-)

Ion 137.00 (136.70 to 137.70): BM017163.D (-1261) (-)

Ion 54.00 (53.70 to 54.70): BM017163.D (-1261) (-)

Ion 68.00 (67.70 to 68.70): BM017163.D (-1261) (-)

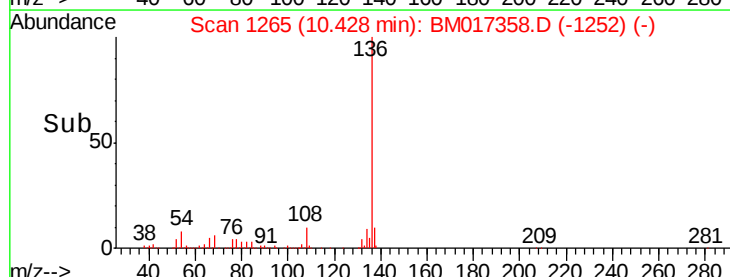


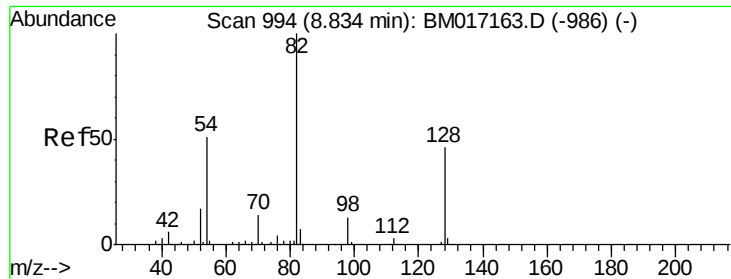




#23
Nitrobenzene-d5
Concen: 87.422 ng
RT: 8.80 min Scan# 989
Delta R.T. -0.03 min
Lab File: BM017358.D
Acq: 26 Oct 2018 21:10

Instrument :
BNA_M
ClientSampled :

Tot Ion: 82 Resp: 1460331
Ion Ratio Lower Upper
82 100
128 41.5 37.0 55.6
54 49.4 40.7 61.1

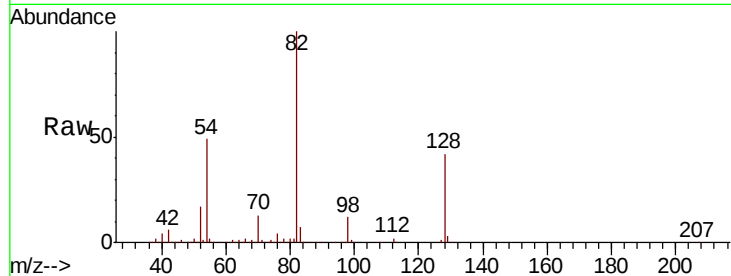


Abundance Ion 82.00 (81.70 to 82.70): BM017163.D (-986) (-)
Ion 128.00 (127.70 to 128.70): BM017163.D (-986) (-)
Ion 54.00 (53.70 to 54.70): BM017163.D (-986) (-)

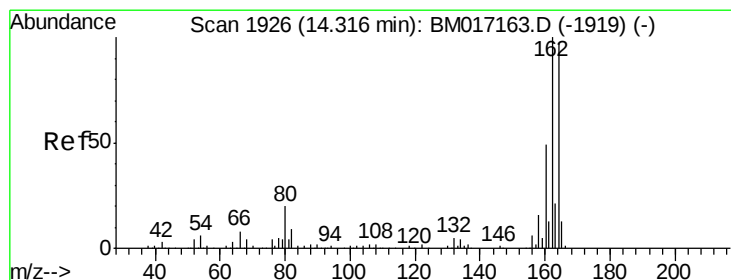
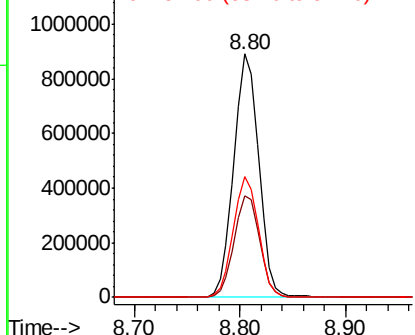



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.29 min Scan# 1922
Delta R.T. -0.02 min
Lab File: BM017358.D
Acq: 26 Oct 2018 21:10

Tgt Ion: 164 Resp: 617407
Ion Ratio Lower Upper
164 100
162 103.6 82.1 123.1
160 45.9 40.2 60.2

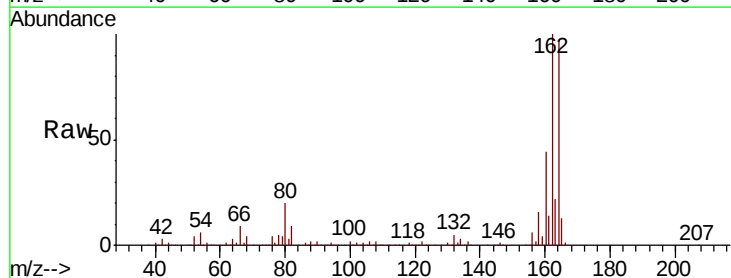

Abundance Ion 164.00 (163.70 to 164.70): BM017163.D (-1919) (-)
Ion 162.00 (161.70 to 162.70): BM017163.D (-1919) (-)
Ion 160.00 (159.70 to 160.70): BM017163.D (-1919) (-)

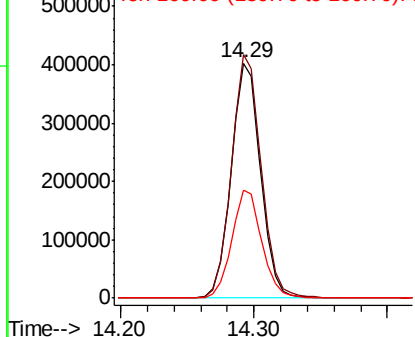


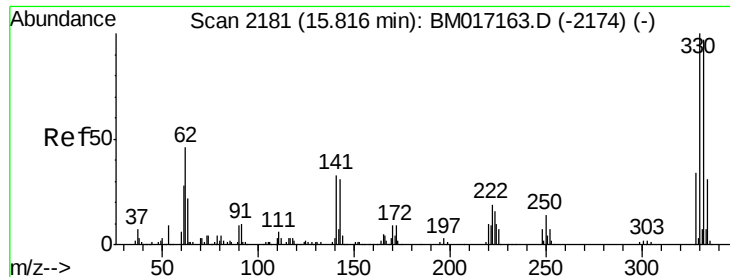




#42
 2,4,6-Tribromophenol
 Concen: 141.363 ng
 RT: 15.79 min Scan# 2177
 Delta R.T. -0.02 min
 Lab File: BM017358.D
 Acq: 26 Oct 2018 21:10

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion:330 Resp: 1180317
 Ion Ratio Lower Upper
 330 100
 332 97.5 77.3 115.9
 141 33.8 27.4 41.0

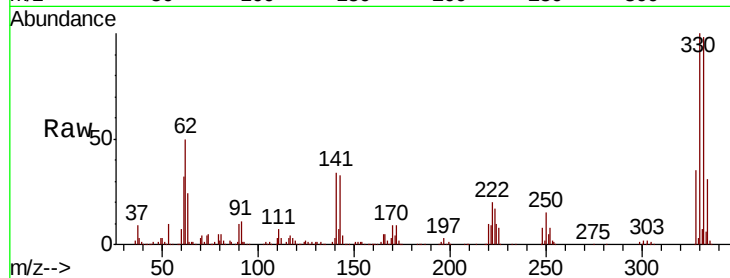


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

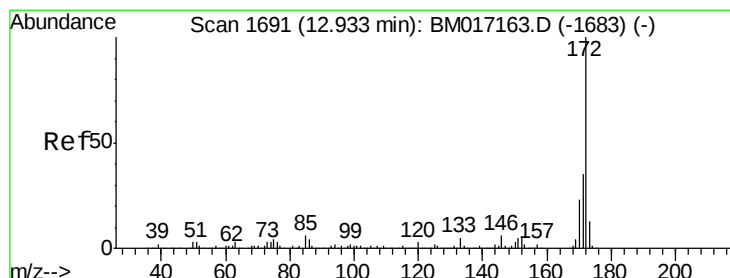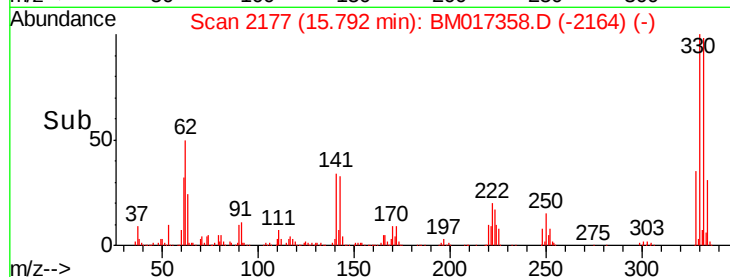
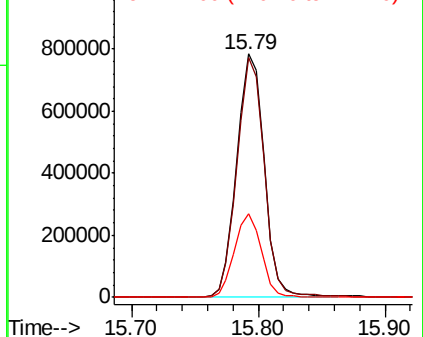



#45
 2-Fluorobiphenyl
 Concen: 78.485 ng
 RT: 12.91 min Scan# 1687
 Delta R.T. -0.02 min
 Lab File: BM017358.D
 Acq: 26 Oct 2018 21:10

Tgt Ion:172 Resp: 3641909
 Ion Ratio Lower Upper
 172 100
 171 34.6 28.3 42.5
 170 22.3 18.3 27.5

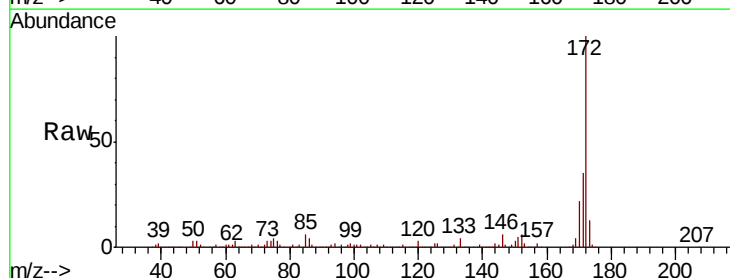

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

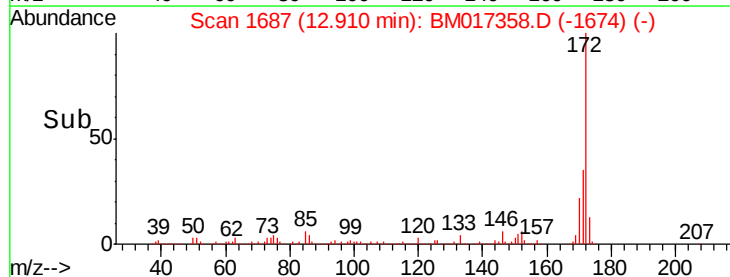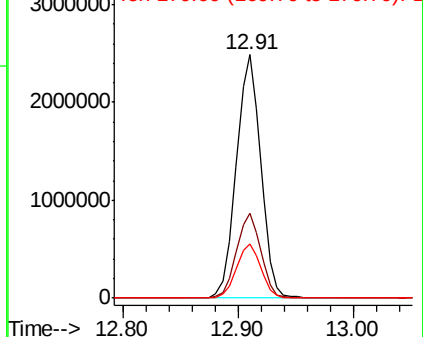


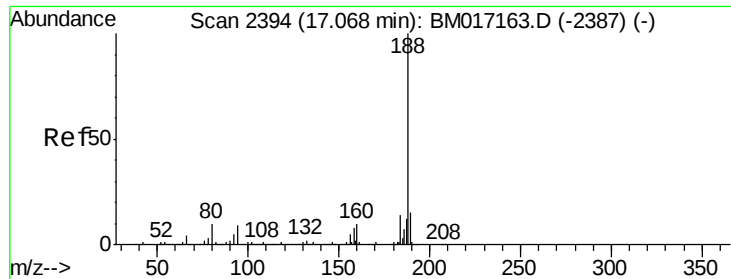




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.05 min Scan# 2390
Delta R.T. -0.02 min
Lab File: BM017358.D
Acq: 26 Oct 2018 21:10

Instrument :
BNA_M
ClientSampled :

Tot Ion:188 Resp: 1594880
Ion Ratio Lower Upper
188 100
94 9.0 7.0 10.4
80 10.3 7.7 11.5

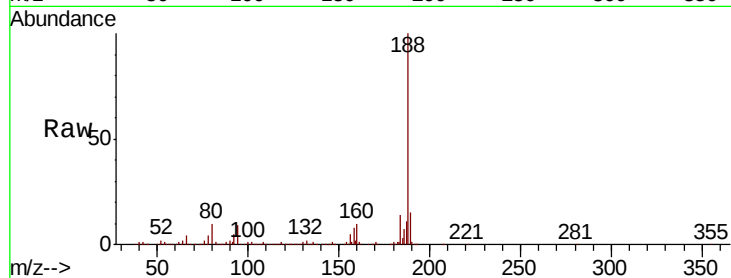


Abundance Ion 188.00 (187.70 to 188.70): E
1500000
Ion 94.00 (93.70 to 94.70): BM
Ion 80.00 (79.70 to 80.70): BM

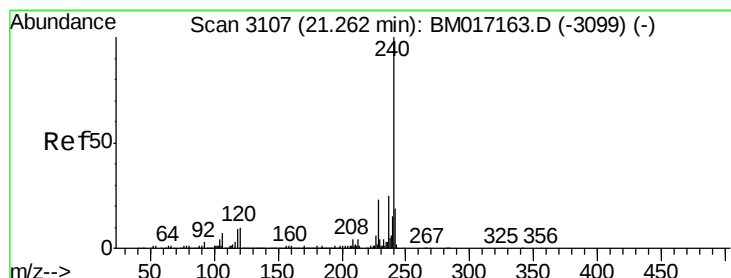
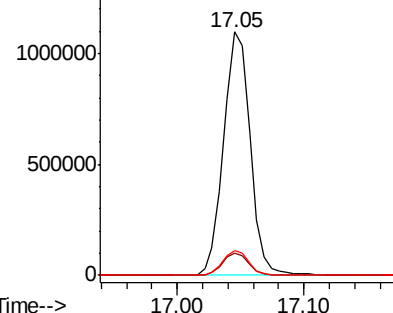



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.24 min Scan# 3104
Delta R.T. -0.02 min
Lab File: BM017358.D
Acq: 26 Oct 2018 21:10

Tgt Ion:240 Resp: 1850019
Ion Ratio Lower Upper
240 100
120 9.1 8.1 12.1
236 25.1 19.9 29.9

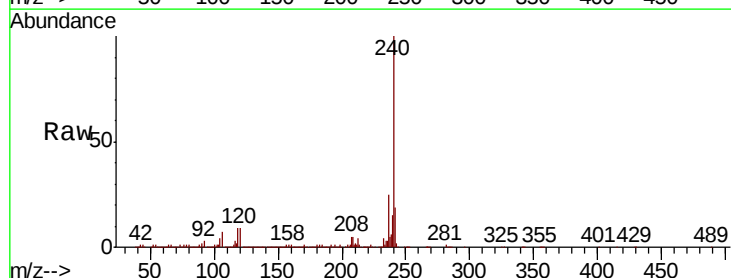

Abundance Ion 240.00 (239.70 to 240.70): E
2000000
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

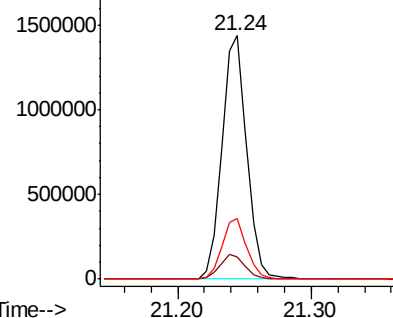



#79

Terphenyl-d14

Concen: 83.419 ng

RT: 19.69 min Scan# 2839

Delta R.T. -0.02 min

Lab File: BM017358.D

Acq: 26 Oct 2018 21:10

Instrument :

BNA_M

ClientSampleId :


Tot Ion:244 Resp: 6846793

Ion Ratio Lower Upper

244 100

212 7.4 5.5 8.3




122 10.9 8.4 12.6

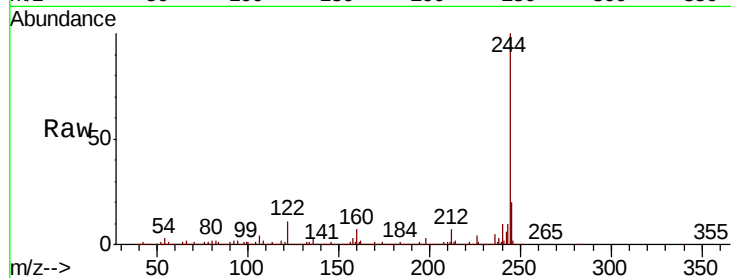

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

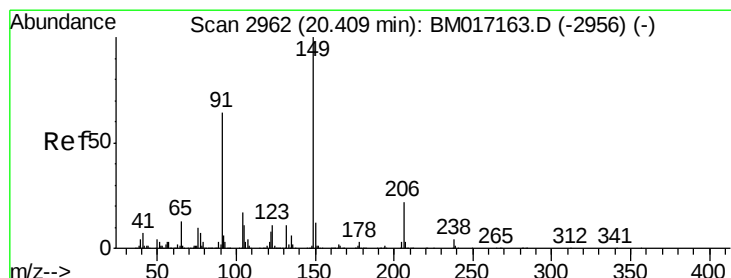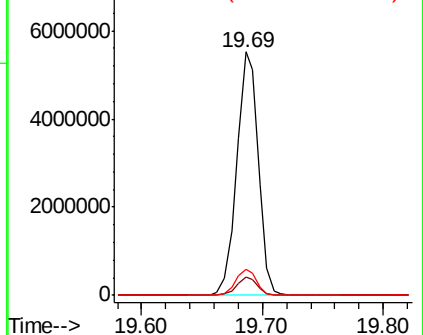

#80

Butylbenzylphthalate

Concen: 7.180 ng

RT: 20.40 min Scan# 2961

Delta R.T. -0.01 min

Lab File: BM017358.D

Acq: 26 Oct 2018 21:10


Tgt Ion:149 Resp: 177

Ion Ratio Lower Upper

149 100

91 52.4 51.3 76.9



206 0.0 18.0 27.0#

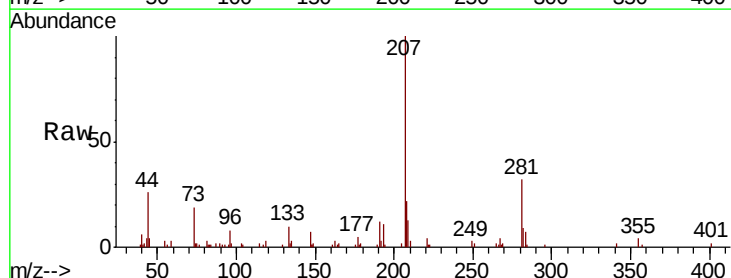


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 91.00 (90.70 to 91.70): BM0

Ion 206.00 (205.70 to 206.70): E




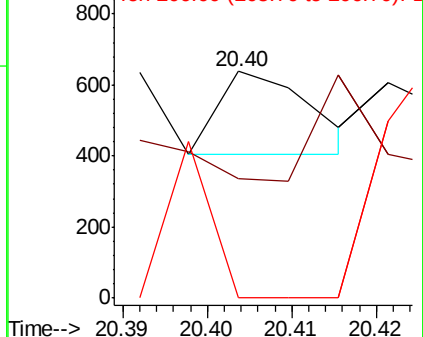




#84
 Bis(2-ethylhexyl)phthalate
 Concen: 5.341 ng
 RT: 21.17 min Scan# 3091
 Delta R.T. -0.02 min
 Lab File: BM017358.D
 Acq: 26 Oct 2018 21:10




Instrument :
 BNA_M
 ClientSampleId :


Tot Ion:149 Resp: 2260
 Ion Ratio Lower Upper
 149 100
 167 24.9 22.2 33.4
 279 13.1 3.6 5.4#

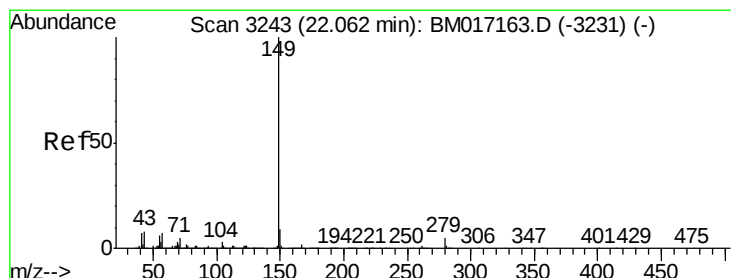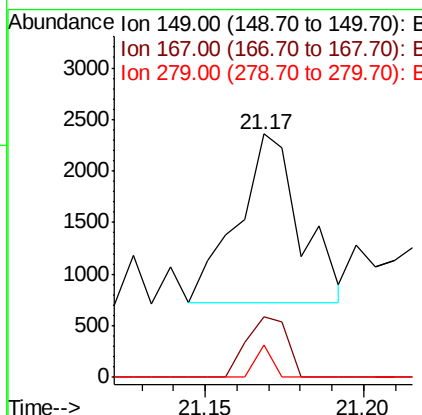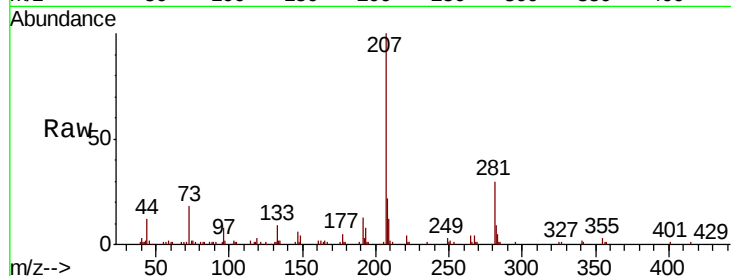

#85
 Di-n-octyl phthalate
 Concen: 5.584 ng
 RT: 22.04 min Scan# 3239
 Delta R.T. -0.02 min
 Lab File: BM017358.D
 Acq: 26 Oct 2018 21:10

Tgt Ion:149 Resp: 1393
 Ion Ratio Lower Upper
 149 100
 167 19.0 1.4 2.0#
 43 63.2 7.2 10.8#

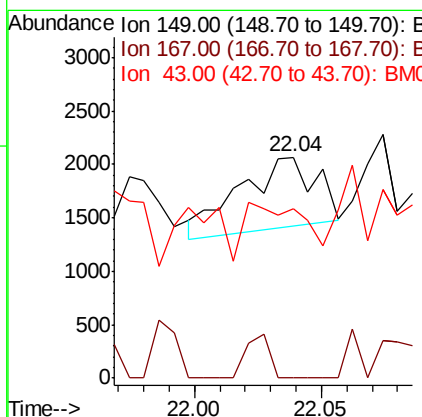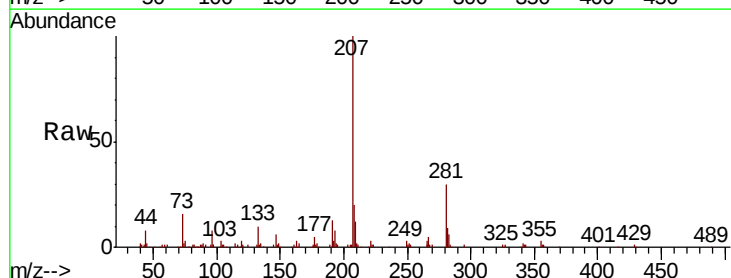



#87
 Pervlene-d12
 Concen: 20.000 ng
 RT: 23.46 min Scan# 3480
 Delta R.T. -0.02 min
 Lab File: BM017358.D
 Acq: 26 Oct 2018 21:10

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion:264 Resp: 1676969
 Ion Ratio Lower Upper
 264 100
 260 22.9 18.6 27.8
 265 22.3 17.8 26.8

