

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102618\
 Data File : BM017352.D
 Acq On : 26 Oct 2018 17:33
 Operator : MJ/SJ
 Sample : PB114216BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB114216BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM101718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.822	307	312	320	rBV	129442	192460	1.17%	0.238%
2	5.275	382	389	406	rBV	3667937	5456016	33.16%	6.751%
3	6.840	647	655	673	rBV	3881067	6098820	37.06%	7.546%
4	7.193	707	715	728	rBV	3923964	6106667	37.11%	7.556%
5	7.651	784	793	801	rBV	886593	1403582	8.53%	1.737%
6	7.969	839	847	857	rBV	2777295	4391721	26.69%	5.434%
7	8.804	981	989	1003	rBV	2147353	3666075	22.28%	4.536%
8	10.428	1256	1265	1284	rBV	1222747	2091828	12.71%	2.588%
9	12.910	1680	1687	1707	rBV	6494708	9481097	57.62%	11.732%
10	14.298	1916	1923	1936	rBV2	1889681	3095582	18.81%	3.830%
11	15.792	2170	2177	2198	rBV	5097892	8028212	48.79%	9.934%
12	17.051	2384	2391	2405	rBV2	2677995	4127837	25.09%	5.108%
13	19.686	2833	2839	2848	rBV	13310395	16455010	100.00%	20.361%
14	21.245	3099	3104	3115	rBV	4145005	5458818	33.17%	6.755%
15	23.456	3473	3480	3493	rVB	2447260	4763520	28.95%	5.894%


Sum of corrected areas: 80817245

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102618\
Data File : BM017352.D
Acq On : 26 Oct 2018 17:33
Operator : MJ/SJ
Sample : PB114216BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB114216BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM101718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

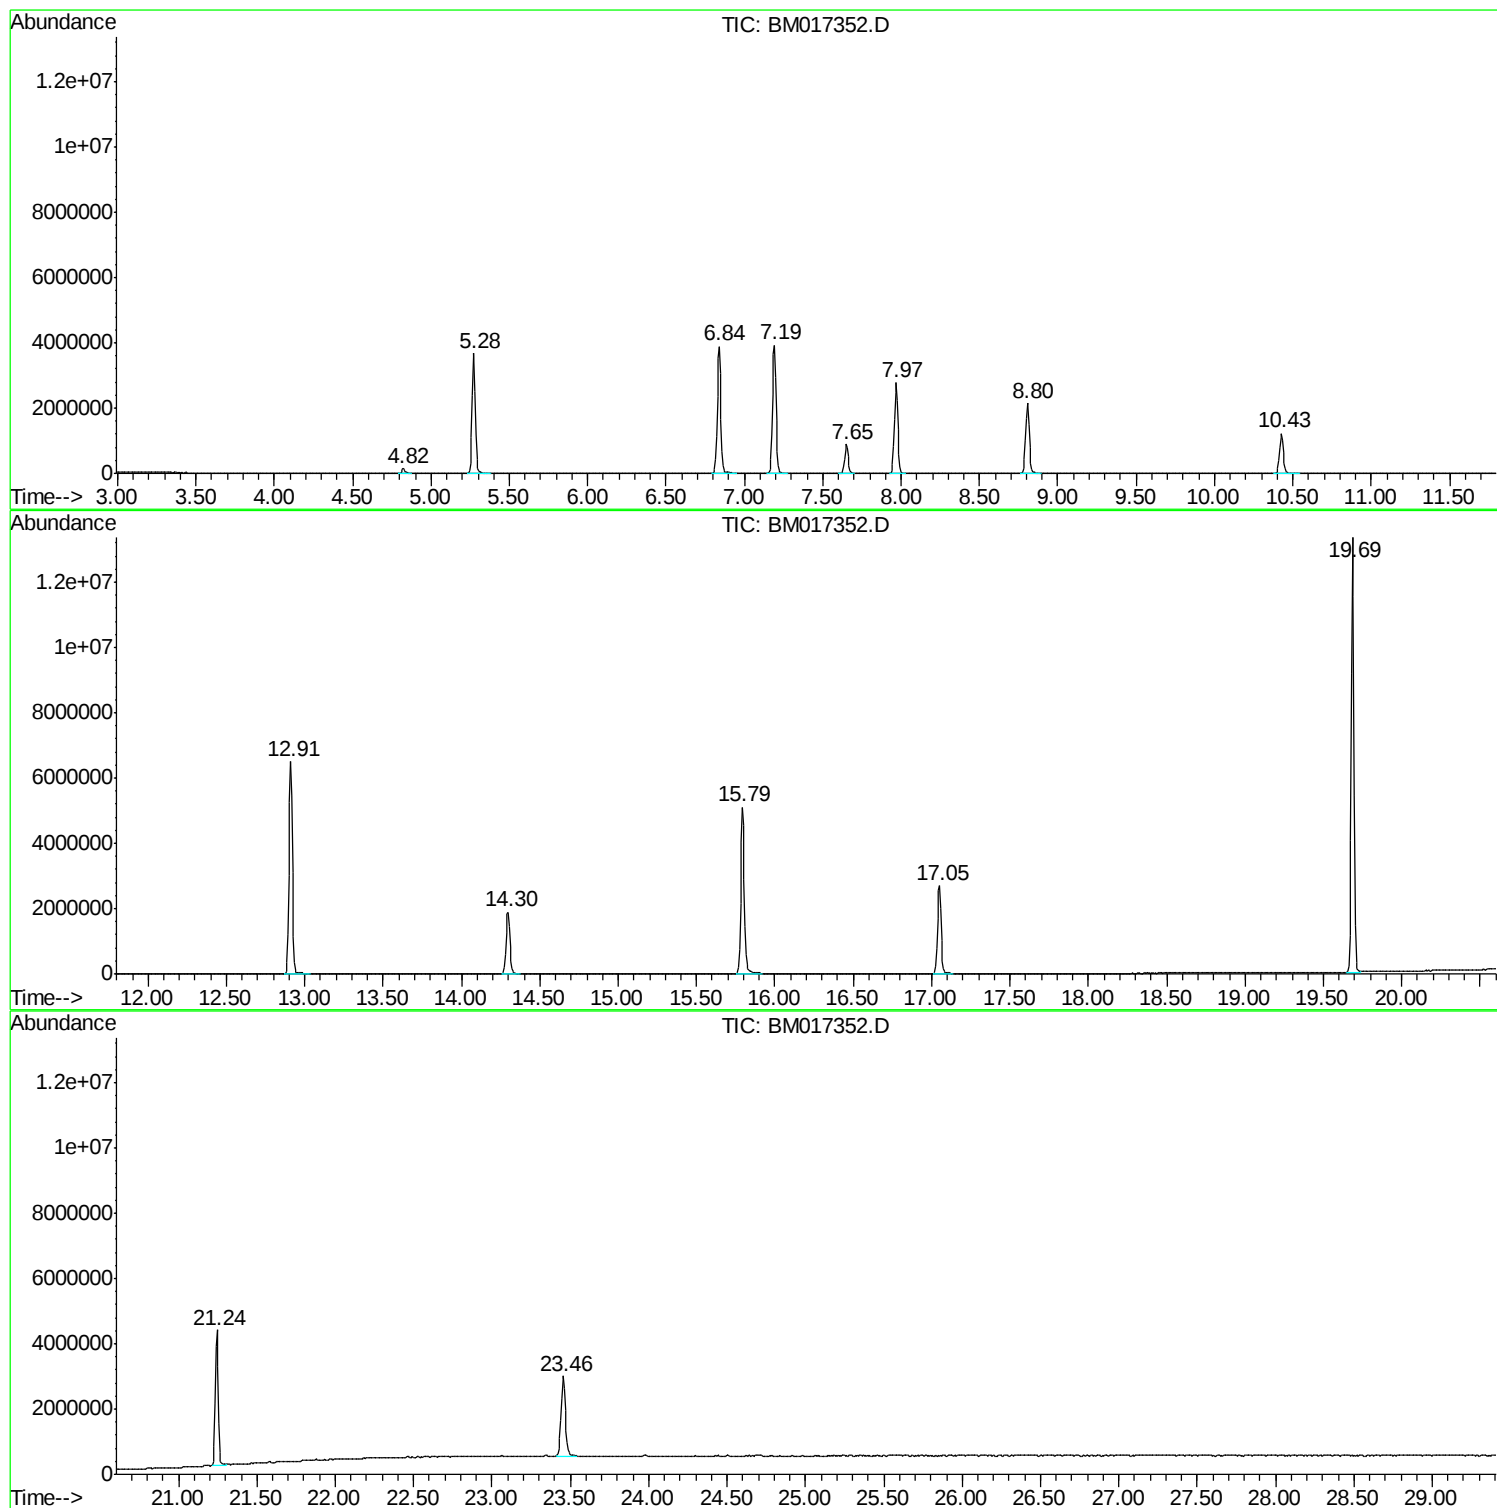

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102618\
Data File : BM017352.D
Acq On : 26 Oct 2018 17:33
Operator : MJ/SJ
Sample : PB114216BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB114216BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM101718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.82	2.74 ng	192460	1,4-Dichlorobenzene-d4	7.65

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50
2		2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	35
3		Dimethadione	129	C5H7NO3	000695-53-4	33
4		Hydrazine, 1,1-bis(1-methylethyl)-	116	C6H16N2	000921-14-2	28
5		(+)-4-Amino-4,5-dihydro-2(3H)-f...	101	C4H7NO2	016504-58-8	9

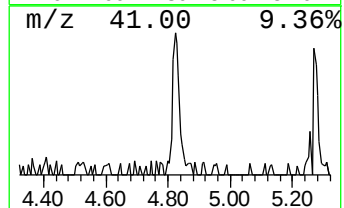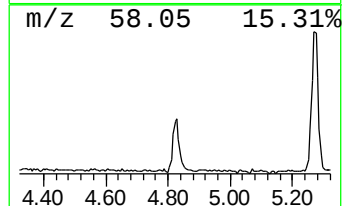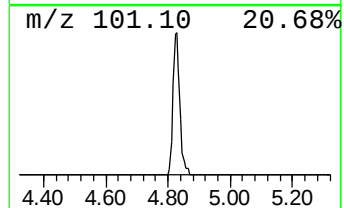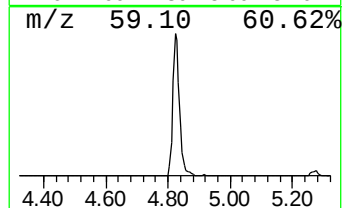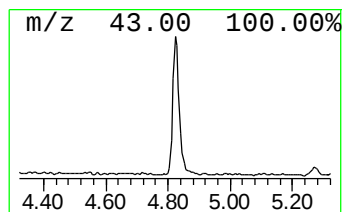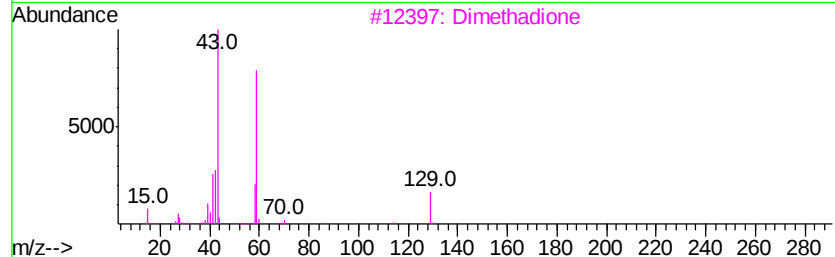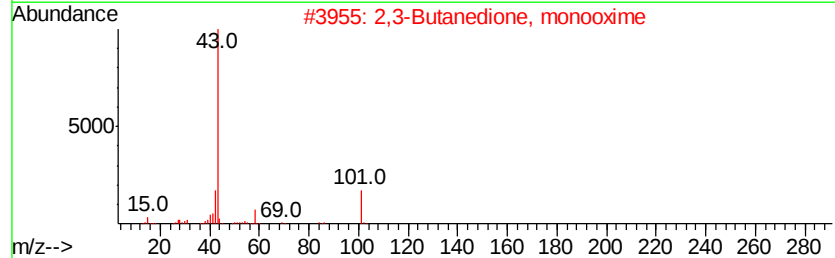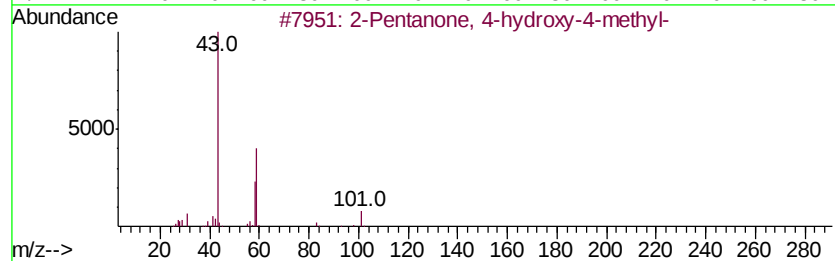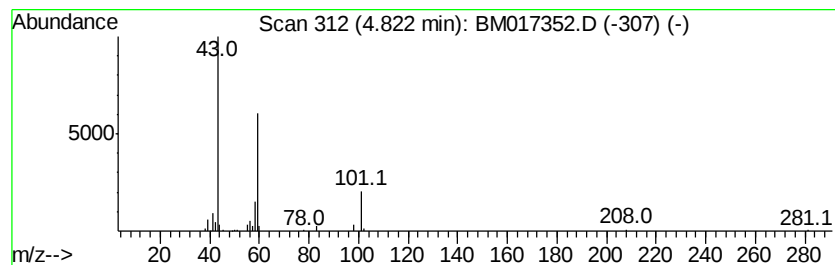

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102618\
Data File : BM017352.D
Acq On : 26 Oct 2018 17:33
Operator : MJ/SJ
Sample : PB114216BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB114216BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM101718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.19 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.19	87.02 ng	6106670	1,4-Dichlorobenzene-d4	7.65

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	12
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	12
4		5-Aminoindole	132	C8H8N2	005192-03-0	9
5		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9

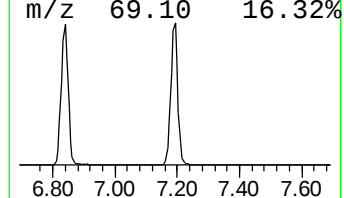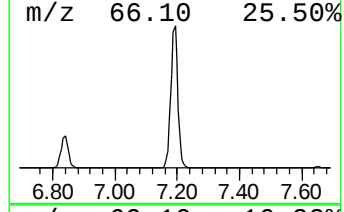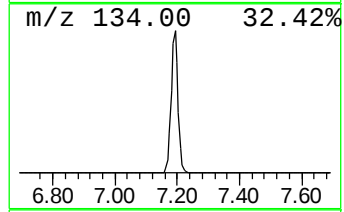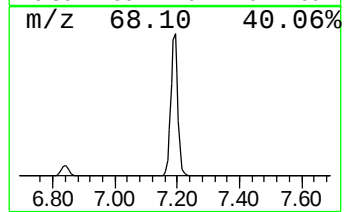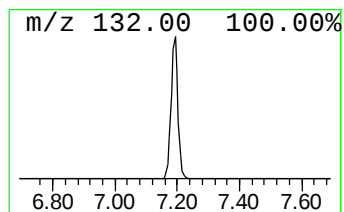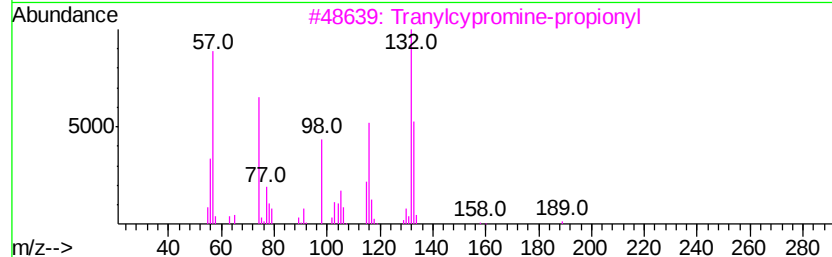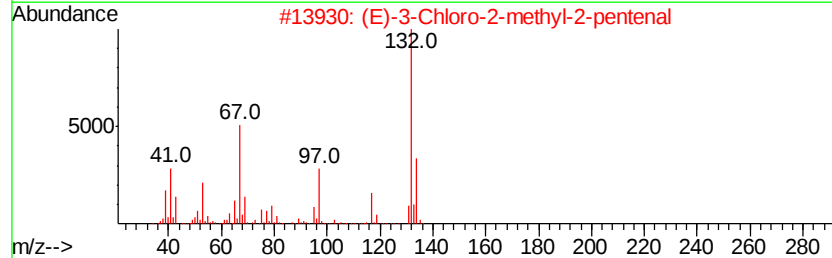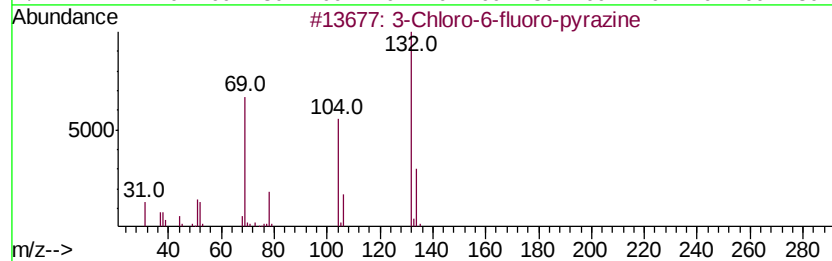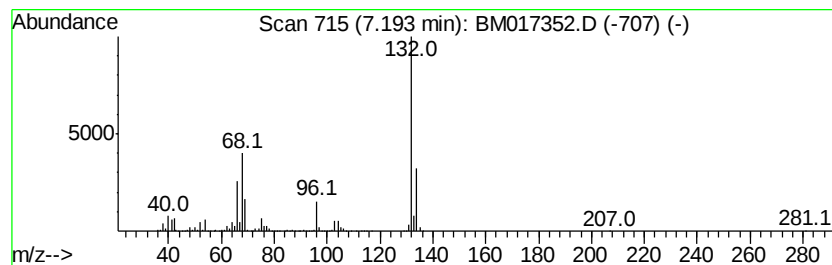

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM102618\
Data File : BM017352.D
Acq On : 26 Oct 2018 17:33
Operator : MJ/SJ
Sample : PB114216BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB114216BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM101718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.82	2.7	ng	192460	1	7.65	1403580	20.0
unknown7.19	7.19	87.0	ng	6106670	1	7.65	1403580	20.0