


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM102618\
 Data File : BM017349.D
 Acq On : 26 Oct 2018 15:45
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM101718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 17 14:23:17 2018

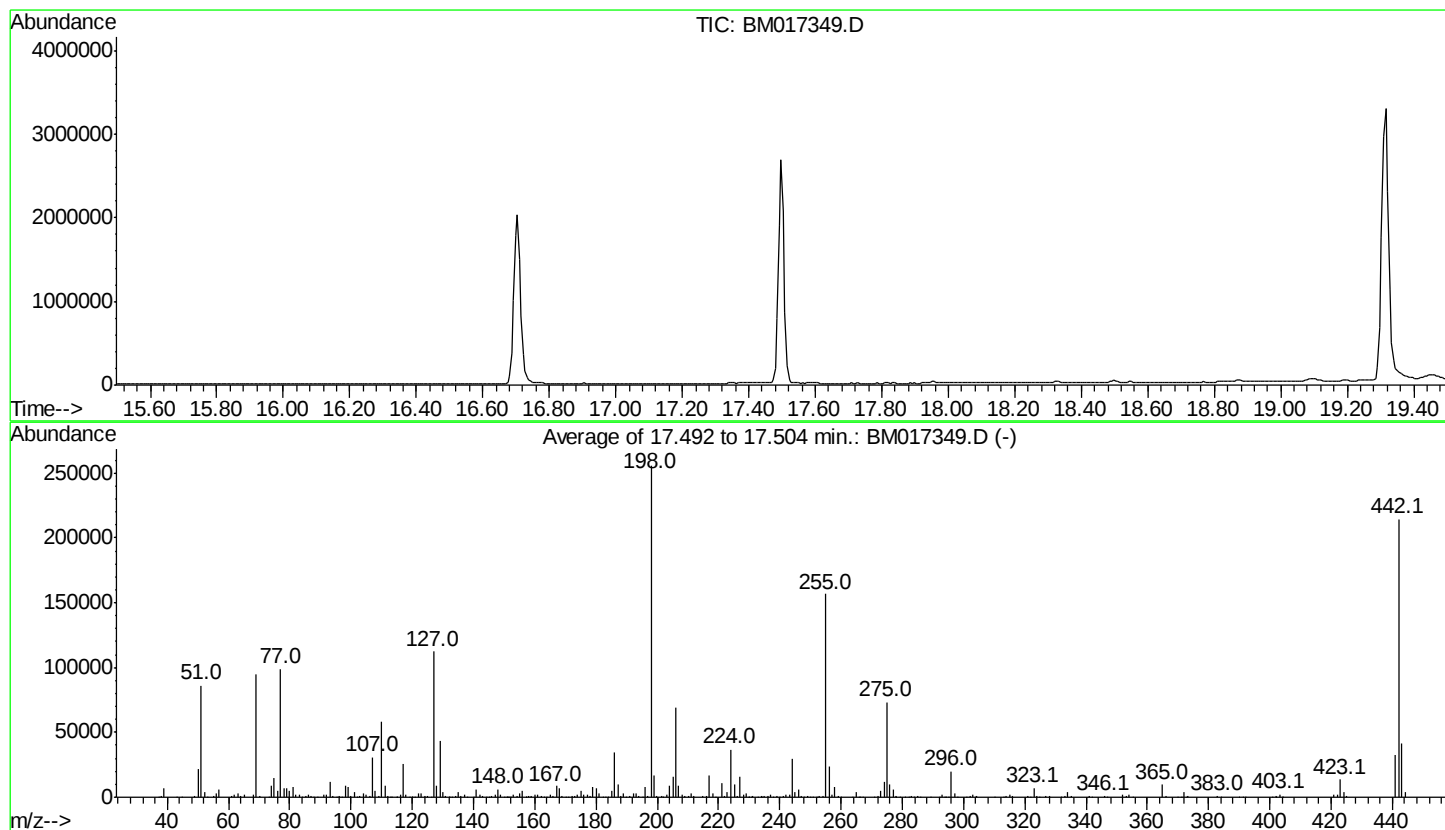

AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	86160	PASS
68	69	0.00	2	1.8	1690	PASS
69	198	0.00	100	36.9	94410	PASS
70	69	0.00	2	0.7	621	PASS
127	198	10	80	43.9	112360	PASS
197	198	0.00	2	0.6	1448	PASS
198	198	100	100	100.0	255658	PASS
199	198	5	9	6.4	16483	PASS
275	198	10	60	28.8	73514	PASS
365	198	1	100	3.7	9480	PASS
441	198	0.01	100	12.8	32674	PASS
442	198	50	100	84.0	214634	PASS
443	442	15	24	19.2	41130	PASS