


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102623\
 Data File : BM042452.D
 Acq On : 26 Oct 2023 14:45
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Oct 21 02:32:53 2023

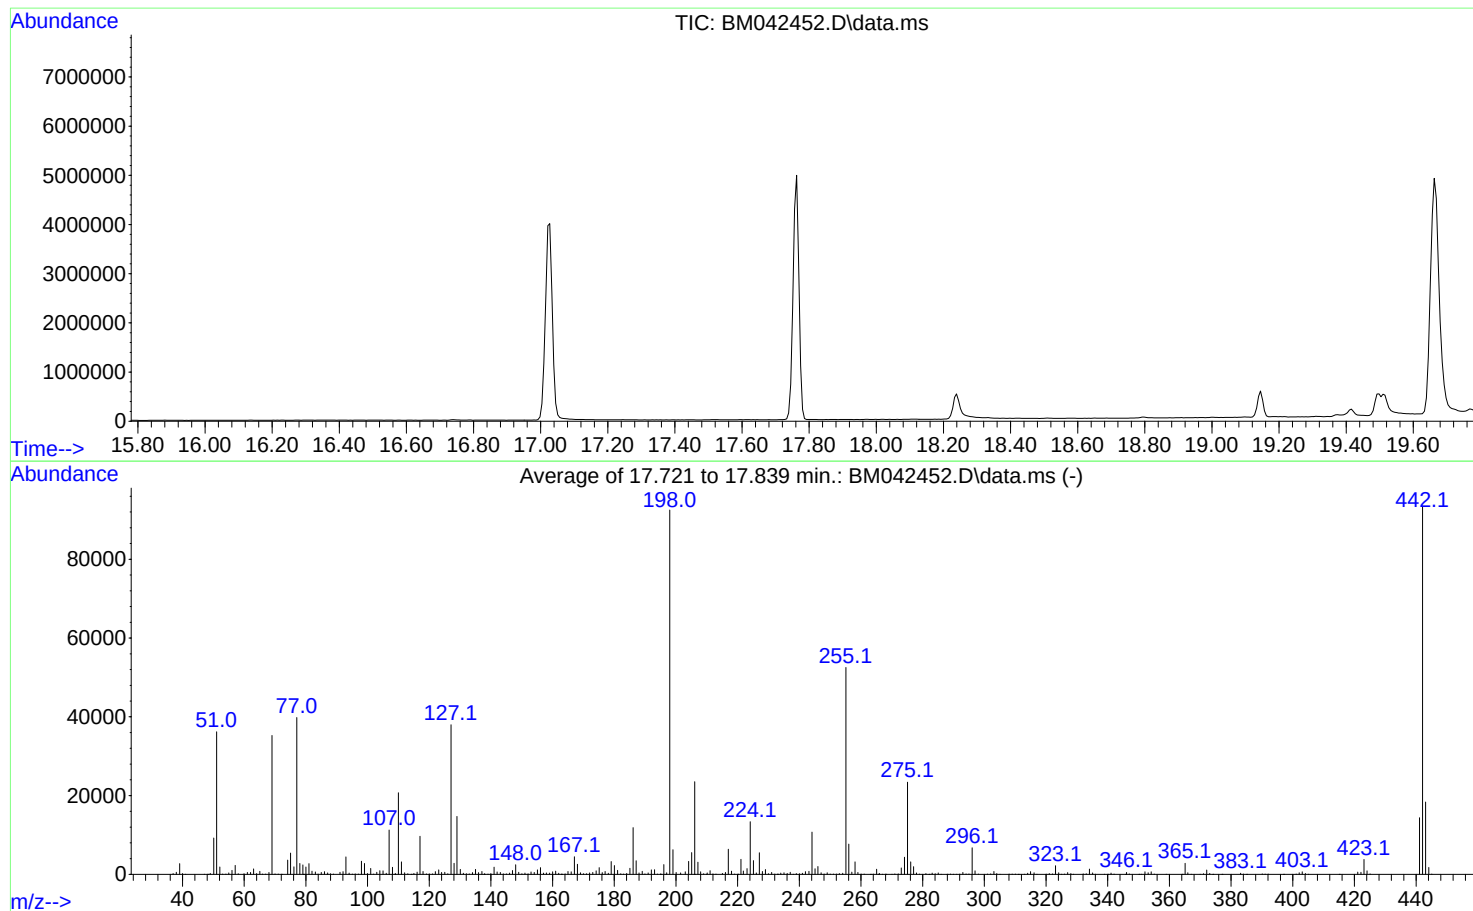




AutoFind: Averaged scan 2471 to 2491; Bkg corrected with scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	36191	PASS
68	69	0.00	2	1.4	502	PASS
69	198	0.00	100	38.1	35276	PASS
70	69	0.00	2	0.3	123	PASS
127	198	10	80	41.1	37997	PASS
197	198	0.00	2	0.4	394	PASS
198	198	100	100	100.0	92499	PASS
199	198	5	9	6.8	6247	PASS
275	198	10	60	25.3	23404	PASS
365	198	1	100	3.1	2822	PASS
441	198	0.01	100	15.6	14393	PASS
442	442	50	100	100.0	93404	PASS
443	442	15	24	19.7	18354	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102623\
 Data File : BM042452.D
 Acq On : 26 Oct 2023 14:45
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Oct 27 02:20:54 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 21 02:32:53 2023
 Response via : Initial Calibration

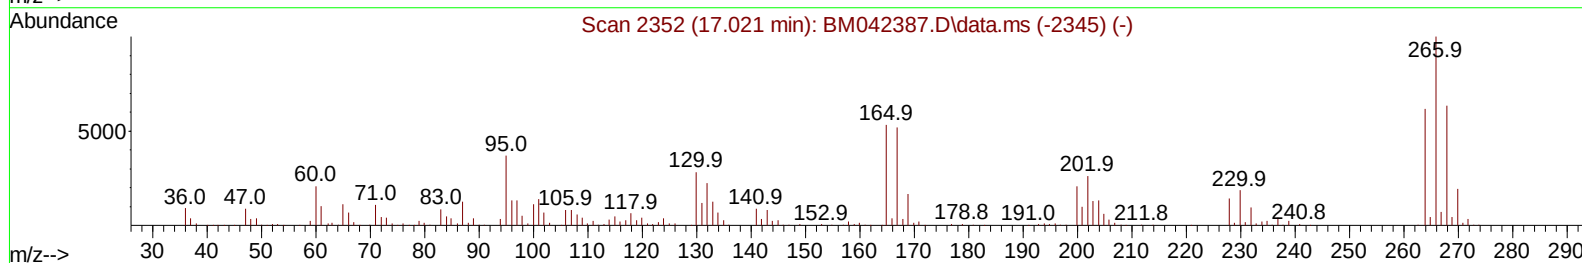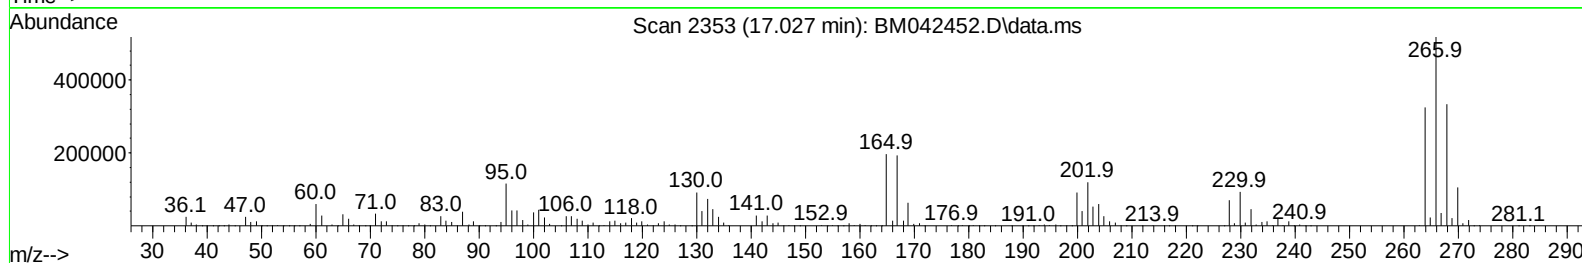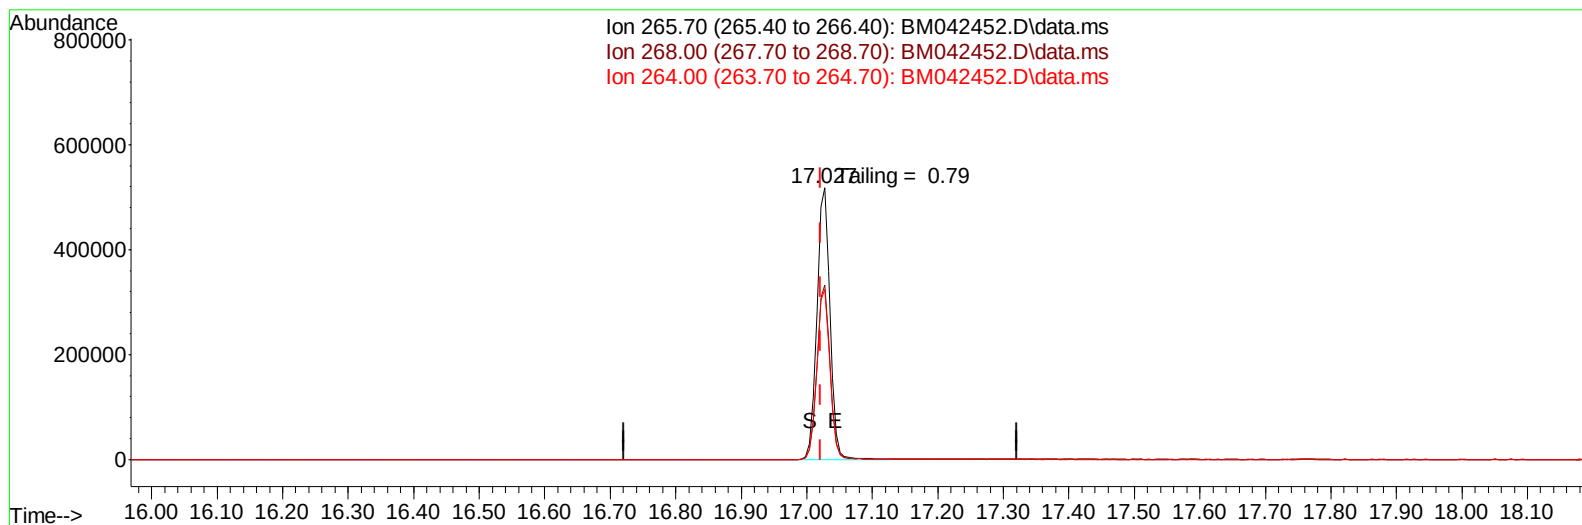

TIC: BM042452.D\data.ms

(70) Pentachlorophenol (C)

17.027min (+ 0.006) 168521.84 ng




response 723079

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	64.35
264.00	61.70	62.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102623\
Data File : BM042452.D
Acq On : 26 Oct 2023 14:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Oct 27 02:20:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 21 02:32:53 2023
Response via : Initial Calibration

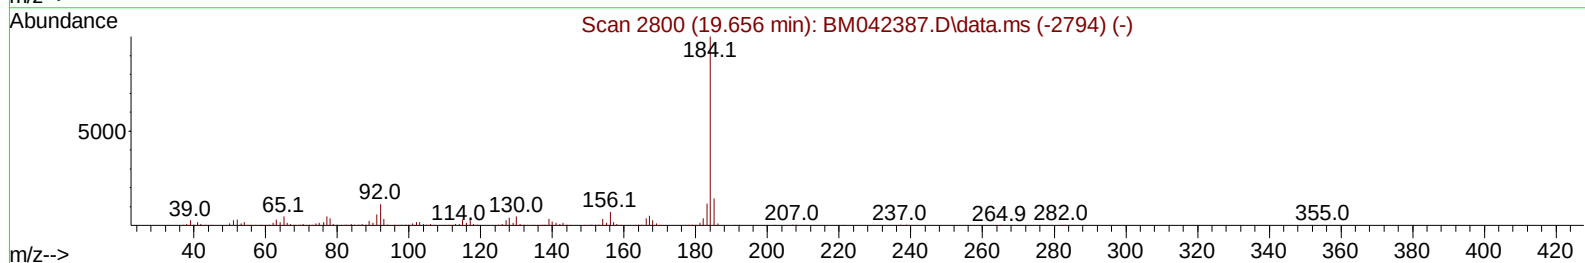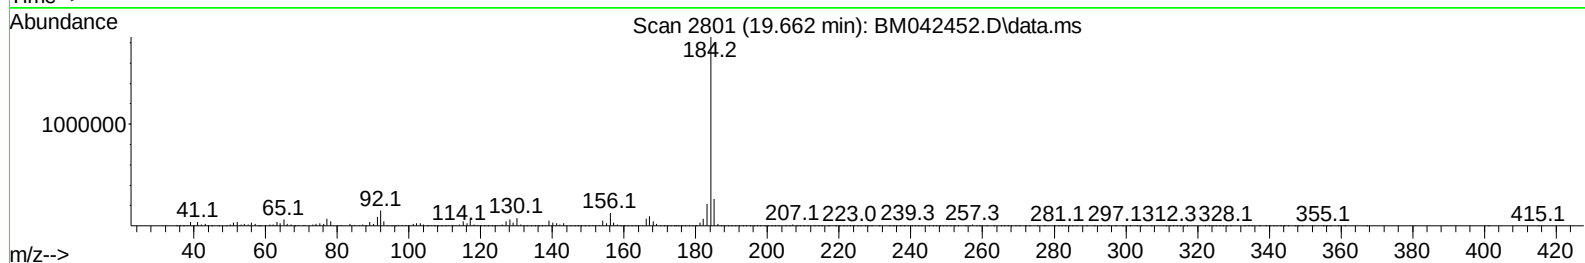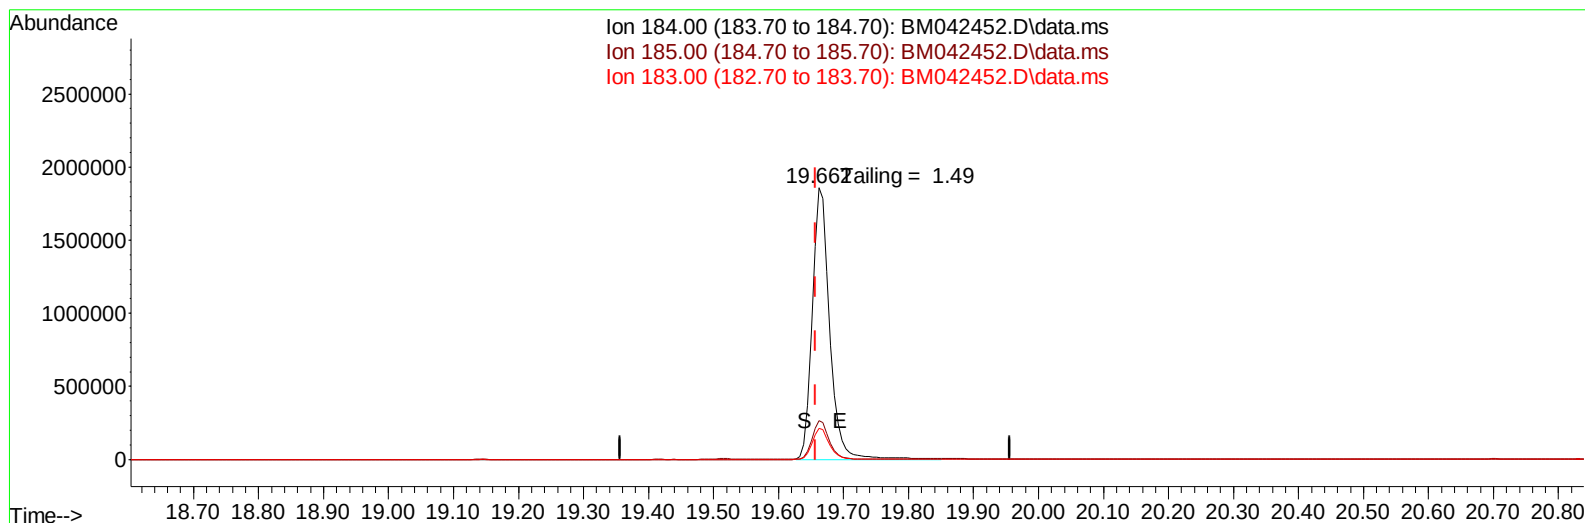

TIC: BM042452.D\data.ms

(77) Benzidine**19.662min (+ 0.006) 53226.65 ng****response 3435222**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.37
183.00	11.50	11.45
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/26/2023	BNA_M	<u>BM042452.D</u>
Compound Name	Response	Retention Time
DDT	1794497	20.851
DDD	35114	20.451
DDE	1259	19.898
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
36373	1830870	1.99

Instrument :
BNA_M
ClientSampleId :
DFTPP