

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102718\
 Data File : BM017376.D
 Acq On : 27 Oct 2018 08:09
 Operator : MJ/SJ
 Sample : J5673-20
 Misc : GCMS Confirmation
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0BM4

Quant Time: Oct 29 15:23:59 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 26 01:13:26 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	238566	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	1027624	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	647664	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.05	188	1587447	20.00	ng/ul	0.00
78) Chrysene-d12	21.24	240	1864934	20.00	ng/ul	0.00
86) Perylene-d12	23.45	264	1845195	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0d	0.00	ng/uL
5) Phenol-d5	0.00	99	0	0.00	ng/ul
7) Bis-(2-Chloroethyl)ether-d	0.00	67	0	0.00	ng/ul
9) 2-Chlorophenol-d4	0.00	132	0	0.00	ng/ul
13) 4-Methylphenol-d8	0.00	113	0	0.00	ng/ul
19) Nitrobenzene-d5	0.00	128	0	0.00	ng/ul
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul
44) Dimethylphthalate-d6	0.00	166	0d	0.00	ng/ul
47) Acenaphthylene-d8	0.00	160	0d	0.00	ng/ul
52) 4-Nitrophenol-d4	0.00	143	0d	0.00	ng/ul
58) Fluorene-d10	0.00	176	0d	0.00	ng/ul
63) 4,6-Dinitro-2-methylphenol	0.00	200	0d	0.00	ng/ul
71) Anthracene-d10	0.00	188	0d	0.00	ng/ul
79) Pyrene-d10	0.00	212	0d	0.00	ng/ul
90) Benzo(a)pyrene-d12	0.00	264	0d	0.00	ng/ul

Target Compounds


				Ovalue
37) 1,2,4,5-Tetrachlorobenzene	12.47	216	213457	9.806 ng/ul 97
70) Phenanthrene	17.09	178	116092	1.274 ng/ul# 51
73) 1,2,3,4-Tetrachlorobenzene	13.08	216	247100	11.040 ng/uL 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102718\
Data File : BM017376.D
Acq On : 27 Oct 2018 08:09
Operator : MJ/SJ
Sample : J5673-20
Misc : GCMS Confirmation
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0BM4

Quant Time: Oct 29 15:23:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 26 01:13:26 2018
Response via : Initial Calibration

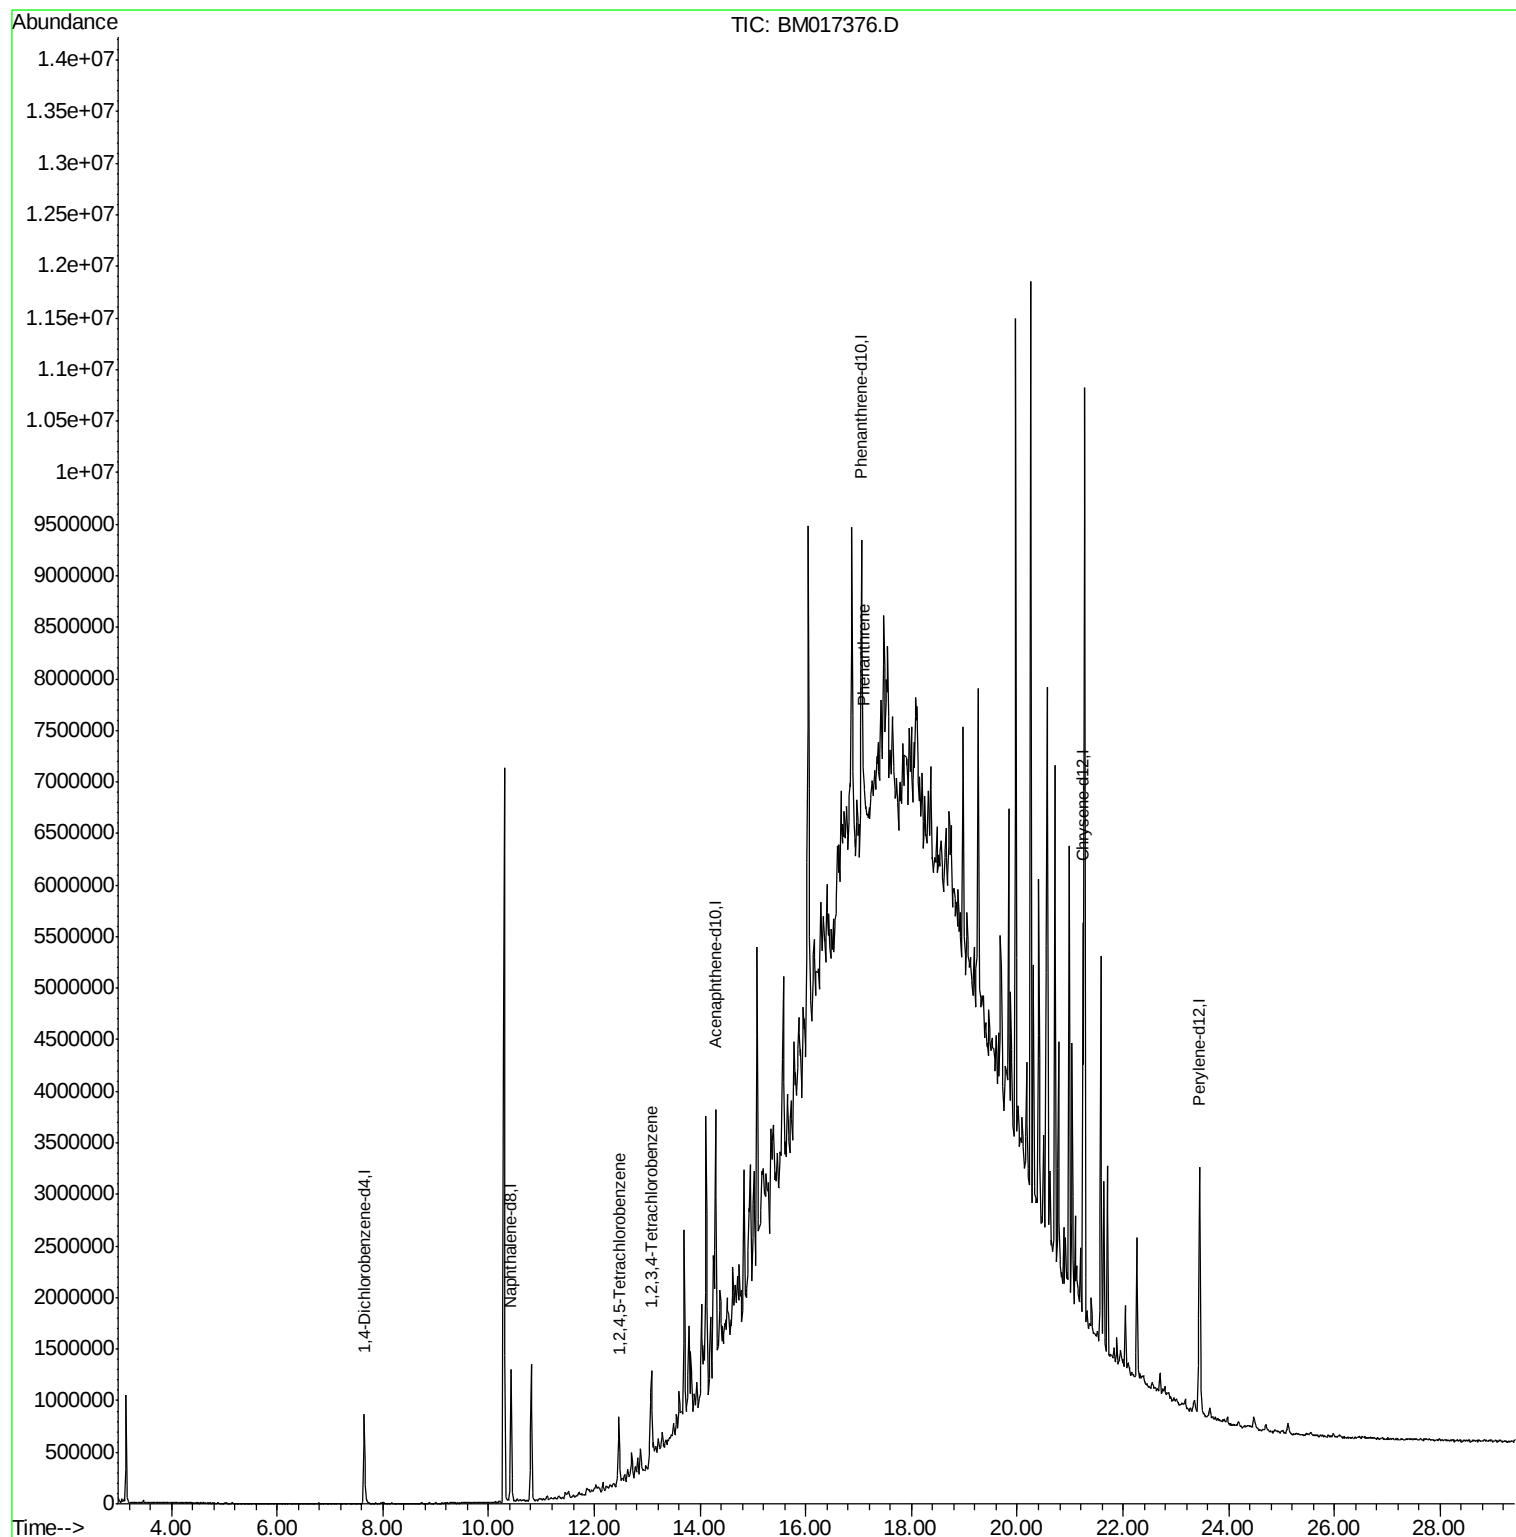

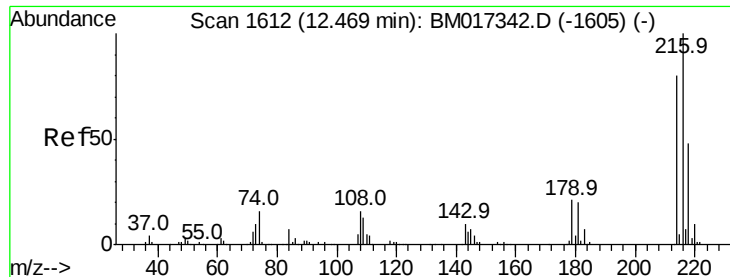

#37

1,2,4,5-Tetrachlorobenzene

Concen: 9.806 ng/ul

RT: 12.47 min Scan# 1612

Delta R.T. -0.00 min

Lab File: BM017376.D

Acq: 27 Oct 2018 08:09

Instrument :

BNA_M

ClientSampleId :

C0BM4

Tot Ion:216 Resp: 213457


Ion Ratio Lower Upper

216 100

214 78.6 61.7 92.5

179 22.9 16.0 24.0

108 17.5 12.6 18.8



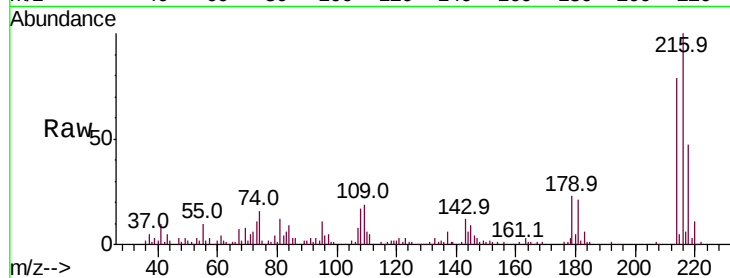


Abundance Ion 216.00 (215.70 to 216.70): E

Ion 214.00 (213.70 to 214.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 108.00 (107.70 to 108.70): E

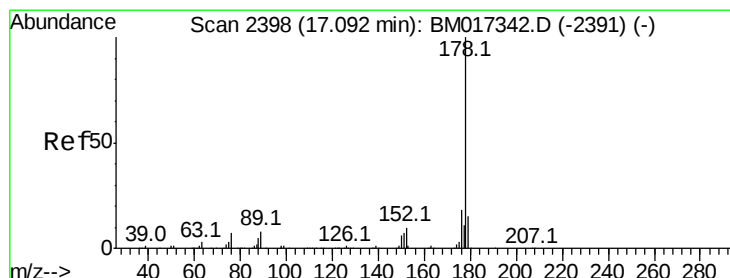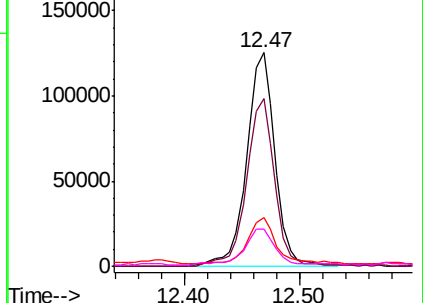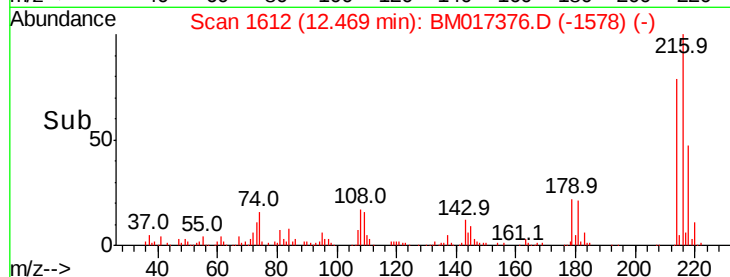

#70

Phenanthrene

Concen: 1.274 ng/ul

RT: 17.09 min Scan# 2398

Delta R.T. -0.00 min

Lab File: BM017376.D

Acq: 27 Oct 2018 08:09


Tgt Ion:178 Resp: 116092

Ion Ratio Lower Upper

178 100

179 50.4 12.2 18.2#



176 27.8 14.9 22.3#

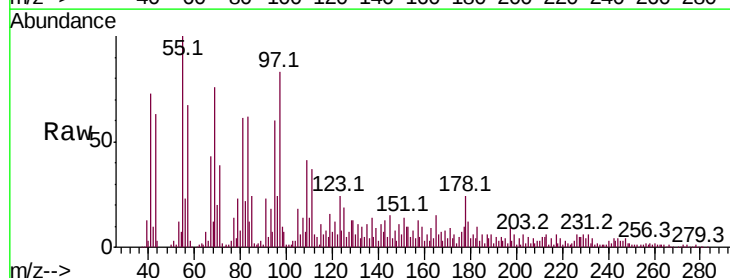


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

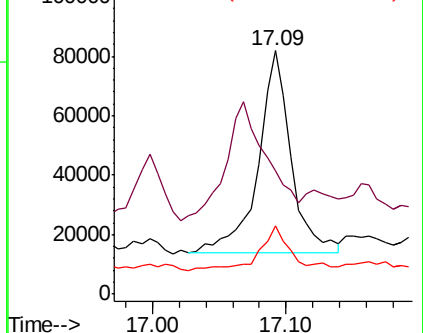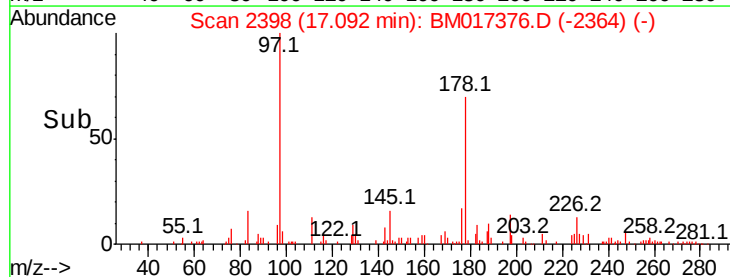

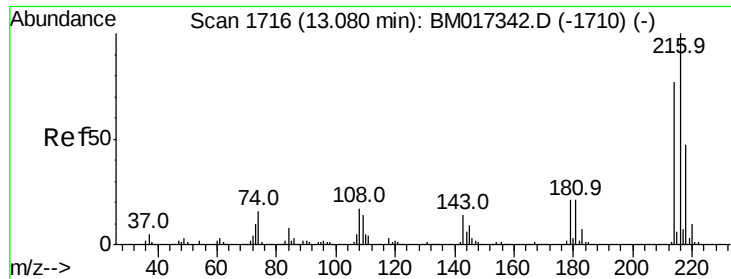

#73

1,2,3,4-Tetrachlorobenzene

Concen: 11.040 ng/uL

RT: 13.08 min Scan# 1716

Delta R.T. -0.00 min

Lab File: BM017376.D

Acq: 27 Oct 2018 08:09

Instrument :

BNA_M

ClientSampleId :

C0BM4


Tot Ion:216 Resp: 247100

Ion Ratio Lower Upper

216 100

214 77.4 63.4 95.0

218 45.9 37.3 55.9

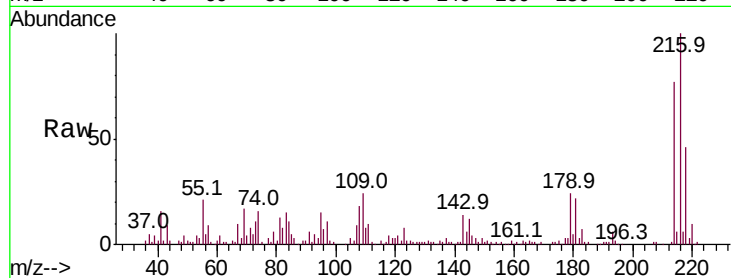

Abundance Ion 216.00 (215.70 to 216.70): E

Ion 214.00 (213.70 to 214.70): E

Ion 218.00 (217.70 to 218.70): E

