

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102718\
 Data File : BM017392.D
 Acq On : 27 Oct 2018 17:47
 Operator : MJ/SJ
 Sample : J5673-16
 Misc : GCMS Confirmation
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COBM0

Quant Time: Oct 29 04:20:22 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 26 01:13:26 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	272827	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	1227140	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	785611	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	1771810	20.00	ng/ul	0.00
78) Chrysene-d12	21.24	240	1981871	20.00	ng/ul	0.00
86) Perylene-d12	23.46	264	1978468	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0d	0.00	ng/uL
5) Phenol-d5	0.00	99	0	0.00	ng/ul
7) Bis-(2-Chloroethyl)ether-d	0.00	67	0d	0.00	ng/ul
9) 2-Chlorophenol-d4	0.00	132	0	0.00	ng/ul
13) 4-Methylphenol-d8	0.00	113	0	0.00	ng/ul
19) Nitrobenzene-d5	0.00	128	0	0.00	ng/ul
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul
44) Dimethylphthalate-d6	0.00	166	0	0.00	ng/ul
47) Acenaphthylene-d8	0.00	160	0	0.00	ng/ul
52) 4-Nitrophenol-d4	0.00	143	0d	0.00	ng/ul
58) Fluorene-d10	0.00	176	0d	0.00	ng/ul
63) 4,6-Dinitro-2-methylphenol	0.00	200	0d	0.00	ng/ul
71) Anthracene-d10	0.00	188	0d	0.00	ng/ul
79) Pyrene-d10	0.00	212	0d	0.00	ng/ul
90) Benzo(a)pyrene-d12	0.00	264	0d	0.00	ng/ul

Target Compounds


				Ovalue
73) 1,2,3,4-Tetrachlorobenzene	13.09	216	30265	1.211 ng/uL 95
77) Fluoranthene	19.11	202	163612	1.403 ng/ul# 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102718\
Data File : BM017392.D
Acq On : 27 Oct 2018 17:47
Operator : MJ/SJ
Sample : J5673-16
Misc : GCMS Confirmation
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0BM0

Quant Time: Oct 29 04:20:22 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 26 01:13:26 2018
Response via : Initial Calibration




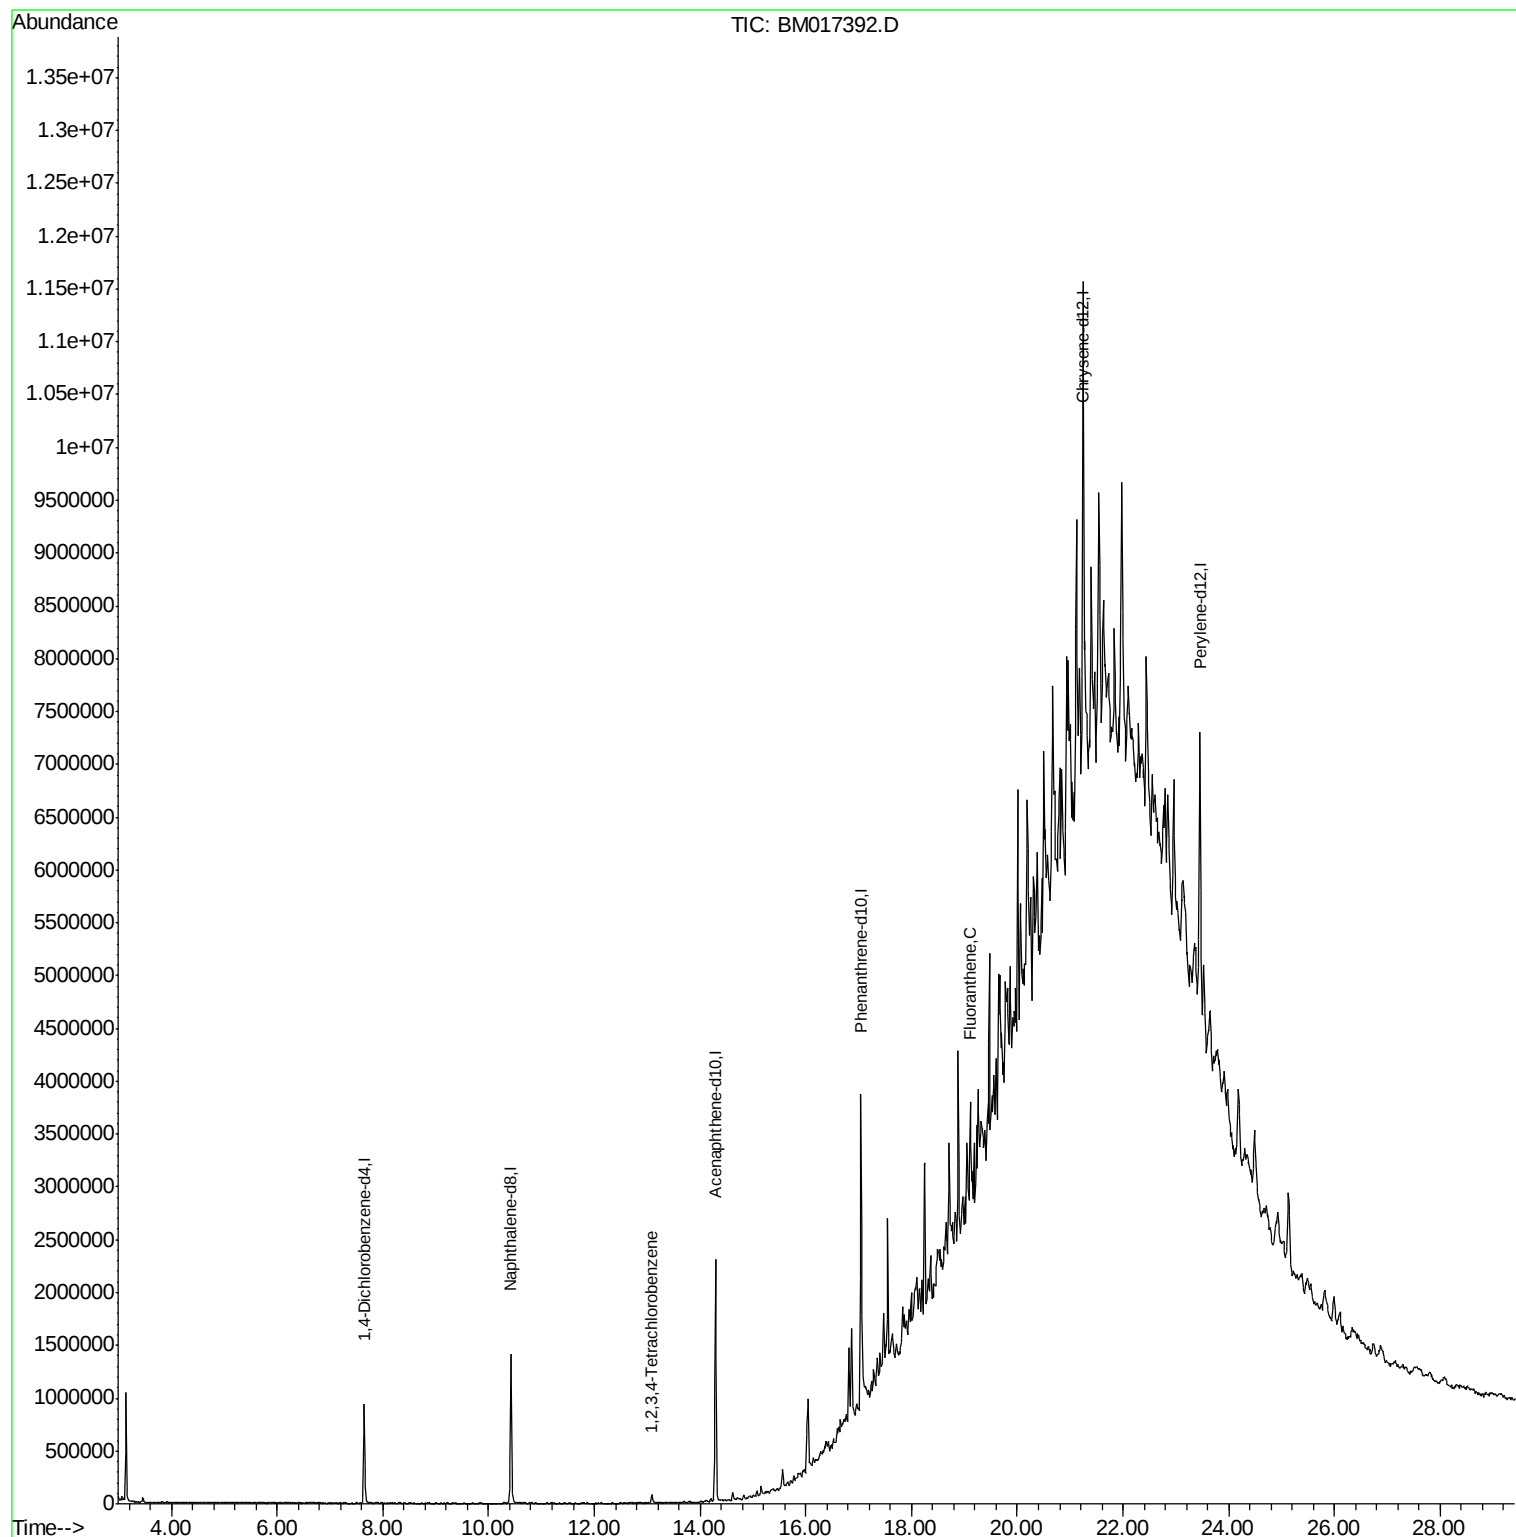


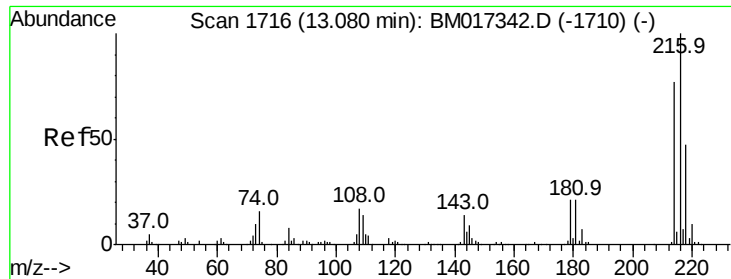

#73
 1,2,3,4-Tetrachlorobenzene
 Concen: 1.211 ng/uL
 RT: 13.09 min Scan# 1717
 Delta R.T. 0.01 min
 Lab File: BM017392.D
 Acq: 27 Oct 2018 17:47

Instrument :
 BNA_M
 ClientSampleId :
 COBM0

Tot Ion:	216	Resp:	30265
Ion	Ratio	Lower	Upper
216	100		
214	81.3	63.4	95.0
218	40.5	37.3	55.9

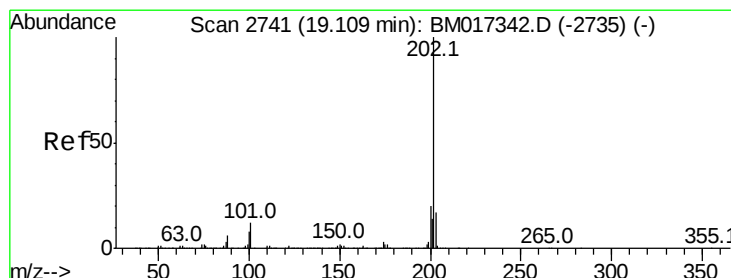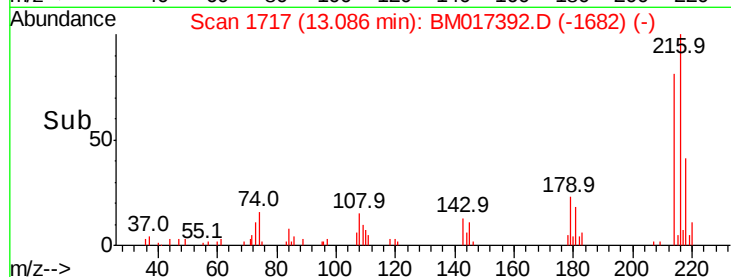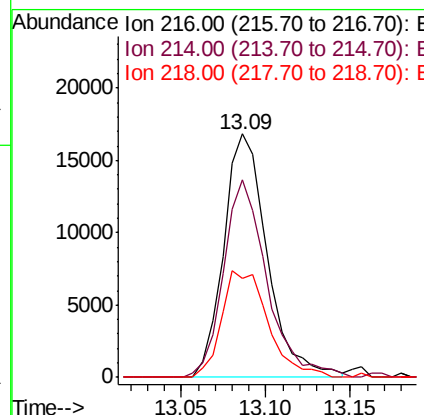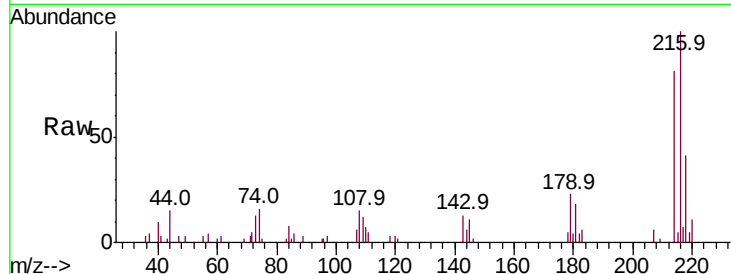

#77
 Fluoranthene
 Concen: 1.403 ng/uL
 RT: 19.11 min Scan# 2741
 Delta R.T. -0.00 min
 Lab File: BM017392.D
 Acq: 27 Oct 2018 17:47

Tgt Ion:	202	Resp:	163612
Ion	Ratio	Lower	Upper
202	100		
101	11.6	8.2	12.4
100	11.3	6.3	9.5#

