

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102718\
 Data File : BM017398.D
 Acq On : 27 Oct 2018 21:25
 Operator : MJ/SJ
 Sample : J5673-08
 Misc : GCMS Confirmation
 ALS Vial : 80 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0BL2

Quant Time: Oct 29 05:22:15 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 26 01:13:26 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	341177	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	1508716	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	891371	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.05	188	1897682	20.00	ng/ul	0.00
78) Chrysene-d12	21.24	240	1930789	20.00	ng/ul	0.00
86) Perylene-d12	23.46	264	1758635	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0d	0.00	ng/uL
5) Phenol-d5	0.00	99	0	0.00	ng/ul
7) Bis-(2-Chloroethyl)ether-d	0.00	67	0d	0.00	ng/ul
9) 2-Chlorophenol-d4	0.00	132	0	0.00	ng/ul
13) 4-Methylphenol-d8	0.00	113	0d	0.00	ng/ul
19) Nitrobenzene-d5	0.00	128	0	0.00	ng/ul
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul
44) Dimethylphthalate-d6	0.00	166	0d	0.00	ng/ul
47) Acenaphthylene-d8	0.00	160	0d	0.00	ng/ul
52) 4-Nitrophenol-d4	0.00	143	0d	0.00	ng/ul
58) Fluorene-d10	0.00	176	0d	0.00	ng/ul
63) 4,6-Dinitro-2-methylphenol	0.00	200	0d	0.00	ng/ul
71) Anthracene-d10	0.00	188	0d	0.00	ng/ul
79) Pyrene-d10	0.00	212	0d	0.00	ng/ul
90) Benzo(a)pyrene-d12	0.00	264	0d	0.00	ng/ul


Target Compounds					Ovalue
73) 1,2,3,4-Tetrachlorobenzene	13.09	216	30334	1.134	ng/uL 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102718\
Data File : BM017398.D
Acq On : 27 Oct 2018 21:25
Operator : MJ/SJ
Sample : J5673-08
Misc : GCMS Confirmation
ALS Vial : 80 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0BL2

Quant Time: Oct 29 05:22:15 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 26 01:13:26 2018
Response via : Initial Calibration

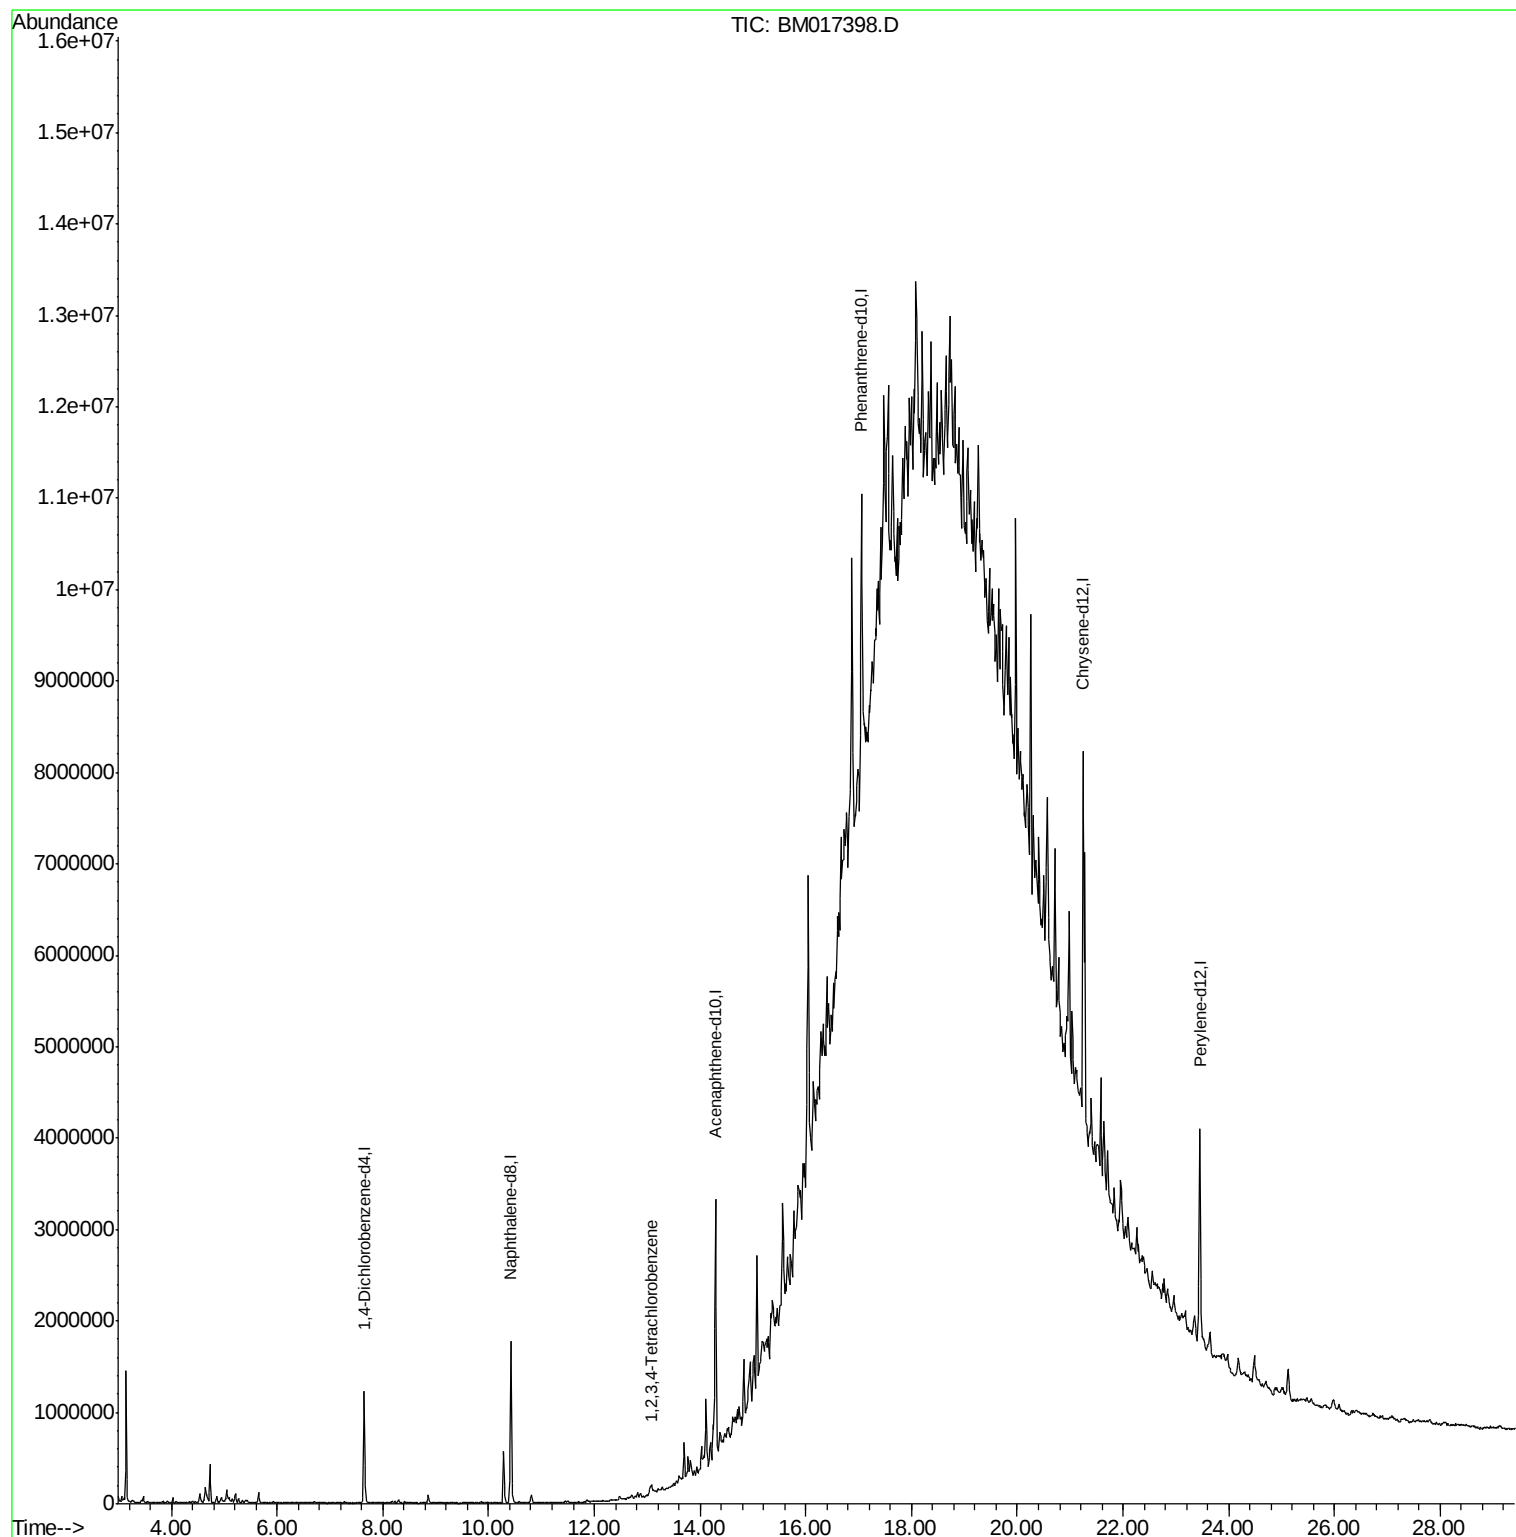

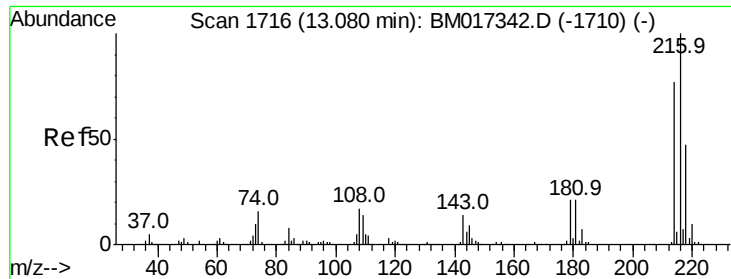

#73

1,2,3,4-Tetrachlorobenzene

Concen: 1.134 ng/uL

RT: 13.09 min Scan# 1717

Delta R.T. 0.01 min

Lab File: BM017398.D

Acq: 27 Oct 2018 21:25

Instrument :

BNA_M

ClientSampleId :

C0BL2


Tot Ion:216 Resp: 30334

Ion Ratio Lower Upper

216 100

214 71.8 63.4 95.0

218 48.6 37.3 55.9

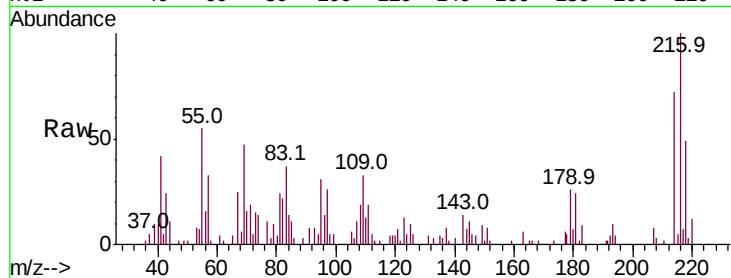

Abundance Ion 216.00 (215.70 to 216.70): E

Ion 214.00 (213.70 to 214.70): E

Ion 218.00 (217.70 to 218.70): E

