
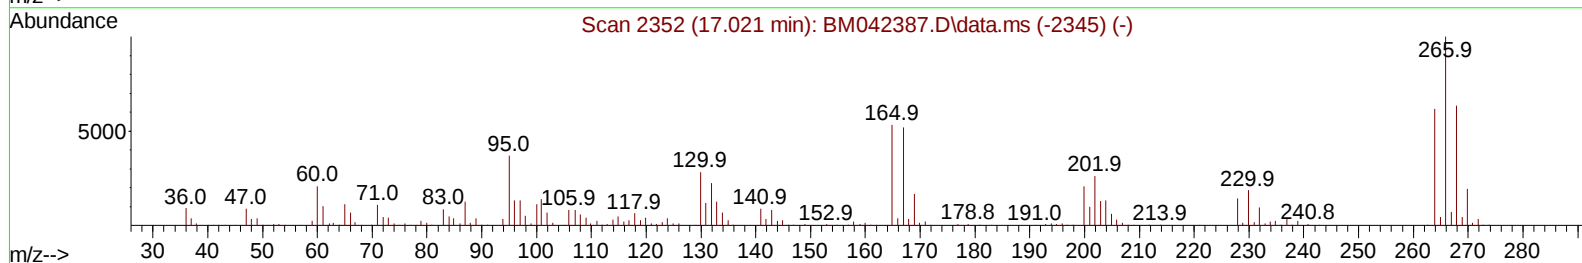
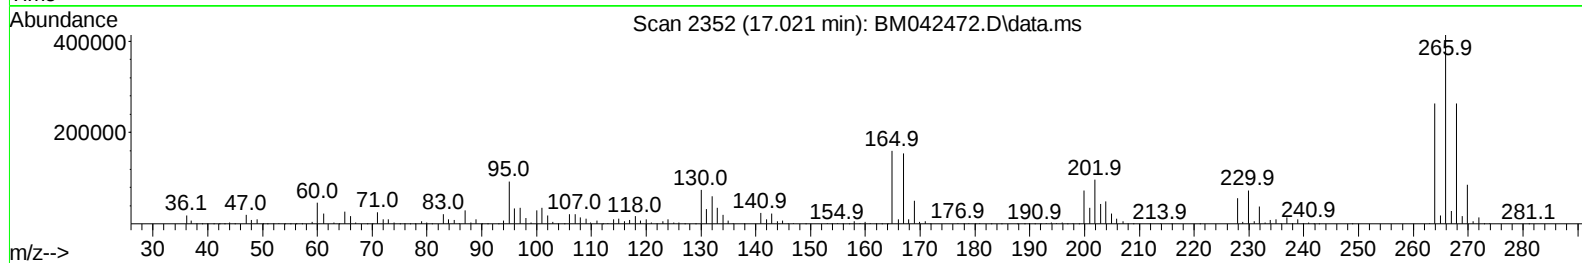


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102723\
Data File : BM042472.D
Acq On : 27 Oct 2023 10:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 01:42:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 28 00:26:13 2023
Response via : Initial Calibration

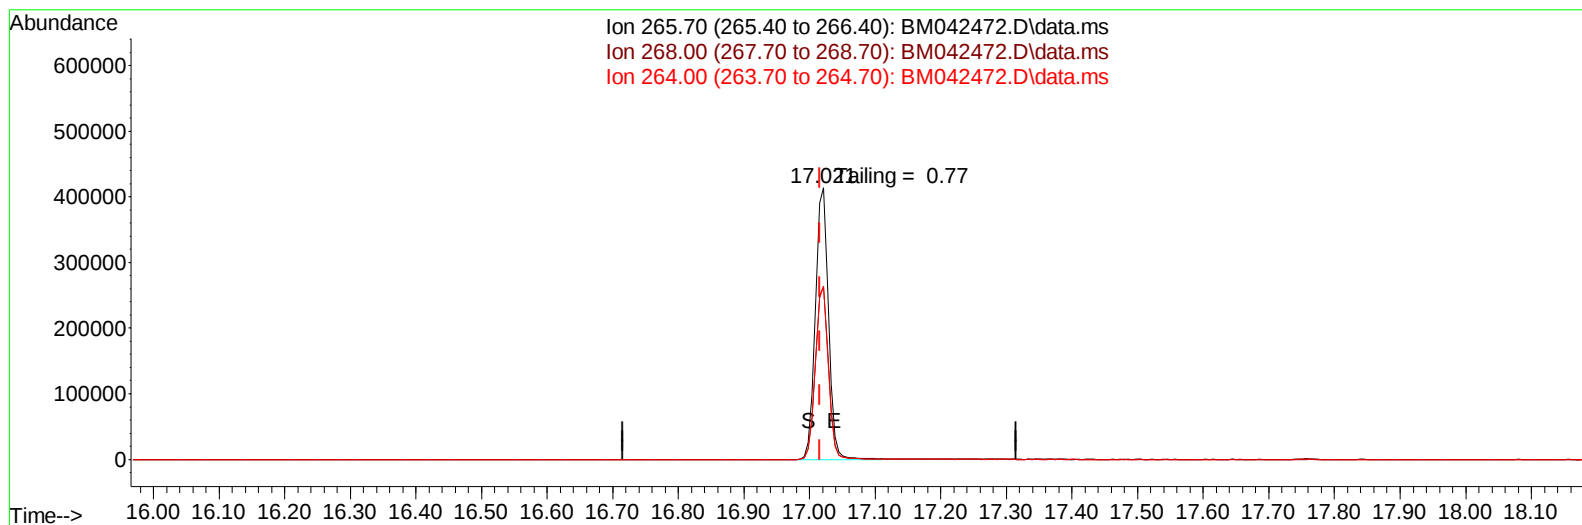

TIC: BM042472.D\data.ms

(70) Pentachlorophenol (C)




17.021min (+ 0.006) 388502.89 ng

response 579973

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	63.72
264.00	61.70	63.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102723\
Data File : BM042472.D
Acq On : 27 Oct 2023 10:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 01:42:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 28 00:26:13 2023
Response via : Initial Calibration

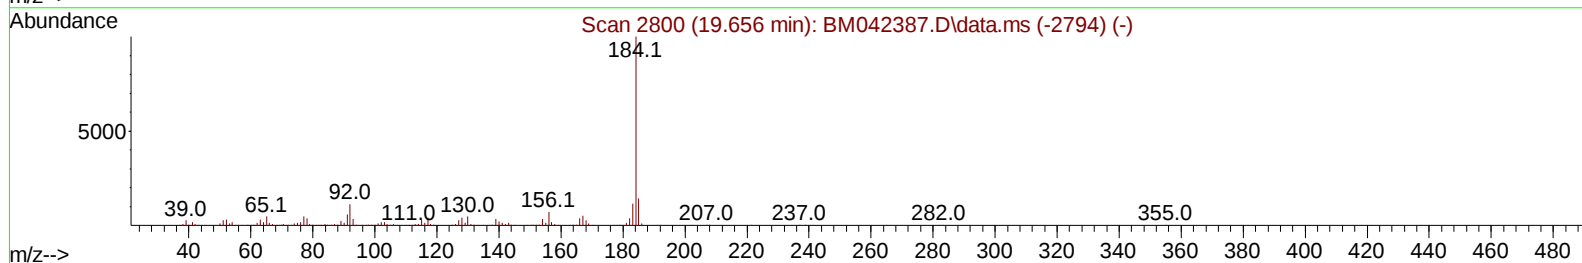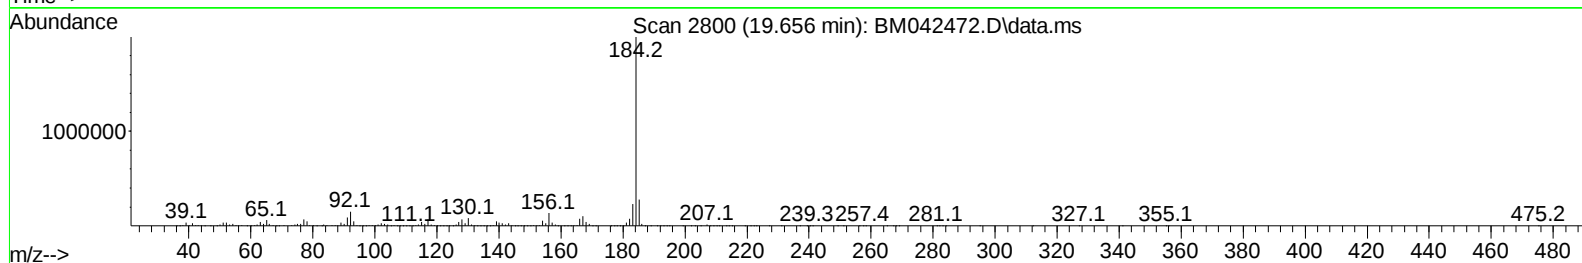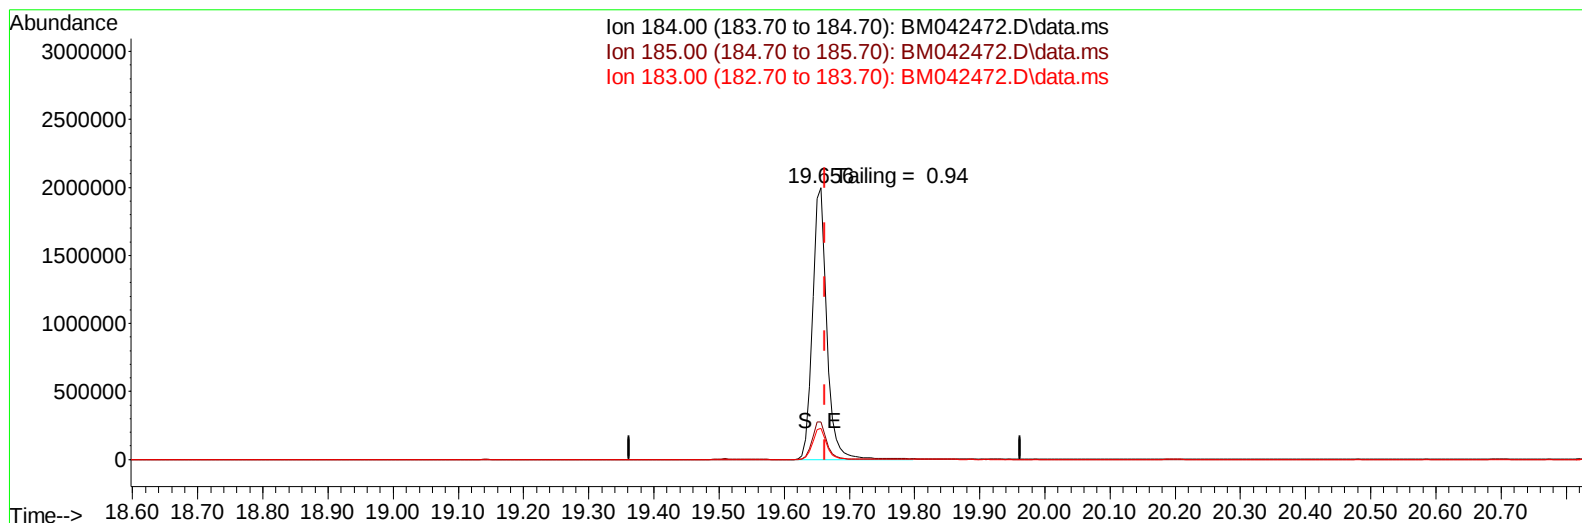

TIC: BM042472.D\data.ms

(77) Benzidine**19.656min (-0.006) 67180.47 ng****response 3044385**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.87
183.00	11.50	11.50
0.00	0.00	0.00