
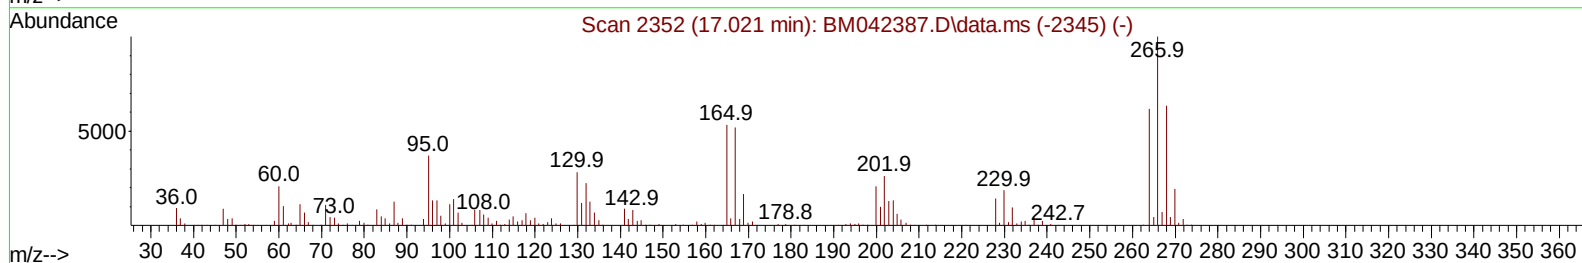
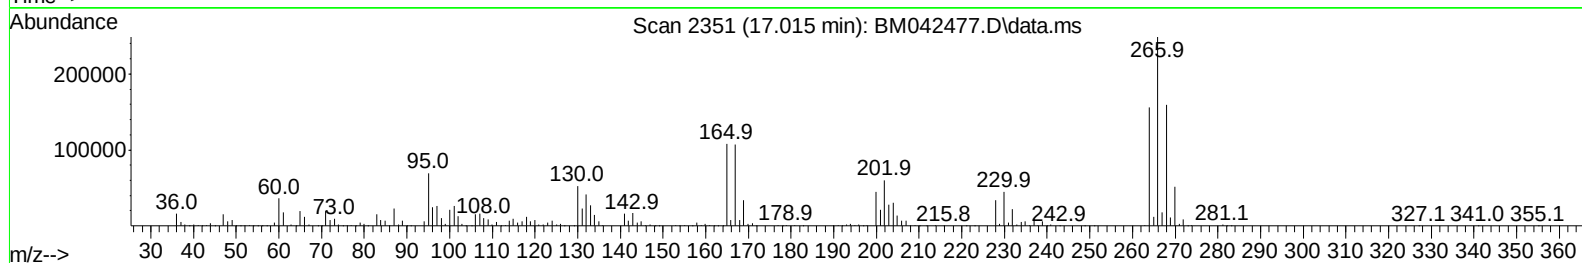


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM102723\  
Data File : BM042477.D  
Acq On : 27 Oct 2023 17:56  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 27 19:01:14 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM102123.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Oct 21 02:32:53 2023  
Response via : Initial Calibration

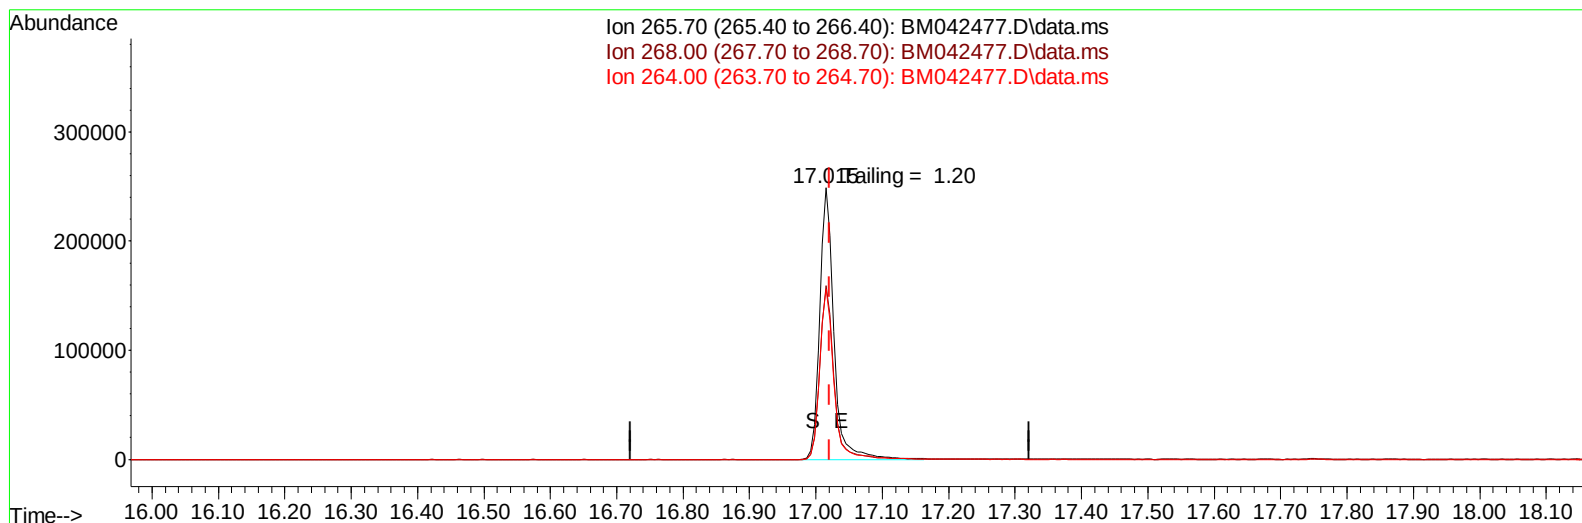

TIC: BM042477.D\data.ms

**(70) Pentachlorophenol (C)**




17.015min (-0.006) 0.00 ng

response 374667

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.30  | 64.00  |
| 264.00 | 61.70  | 62.76  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM102723\  
Data File : BM042477.D  
Acq On : 27 Oct 2023 17:56  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 27 19:01:14 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM102123.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Oct 21 02:32:53 2023  
Response via : Initial Calibration

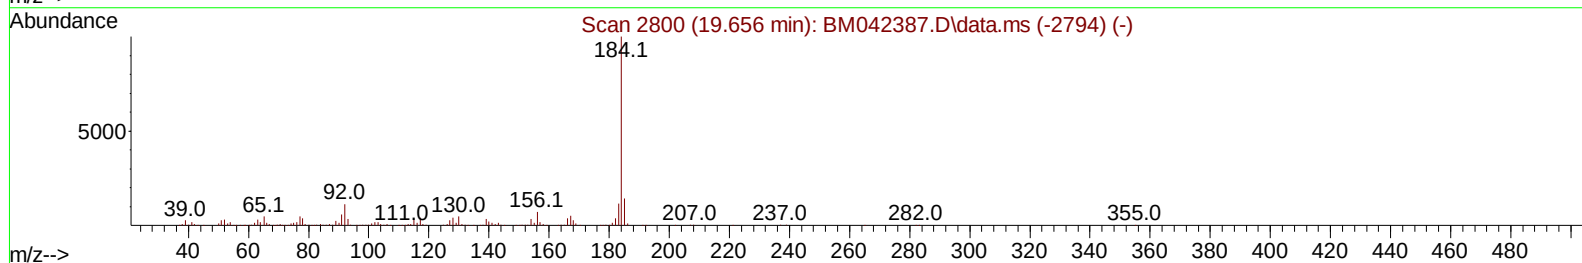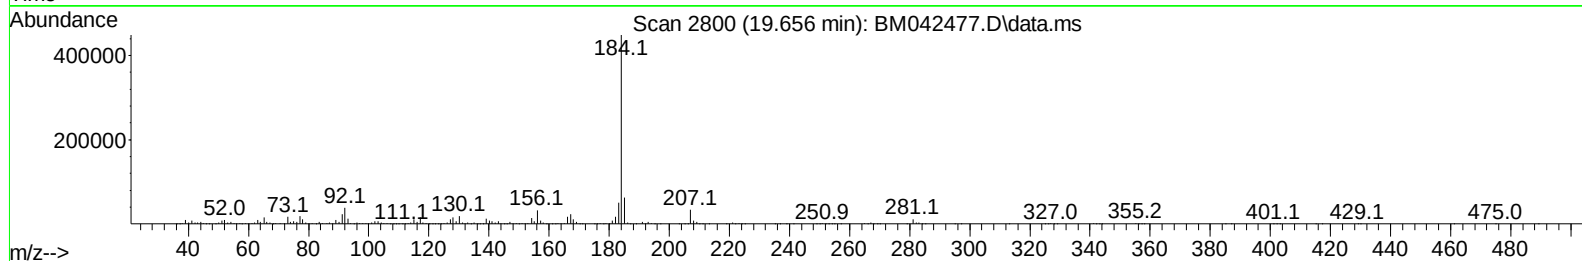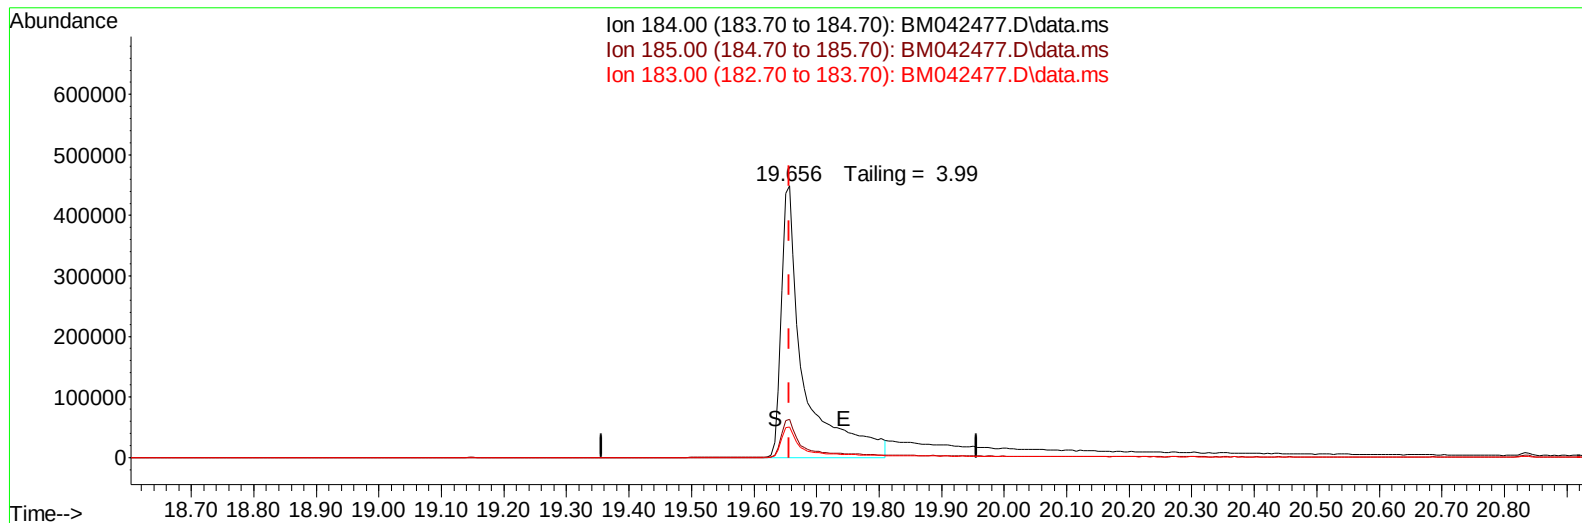

TIC: BM042477.D\data.ms

**(77) Benzidine****19.656min (-0.000) 78880.40 ng****response 1276719**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.40  | 13.94  |
| 183.00 | 11.50  | 11.34  |
| 0.00   | 0.00   | 0.00   |