
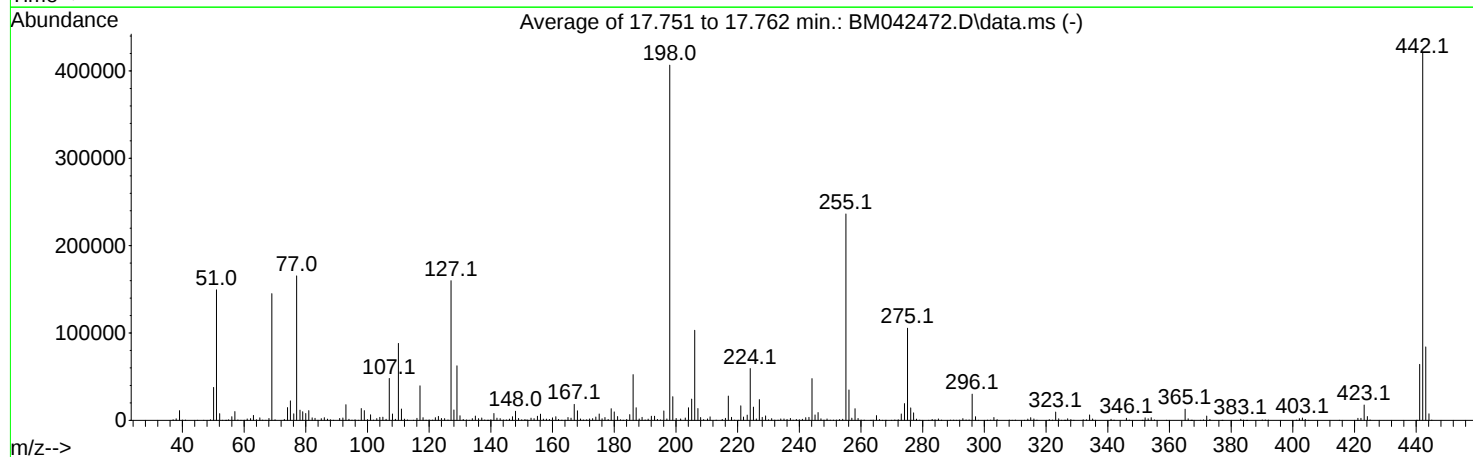


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102723\
Data File : BM042472.D
Acq On : 27 Oct 2023 10:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Oct 28 00:26:13 2023

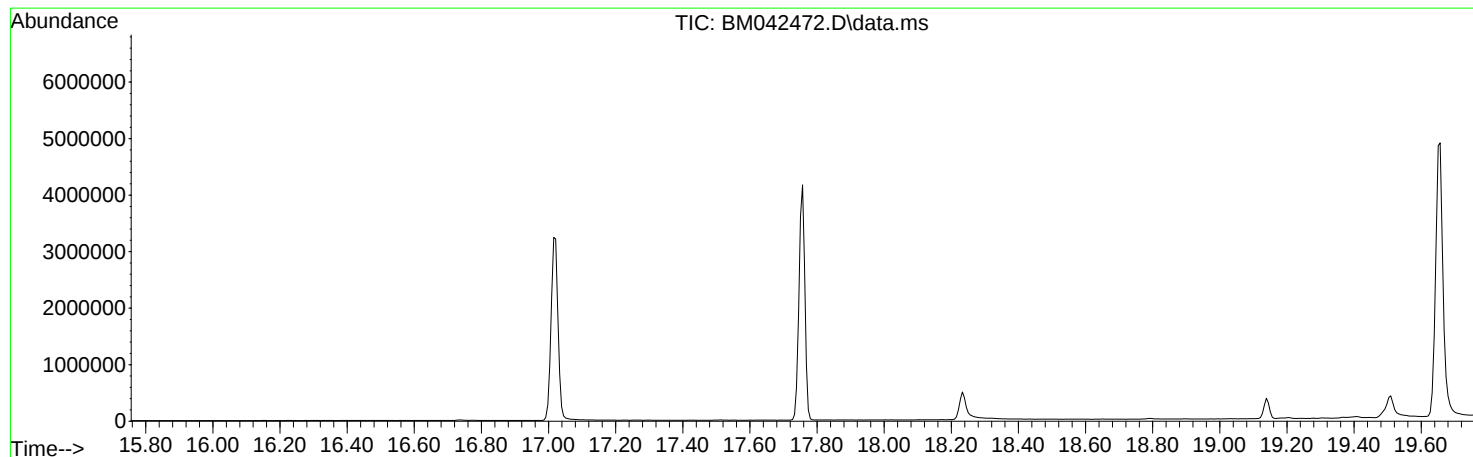




AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	149438	PASS
68	69	0.00	2	1.5	2228	PASS
69	198	0.00	100	35.7	145107	PASS
70	69	0.00	2	0.6	808	PASS
127	198	10	80	39.3	159965	PASS
197	198	0.00	2	0.4	1726	PASS
198	198	100	100	100.0	406656	PASS
199	198	5	9	6.7	27133	PASS
275	198	10	60	25.9	105491	PASS
365	198	1	100	3.2	12876	PASS
441	198	0.01	100	15.8	64192	PASS
442	442	50	100	100.0	421163	PASS
443	442	15	24	20.0	84115	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102723\
Data File : BM042472.D
Acq On : 27 Oct 2023 10:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Oct 28 01:42:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 28 00:26:13 2023
Response via : Initial Calibration

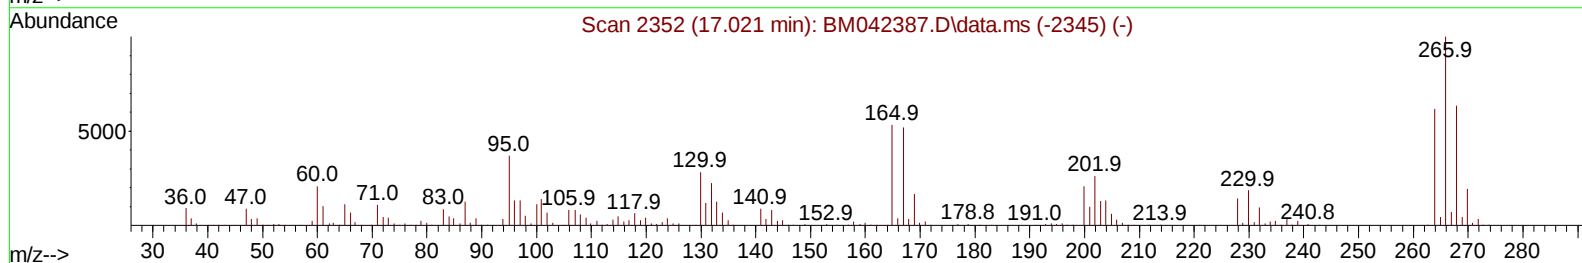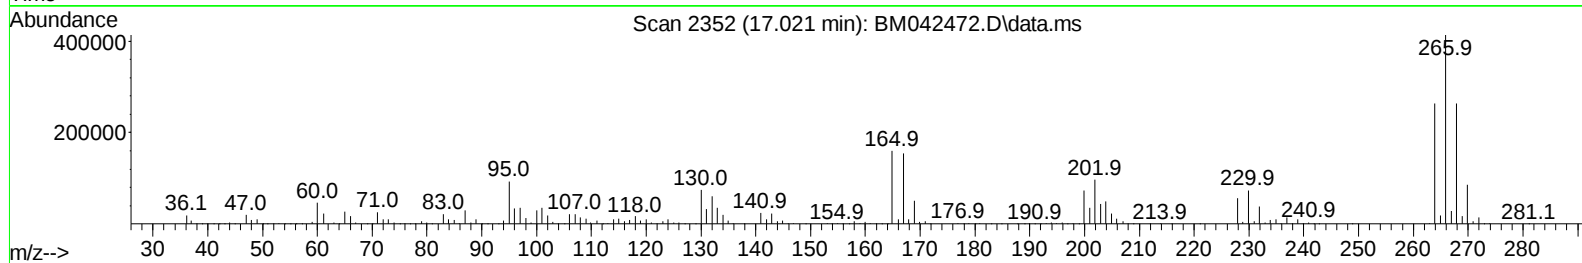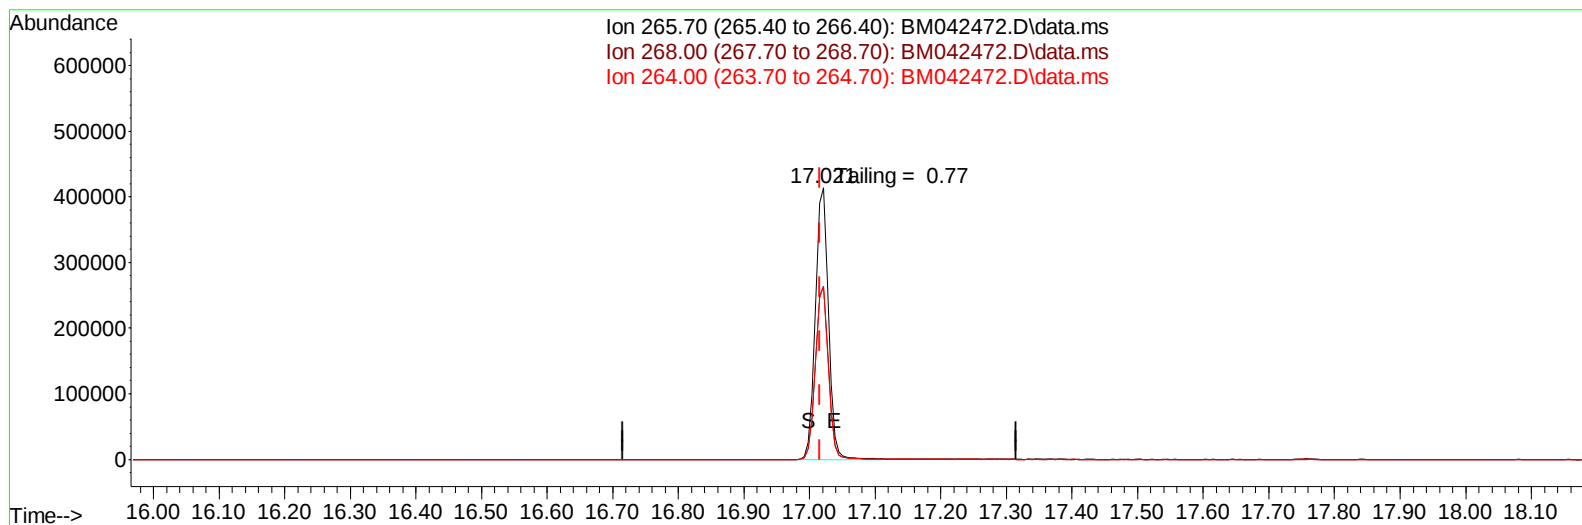

TIC: BM042472.D\data.ms

(70) Pentachlorophenol (C)

17.021min (+ 0.006) 388502.89 ng




response 579973

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	63.72
264.00	61.70	63.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102723\
Data File : BM042472.D
Acq On : 27 Oct 2023 10:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Oct 28 01:42:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 28 00:26:13 2023
Response via : Initial Calibration

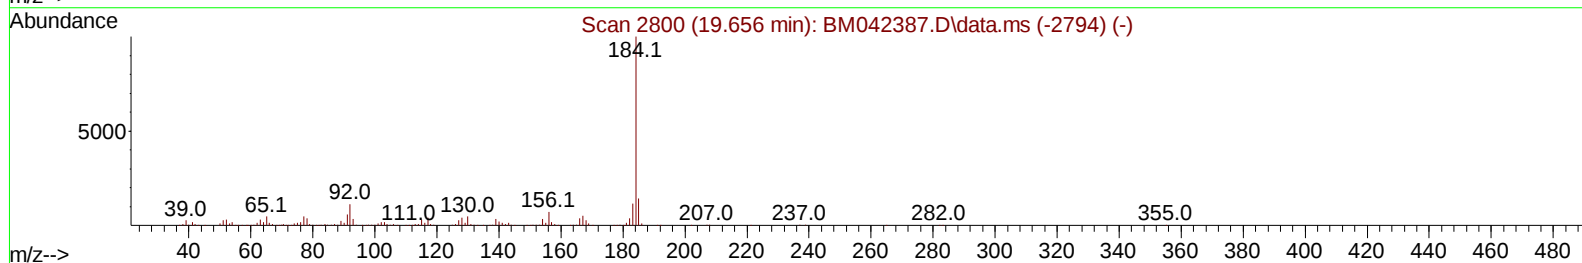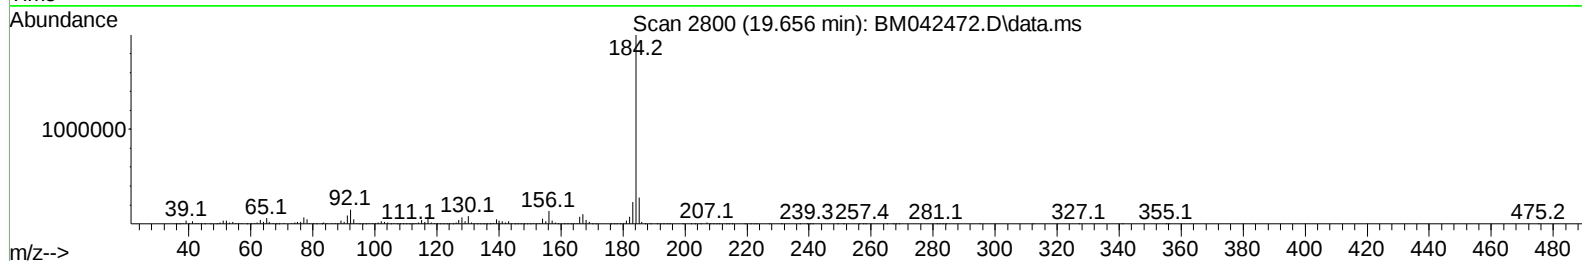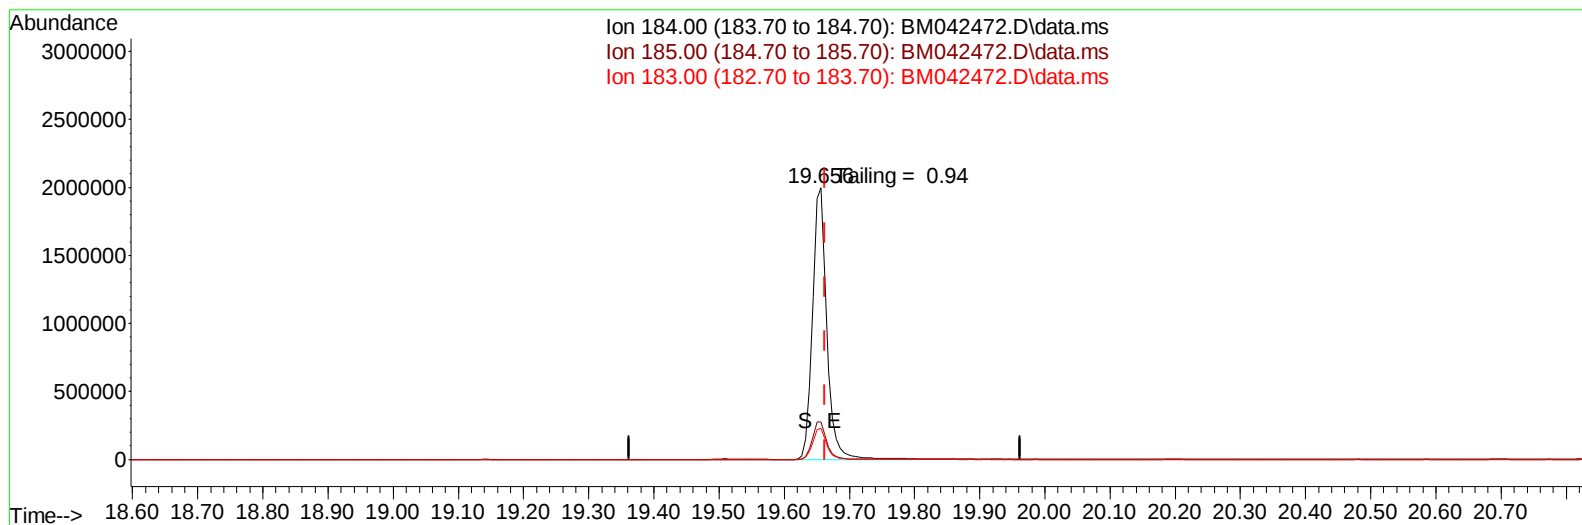

TIC: BM042472.D\data.ms

(77) Benzidine

19.656min (-0.006) 67180.47 ng

response 3044385

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.87
183.00	11.50	11.50
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/27/2023	BNA_M	<u>BM042472.D</u>
Compound Name	Response	Retention Time
DDT	1649913	20.845
DDD	46579	20.403
DDE	1437	19.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
48016	1697929	2.83

Instrument :
BNA_M
ClientSampleId :
DFTPP