


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102723\
Data File : BM042477.D
Acq On : 27 Oct 2023 17:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Oct 28 00:26:13 2023

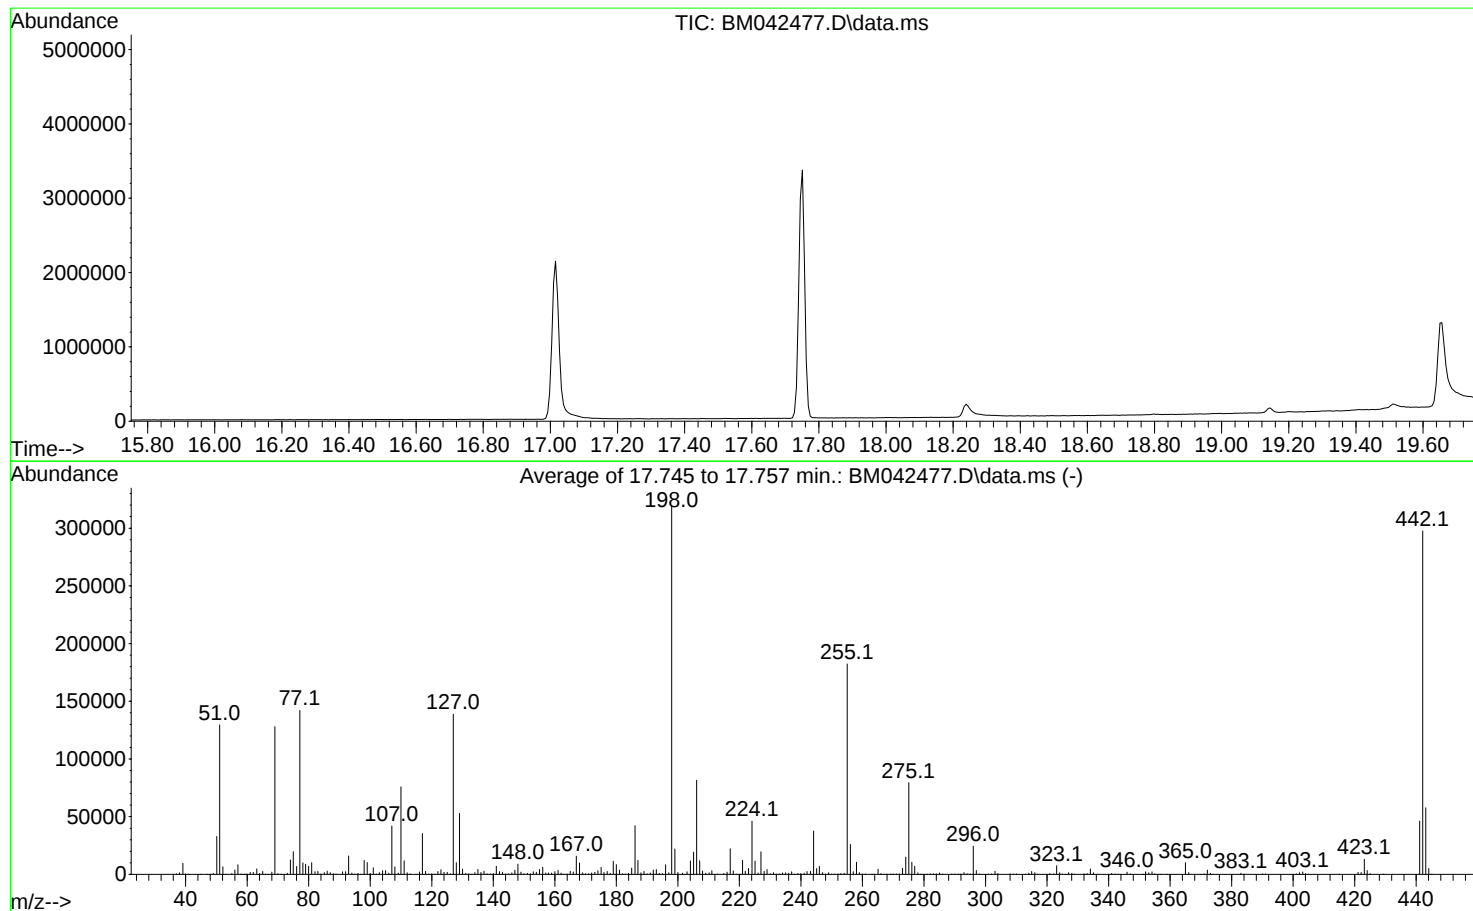




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.6	129496	PASS
68	69	0.00	2	1.5	1940	PASS
69	198	0.00	100	40.2	128008	PASS
70	69	0.00	2	0.6	741	PASS
127	198	10	80	43.6	138861	PASS
197	198	0.00	2	0.4	1370	PASS
198	198	100	100	100.0	318805	PASS
199	198	5	9	6.9	22113	PASS
275	198	10	60	24.9	79427	PASS
365	198	1	100	3.2	10146	PASS
441	198	0.01	100	14.5	46160	PASS
442	442	50	100	100.0	297557	PASS
443	442	15	24	19.4	57661	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102723\
Data File : BM042477.D
Acq On : 27 Oct 2023 17:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Oct 27 19:01:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 21 02:32:53 2023
Response via : Initial Calibration

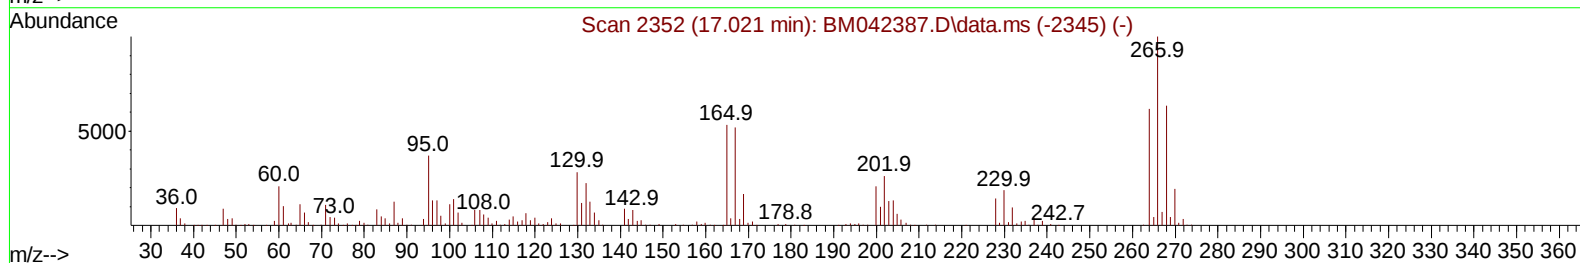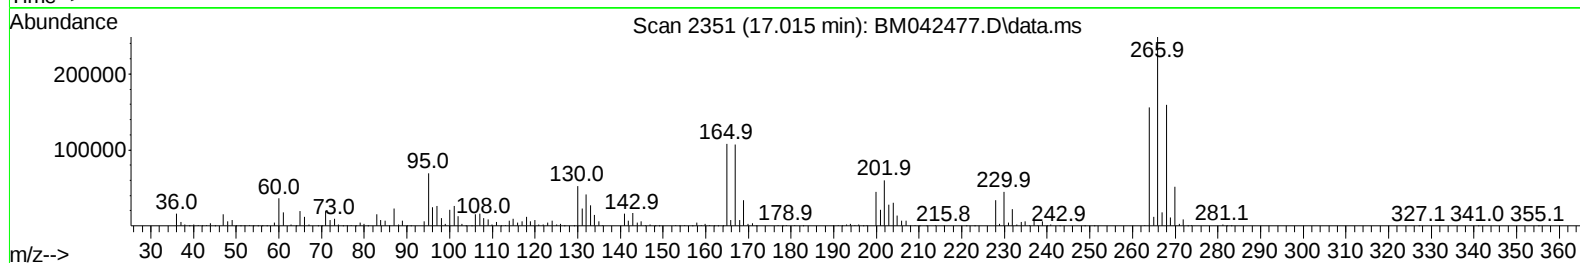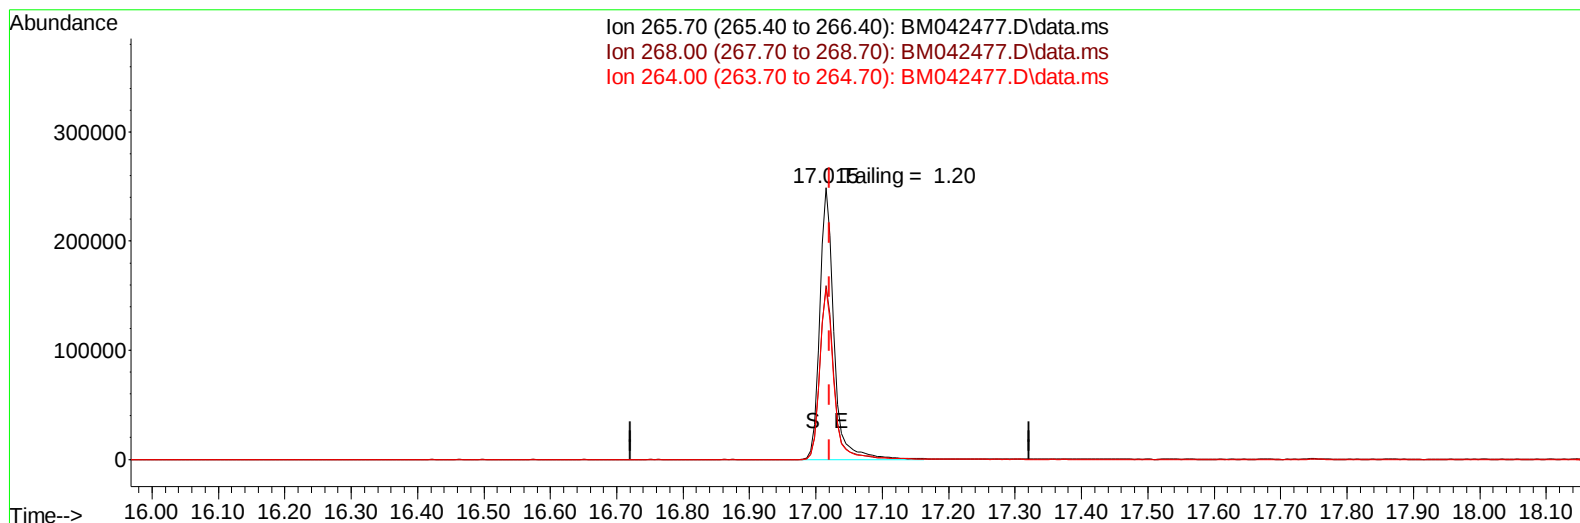

TIC: BM042477.D\data.ms

(70) Pentachlorophenol (C)

17.015min (-0.006) 0.00 ng




response 374667

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	64.00
264.00	61.70	62.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102723\
Data File : BM042477.D
Acq On : 27 Oct 2023 17:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Oct 27 19:01:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 21 02:32:53 2023
Response via : Initial Calibration

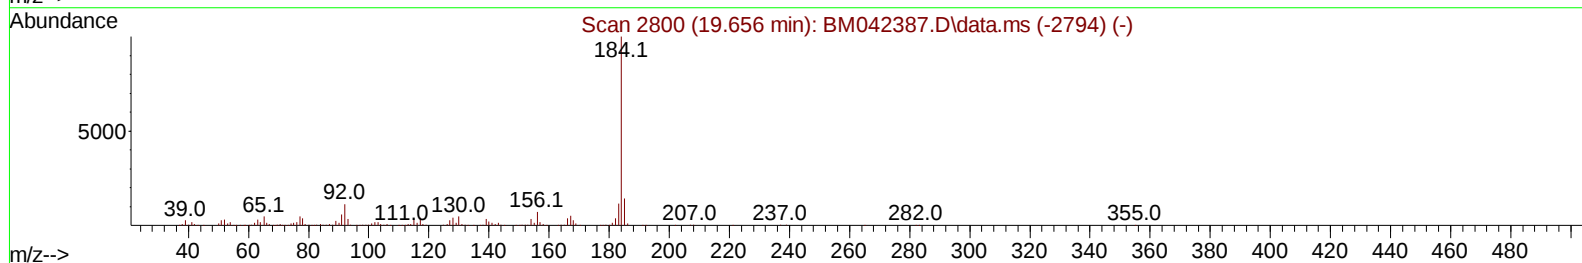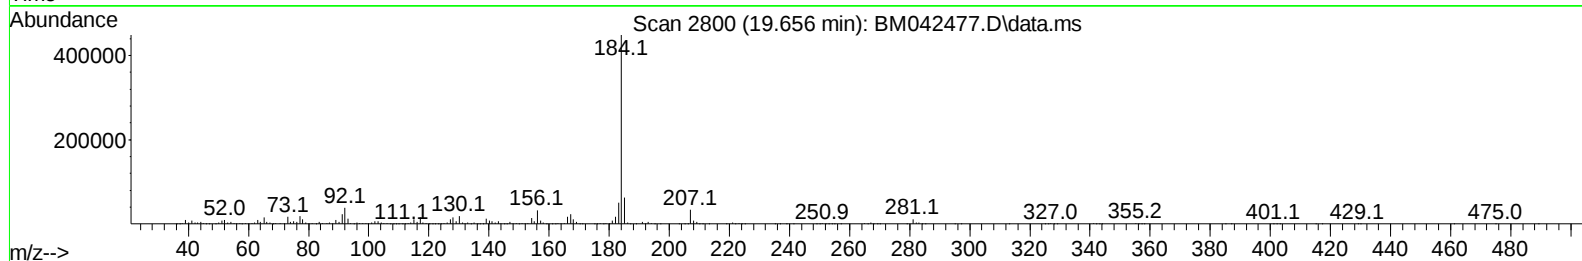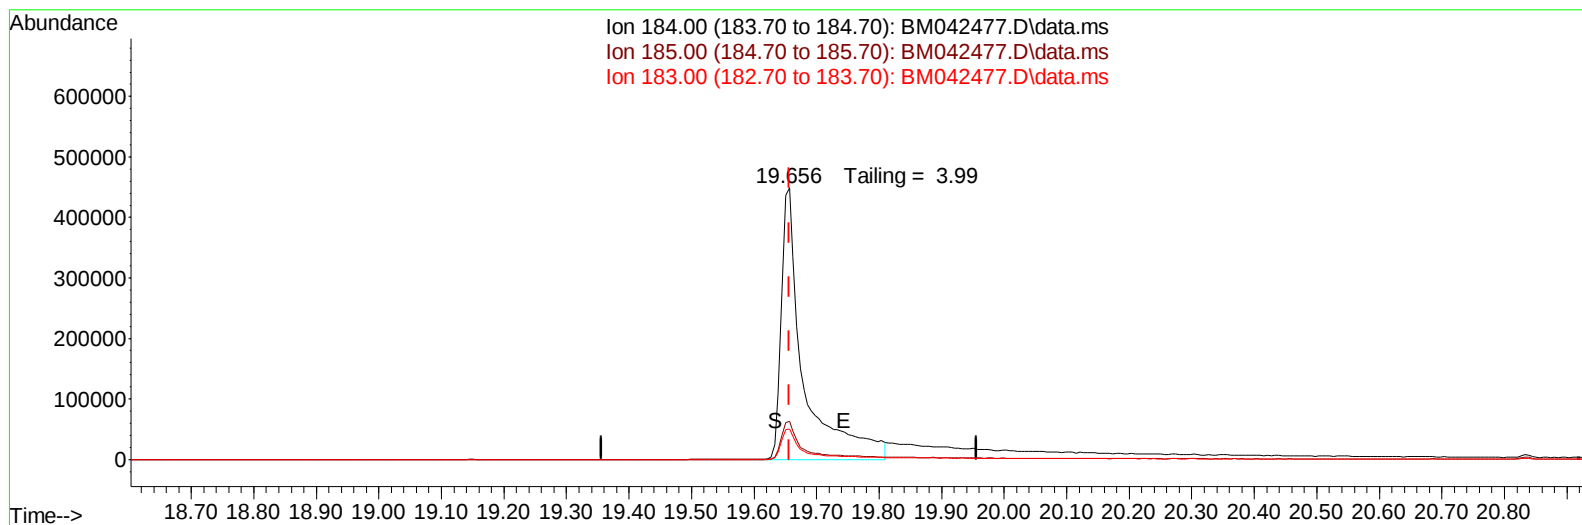

TIC: BM042477.D\data.ms

(77) Benzidine**19.656min (-0.000) 78880.40 ng****response 1276719**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.94
183.00	11.50	11.34
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/27/2023	BNA_M	<u>BM042477.D</u>
Compound Name	Response	Retention Time
DDT	982364	20.833
DDD	29948	20.403
DDE	929	19.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
30877	1013241	3.05

Instrument :
BNA_M
ClientSampleId :
DFTPP