

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM103023\  
 Data File : BM042503.D  
 Acq On : 30 Oct 2023 20:43  
 Operator : MA/JU  
 Sample : 05011-01DL 10X  
 Misc :  
 ALS Vial : 17 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 RBR-200027DL

Quant Time: Oct 31 03:46:40 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM103023.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Oct 31 02:55:18 2023  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.928	152	94486	20.000	ng	0.00
21) Naphthalene-d8	10.745	136	348584	20.000	ng	0.00
39) Acenaphthene-d10	14.574	164	196005	20.000	ng	0.00
64) Phenanthrene-d10	17.333	188	337501	20.000	ng	# 0.00
76) Chrysene-d12	21.509	240	277856	20.000	ng	0.00
86) Perylene-d12	23.927	264	347497	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.469	112	44435	7.590	ng	0.00
7) Phenol-d6	7.098	99	53728	6.691	ng	0.00
23) Nitrobenzene-d5	9.128	82	35648	4.767	ng	0.00
42) 2,4,6-Tribromophenol	16.074	330	16241	6.347	ng	0.00
45) 2-Fluorobiphenyl	13.198	172	74988	5.148	ng	0.00
79) Terphenyl-d14	19.945	244	78333	4.780	ng	0.00
Target Compounds						
26) 2-Nitrophenol	10.010	139	60	3.535	ng	# 1
32) Benzoic acid	10.016	122	419	4.204	ng	# 46
48) 2-Nitroaniline	13.727	65	3071	4.980	ng	# 62
53) 3-Nitroaniline	14.498	138	5846	5.922	ng	# 29
54) 2,4-Dinitrophenol	14.898	184	63	7.774	ng	# 1
55) Dibenzofuran	14.974	168	51659	2.876	ng	# 82
56) 4-Nitrophenol	14.857	139	3634	8.163	ng	# 1
57) 2,4-Dinitrotoluene	14.951	165	13170	6.612	ng	# 40
58) Fluorene	15.627	166	53599	3.688	ng	# 80
62) 4-Nitroaniline	15.715	138	1681	6.229	ng	# 36
65) 4,6-Dinitro-2-methylph...	15.733	198	2647	6.906	ng	# 1
66) n-Nitrosodiphenylamine	15.880	169	20521	2.156	ng	# 59
71) Phenanthrene	17.374	178	504211	28.587	ng	# 96
72) Anthracene	17.468	178	72149	4.130	ng	# 73
73) Carbazole	17.757	167	43218	3.041	ng	# 29
75) Fluoranthene	19.386	202	224039	10.814	ng	93
78) Pyrene	19.756	202	150613	7.894	ng	# 91
81) Benzo(a)anthracene	21.492	228	40924	2.315	ng	# 90
83) Chrysene	21.545	228	50176	2.794	ng	# 92
84) Bis(2-ethylhexyl)phtha...	21.374	149	42084	3.417	ng	# 92
88) Benzo(b)fluoranthene	23.186	252	44824	2.315	ng	# 80
89) Benzo(k)fluoranthene	23.186	252	44824	2.078	ng	# 80
91) Dibenzo(a,h)anthracene	26.438	278	685	4.171	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM103023\  
 Data File : BM042503.D  
 Acq On : 30 Oct 2023 20:43  
 Operator : MA/JU  
 Sample : 05011-01DL 10X  
 Misc :  
 ALS Vial : 17 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 RBR-200027DL


Quant Time: Oct 31 03:46:40 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM103023.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Oct 31 02:55:18 2023  
 Response via : Initial Calibration








#1  
 1,4-Dichlorobenzene-d4  
 Concen: 20.000 ng  
 RT: 7.928 min Scan# 80  
 Delta R.T. -0.000 min  
 Lab File: BM042503.D  
 Acq: 30 Oct 2023 20:43


Instrument : BNA\_M  
 ClientSampleId : RBR-200027DL





Tgt Ion:152 Resp: 94486  
 Ion Ratio Lower Upper  
 152 100  
 150 157.9 127.4 191.0  
 115 62.1 47.9 71.9




#5  
 2-Fluorophenol  
 Concen: 7.590 ng  
 RT: 5.469 min Scan# 388  
 Delta R.T. 0.006 min  
 Lab File: BM042503.D  
 Acq: 30 Oct 2023 20:43




Tgt Ion:112 Resp: 44435  
 Ion Ratio Lower Upper  
 112 100  
 64 60.5 52.1 78.1  
 63 36.4 28.3 42.5








#7  
 Phenol-d6  
 Concen: 6.691 ng  
 RT: 7.098 min Scan# 6  
 Delta R.T. -0.000 min  
 Lab File: BM042503.D  
 Acq: 30 Oct 2023 20:43


Instrument :  
 BNA\_M  
 ClientSampleId :  
 RBR-200027DL





Tgt Ion: 99 Resp: 53728  
 Ion Ratio Lower Upper  
 99 100  
 42 24.2 18.7 28.1  
 71 38.7 29.1 43.7




#21  
 Naphthalene-d8  
 Concen: 20.000 ng  
 RT: 10.745 min Scan# 1285  
 Delta R.T. -0.006 min  
 Lab File: BM042503.D  
 Acq: 30 Oct 2023 20:43




Tgt Ion: 136 Resp: 348584  
 Ion Ratio Lower Upper  
 136 100  
 137 10.6 9.0 13.6  
 54 9.9 8.0 12.0  
 68 6.6 5.7 8.5








#23  
 Nitrobenzene-d5  
 Concen: 4.767 ng  
 RT: 9.128 min Scan# 1160  
 Delta R.T. -0.006 min  
 Lab File: BM042503.D  
 Acq: 30 Oct 2023 20:43

Instrument :  
 BNA\_M  
 ClientSampleId :  
 RBR-200027DL



Tgt Ion: 82 Resp: 35648




Ion	Ratio	Lower	Upper
82	100		
128	38.6	30.7	46.1
54	59.1	45.3	67.9




#26  
 2-Nitrophenol  
 Concen: 3.535 ng  
 RT: 10.010 min Scan# 1160  
 Delta R.T. 0.135 min  
 Lab File: BM042503.D  
 Acq: 30 Oct 2023 20:43

Tgt Ion: 139 Resp: 60


Ion	Ratio	Lower	Upper
139	100		
109	362.7	25.2	37.8#
65	116.0	51.4	77.0#








#32  
 Benzoic acid  
 Concen: 4.204 ng  
 RT: 10.016 min Scan# 1171  
 Delta R.T. -0.059 min  
 Lab File: BM042503.D  
 Acq: 30 Oct 2023 20:43

Instrument :  
 BNA\_M  
 ClientSampleId :  
 RBR-200027DL







Tgt Ion:122 Resp: 419  
 Ion Ratio Lower Upper  
 122 100  
 105 101.5 105.2 145.2#  
 77 201.5 84.8 124.8#



#39  
 Acenaphthene-d10  
 Concen: 20.000 ng  
 RT: 14.574 min Scan# 1936  
 Delta R.T. -0.006 min  
 Lab File: BM042503.D  
 Acq: 30 Oct 2023 20:43


Tgt Ion:164 Resp: 196005  
 Ion Ratio Lower Upper  
 164 100  
 162 98.4 81.6 122.4  
 160 45.6 36.2 54.4








#42  
 2,4,6-Tribromophenol  
 Concen: 6.347 ng  
 RT: 16.074 min Scan# 21  
 Delta R.T. 0.000 min  
 Lab File: BM042503.D  
 Acq: 30 Oct 2023 20:43


Instrument :  
 BNA\_M  
 ClientSampleId :  
 RBR-200027DL





Tgt Ion:330 Resp: 16241  
 Ion Ratio Lower Upper  
 330 100  
 332 97.6 78.8 118.2  
 141 58.5 31.1 46.7#




#45  
 2-Fluorobiphenyl  
 Concen: 5.148 ng  
 RT: 13.198 min Scan# 1702  
 Delta R.T. -0.000 min  
 Lab File: BM042503.D  
 Acq: 30 Oct 2023 20:43



Tgt Ion:172 Resp: 74988  
 Ion Ratio Lower Upper  
 172 100  
 171 35.0 28.2 42.2  
 170 23.5 19.0 28.4









#48  
 2-Nitroaniline  
 Concen: 4.980 ng  
 RT: 13.727 min Scan# 11  
 Delta R.T. 0.023 min  
 Lab File: BM042503.D  
 Acq: 30 Oct 2023 20:43




Instrument : BNA\_M  
 ClientSampleId : RBR-200027DL

Tgt Ion	Resp	Ion Ratio	Lower	Upper
65	3071	100		
92	39.4	49.4	74.2#	
138	44.0	66.9	100.3#	




#53  
 3-Nitroaniline  
 Concen: 5.922 ng  
 RT: 14.498 min Scan# 1923  
 Delta R.T. -0.035 min  
 Lab File: BM042503.D  
 Acq: 30 Oct 2023 20:43

Tgt Ion	Resp	Ion Ratio	Lower	Upper
138	5846	100		
108	84.8	7.9	11.9#	
92	56.4	100.7	151.1#	











#54  
 2,4-Dinitrophenol  
 Concen: 7.774 ng  
 RT: 14.898 min Scan# 11  
 Delta R.T. 0.165 min  
 Lab File: BM042503.D  
 Acq: 30 Oct 2023 20:43

Instrument :  
 BNA\_M  
 ClientSampleId :  
 RBR-200027DL



Tgt Ion:184 Resp: 63




Ion	Ratio	Lower	Upper
184	100		
63	856.7	69.2	103.8#
154	733.1	53.2	79.8#




#55  
 Dibenzofuran  
 Concen: 2.876 ng  
 RT: 14.974 min Scan# 2004  
 Delta R.T. -0.006 min  
 Lab File: BM042503.D  
 Acq: 30 Oct 2023 20:43

Tgt Ion:168 Resp: 51659

Ion	Ratio	Lower	Upper
168	100		
139	47.6	30.4	45.6#
169	22.2	10.6	15.8#









#56  
 4-Nitrophenol  
 Concen: 8.163 ng  
 RT: 14.857 min Scan# 14  
 Delta R.T. 0.024 min  
 Lab File: BM042503.D  
 Acq: 30 Oct 2023 20:43




Instrument :  
 BNA\_M  
 ClientSampleId :  
 RBR-200027DL


Tgt Ion:139 Resp: 3634  
 Ion Ratio Lower Upper  
 139 100  
 109 649.6 61.3 101.3#  
 65 156.5 100.2 140.2#



#57  
 2,4-Dinitrotoluene  
 Concen: 6.612 ng  
 RT: 14.951 min Scan# 2000  
 Delta R.T. -0.023 min  
 Lab File: BM042503.D  
 Acq: 30 Oct 2023 20:43


Tgt Ion:165 Resp: 13170  
 Ion Ratio Lower Upper  
 165 100  
 63 45.9 66.7 100.1#  
 89 23.3 80.2 120.4#  
 182 10.8 2.0 3.0#








#58  
 Fluorene  
 Concen: 3.688 ng  
 RT: 15.627 min Scan# 2115  
 Delta R.T. -0.000 min  
 Lab File: BM042503.D  
 Acq: 30 Oct 2023 20:43

Instrument : BNA\_M  
 ClientSampleId : RBR-200027DL







Tgt Ion:166 Resp: 53599  
 Ion Ratio Lower Upper  
 166 100  
 165 119.0 79.3 118.9#  
 167 21.5 10.5 15.7#



#62  
 4-Nitroaniline  
 Concen: 6.229 ng  
 RT: 15.715 min Scan# 2130  
 Delta R.T. 0.017 min  
 Lab File: BM042503.D  
 Acq: 30 Oct 2023 20:43

Tgt Ion:138 Resp: 1681  
 Ion Ratio Lower Upper  
 138 100  
 92 92.6 37.0 77.0#  
 108 156.4 67.2 107.2#









#64  
 Phenanthrene-d10  
 Concen: 20.000 ng  
 RT: 17.333 min Scan# 2405  
 Delta R.T. 0.006 min  
 Lab File: BM042503.D  
 Acq: 30 Oct 2023 20:43

Instrument :  
 BNA\_M  
 ClientSampleId :  
 RBR-200027DL

Tgt Ion:188 Resp: 337501




Ion	Ratio	Lower	Upper
188	100		
94	13.1	8.2	12.4#
80	14.3	9.4	14.2#




#65  
 4,6-Dinitro-2-methylphenol  
 Concen: 6.906 ng  
 RT: 15.733 min Scan# 2133  
 Delta R.T. 0.012 min  
 Lab File: BM042503.D  
 Acq: 30 Oct 2023 20:43

Tgt Ion:198 Resp: 2647

Ion	Ratio	Lower	Upper
198	100		
51	251.2	42.4	82.4#
105	1140.4	29.2	69.2#









#66  
 n-Nitrosodiphenylamine  
 Concen: 2.156 ng  
 RT: 15.880 min Scan# 2158  
 Delta R.T. 0.035 min  
 Lab File: BM042503.D  
 Acq: 30 Oct 2023 20:43

Instrument : BNA\_M  
 ClientSampleId : RBR-200027DL

Tgt Ion:169 Resp: 20521




Ion	Ratio	Lower	Upper
169	100		
168	20.1	55.9	83.9#
167	35.6	29.8	44.8




#71  
 Phenanthrene  
 Concen: 28.587 ng  
 RT: 17.374 min Scan# 2412  
 Delta R.T. -0.000 min  
 Lab File: BM042503.D  
 Acq: 30 Oct 2023 20:43

Tgt Ion:178 Resp: 504211

Ion	Ratio	Lower	Upper
178	100		
176	20.2	15.8	23.8
179	18.9	12.2	18.4#









#72  
 Anthracene  
 Concen: 4.130 ng  
 RT: 17.468 min Scan# 2427  
 Delta R.T. 0.006 min  
 Lab File: BM042503.D  
 Acq: 30 Oct 2023 20:43




Instrument : BNA\_M  
 ClientSampleId : RBR-200027DL


Tgt Ion	Resp	Lower	Upper
178	72149		
176	22.6	15.2	22.8
179	36.9	12.3	18.5#



#73  
 Carbazole  
 Concen: 3.041 ng  
 RT: 17.757 min Scan# 2477  
 Delta R.T. 0.006 min  
 Lab File: BM042503.D  
 Acq: 30 Oct 2023 20:43

Tgt Ion	Resp	Lower	Upper
167	43218		
166	48.6	17.4	26.2#
139	51.0	10.5	15.7#









#75  
 Fluoranthene  
 Concen: 10.814 ng  
 RT: 19.386 min Scan# 21  
 Delta R.T. -0.000 min  
 Lab File: BM042503.D  
 Acq: 30 Oct 2023 20:43




Instrument :  
 BNA\_M  
 ClientSampleId :  
 RBR-200027DL


Tgt Ion	Resp	Lower	Upper
202	100		
101	10.6	0.0	30.5
203	21.9	0.0	37.0



#76  
 Chrysene-d12  
 Concen: 20.000 ng  
 RT: 21.509 min Scan# 3115  
 Delta R.T. -0.000 min  
 Lab File: BM042503.D  
 Acq: 30 Oct 2023 20:43

Tgt Ion	Resp	Lower	Upper
240	100		
120	10.2	8.3	12.5
236	26.6	20.8	31.2









#78  
 Pyrene  
 Concen: 7.894 ng  
 RT: 19.756 min Scan# 2816  
 Delta R.T. 0.006 min  
 Lab File: BM042503.D  
 Acq: 30 Oct 2023 20:43

Instrument :  
 BNA\_M  
 ClientSampleId :  
 RBR-200027DL

Tgt Ion:202 Resp: 150613




Ion	Ratio	Lower	Upper
202	100		
200	22.1	16.9	25.3
203	24.8	13.7	20.5




#79  
 Terphenyl-d14  
 Concen: 4.780 ng  
 RT: 19.945 min Scan# 2849  
 Delta R.T. -0.000 min  
 Lab File: BM042503.D  
 Acq: 30 Oct 2023 20:43

Tgt Ion:244 Resp: 78333

Ion	Ratio	Lower	Upper
244	100		
212	9.7	5.4	8.2
122	17.5	7.2	10.8











#81  
 Benzo(a)anthracene  
 Concen: 2.315 ng  
 RT: 21.492 min Scan# 3112  
 Delta R.T. -0.000 min  
 Lab File: BM042503.D  
 Acq: 30 Oct 2023 20:43




Instrument : BNA\_M  
 ClientSampleId : RBR-200027DL


Tgt Ion	Resp	Lower	Upper
228	40924		
226	31.1	22.3	33.5
229	26.6	15.8	23.8

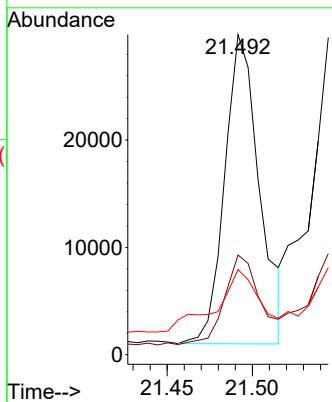

#83  
 Chrysene  
 Concen: 2.794 ng  
 RT: 21.545 min Scan# 3121  
 Delta R.T. -0.006 min  
 Lab File: BM042503.D  
 Acq: 30 Oct 2023 20:43

Tgt Ion	Resp	Lower	Upper
228	50176		
226	31.9	24.4	36.6
229	27.4	15.7	23.5









#84  
Bis(2-ethylhexyl)phthalate  
Concen: 3.417 ng  
RT: 21.374 min Scan# 3093  
Delta R.T. -0.006 min  
Lab File: BM042503.D  
Acq: 30 Oct 2023 20:43




Instrument :  
BNA\_M  
ClientSampleId :  
RBR-200027DL


Tgt Ion:149 Resp: 42084  
Ion Ratio Lower Upper  
149 100  
167 30.8 21.4 32.0  
279 5.8 3.4 5.2#



#86  
Perylene-d12  
Concen: 20.000 ng  
RT: 23.927 min Scan# 3526  
Delta R.T. -0.006 min  
Lab File: BM042503.D  
Acq: 30 Oct 2023 20:43

Tgt Ion:264 Resp: 347497  
Ion Ratio Lower Upper  
264 100  
260 24.4 19.0 28.4  
265 24.5 18.7 28.1









#88  
 Benzo(b)fluoranthene  
 Concen: 2.315 ng  
 RT: 23.186 min Scan# 3400  
 Delta R.T. -0.000 min  
 Lab File: BM042503.D  
 Acq: 30 Oct 2023 20:43

Instrument :  
 BNA\_M  
 ClientSampleId :  
 RBR-200027DL

Tgt Ion:252 Resp: 44824




Ion	Ratio	Lower	Upper
252	100		
253	28.5	17.5	26.3#
125	22.5	7.8	11.6#




#89  
 Benzo(k)fluoranthene  
 Concen: 2.078 ng  
 RT: 23.186 min Scan# 3400  
 Delta R.T. -0.047 min  
 Lab File: BM042503.D  
 Acq: 30 Oct 2023 20:43

Tgt Ion:252 Resp: 44824


Ion	Ratio	Lower	Upper
252	100		
253	28.5	17.6	26.4#
125	22.5	8.2	12.4#





#91  
 Dibenzo(a,h)anthracene  
 Concen: 4.171 ng  
 RT: 26.438 min Scan# 3960  
 Delta R.T. -0.042 min  
 Lab File: BM042503.D  
 Acq: 30 Oct 2023 20:43

Instrument :  
 BNA\_M  
 ClientSampleId :  
 RBR-200027DL



Tgt Ion: 278 Resp: 685

Ion	Ratio	Lower	Upper
278	100		
139	99.6	13.4	20.2#
279	57.9	19.7	29.5#

