
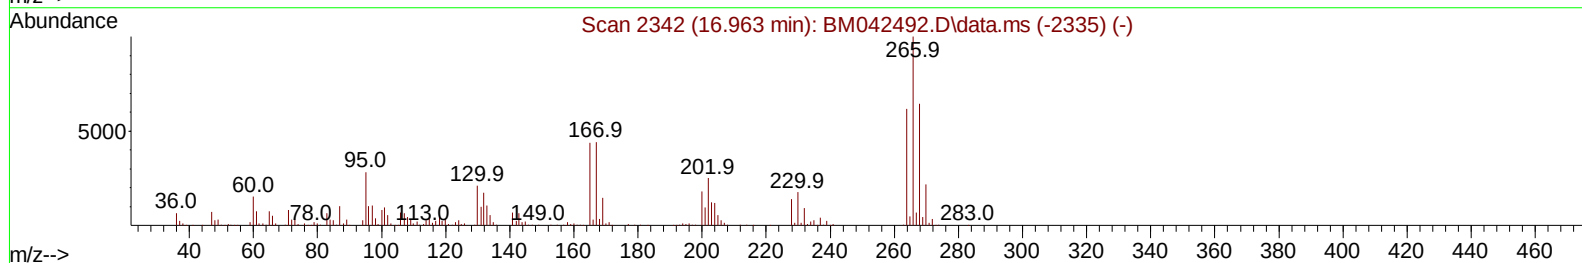
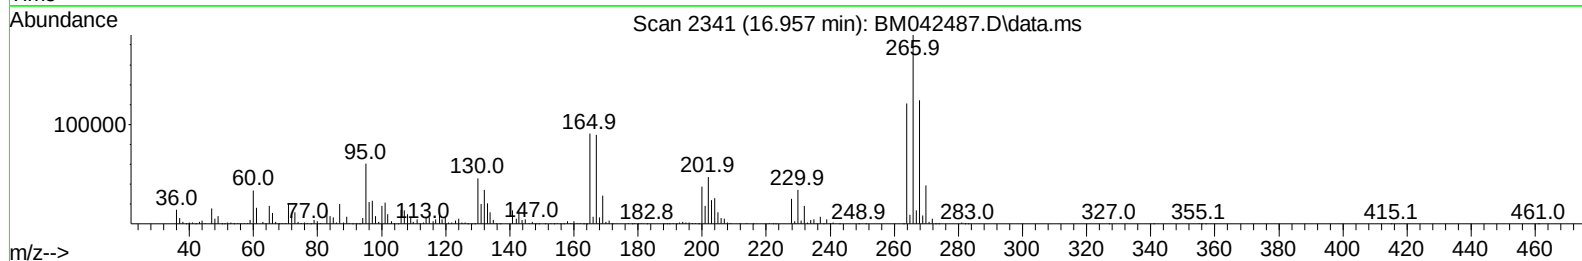


Quant Time: Oct 30 16:45:15 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM103023.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Oct 30 16:44:27 2023  
Response via : Initial Calibration

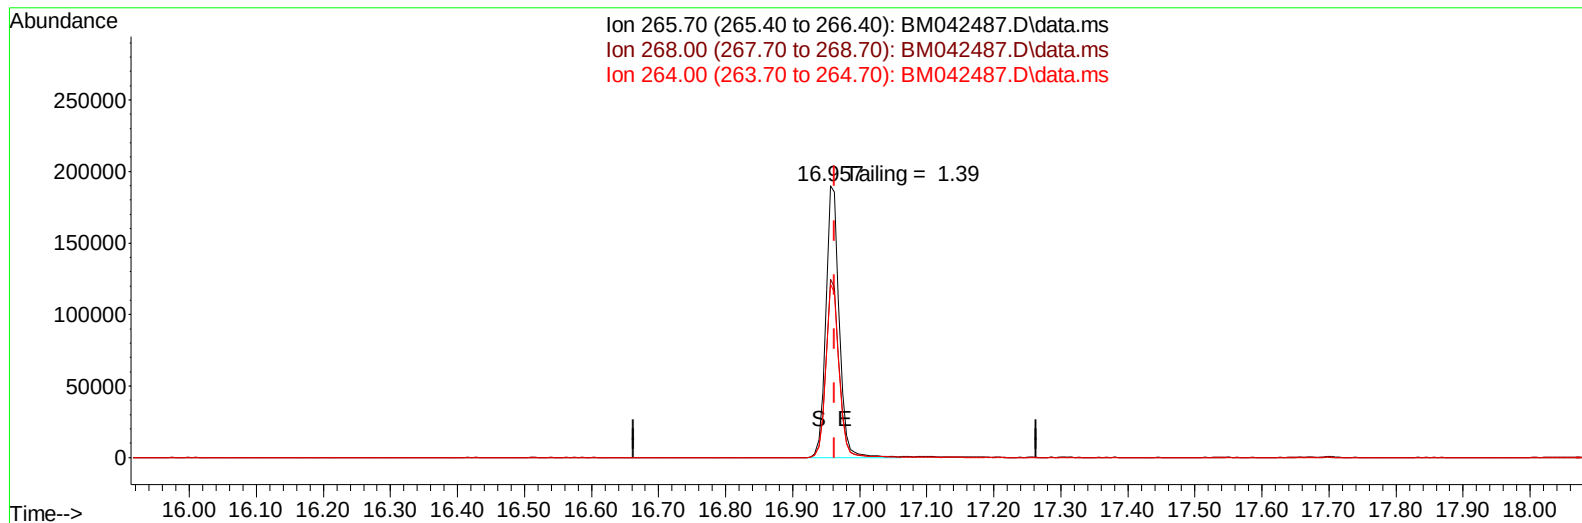

TIC: BM042487.D\data.ms

(70) Pentachlorophenol (C)




**16.957min (-0.006) 0.00 ng**

**response**      **264555**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.60  | 65.61  |
| 264.00 | 61.80  | 63.70  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM103023\  
Data File : BM042487.D  
Acq On : 30 Oct 2023 09:52  
Operator : MA/JU  
Sample : DFTTP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 30 16:45:15 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM103023.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Oct 30 16:44:27 2023  
Response via : Initial Calibration

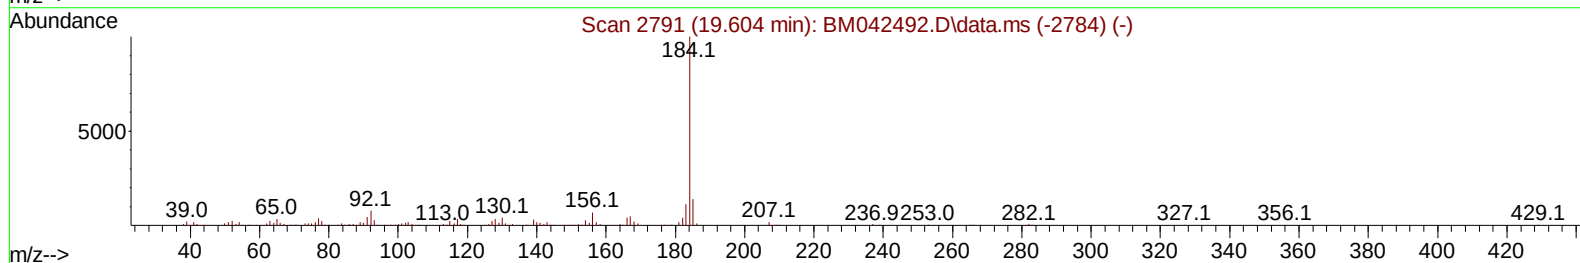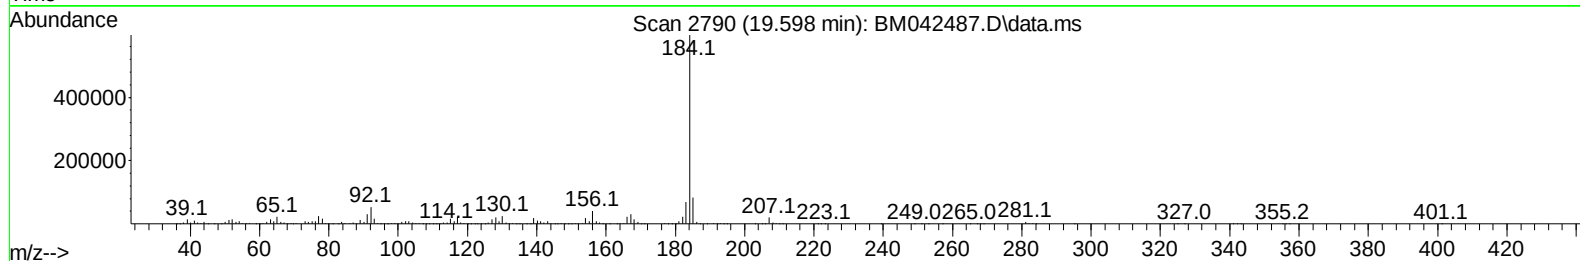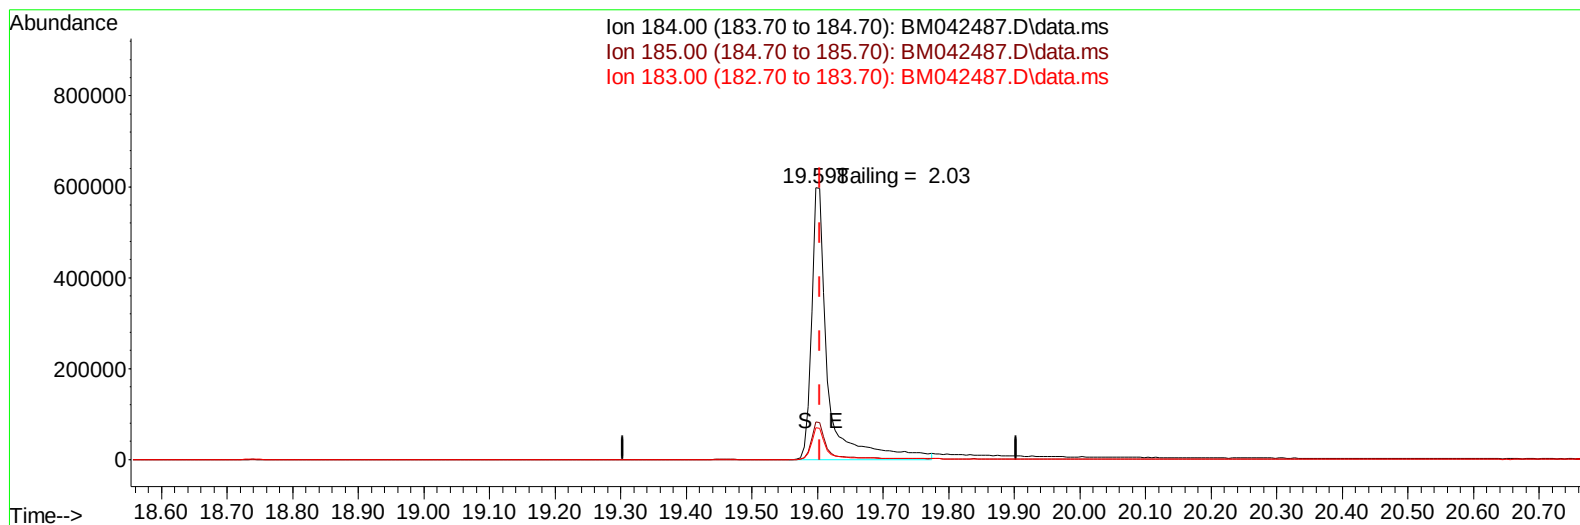

TIC: BM042487.D\data.ms

**(77) Benzidine****19.598min (-0.006) 107031.09 ng****response 1037677**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.00  | 13.89  |
| 183.00 | 11.20  | 11.58  |
| 0.00   | 0.00   | 0.00   |